


# THERMISTOR MOUNTS

OPERATING NOTE 6 DEC 66

## GENERAL INFORMATION

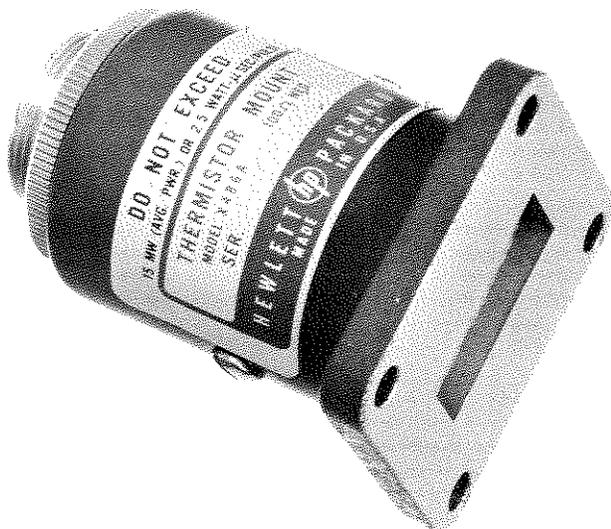

Ⓜ Model 486A Thermistor Mount

### 1. INTRODUCTION.

2. The Ⓜ Model 486A Thermistor Mounts are designed for use with the Ⓜ Model 431 Power Meter in the measurement of microwave power from 1  $\mu$ W to 10 mw in the range from 2.6 to 40.0 GHz. Design of power meter and thermistor mount are such that the measurement system is temperature-compensated. This feature permits microwave power measurements that are relatively free of the drift in meter indication that otherwise occurs with changes in ambient temperature.

3. For improved accuracy of measurement results, Calibration Factor and Effective Efficiency are measured at six selected frequencies across the operating range of each mount, and the results recorded on the label of the mount. In addition, each mount is tested on a swept-frequency basis to assure that interpolation between measured points is valid.

Table 1. Specifications

Model	Freq Range (Gc)	Max SWR	Operating Resistance (ohms)	Fits Waveguide Size		Equiv Flange JAN Type	Approx Length		Net Weight	
				Nominal OD (inches)	EIA		(inches)	(mm)	(oz)	(g)
S486A	2.6 - 3.95	1.35	100	3 x 1-1/2	WR284	UG-53/U	2-7/8	74	24	670
G486A	3.95 - 5.85	1.5	100	2 x 1	WR187	UG-149A/U	3-9/32	83	11	310
J486A	5.3 - 8.2	1.5	100	1-1/2 x 3/4	WR137	UG-344/U	3-5/32	80	8-1/2	240
H486A	7.05 - 10.0	1.5	100	1-1/4 x 5/8	WR112	UG-51/U	2-3/4	70	5-1/4	150
X486A	8.2 - 12.4	1.5	100	1 x 1/2	WR90	UG-39/U	2-1/8	54	3	80
M486A	10.0 - 15.0	1.5	100	0.850 x 0.475	WR75	--	2-1/8	54	3-1/4	90
P486A	12.4 - 18.0	1.5	100	0.702 x 0.391	WR51	UG-419/U	2-3/8	60	3-1/4	90
K486A <sup>1</sup>	18.0 - 26.5	2.0	200	1/2 x 1/4	WR42	UG-595/U	3	76	4-1/2	126
R486A <sup>1</sup>	26.5 - 40.0	2.0	200	0.360 x 0.220	WR28	UG-599/U	3	76	4-1/2	126

Mount Calibration: Calibration Factor and Effective Efficiency furnished at six frequencies. Maximum uncertainty of data:			Power Range (with Model 431): 1 $\mu$ w to 10 mw		
S- thru P-band	K- and R-band	431 Power Range (mw)	Power-Sensing Element: Permanently installed thermistor		
±1.5%	±2.5%	10	Output Connector: 6-pin connector mates with cable furnished with Ⓜ Model 431 Power Meter		
±1.5%	±2.5%	3			
±1.5%	±2.5%	1			
±1.5%	±2.5%	0.3			
±2%	±3%	0.1			
±3%	±4%	0.03			
±4%	±5%	0.01			
Plus uncertainty of reference standard. <sup>2</sup> See text for methods of obtaining increased accuracy.			<sup>1</sup> Circular contact flange adapter available: K-band (UG-425/U) order Ⓜ 11515A, R-band (UG-381/U) order Ⓜ 11516A		
			<sup>2</sup> Directly traceable to the National Bureau of Standards at those frequencies at which the Bureau offers calibration service.		

01189-10



4. Each Model 486A Mount is designed to provide a good impedance match (low SWR) over the full frequency range of its waveguide size without external tuning.

#### 5. INCOMING INSPECTION.

6. Unpack and inspect the Model 486A as soon as it is received. Inspect for mechanical damage such as dents, scratches, etc. Also check it electrically; if the mount was subjected to severe mechanical shock during shipment, the match between the thermistors will be affected. To check thermistor match, proceed as described in Paragraph 50.

7. If any damage is found, notify the carrier and your Hewlett-Packard Sales and Service Office immediately.

## OPERATION

#### 8. PRECAUTIONS.

#### 9. MECHANICAL SHOCK.

10. DO NOT DROP OR SUBJECT TO SEVERE MECHANICAL SHOCK. SHOCK MAY DESTROY THE MATCH BETWEEN THERMISTORS AND INCREASE SUSCEPTIBILITY TO DRIFT.

#### 11. BIASING THERMISTORS.

##### CAUTION

Before connecting a 200-ohm thermistor mount (K or R486A) to Model 431 Power Meters set MOUNT RES switch to 200  $\Omega$  position. CONNECTING A 200-OHM MOUNT TO A POWER METER SET FOR A 100-OHM MOUNT CAN RESULT IN THERMISTOR DAMAGE.

#### 12. MAXIMUM INPUT.

13. The Model 486A/431 combination responds to the average RF power applied. The maximum signal applied to the thermistor mount should not exceed the limitations for 1) average power, 2) pulse energy, and 3) peak pulse power. Excessive input can permanently damage the Model 486A by altering the match between the RF and compensation thermistors (resulting in excessive drift or zero shift) or cause error in indicated power.

14. **AVERAGE POWER.** The 486A/431 combination can measure average power up to 10 mW. To measure power in excess of 10 mW, a directional coupler (such as one of the Model 752 series) can be inserted between the mount and the source. UNDER NO CIRCUMSTANCES APPLY MORE THAN 15 MW AVERAGE TO THE MOUNT.

15. **PULSE ENERGY AND PEAK POWER.** In measuring pulse power, there is a limit on the energy per pulse which may be applied to the mount. For a pulse repetition frequency (PRF) less than 1 kHz, energy per pulse can be up to 2.5 Watt- $\mu$ sec; for a PRF 1 kHz and above, up to 5 Watt- $\mu$ sec (for lack of space, only the lower limit is shown on the mount name plate). However, this energy limit applies only to pulses shorter than 250  $\mu$ sec. In Figure 1, the pulse energy limit is translated into a maximum power-meter reading for any PRF. For pulses in this category, allowable peak power is inversely proportional to pulse width but should never exceed 100 Watts.

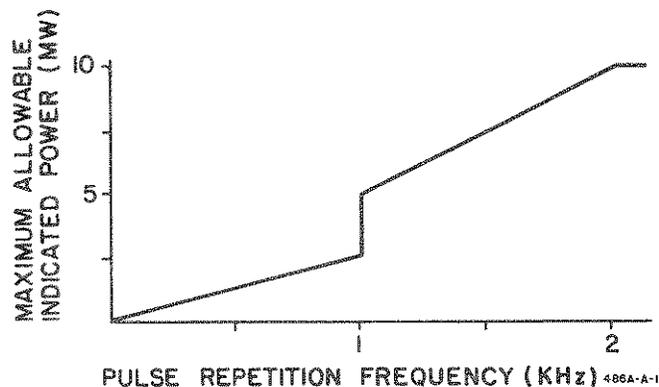


Figure 1. Maximum Power Meter Reading vs. PRF for Pulses Shorter than 250  $\mu$ sec

16. For pulses longer than 250  $\mu$ sec, the peak power limitation can be expressed in terms of PRF: 10 mW for a PRF below 1 kHz, 20 mW for a PRF 1 kc or above provided 15 mW average is not exceeded. In Figure 2, the peak power limit is translated into power-meter reading versus duty cycle. (For a PRF less than 1 kHz and an indicated power between 2 and 3 mW, use the 10-mW range. Errors as much as 2% may be introduced if the 3-mW range is used.)

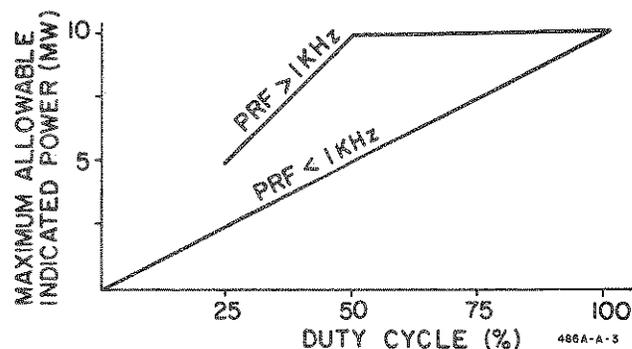


Figure 2. Maximum Power Meter Reading vs. Duty Cycle for Pulses Longer than 250  $\mu$ sec

17. Square-wave modulation is a special case of pulse modulation, and maximum power-meter reading versus square-wave frequency is illustrated in Figure 3. This figure also holds for sine-wave modulation.

18. In the discussions above, the primary consideration is maximum power or energy. However, for modulation frequencies less than 100 Hz, the low

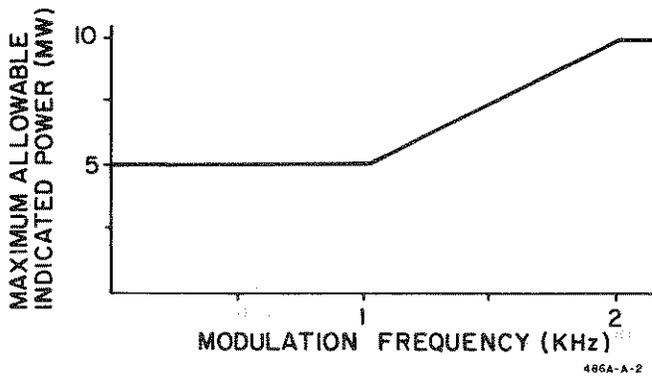


Figure 3. Maximum Power Meter Reading vs. Square- and Sine-Wave Modulation Frequency

repetition frequency itself causes errors in indicated power. These errors may be as large as 2% regardless of range or reading.

#### 19. DRIFT.

20. Thermistors are inherently temperature sensitive devices. A cold thermistor mount connected to a warm piece of equipment or vice versa, produces rapid drift. FOR MINIMUM DRIFT ON SENSITIVE RANGES MAKE SURE THAT THE MOUNT AND THE EQUIPMENT CONNECTED TO IT ARE AT NEARLY THE SAME TEMPERATURE BEFORE MAKING A MEASUREMENT.

#### 21. ZERO-SET.

22. It is necessary to electrically zero-set the Model 431 Power Meter before making a power measurement. To preserve the same zero reference throughout the measurement, especially when operating on the more sensitive ranges, maintain the same thermal environment when RF power is applied. Three recommended setups for zero-set are presented below:

a. RF Power Turned Off for Zero-Set. There is minimum zero drift when zero is set with the RF system connected to the thermistor mount and RF power turned off at the generator or shorted out by a shorting switch. After allowing time for the mount to stabilize thermally, follow the steps for zero-set described in the Model 431 Power Meter manual, and then turn on the RF power for measurement.

b. Use of High Attenuation with RF Source On. When it is inconvenient to turn off the RF source for zero-set, connect a waveguide variable attenuator, such as the  $\Phi$  Model 382A, between the RF system and the thermistor mount. Attenuate the RF power approximately 30 dB for zero-set, and reduce attenuation to zero during the measurement.

c. Disconnect the Mount for Zero-Set. When the RF source cannot be turned off, shorted, or attenuated, connect the mount to the source, and set the range of the Model 431 Power Meter for approximately a mid-scale reading. When the reading no longer drifts, disconnect the mount from the RF source and im-

mediately zero-set the power meter according to the procedure described in the Model 431 manual. Immediately reconnect the mount to the RF source for the power measurement. IN THE PROXIMITY OF A HIGH RF FIELD, SHIELD THE DISCONNECTED THERMISTOR MOUNT FROM POSSIBLE STRAY RF PICK-UP DURING THE ZERO SET.

#### 23. POWER MEASUREMENT.

24. The thermistor has a long thermal time constant, which causes it to respond to average microwave power whether CW or modulated (pulse, sine wave, or square wave).

25. In pulse modulation, response is proportional to the amplitude and the duty cycle of the pulse. The power level of an individual pulse can be determined by dividing the average power reading by the duty cycle of the pulse. Accurate measurements can be made with pulse repetition rates as low as 50 Hz.

26. To measure microwave power in excess of 10 mW insert a calibrated attenuator, such as one of the  $\Phi$  382A, or 375A series, or a directional coupler, such as one of the  $\Phi$  752/750 series, between the mount and the RF source to be measured.

#### 27. RESPONSE TO DC (POLARIZATION EFFECT).

28. When a DC current is applied to a thermistor, the power apparently dissipated (as indicated by the power meter when the thermistor is part of a power-measuring bridge) will be slightly different from the power found by calculating  $I^2R$ , and the magnitude of this small difference between apparent and actual power will change with a reversal of current-flow through the thermistor. This behavior of the thermistor is called the polarization effect. Maximum error introduced by polarization effect is about  $0.3 \mu\text{W}$ , and typically this error will be only  $0.1 \mu\text{W}$ . Except on the three lowest ranges of the Model 431, therefore, polarization error is insignificant. To determine the polarization-effect correction factor for any given thermistor, apply a known low-level DC power, such as  $10 \mu\text{W}$ , to the Model 431, and take a reading ( $P_{DCa}$ ); reverse connection between DC source and Model 431 to get a reverse in current flow, and again take a reading ( $P_{DCb}$ ). Assuming that, under measurement conditions, current-flow will have the direction it had when reading  $P_{DCa}$  was made, subtract  $P_{DCa}$  from  $P_{DCb}$ , and divide the difference by two; this is the polarization-effect correction factor. Step-by-step instructions for determining and applying this correction factor are given in the manual for the HP Model 8402 Power Meter Calibrator.

#### 29. CALIBRATION DATA.

30. The calibration points marked on the label of each 486A permit increased accuracy in measurement results. Both Calibration Factor and Effective Efficiency are shown at specific frequencies, and the

mounts are tested on a swept-frequency basis to assure that interpolation between measured points is valid. Effective Efficiency and Calibration Factor are traceable to the National Bureau of Standards to the extent allowed by the Bureau's calibration facilities.

31. **CALIBRATION FACTOR.** Calibration Factor is the ratio of substituted audio or DC power in a thermistor mount to the microwave RF power incident upon the mount.

$$\text{Calibration Factor} = \frac{P_{\text{DC Substituted}}}{P_{\mu\text{wave Incident}}}$$

32. Calibration Factor is a figure of merit assigned to a thermistor mount to correct for the following sources of error: 1) RF reflected by the mount due to mismatch, 2) RF loss caused by absorption within the detection thermistor elements, and 3) DC-to-microwave power substitution error. Calibration Factor is applied as a correction factor to all measurements made without a tuner. When these factors and thermoelectric effect (refer to Paragraph 37) are taken into consideration, the power indicated is the power that would be delivered by the RF source to the characteristic impedance of the transmission line. The total SWR in the transmission line determines a region of uncertainty about the measured power. This subject is discussed in Application Note 64, available from any Hewlett-Packard Sales and Service Office.

33. **EFFECTIVE EFFICIENCY.** Effective Efficiency is the ratio of substituted audio or DC power in a thermistor mount to the microwave RF power dissipated within the mount.

$$\text{Effective Efficiency} = \frac{P_{\text{DC Substituted}}}{P_{\mu\text{wave Dissipated}}}$$

34. Effective Efficiency corrects for power absorbed in parts of the mount other than the detection thermistor elements and DC-to-microwave power substitution error in the thermistor mount. Effective Efficiency is applied as a correction factor when a tuner is used to match the thermistor mount to the transmission line or RF source. In this case, all of the RF power incident upon the mount is absorbed in the mount. Since all power is absorbed in the mount, measurement uncertainty due to mount SWR is eliminated.

### 35. MISMATCH ERROR.

36. Errors caused by mismatch result when the mount does not provide a  $Z_0$  termination. The term Calibration Factor describes the combination of Effective Efficiency and mismatch errors. The Calibration Factor of a thermistor mount equals the percentage of incident power which effectively heats the thermistor. Calibration Factor is always equal to or less than Effective Efficiency. The terms are related by the equation:

$$\text{CAL FACTOR} = \text{EFF EFFICIENCY} (1 - \rho_m^2)$$

( $\rho_m^2$  = reflection coefficient of the mount)

### 37. CALIBRATION DATA APPLICATION.

38. When the 486A is used with the Model 431C Power Meter, Calibration Factor or Effective Efficiency correction can be made by the setting of a front panel switch. With the proper setting, the 431C compensates for the Calibration Factor or Effective Efficiency of the 486A. If the 486A is used with a power meter other than the 431C, Calibration Factor or Effective Efficiency correction can be made by dividing the measured power by the Calibration Factor or Effective Efficiency value respectively.

### 39. THERMOELECTRIC EFFECT.

40. Mount calibration uncertainties given in Table 1 include inaccuracies caused by thermoelectric effect error. Calibration Factor uncertainty of  $\pm 1.5\%$  and Effective Efficiency uncertainty of  $\pm 2.5\%$  can be maintained on the three lowest power ranges of the Model 431 series Power Meters by correcting for the measurement error introduced by thermoelectric effect. An error correction procedure is given in Paragraph 44.

41. A mild thermocouple exists at each point of contact where the connecting wires join to the thermistor elements. Each thermocouple creates a DC voltage. Thus, two thermocouple voltages of opposite relative polarity are formed, one at each junction to each thermistor element.

42. Ideally, each thermocouple voltage would be equal in magnitude so that they cancel with no resultant effect on the accuracy of power measurement. In practice, however, each point of contact does not have identical thermocouple characteristics, and in addition, the temperatures at each junction may not be the same. These differences cause an incomplete cancellation of the thermoelectric voltages, resulting in a voltage that causes a thermoelectric effect error. The magnitude of the error is important when making DC substitution measurements on the 0.1 mW, 0.03 mW, and 0.01 mW ranges with one of the Model 431-series Power Meters. On other ranges, the effect is negligible. Maximum error introduced by thermoelectric effect is about  $0.3 \mu\text{W}$  and is typically  $0.1 \mu\text{W}$  on the .01 mW range.

### 43. THERMOELECTRIC EFFECT ERROR CORRECTION.

44. Use the following technique to correct for thermoelectric effect error.

a. Measure power.

b. Connect an  $\text{\textcircled{P}}$  Model 8402 Power Meter Calibrator to the power meter DC CALIBRATION AND SUBSTITUTION jack.

c. Zero and null power meter.

d. By DC Substitution (refer to procedure in 431 Manual), duplicate power measurement made in step a. Calculate and record substituted power as  $P_1$ .

e. Reverse connection polarity between the calibrator and power meter.

f. Re-zero and re-null power meter, if necessary.

g. By DC Substitution, duplicate power measurement made in step a. Calculate and record substituted power as  $P_2$ .

h. Calculate arithmetic mean of the two substitution powers  $P_1$  and  $P_2$ . This mean power includes a correction for thermoelectric effect error.

$$\text{Power} = \frac{P_1 + P_2}{2}$$

### OPERATING PRINCIPLES

45. The matched thermistor pair, C and D (C is used for thermal compensation, and D for RF detection), are mounted in an isolated common thermal environment represented by the shaded rectangle in Figure 4. Electrically, however, the thermistors are isolated from each other, D being mounted inside the waveguide and exposed to incoming RF, while C is entirely shielded from RF. A correct amount of 10-kHz bias is supplied through a cable from the Model 431 Power Meter to heat D to its operating resistance (100 ohms  $\pm 1\%$  or 200 ohms  $\pm 1\%$ ). An equal amount of 10-kHz bias, together with a DC bias, is supplied to heat C to the same operating resistance. As indicated in Figure 4, the total power applied to heat thermistor D consists of incoming RF, 10-kHz bias, and heat from the environment. The total heating power to compensating thermistor C consists of DC bias, 10-kHz bias, and the same environmental heat. As D and C are matched thermally, only equal amounts of heating power can bias them to equal operating resistances. Restating the foregoing algebraically: under normal operation

$$P_{\text{total to D}} = P_{\text{total to C}}$$

where

$$P_{\text{total to D}} = P_{\text{RF to D}} + P_{\text{10kHz to D}} + P_{\text{env heat to D}}$$

and

$$P_{\text{total to C}} = P_{\text{DC to C}} + P_{\text{10kHz to C}} + P_{\text{env heat to C}}$$

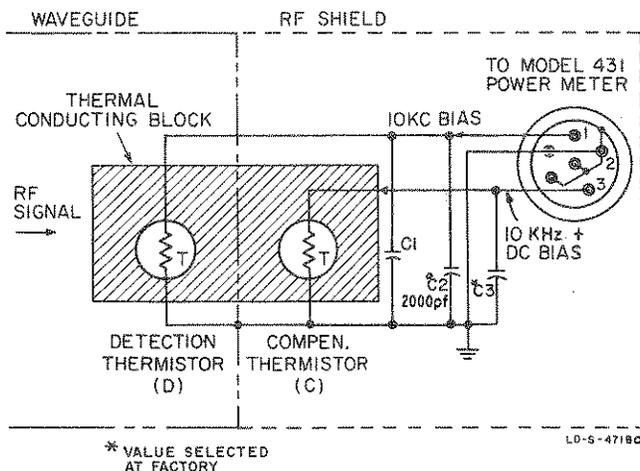


Figure 4. Thermistor Mount Schematic Diagram

Since the thermistors share the same thermal environment

$$P_{\text{env heat to D}} = P_{\text{env heat to C}}$$

and since

$$P_{\text{10kHz to D}} \text{ is made} = P_{\text{10 kHz to C}}$$

this leaves

$$P_{\text{RF to D}} = P_{\text{DC to C}}$$

The  $P_{\text{DC to C}}$  is monitored by the Model 431 Power Meter, and since  $P_{\text{DC}}$  is made equal to  $P_{\text{RF}}$ , the Model 431 meter indicates the magnitude of the RF power.

46. The above equations assume perfect accuracy in the components; in practice, however, there is a small offset which is balanced out by the zero-set adjustment so that the meter indication will be zero with no RF power applied. Also, for best accuracy, the slight differential thermal drift between components may require occasional zero reset on the most sensitive ranges.

### MAINTENANCE

#### 47. CHECK ON THERMISTOR MATCH.

48. Damage to the match between the thermistors may be checked at room temperature by comparing the thermistor resistances under simulated operating conditions. Connect the equipment to the pins of the connector at the rear of the thermistor mount as shown in Figure 5. Select a suitable bucking DC voltage to reduce the voltage across the digital voltmeter for readings down to the nearest 0.001 volt. Take readings with switches connected to pin 1 and then to pin 3. Thermistor match is satisfactory if the two readings do not differ by more than 0.015 volt.

#### 49. CLEANLINESS.

50. Except for the K and R Models, thermistor D (mounted inside the waveguide) is protected against air currents, dirt, and mechanical damage by two layers of polyfoam plastic. Polyfoam is soluble in most volatile solvents, such as gasoline, alcohol, benzene, carbon tetrachloride, acetone, etc., so great

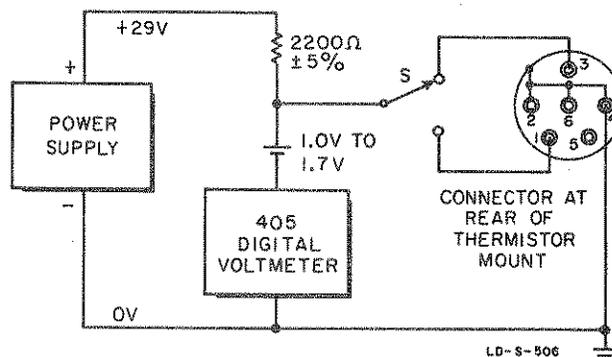


Figure 5. Check on Model 486A Thermistor Resistance Match

care should be used if one of these is used to clean the flange or inner surfaces of the waveguide. Use the plastic flange cover to protect the mount from dirt and mechanical damage whenever it is not in use. Any burn, dents or dirt on the flange or waveguide surfaces will increase the SWR. This is particularly important in the case of the K486A and R486A, which do not have the polyfoam plastic protection.

#### 51. REPAIR.

52. Exceeding the CW or pulse power limits of the Model 486A Thermistor Mount may result in damage such that the mount will no longer zero on the Model 431 Power Meter.

53. Before adjusting the mount in any way, make sure that the mount is the cause of the problem. If the 431 Power Meter remains pegged downscale when ZERO is rotated through its range, measure the resistance between pins 1 and 2, and between pins 2 and 3 of the 6-pin connector. This resistance should be between 500 and 5000 ohms. If the resistance in both cases is within this range, the mount may be repairable. An open or short indication calls for factory repair.

54. If possible, test the mount by connecting it to a Model 431 and cable which are known to be good. A faulty cable will not have continuity through the respective connector pins, or may have poor contact at the mount connector. Poor contact will show up as intermittence or a great deal of noise (visible on the 431 meter) when the cable is gently flexed near the connector end.

55. If the 431 meter remains pegged upscale, factory repair of the mount is indicated.

#### CAUTION

Under no conditions should the mount be required to carry current higher than 10 ma.

#### 56. MOUNT COMPENSATION.

57. If the resistance reading of the mount is satisfactory, it may be possible to recompensate the mount, and return it to service. The drift with temperature changes will be higher because of damage to the thermistors, but it will be possible to zero the meter and to make measurements.

#### NOTE

After recompensation the Calibration Factor and Effective Efficiency recorded on the label of the mount will no longer be valid. If desired, the instrument may be sent to the factory for repair and recalibration. Any Hewlett-Packard Sales and Service Office will arrange for such repair.

58. There is an adjusting screw inside the instrument which permits recompensation within limits. Instruments which were manufactured without the adjusting screw are modified when they are sent in for repair.

59. To recompensate the mount, refer to Figure 6, and proceed as follows:

- a. Remove cover screws (A).
- b. Slide instrument out of cover.
- c. Set 431 MOUNT RES to proper value.
- d. Plug cover into mount cable.
- e. Set ZERO and VERNIER to mid-range.
- f. Set RANGE to 10 mW.
- g. If meter is pegged upscale, turn compensating screw (B) counterclockwise to zero meter.
- h. If meter is pegged downscale, turn screw clockwise to zero meter.

#### WARNING

If there is a sudden jump in meter indication when turning compensating screw clockwise, back off 1/8 turn. If screw bottoms, do not apply force. Factory repair is indicated.

- i. Replace cover and cover screws (A).

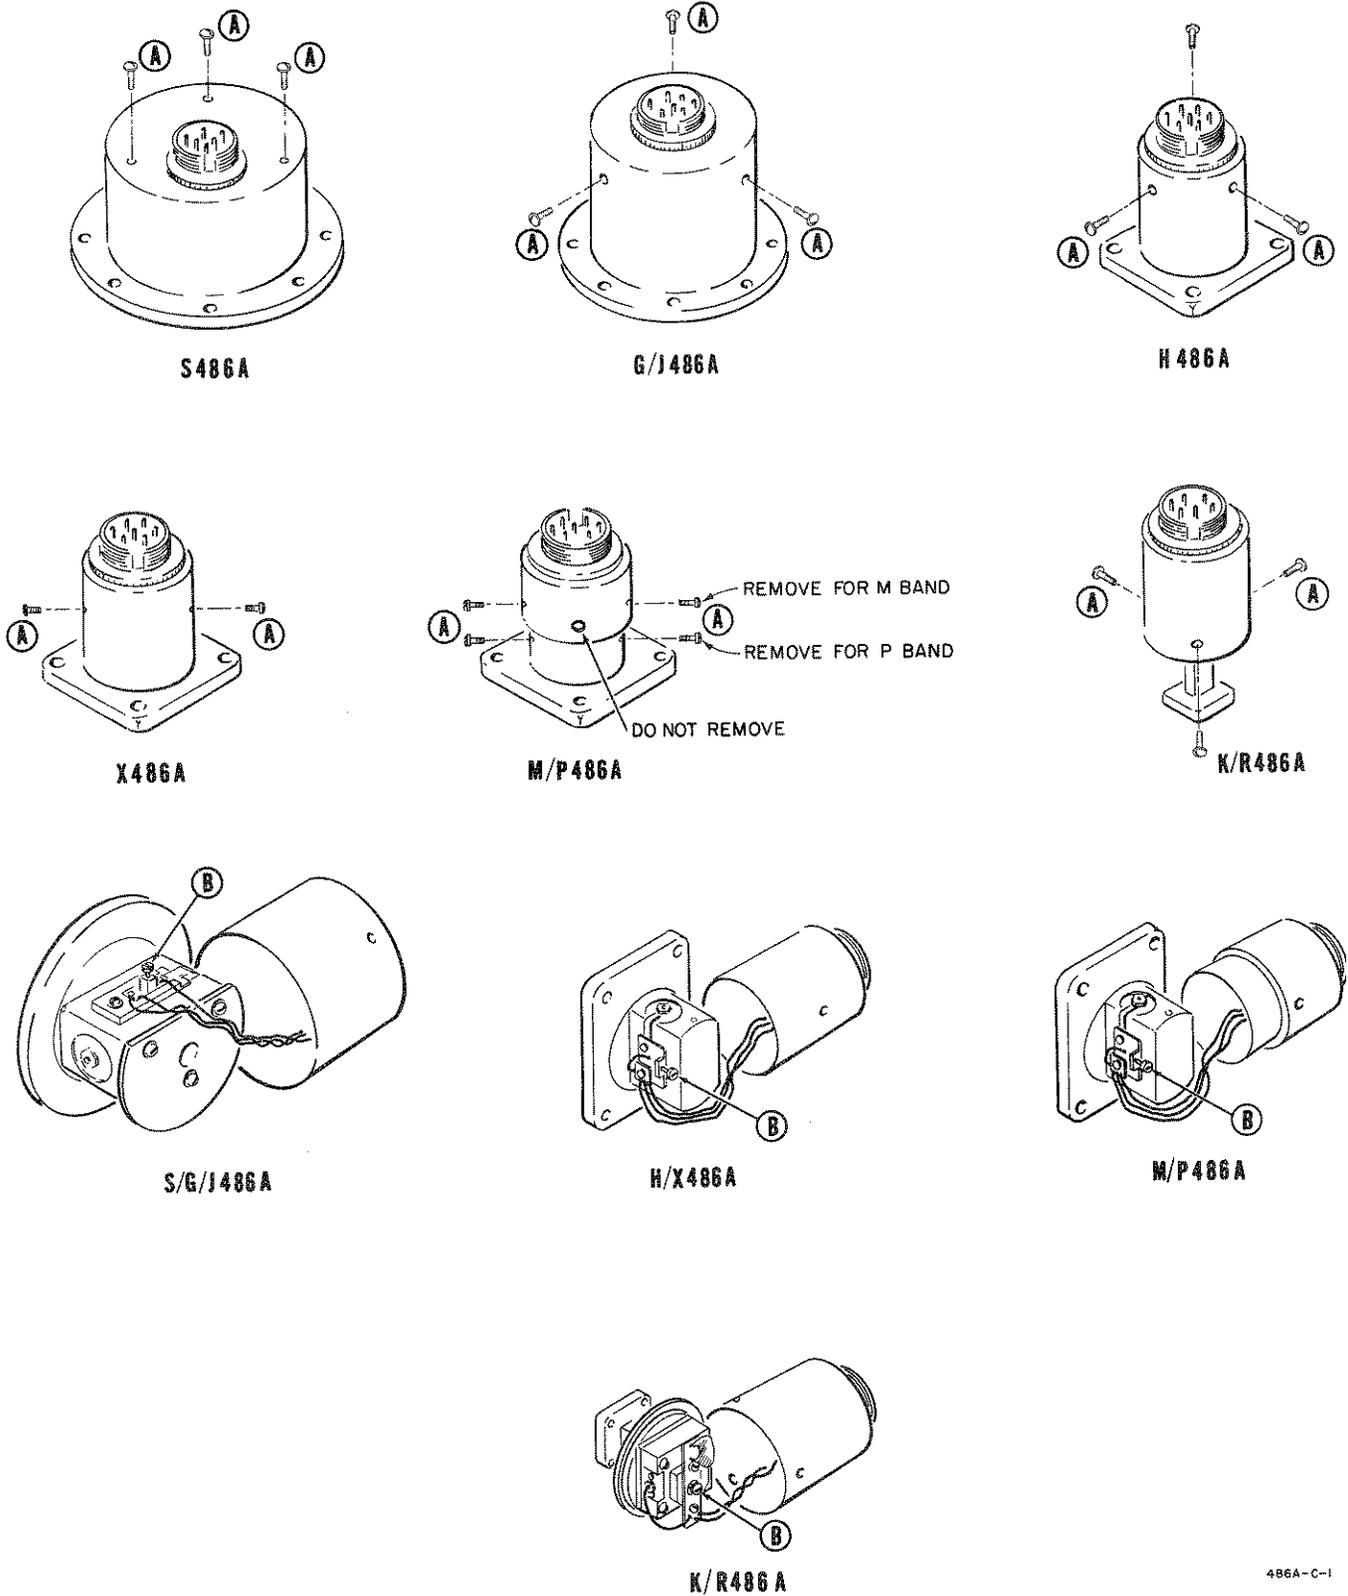


Figure 6. Cover Screws (A) and Compensating Screws (B) in Model 486A Thermistor Mounts

## HEWLETT·PACKARD

## ELECTRONIC INSTRUMENTATION SALES AND SERVICE

UNITED STATES, CENTRAL AND SOUTH AMERICA, CANADA

## UNITED STATES

**ALABAMA**  
P.O. Box 4207  
2003 Byrd Spring Road S.W.  
Huntsville 35802  
Tel: (205) 881-4591  
TWX: 810-726-2204

**ARIZONA**  
3009 North Scottsdale Road  
Scottsdale 85251  
Tel: (602) 945-7601  
TWX: 910-850-1282

5737 East Broadway  
Tucson 85716  
Tel: (602) 298-2313  
TWX: 910-952-1162

**CALIFORNIA**  
3939 Lankershim Boulevard  
North Hollywood 91604  
Tel: (213) 877-1282  
TWX: 910-499-2170

1101 Embarcadero Road  
Palo Alto 94303  
Tel: (415) 327-6500  
TWX: 910-373-1280

2581 Carlsbad Avenue  
Sacramento 95821  
Tel: (916) 482-1463  
TWX: 910-267-2092

1955 Shafter Street  
San Diego 92106  
Tel: (714) 223-8103  
TWX: 910-335-2000

**COLORADO**  
7965 East Prentice  
Englewood 80110  
Tel: (303) 771-3455  
TWX: 910-935-0705

**CONNECTICUT**  
508 Tolland Street  
East Hartford 06108  
Tel: (203) 289-9394  
TWX: 710-425-3476

111 East Avenue  
Norwalk 06851  
Tel: (203) 853-1251  
TWX: 710-468-3750

**DELAWARE**  
3941 Kennett Pike  
Wilmington 19807  
Tel: (302) 655-6161  
TWX: 510-666-2214

**FLORIDA**  
P.O. Box 545  
Suite 106  
9999 N.E. 2nd Avenue  
Miami Shores 33153  
Tel: (305) 758-3626  
TWX: 810-848-7262

P.O. Box 20007  
Herndon Station 32814  
621 Commonwealth Avenue  
Orlando  
Tel: (305) 841-3970  
TWX: 810-850-0113

P.O. Box 8128  
Melrose Beach 33708  
410 150th Avenue  
St. Petersburg  
Tel: (813) 391-0211  
TWX: 810-863-0366

**GEORGIA**  
P.O. Box 28234  
2340 Interstate Parkway  
Atlanta 30328  
Tel: (404) 436-6181  
TWX: 910-766-4890

**ILLINOIS**  
5500 Howard Street  
Skokie 60076  
Tel: (312) 677-0400  
TWX: 910-223-3613

**INDIANA**  
4002 Meadows Drive  
Indianapolis 46205  
Tel: (317) 546-4891  
TWX: 810-341-3263

**LOUISIANA**  
P.O. Box 856  
1942 Williams Boulevard  
Kenner 70062  
Tel: (504) 721-6201  
TWX: 810-955-5524

**MARYLAND**  
6707 Whitestone Road  
Baltimore 21207  
Tel: (301) 944-5400  
TWX: 710-862-0850

P.O. Box 727  
Twinbrook Station 20851  
12303 Twinbrook Parkway  
Rockville  
Tel: (301) 427-7560  
TWX: 710-828-9684

**MASSACHUSETTS**  
32 Hartwell Road  
Lexington 02173  
Tel: (617) 861-8960  
TWX: 710-332-0382

**MICHIGAN**  
24315 Northwestern Highway  
Southfield 48075  
Tel: (313) 353-9200  
TWX: 810-232-1532

**MINNESOTA**  
2459 University Avenue  
St. Paul 55114  
Tel: (612) 645-9461  
TWX: 910-563-3734

**MISSOURI**  
9208 Wyoming Place  
Kansas City 64114  
Tel: (816) 333-2445  
TWX: 910-771-2087

2812 South Brentwood Blvd.  
St. Louis 63144  
Tel: (314) 644-0220  
TWX: 910-760-1670

**NEW JERSEY**  
W. 120 Century Road  
Paramus 07652  
Tel: (201) 265-5000  
TWX: 710-990-4951

**NEW MEXICO**  
P.O. Box 8366  
Station C  
6501 Lomas Boulevard N.E.  
Albuquerque 87108  
Tel: (505) 255-5586  
TWX: 910-989-1665

156 Wyatt Drive  
Las Cruces 88001  
Tel: (505) 526-2485  
TWX: 910-983-0550

**NEW YORK**  
1702 Central Avenue  
Albany 12205  
Tel: (518) 858-8452  
TWX: 710-441-8270

1219 Campville Road  
Endicott 13764  
Tel: (607) 754-0050  
TWX: 510-252-0890

82 Washington Street  
Poughkeepsie 12601  
Tel: (914) 454-7330  
TWX: 510-248-0012

39 Saginaw Drive  
Rochester 14623  
Tel: (716) 473-9500  
TWX: 510-253-5981

1025 Northern Boulevard  
Roslyn, Long Island 11576  
Tel: (516) 869-8400  
TWX: 510-223-0811

5858 East Molloy Road  
Syracuse 13211  
Tel: (315) 454-2486  
TWX: 710-541-0482

**NORTH CAROLINA**  
P.O. Box 5188  
1923 North Main Street  
High Point 27262  
Tel: (919) 882-6873  
TWX: 910-926-1516

**OHIO**  
5579 Pearl Road  
Cleveland 44129  
Tel: (216) 884-9209  
TWX: 810-421-6500

3460 South Dixie Drive  
Dayton 45428  
Tel: (513) 298-0351  
TWX: 810-459-1925

**OKLAHOMA**  
2919 United Founders Boulevard  
Oklahoma City 73112  
Tel: (405) 848-2801  
TWX: 910-830-6862

**OREGON**  
Westhill Mall, Suite 158  
4475 S.W. Scholls Ferry Road  
Portland 97225  
Tel: (503) 292-9171  
TWX: 910-464-6103

**PENNSYLVANIA**  
2500 Moss Side Boulevard  
Menroville 15146  
Tel: (412) 271-0724  
TWX: 710-797-3650

144 Elizabeth Street  
West Conshohocken 19428  
Tel: (215) 248-1600, 828-6200  
TWX: 510-660-8715

**TEXAS**  
P.O. Box 7166  
3605 Inwood Road  
Dallas 75209  
Tel: (214) 357-1881  
TWX: 910-861-4081

P.O. Box 22813  
4242 Richmond Avenue  
Houston 77027  
Tel: (713) 667-2407  
TWX: 910-881-2645

**GOVERNMENT CONTRACT OFFICE**  
225 Billy Mitchell Road  
San Antonio 78226  
Tel: (512) 434-4171  
TWX: 910-871-1170

**UTAH**  
2890 South Main Street  
Salt Lake City 84115  
Tel: (801) 486-8165  
TWX: 910-925-5681

**VIRGINIA**  
P.O. Box 6514  
2111 Spencer Road  
Richmond 23230  
Tel: (703) 282-5451  
TWX: 710-956-0157

**WASHINGTON**  
433-108th N.E.  
Bellevue 98004  
Tel: (206) 454-3571  
TWX: 910-443-2303

**FOR U.S. AREAS NOT LISTED:**  
Contact the regional office nearest you:  
Atlanta, Georgia... North Hollywood, California... Paramus, New Jersey... Skokie, Illinois. Their complete addresses are listed above.

## CENTRAL AND SOUTH AMERICA

**ARGENTINA**  
Hewlett-Packard Argentina  
S.A.C.e.I.  
Lavalle 1171 - 3º  
Buenos Aires  
Luz, Ferrando y Cla. S. A.  
Florida 240 (R.5)  
Buenos Aires  
Tel: 46-7241, 46-1635  
Cable: OPTICA Buenos Aires

**BRAZIL**  
Hewlett-Packard Do Brasil  
l.e.C. Ltda.  
Rua Cel. Oscar Porto, 691  
Sao Paulo - 8, SP  
Tel: 71-1503  
Cable: HEWPAK Sao Paulo

Hewlett-Packard Do Brasil  
l.e.C. Ltda.  
Avenida Franklin Roosevelt 84  
Grupo 203  
Rio de Janeiro, 20-39, GB  
Tel: 32-9733  
Cable: HEWPAK Rio de Janeiro

**CHILE**  
Hector Calcagni P.  
Casilla 13942  
Estado 215 - Oficina 1016  
Santiago  
Tel: 31-890, 490-505

**COLOMBIA**  
Instrumentacion  
Henrik A. Langebaek & Cia. Ltda.  
Carrera 7 # 48-59  
Apartado Aéreo 6287  
Bogota, l. D.E.  
Tel: 45-78-06, 45-55-46  
Cable: AARIS Bogota

**COSTA RICA**  
Lic. Alfredo Gallagos Gardian  
Apartado 3243  
San José  
Tel: 21-86-13  
Cable: GALGUR San José

**ECUADOR**  
Laboratorios de Radio-Ingenieria  
Calle Guayaquil 1246  
Post Office Box 3199  
Quito  
Tel: 12496  
Cable: HORVATH Quito

**EL SALVADOR**  
Electronica  
Apartado Postal 1589  
27 Avenida Norte 1133  
San Salvador  
Tel: 25 74 50  
Cable: ELECTRONICA San Salvador

**GUATEMALA**  
Olander Associates Latin America  
Apartado 1226  
7a. Calle, 0-22, Zona 1  
Guatemala City  
Tel: 22812  
Cable: OLALA Guatemala City

**MEXICO**  
Hewlett-Packard Mexicana, S.A.  
de C.V.  
Apartado Postal 12-832  
Eugenia 408, Dept. 1  
Mexico 12, D.F.  
Tel: 43-03-79, 36-08-78

**NICARAGUA**  
Roberto Terán G.  
Apartado Postal 689  
Edificio Terán  
Managua  
Tel: 3451, 3452  
Cable: ROTERAN Managua

**PANAMA**  
Electronica Balboa, S.A.  
Apartado Postal 4929  
Ave. Manuel Espinosa No. 13-50  
Bldg. Alina  
Panama City  
Tel: 30833  
Cable: ELECTRON Panama City

**PERU**  
Fernando Ezeta B.  
Avenida Petit Thouars 4719  
Miraflores  
Casilla 3061  
Lima  
Tel: 50346  
Cable: FEPERU Lima

**PUERTO RICO**  
San Juan Electronics, Inc.  
P.O. Box 5167  
Ponce de Leon 154  
Pda. 3-Pta. de Tierra  
San Juan, P.R. 00906  
Tel: (174) 725-3342  
Cable: SATRONICS San Juan

Hewlett-Packard (Canada) Ltd.  
1415 Lawrence Avenue West  
Toronto  
Tel: (416) 249-9196  
TWX: 610-492-2362

**URUGUAY**  
Pablo Ferrando S.A.  
Comercial e Industrial  
Avenida Italia 2877  
Casilla de Correo 370  
Montevideo  
Tel: 40-3102  
Cable: RADIOM Montevideo

**VENEZUELA**  
Hewlett-Packard De Venezuela C.A.  
Edificio Arisan-Of. 4  
Ave. Francisco de Miranda  
Chacarito  
Caracas  
Tel: 71-88-05  
Cable: HEWPAK Caracas  
Mailing Address: Apartado del  
Este 10934 Caracas

**FOR AREAS NOT LISTED,  
CONTACT:**  
Hewlett-Packard Inter-Americas  
1501 Page Mill Road  
Palo Alto, California 94304  
Tel: (415) 326-7000  
TWX: 910-373-1267  
Telex: 034-8461  
Cable: HEWPAK Palo Alto

## CANADA

**ALBERTA**  
Hewlett-Packard (Canada) Ltd.  
11745 Jasper Avenue  
Edmonton  
Tel: (403) 482-5561  
TWX: 610-831-2431

**BRITISH COLUMBIA**  
Hewlett-Packard (Canada) Ltd.  
305-1037 West Broadway  
Vancouver 9  
Tel: (604) 731-5301  
TWX: 610-922-5059

**NOVA SCOTIA**  
Hewlett-Packard (Canada) Ltd.  
7091 Mumford Road  
Suite 356  
Halifax  
Tel: (902) 455-0511  
TWX: 610-271-4482

**ONTARIO**  
Hewlett-Packard (Canada) Ltd.  
880 Lady Ellen Place  
Ottawa 3  
Tel: (613) 722-4223  
TWX: 610-562-1952

Hewlett-Packard (Canada) Ltd.  
1415 Lawrence Avenue West  
Toronto  
Tel: (416) 249-9196  
TWX: 610-492-2362

**QUEBEC**  
Hewlett-Packard (Canada) Ltd.  
275 Hymus Boulevard  
Pointe Claire  
Tel: (514) 697-4232  
TWX: 610-422-3022  
Telex: 01-20607

**FOR CANADIAN AREAS NOT LISTED:**  
Contact Hewlett-Packard (Canada) Ltd. in  
Pointe Claire, at the complete address  
listed above.