


OPERATING MANUAL

SYNTHESIZER/ FUNCTION GENERATOR

3325A

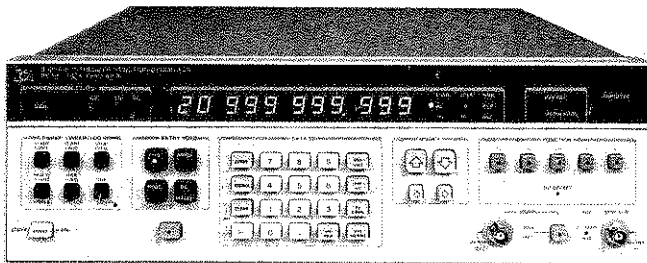

 HEWLETT
PACKARD



OPERATING MANUAL

MODEL 3325A SYNTHESIZER/FUNCTION GENERATOR

Serial Numbers: All

IMPORTANT NOTICE

This manual applies to all instruments. Documentation changes required after the printing of this manual are shown on a manual changes supplement which accompanies this manual.

WARNING

To prevent potential fire or shock hazard, do not expose equipment to rain or moisture.

Manual Part No. 03325-90013

© Copyright Hewlett-Packard Company 1978, 1981, 1984
P.O. Box 69, Marysville, Washington 98270

Printed: May 1984



SAFETY SUMMARY

The following general safety precautions must be observed during all phases of operation, service, and repair of this instrument. Failure to comply with these precautions or with specific warnings elsewhere in this manual violates safety standards of design, manufacture, and intended use of the instrument. Hewlett-Packard Company assumes no liability for the customer's failure to comply with these requirements. This is a Safety Class 1 instrument.

GROUND THE INSTRUMENT

To minimize shock hazard, the instrument chassis and cabinet must be connected to an electrical ground. The instrument is equipped with a three-conductor ac power cable. The power cable must either be plugged into an approved three-contact electrical outlet or used with a three-contact to two-contact adapter with the grounding wire (green) firmly connected to an electrical ground (safety ground) at the power outlet. The power jack and mating plug of the power cable meet International Electrotechnical Commission (IEC) safety standards.

DO NOT OPERATE IN AN EXPLOSIVE ATMOSPHERE

Do not operate the instrument in the presence of flammable gases or fumes. Operation of any electrical instrument in such an environment constitutes a definite safety hazard.

KEEP AWAY FROM LIVE CIRCUITS

Operating personnel must not remove instrument covers. Component replacement and internal adjustments must be made by qualified maintenance personnel. Do not replace components with power cable connected. Under certain conditions, dangerous voltages may exist even with the power cable removed. To avoid injuries, always disconnect power and discharge circuits before touching them.

DO NOT SERVICE OR ADJUST ALONE

Do not attempt internal service or adjustment unless another person, capable of rendering first aid and resuscitation, is present.

DO NOT SUBSTITUTE PARTS OR MODIFY INSTRUMENT

Because of the danger of introducing additional hazards, do not install substitute parts or perform any unauthorized modification to the instrument. Return the instrument to a Hewlett-Packard Sales and Service Office for service and repair to ensure that safety features are maintained.

DANGEROUS PROCEDURE WARNINGS

Warnings, such as the example below, precede potentially dangerous procedures throughout this manual. Instructions contained in the warnings must be followed.

WARNING

Dangerous voltages, capable of causing death, are present in this instrument. Use extreme caution when handling, testing, and adjusting.

SAFETY SYMBOLS


General Definitions of Safety Symbols Used On Equipment or In Manuals.



Instruction manual symbol: the product will be marked with this symbol when it is necessary for the user to refer to the instruction manual in order to protect against damage to the instrument.




Indicates dangerous voltage (terminals fed from the interior by voltage exceeding 1000 volts must be so marked).



Protective conductor terminal. For protection against electrical shock in case of a fault. Used with field wiring terminals to indicate the terminal which must be connected to ground before operating equipment.



Low-noise or noiseless, clean ground (earth) terminal. Used for a signal common, as well as providing protection against electrical shock in case of a fault. A terminal marked with this symbol must be connected to ground in the manner described in the installation (operating) manual, and before operating the equipment.



Frame or chassis terminal. A connection to the frame (chassis) of the equipment which normally includes all exposed metal structures.



Alternating current (power line).



Direct current (power line).



Alternating or direct current (power line).

WARNING

The **WARNING** sign denotes a hazard. It calls attention to a procedure, practice, condition or the like, which, if not correctly performed or adhered to, could result in injury or death to personnel.

CAUTION

The **CAUTION** sign denotes a hazard. It calls attention to an operating procedure, practice, condition or the like, which, if not correctly performed or adhered to, could result in damage to or destruction of part or all of the product.

NOTE:

The **NOTE** sign denotes important information. It calls attention to procedure, practice, condition or the like, which is essential to highlight.

TABLE OF CONTENTS

Section	Page
I. GENERAL INFORMATION	1-1
1-1. Introduction	1-1
1-5. Instrument Description	1-1
1-9. Specifications	1-1
1-11. Supplemental Operating Information	1-1
1-13. Remote Control	1-1
1-15. Options	1-1
1-17. Accessories Supplied	1-5
1-19. Accessories Available	1-5
1-21. Instrument and Manual Identification	1-6
1-24. Safety Considerations	1-6
1-27. Recommended Test Equipment	1-6

Section	Page
II. INSTALLATION	2-1
2-1. Introduction	2-1
2-3. Initial Inspection	2-1
2-5. Preparation For Use	2-1
2-6. Power Requirements	2-1
2-8. Line Voltage Selection	2-1
2-10. Power Cable	2-1
2-12. HP-IB Connections	2-1
2-15. 3325A Listen/Talk Address	2-2
2-17. HP-IB Description	2-3
2-19. Connecting Oven Option 001	2-3
2-21. Operating Environment	2-3
2-23. Cooling System	2-3
2-26. Bench Operation	2-3
2-28. Rack Mounting	2-3
2-30. Storage and Shipment	2-3
2-31. Environment	2-3
2-33. Instrument Identification	2-5
2-35. Packaging	2-5

Section	Page
III. OPERATION	3-1
3-1. Introduction	3-1
3-3. Panel Features	3-3
3-5. Power/Warm-Up	3-3
3-8. Initial Conditions	3-3
3-10. Self Test	3-3
3-12. Front/Rear Signal Output	3-3
3-14. Sync Output	3-3
3-16. External Reference Input	3-4
3-18. 10MHz Oven Option 001	3-4
3-20. Manual Programming	3-4
3-22. Clear Display	3-4
3-24. Entry Errors	3-4
3-26. Function Selection	3-4
3-28. Frequency Entry	3-4

Section	Page
3-30. Frequency Limits	3-4
3-32. Frequency Display and Resolution	3-5
3-34. Auxiliary Output (Sine Function Only)	3-5
3-36. Amplitude Entry	3-5
3-39. Amplitude Calibration	3-5
3-41. High Voltage Output Option 002	3-6
3-43. DC Offset	3-6
3-46. Phase Entry	3-7
3-49. Frequency Sweep	3-7
3-55. Sweep Marker	3-9
3-58. Sweep X Drive Output	3-10
3-60. Sweep Z Blank Output	3-10
3-62. Amplitude Modulation	3-10
3-66. Phase Modulation	3-11
3-68. Modify Keys	3-11
3-70. Store and Recall	3-11
3-72. Operator's Checks	3-11
3-74. Self Test	3-11
3-76. Output Checks	3-11
3-78. Operator's Maintenance	3-12
3-81. HP-IB Operation	3-12
3-83. General HP-IB Description	3-13
3-88. Definition of HP-IB Terms and Concepts	3-13
3-89. Basic Device Communication Capability	3-14
3-91. Message Definitions	3-14
3-93. 3325A Response to Messages	3-14
3-95. HP-IB Work Sheet	3-14
3-97. HP-IB Addressing	3-14
3-100. 3325A Remote Programming	3-14
3-101. 3325A HP-IB Capabilities	3-14
3-103. Developing an HP-IB Program	3-15
3-107. Universal and Addressed Commands	3-17
3-109. Placing the 3325A in Remote	3-17
3-111. The 3325A Address	3-17
3-113. 3325A Data Message Formats	3-17
3-115. Data Transfer Mode	3-20
3-118. Programming Data Transfer Mode	3-21
3-120. Programming Entry Parameters	3-21
3-122. Programming Waveform Function	3-21
3-124. Programming Binary (On or Off) Functions	3-22
3-126. Programming Selection Functions	3-22
3-128. Programming Execution Functions	3-22
3-130. Programming Amplitude Units Conversion	3-23
3-132. Programming Storage Registers	3-23

TABLE OF CONTENTS (Cont'd)

Section	Page	Section	Page
3-134. Service Requests	3-23	IV. PERFORMANCE TESTS	4-1
3-136. Serial Poll	3-23	4-1. Introduction	4-1
3-138. Status Byte	3-24	4-3. Calculator-Controlled Test	4-1
3-140. Busy Flag	3-24	4-5. Operational Verification	4-1
3-142. Sweep Flag	3-24	4-8. Required Test Equipment	4-1
3-144. Masking or Enabling Service Requests	3-24	4-10. Self Test	4-1
3-146. Interrogating Program Errors	3-24	4-12. Sine Wave Verification	4-1
3-148. Interrogating Entry Parameters	3-25	4-14. Square Wave Verification	4-2
3-150. Interrogating Function (Waveform)	3-25	4-16. Triangle and Ramp Verification	4-3
3-152. Interrogating Miscellaneous Parameters	3-26	4-18. Amplitude Flatness Check	4-3
3-154. Using the Interrogate Capability	3-26	4-20. Sync Output Check	4-4
3-156. 3325A Programming Procedure	3-27	4-22. Frequency Accuracy	4-4
Appendix A. Meta Messages Block Diagrammed	A-1	4-24. Output Level and Attenuator Check	4-4
Appendix B. Programming the Model 3325A with the 9825A Calculator	B-1	4-26. Harmonic Distortion Test	4-5
		4-28. Close-In Spurious Signal Test	4-6
		4-30. HP-IB Interface Test	4-6

LIST OF TABLES

Table	Page	Table	Page
1-1. Specifications	1-2	3-5. General Interface Management Lines	3-14
1-2. Supplemental Information	1-3	3-6. Definition of Meta Messages	3-15
1-3. HP-IB Interface Capability	1-6	3-7. 3325A Implementation of Messages	3-16
1-4. HP-IB Response Times	1-7	3-8. Interface Functions	3-16
1-5. Recommended Test Equipment	1-8	3-9. Summary of 3325A Programming (ASCII)	3-18
2-1. HP-IB Addresses	2-4	3-10. Programming Codes	3-19
3-1. Operating Information	3-1	3-11. SRQ Mask/Enable Data	3-25
3-2. Amplitude Limits of AC Functions	3-5	4-1. Test Equipment Required for Operational Verification	4-2
3-3. High Voltage Output Amplitudes (Option 002)	3-6		
3-4. Maximum DC Offset with any AC Function	3-7		

LIST OF ILLUSTRATIONS

Figure	Page	Figure	Page
2-1. Power Cables	2-2	3-3. Interface Connections and Bus Structure	3-13
2-2. HP-IB Connector	2-2	4-1. Harmonic Distortion Verification (High Voltage Output)	4-5
2-3. Rack Mount and Handle Kits	2-5		
3-1. Front and Rear Panel Controls	3-2		
3-2. Maximum DC Offset with AC Functions	3-8		

SECTION I

GENERAL INFORMATION

TABLE OF CONTENTS

Paragraph	Page
1-1. Introduction	1-1
1-5. Instrument Description	1-1
1-9. Specifications	1-1
1-11. Supplemental Operating Information	1-1
1-13. Remote Control	1-1
1-15. Options	1-1
1-17. Accessories Supplied	1-5
1-19. Accessories Available	1-5
1-21. Instrument and Manual Identification	1-6
1-24. Safety Considerations	1-6
1-27. Recommended Test Equipment	1-6

LIST OF TABLES

Table	Page
1-1. Specifications	1-2
1-2. Supplemental Information	1-3
1-3. HP-IB Interface Capability	1-6
1-4. HP-IB Response Times	1-7
1-5. Recommended Test Equipment	1-8

SECTION I

GENERAL INFORMATION

1-1. INTRODUCTION.

1-2. The Operating and Service Manual contains information required to install, operate, test, adjust, and service the Hewlett-Packard Model 3325A Synthesizer/Function Generator. The Operating Manual supplement is a copy of the first three sections of the Operating and Service Manual, plus the Operational Verification procedures from Section IV. The supplement should be kept with the instrument for use by the operator. The part numbers of both the Operating and Service Manual and the Operating Manual supplement are shown on the title pages.

1-3. Also shown on the title page of this manual is a Microfiche part number. This number can be used to order 4 × 6 inch transparencies of the Operating and Service Manual. Each Microfiche contains up to 96 photo-duplicates of the manual pages. The Microfiche package includes the latest Manual Changes supplement as well as pertinent Service Notes.

1-4. Additional copies of the Operating and Service Manual, Operating Information Supplement, or Service Notes can be ordered through your nearest Hewlett-Packard Sales and Service Office. (A list of these offices is provided at the end of this manual.)

1-5. INSTRUMENT DESCRIPTION.

1-6. The Model 3325A Synthesizer/Function Generator produces the following signals at a minimum frequency of 1 μ Hz and maximum frequency of:

Sine wave	20 MHz
Square wave	10 MHz
Triangle	10 kHz
Positive slope ramp	10 kHz
Negative slope ramp	10 kHz

Frequency may be selected with up to eleven digits of resolution. Output amplitude is 1 mV to 10 V peak-to-peak. The output level may also be selected or displayed in V rms or in dBm (50 ohms). Any function may be dc offset up to ± 4.5 V, or the output may be dc only up to ± 5 V. An optional high voltage output produces up to 40 V p-p into ≥ 500 ohms load.

1-7. Frequency sweep of all functions is provided in linear or log sweep, at sweep times of 10 milliseconds to 99.99 seconds for linear sweep. Maximum time for log sweep is 99.99 seconds and minimum time is 2 seconds for single log sweep and 0.1 second for continuous log sweep. Single linear sweep may be up or down, while continuous sweep is up/down/up, etc., in the linear mode and up/up, etc., in log mode.

1-8. The Model 3325A is fully programmable through the rear panel Hewlett-Packard Interface Bus (HP-IB) connector. A device such as a programmable calculator is capable of remotely controlling the 3325A. Interface information is given in Section II of this manual, and programming information is in Section III.

1-9. SPECIFICATIONS.

1-10. Instrument specifications are listed in Table 1-1. These specifications are the performance standards or limits against which the instrument is tested. Any changes in specifications due to manufacturing, design or traceability to the U.S. National Bureau of Standards are included in Table 1-1 of this manual and/or the Manual Changes Supplement.

1-11. SUPPLEMENTAL OPERATING INFORMATION.

1-12. Table 1-2 contains information describing general operating characteristics of the 3325A. This information is supplemental operating information and is not to be considered as specifications.

1-13. REMOTE CONTROL.

1-14. Table 1-3 lists the HP-IB interface capabilities of the Model 3325A in conformity with IEEE Standard 488-1978, "Standard Digital Interface for Programmable Instrumentation". HP-IB response times are given in Table 1-4.

1-15. OPTIONS.

1-16. The following options extend the frequency stability and output amplitude capabilities of the Model 3325A:

Option 001	High Stability Frequency Reference
Option 002	High Voltage Output

The following options indicate the line voltage to which the instrument was set at the factory:

Option 100	Nominal 100 V ac
Option 120	Nominal 120 V ac
Option 220	Nominal 220 V ac
Option 240	Nominal 240 V ac

Table 1-1. Specifications (Cont'd).

<p>Accuracy of DC Offset (into 50 ohms): DC Only (No AC Function): $\pm 0.4\%$ of full peak output for each range* *Except lowest attenuator range where accuracy is $\pm 20 \mu V$.</p> <p>DC + AC, ≤ 1 MHz: $\pm 1.2\%$, Ramps $\pm 2.4\%$</p> <p>DC + AC, > 1 MHz: $\pm 3\%$</p> <p>AMPLITUDE MODULATION (of Sine Function only)</p> <p>Modulation Envelope Distortion: -30 dB to 80% modulation at 1 kHz, 0 V dc Offset</p> <p>PHASE OFFSET</p> <p>Range: $\pm 719.9^\circ$ with respect to arbitrary starting phase, or assigned zero phase</p> <p>Resolution: 0.1° Stability: $\pm 1^\circ$ phase/$^\circ C$ Increment Accuracy: $\pm 0.2^\circ$</p> <p>PHASE MODULATION</p> <p>Linearity (Sine Function): $\pm 0.5\%$, best fit straight line</p> <p>SYNC OUTPUT</p> <p>Output Levels into 50 ohms: Square wave with $V_{high} \geq + 1.2V$, $V_{low} \leq + 0.2V$</p> <p>X DRIVE OUTPUT</p> <p>Amplitude: 0 to + 10 V dc linear ramp proportional to sweep frequency (sweep up only)</p> <p>Linearity, 10% to 90%, best fit straight line: $\pm 0.1\%$ of final value. Specified for all linear sweep widths which are integral multiples of the minimum sweep width for each function and sweep time.</p> <p>OPTION 001</p> <p>HIGH STABILITY FREQUENCY REFERENCE</p> <p>Ambient Stability: $\pm 5 \times 10^{-8}$ (0° to $55^\circ C$ referenced to $+ 30^\circ C$)</p>	<p>Aging Rate: $\pm 5 \times 10^{-8}$ per week (after 72 hours continuous operation) $\pm 1 \times 10^{-7}$ per month (after 15 days continuous operation)</p> <p>OPTION 002</p> <p>HIGH VOLTAGE OUTPUT</p> <p>Frequency Range: Sine and Square Wave: 1 μHz to 1 MHz Triangle and Ramps: 1 μHz to 10 kHz</p> <p>Amplitude: Range: 4mVp-p to 40Vp-p ($\geq 500\Omega$, $< 500pF$ load) maximum output current, $\pm 40mA$ Accuracy (at 2 kHz): $\pm 2\%$ of full output for each range Flatness: $\pm 10\%$ of programmed amplitude</p> <p>DC Offset: Range: 4 times the range of the standard instrument Accuracy: $\pm (1\% + 25 mV)$ of full output for each range</p> <p>Signal Characteristics: Sine Wave Harmonic Distortion (relative to the fundamental frequency at full output into ≥ 500 ohms, $< 500 pF$)</p> <table border="1"> <thead> <tr> <th>Fundamental Frequency</th> <th>No Harmonic Greater Than</th> </tr> </thead> <tbody> <tr> <td>10 Hz to 50 kHz</td> <td>- 65 dB</td> </tr> <tr> <td>50 kHz to 200 kHz</td> <td>- 60 dB</td> </tr> <tr> <td>200 kHz to 1 MHz</td> <td>- 40 dB</td> </tr> </tbody> </table> <p>Square Wave: Rise/Fall Time: ≤ 125 nanoseconds, 10% to 90% at full output with ≥ 500 ohm, $< 500pF$ load Overshoot: $< 10\%$ of peak amplitude with ≥ 500 ohm, $< 500 pF$ load</p>	Fundamental Frequency	No Harmonic Greater Than	10 Hz to 50 kHz	- 65 dB	50 kHz to 200 kHz	- 60 dB	200 kHz to 1 MHz	- 40 dB
Fundamental Frequency	No Harmonic Greater Than								
10 Hz to 50 kHz	- 65 dB								
50 kHz to 200 kHz	- 60 dB								
200 kHz to 1 MHz	- 40 dB								

Table 1-2 Supplemental Information

<p>MAIN SIGNAL OUTPUT</p> <p>50 Ω Impedance</p> <p>BNC Connector, switchable to front or rear panel (not switchable with Option 002)</p> <p>May be floated a maximum of ± 42 V peak (ac + dc) from chassis (earth) ground</p> <p>Amplitude Ranges: All AC Functions (with no dc offset):</p> <table border="1"> <thead> <tr> <th>Range No.</th> <th>Attenuation Factor</th> <th>Amplitude (Peak-to-Peak)</th> </tr> </thead> <tbody> <tr> <td>1</td> <td>1</td> <td>10.00 V to 3.000 V</td> </tr> <tr> <td>2</td> <td>3</td> <td>2.999 V to 1.000 V</td> </tr> <tr> <td>3</td> <td>10</td> <td>999.9 mV to 300.0 mV</td> </tr> </tbody> </table>	Range No.	Attenuation Factor	Amplitude (Peak-to-Peak)	1	1	10.00 V to 3.000 V	2	3	2.999 V to 1.000 V	3	10	999.9 mV to 300.0 mV	<table border="1"> <tbody> <tr> <td>4</td> <td>30</td> <td>299.9 mV to 100.0 mV</td> </tr> <tr> <td>5</td> <td>100</td> <td>99.99 mV to 30.00 mV</td> </tr> <tr> <td>6</td> <td>300</td> <td>29.99 mV to 10.00 mV</td> </tr> <tr> <td>7</td> <td>1000</td> <td>9.999 mV to 3.000 mV</td> </tr> <tr> <td>8</td> <td>3000</td> <td>2.999 mV to 1.000 mV</td> </tr> </tbody> </table>	4	30	299.9 mV to 100.0 mV	5	100	99.99 mV to 30.00 mV	6	300	29.99 mV to 10.00 mV	7	1000	9.999 mV to 3.000 mV	8	3000	2.999 mV to 1.000 mV
	Range No.	Attenuation Factor	Amplitude (Peak-to-Peak)																									
1	1	10.00 V to 3.000 V																										
2	3	2.999 V to 1.000 V																										
3	10	999.9 mV to 300.0 mV																										
4	30	299.9 mV to 100.0 mV																										
5	100	99.99 mV to 30.00 mV																										
6	300	29.99 mV to 10.00 mV																										
7	1000	9.999 mV to 3.000 mV																										
8	3000	2.999 mV to 1.000 mV																										
	<p>DC Offset Only:</p> <table border="1"> <thead> <tr> <th>Range No.</th> <th>Attenuation Factor</th> <th>Amplitude (Peak-to-Peak)</th> </tr> </thead> <tbody> <tr> <td>1</td> <td>1</td> <td>5.000 V to 1.500 V</td> </tr> <tr> <td>2</td> <td>3</td> <td>1.499 V to 500.0 mV</td> </tr> <tr> <td>3</td> <td>10</td> <td>499.9 mV to 150.0 mV</td> </tr> <tr> <td>4</td> <td>30</td> <td>149.9 mV to 50.00 mV</td> </tr> <tr> <td>5</td> <td>100</td> <td>49.99 mV to 15.00 mV</td> </tr> <tr> <td>6</td> <td>300</td> <td>14.99 mV to 5.000 mV</td> </tr> <tr> <td>7</td> <td>1000</td> <td>4.999 mV to 1.500 mV</td> </tr> <tr> <td>8</td> <td>3000</td> <td>1.499 mV to 1.000 mV</td> </tr> </tbody> </table>	Range No.	Attenuation Factor	Amplitude (Peak-to-Peak)	1	1	5.000 V to 1.500 V	2	3	1.499 V to 500.0 mV	3	10	499.9 mV to 150.0 mV	4	30	149.9 mV to 50.00 mV	5	100	49.99 mV to 15.00 mV	6	300	14.99 mV to 5.000 mV	7	1000	4.999 mV to 1.500 mV	8	3000	1.499 mV to 1.000 mV
Range No.	Attenuation Factor	Amplitude (Peak-to-Peak)																										
1	1	5.000 V to 1.500 V																										
2	3	1.499 V to 500.0 mV																										
3	10	499.9 mV to 150.0 mV																										
4	30	149.9 mV to 50.00 mV																										
5	100	49.99 mV to 15.00 mV																										
6	300	14.99 mV to 5.000 mV																										
7	1000	4.999 mV to 1.500 mV																										
8	3000	1.499 mV to 1.000 mV																										

Table 1-2. Supplemental Information (Cont'd).

AC Function with DC Offset:

Range No.	Attenuation Factor	AC Function Amplitude (p-p)	Maximum DC (+ or -)	Min. DC (+ or -)
1	1	9.998 V to 1.000 V	1.000 mV to 4.500 V	1.000 mV
2	3	999.9 mV to 333.4 mV	1.166 V to 1.499 V	0.100 mV
3	10	333.3 mV to 100.0 mV	333.3 mV to 450.0 mV	0.100 mV
4	30	99.99 mV to 33.34 mV	116.6 mV to 149.9 mV	0.010 mV
5	100	33.33 mV to 10.00 mV	33.33 mV to 45.00 mV	0.010 mV
6	300	9.999 mV to 3.334 mV	11.66 mV to 14.99 mV	0.001 mV
7	1000	3.333 mV to 1.000 mV	3.333 mV to 4.500 mV	0.001 mV

High Voltage Output Option 002:

Amplitude and Ranges: 4 times the standard instrument amplitudes

Output Impedance: < 2 Ω at DC to < 10 Ω at 1 MHz

Square Wave Settling Time: < 1 μs to settle to within .05% of final value for frequencies of 10 Hz to 500 kHz, tested at full output with no load

FREQUENCY SWEEP

Sweep Time:

Linear Sweep: 0.01 second to 99.99 seconds (single or continuous)

Log Sweep:

Single Sweep: 2 seconds to 99.99 seconds
Continuous Sweep: 0.1 second to 99.99 seconds

Maximum Sweep Width: 1 Hz to maximum frequency of the function selected

Minimum Sweep Width (Linear):

Minimum Sweep Width

Function	Sweep Time 0.01 second	Sweep Time 99.99 seconds
Sine	0.1 mHz	999.9 mHz
Square	0.05 mHz	499.5 mHz
Triangle	0.005 mHz	49.95 mHz
Ramps	0.01 mHz	99.99 mHz

Minimum Sweep Width (Log): 1 decade

Phase Continuity: Sweep is phase continuous over the full frequency range

WARMUP TIME

Standard Instrument: 20 minutes to within specified accuracy

Option 001 High Stability Frequency Reference:

Reference will be within $\pm 1 \times 10^{-7}$ of final value 15 minutes after turn-on at 25°C for an off time of less than 24 hours

AUXILIARY INPUTS (May be floated a maximum of ±42 V peak [ac + dc] from chassis [earth] ground)

Reference: For phase-locking the 3325A to an external frequency reference of 10 MHz or a subharmonic of 10 MHz down to 1 MHz. Level must be 0 dBm to +20 dBm into 50 ohms. Rear panel BNC connector.

Amplitude Modulation Input (Sine Function Only):

Modulation depth at full output for each range: 0 to 100%

Modulation frequency range: DC to 500 kHz (0 to 21 MHz carrier frequency)

Sensitivity: 5 V peak for 100% modulation

Input Impedance: 10 kΩ

Connector: Rear panel BNC

Phase Modulation:

Modulation Frequency Range: DC to 5 kHz

Modulation Depth

Function	Depth (+ or -)
Sine	850°
Square	425°
Triangle	42.5°
Ramps	85°

Input Impedance: 20 kΩ

Connector: Rear panel BNC

AUXILIARY OUTPUTS (May be floated a maximum of ±42 V peak [ac + dc] from chassis [earth] ground)

Auxiliary Frequency Output (ac coupled output):

Frequency Range: 21 MHz to 60.999 999 999 MHz, with under-range coverage to 19.000 000 001 MHz

Amplitude: 0 dBm

Output Impedance: 50 ohms

Connector: Rear panel BNC

1 MHz Reference Output (for phase-locking other instruments to 3325A):

Amplitude: 0 dBm

Output Impedance: 50 ohms

Connector: Rear panel BNC

Marker Output (Linear sweep only):

Levels: High to Low TTL compatible voltage transition at selected marker frequency, sweep up only.

Connector: Rear panel BNC

Table 1-2. Supplemental Information (Cont'd).

<p>X Drive Output (Sweep up only): Amplitude: 0 to + 10 V linear ramp proportional to sweep frequency</p> <p>Connector: Rear panel BNC</p> <p>Z Blank Output: Levels (TTL compatible voltage levels): Linear Sweep: Single: Low at start of sweep, High at stop. Remains High until start of next sweep.</p> <p>Continuous: Low during sweep up, High during sweep down.</p> <p>Log Sweep: Single: Low at start of sweep, High at stop. Remains High until start of next sweep.</p> <p>Continuous: Low during sweep. Goes High momentarily at stop frequency.</p> <p>10 MHz Oven Reference Output, Option 001, for phase locking the 3325A to the optional high stability frequency reference:</p> <p>Amplitude: 0 dBm, 50 ohms</p> <p>Connector: Rear panel BNC. Must be connected to the rear panel EXT REF IN connector.</p> <p>REMOTE CONTROL</p> <p>Hewlett-Packard Interface Bus (HP-IB) Control: (HP-IB is Hewlett-Packard Company's implementation of IEEE Standard 488-1978). Time shown is in addition to programming time.</p>	<p>Frequency Switching and Settling Time:*</p> <p>< 10 ms to within 1 Hz of final value for 100 kHz span</p> <p>< 25 ms to within 1 Hz of final value for 1 MHz span</p> <p>< 70 ms to within 1 Hz of final value for 20 MHz span</p> <p>Phase Switching and Settling Time:*</p> <p>< 15 ms to within 90° of phase lock for 20 MHz frequency change</p> <p>Amplitude Switching Time:*</p> <p>< 30 ms to within amplitude specifications</p> <p>*Times shown are in addition to programming time</p> <p>GENERAL</p> <p>Operating Environment:</p> <p>Temperature: 0° to 55°C Relative Humidity: < 95%, 0° to 40°C Altitude: ≤ 15,000 ft.</p> <p>Storage Temperature: - 50° to + 75°C Storage Altitude: ≤ 50,000 ft.</p> <p>Power Requirements:</p> <p>100/120/220/240V + 5%, - 10%, 48 to 66 Hz 60 VA, 100 VA with all options, 10 VA standby</p> <p>Dimensions in millimeters and (inches):</p> <p>132.6 (5¼) high × 425.5 (16¾) wide × 497.8 (19-5/8) deep</p> <p>Weight in kilograms and (lbs):</p> <p>Net weight: 9(20) Shipping Weight: 14.5 (32)</p>
--	--

The following accessory options are also available for the Model 3325A:

- Option 907 Front Handle Assembly
- Option 908 Rack Mount Flange Kit
- Option 909 Rack Mount Flange Kit/Front Handle Assembly
- Option 910 Additional Operating and Service Manual

1-17. ACCESSORIES SUPPLIED.

1-18. A special connector is supplied with the High Stability Frequency Reference Option 001 for connecting the rear panel Reference Output to the Reference Input. This connector is Part No. 1250-1499.

1-19. ACCESSORIES AVAILABLE.

1-20. The following accessories are available for use with the Model 3325A:

Number	Description
11048C	50 ohm Feedthru Termination
11356A	Ground Isolator
03325-80001	Oven Board Assy. (Converts 3325A to Option 001)
03325-80002	High Voltage Option (Converts 3325A to Option 002)
5061-0077	Rack Mount Flange Kit (Option 908)
5061-0083	Rack Mount Flange/Front Handle Kit (Option 909)
5061-0089	Front Handle Kit (Option 907)

1-21. INSTRUMENT AND MANUAL IDENTIFICATION.

1-22. The instrument serial number is located on the rear panel. Hewlett-Packard uses a two-section serial number consisting of a four-digit prefix and a five-digit suffix. A letter between the prefix and suffix identifies the country in which the instrument was manufactured (A=USA, G=West Germany, J=Japan, U=United Kingdom). All correspondence with Hewlett-Packard concerning this instrument should include the complete serial number.


1-23. The serial number prefix is the same for all identical instruments and changes only when a change is made to the instrument. The suffix is assigned sequentially and is different for each instrument. If the serial number of your instrument is lower than the serial number on the title page of this manual, refer to Section VII, MANUAL CHANGES, for the information that will adapt this manual to your instrument. This is especially important if the serial prefix of your instrument is different than the one shown on the title page of this manual. An instrument manufactured after the printing of this manual may differ in some respect from the information in this manual. In this case, a yellow Manual Changes supplement included with the manual explains how to adapt the manual to your instrument.

1-24. SAFETY CONSIDERATIONS.

1-25. To ensure safe operation and to retain the instrument in a safe condition, this Operating and Service Manual contains information, cautions and warnings which must be adhered to by the user or service personnel.

Table 1-3. HP-IB Interface Capability.

Code	Function
SH1	Source handshake capability
AH1	Acceptor handshake capability
T6	Basic talker; Serial poll; Unaddressed to talk if addressed to listen
L3	Basic listener; Listen only; Unaddressed to listen if addressed to talk
SR1	Service Request capability
RL1	Remote/Local capability
PP0	No parallel poll capability
DC1	Device Clear capability
DT0	No device trigger capability
C0	No controller capability
E1	Open collector bus drivers

1-26. The symbol  appearing on the front or rear panel of the 3325A is an international symbol meaning "refer to the Operating and Service Manual". The symbol identifies important instructions required to prevent damage to the instrument. To ensure the safety of the operating and maintenance personnel and retain the safe operating condition of the instrument, these instructions must be adhered to.

1-27. RECOMMENDED TEST EQUIPMENT.

1-28. Equipment required to maintain the Model 3325A is listed in Table 1-5. Other equipment can be substituted if it meets or exceeds the critical specifications listed in the table.

Table 1-4. HP-IB Response Times.

Function	Mnemonic	Input Data Transfer Time	Device Time	Output Data Transfer Time
Function (Waveform) 1 Digit	FU	450-500 μ s 225-250 μ s	1600 ms 2.8 ms	450-500 μ s 225-250 μ s
Frequency \leq 11 Digits + Decimal Delimiters	FR HZ, KH, or MH	450-500 μ s 225-250 μ s each 450-500 μ s	7.0 ms 2.8 ms each 12.5 ms	450-500 μ s 225-250 μ s each 450-500 μ s
Amplitude \leq 4 Digits + Decimal Delimiters	AM VO or MV VR or MR DB	450-500 μ s 225-250 μ s each 450-500 μ s 450-500 μ s 450-500 μ s	6.8 ms 2.8 ms each 90 ms 130 ms 250 ms	450-500 μ s 225-250 μ s each 450-500 μ s 450-500 μ s 450-500 μ s
DC Offset \leq 4 Digits + Decimal Delimiters	OF VO or MV	450-500 μ s 225-250 μ s each 450-500 μ s	6.8 ms 2.8 ms each 82 ms	450-500 μ s 225-250 μ s each 450-500 μ s
Phase \leq 4 Digits + Decimal Delimiter	PH DE	450-500 μ s 225-250 μ s each 450-500 μ s	5 ms 2.8 ms each 28 ms	450-500 μ s 225-250 μ s each 450-500 μ s
Sweep Start Frequency \leq 11 Digits + Decimal Delimiters	ST HZ, KH, or MH	450-500 μ s 225-250 μ s each 450-500 μ s	7.0 ms 2.8 ms each 10.3 ms	450-500 μ s 225-250 μ s each 450-500 μ s
Sweep Stop Frequency \leq 11 Digits + Decimal Delimiters	SP HZ, KH or MH	450-500 μ s 225-250 μ s each 450-500 μ s	7.0 ms 2.8 ms each 10.3 ms	450-500 μ s 225-250 μ s each 450-500 μ s
Sweep Marker Frequency \leq 11 Digits + Decimal Delimiters	MF HZ, KH or MH	450-500 μ s 225-250 μ s each 450-500 μ s	7.0 ms 2.8 ms each 10.3 ms	450-500 μ s 225-250 μ s each 450-500 μ s
Sweep Time \leq 4 Digits + Decimal Delimiter	T1 SE	450-500 μ s 225-250 μ s each 450-500 μ s	5.5 ms 2.8 ms each 7.0 ms	450-500 μ s 225-250 μ s each 450-500 μ s
Store	SR	450-500 μ s	11 ms	
Recall	RE	450-500 μ s	1700 ms	
Assign Zero Phase	AP	450-500 μ s	5.2 ms	
Amptd Cal	AC	450-500 μ s	1500 ms	
Start Single Sweep	SS	450-500 μ s	300 ms	
Start Continuous Sweep	SC	450-500 μ s	300 ms	
Interrogate (Add Parameter Mnemonic Time)	I	225-250 μ s	3 ms	
Mask Service Request	MS	450-500 μ s	4.5 ms	
High Voltage Output	HV	450-500 μ s	48 ms	
Rear/Front Output	RF	450-500 μ s	44.5 ms	
Self Test	TE	450-500 μ s	10,000 ms	
Sweep Mode	SM	450-500 μ s	4.5 ms	
Data Transfer Mode	MD	450-500 μ s	4.5 ms	
Interrogate Function	IFU	675-750 μ s	1603 ms	
Interrogate Error	IER	675-750 μ s	11.5 ms	
Universal Commands		\sim 225 μ s per byte		
Amplitude Modulation	MA	450-500 μ s	7.0 ms	
Phase Modulation	MP	450-500 μ s	7.0 ms	

Table 1-5. Recommended Test Equipment.

Instrument	Critical Specifications	Required For				Recommended Model
		Oper. Ver.	Perf. Tests	Adjustments	Trouble-shooting	
Oscilloscope	Vertical Bandwidth: dc to 100 MHz Deflection: 0.01 V to 10V/div Horizontal Sweep: 0.05 μ s to 1 s/div x10 Magnification Delayed Sweep	X	X	X	X	-hp- 1740A
Electronic Counter	Frequency Measurement Frequency Range: to 20 MHz Resolution: 8 digits Accuracy: \pm 2 counts Time Interval Average A to B Resolution: 0.1 ns	X	X	X		-hp- 5328A with Opt 01 and 040 or 041
Digital Voltmeter	DC Function Ranges: .1 V, 1 V, 10 V, 100 V Accuracy: \pm .2% Resolution: 4 1/2 digits AC Function Ranges: 1 V, 10 V, 100 V Accuracy: \pm .5% Resolution: 4 digits DC Function Ranges: .1 V, 1 V, 10 V, 100 V Accuracy: \pm .05% Resolution: 6 digits AC Function: True RMS Ranges: 1 V, 10 V, 100 V Accuracy: \pm .2% Resolution: 6 digits Crest Factor: 4:1		X	X	X	-hp- 3466A -hp- 3455A
50-ohm Load	Accuracy: \pm .2% Power Rating: 1 W	X	X	X	X	-hp- 11048C
High Frequency Spectrum Analyzer	Frequency Range: 1 kHz to 100 MHz Amplitude Accuracy: \pm .5 dB	X	X	X		-hp- 141T/8552B/8553B/8566A/8568A
Low Frequency Spectrum Analyzer	Frequency Range: 20Hz-50kHz Amplitude Accuracy: \pm .5 dB Spurious Responses: 80 dB below reference	X	X	X		-hp- 3580A/3585A
Sine Wave Signal Source	Frequency: 1 kHz Amplitude: 1 V rms into 20 k Ω Frequency Range:		X	X		-hp- 204C -hp- 3335A 1 MHz-20 MHz Amplitude Range: to +7.0 dBm Output Impedance: 50 Ω Phase Noise (Integrated): 9.9 MHz: < -63 dB 20 MHz: < -70 dB Spurious: > 75 dB below fundamental
Double Balanced Mixer	Impedance: 50 Ω Frequency: to 20 MHz			X		-hp- 10534A or 10514A
1 MHz Low Pass Filter	Cut-off Frequency: 1 MHz Stopband Atten: 50 dB by 4 MHz Stopband Freq: 4 MHz-80 MHz			X		F882 1MHz Low Pass Filter, Impedance 50 Ω , C Shape Factor, Metal Can, BNC's Allen Avionics, Inc. 224 E. Second St. Mineola, NY 11501
15 kHz Noise Equivalent Filter	Consisting of: Resistor: 10 k Ω \pm 1% Capacitor: 1600 pF \pm 5%			X		-hp- 0757-0340 -hp- 0160-2223

Table 1-5. Recommended Test Equipment (Cont'd).

Instrument	Critical Specifications	Required For				Recommended Model
		Oper. Ver.	Perf. Tests	Adjustments	Trouble-shooting	
AC Voltmeter	Ranges: 0.1 V to 1 V Frequency Range: 20 Hz-1 MHz Input Impedance: $\geq 1 \text{ M}\Omega$ Meter: Log scale Acc (100 Hz to 10 kHz): $\pm 1\%$		X			-hp- 400 FL
Resistor	1 k Ω $\pm 5\%$			X		-hp- 0683-1025
Oscilloscope Probe	Division Ratio: 10 to 1 Impedance: 1 M Ω , 12 pF			X	X	-hp- 10041A
DC Power Supply	Volts: 0-10 V Amps: 10 mA Floating output		X	X		-hp- 6214A
Frequency Standard (Required for Option 001 Only)	Frequency: 5 MHz Accuracy: 1×10^{-9}			X		-hp- 105B
Calculator (Required for automatic testing)	HP-IB Control Capability	X	X			-hp- 9825A with 98034A Interface, General I/O ROM, Extended I/O ROM
System Voltmeter	DC Voltage: 0 to $\pm 10 \text{ V}$ Sample/Hold Measurement External Trigger: Low True TTL Edge Trigger Trigger Delay: selectable, 10 μs to 140 μs		X			-hp- 3437A
BNC Tee Adapter BNC-to-Triax Adapter	Male-female-female BNC-to-dual banana plug Female BNC-to-Male Triax	X X	X X X	X X		-hp- 1250-0781 -hp- 1250-2277 -hp- 1250-0595
Signature Analyzer	Signature: 4-digit hexadecimal Characters: 0 thru 9, A, C, F, H, P, U Threshold Logic 1: +2.2 V Logic 0: +0.5 V Clock Frequency: $\geq 1.5 \text{ MHz}$				X	-hp- 5004A
Pulse Generator	Pulse Rate: 500 kHz Pulse Width: $\leq 1 \mu\text{s}$ DC Offset: 1 V				X	-hp- 3312A
Resistor	56.2 Ω 1% 1/8W	X	X			-hp- 0757-0395
Thermal Converter	Input Impedance: 75 Ω Input Voltage: 0.5 V rms Frequency: 2 kHz to 20 MHz Frequency Response: $\pm 0.05 \text{ dB}$ 2 kHz to 20 MHz		X	X		-hp- 11050A
Resistive Divider	Consisting of: Resistor: 36.5 Ω 1% 1/2 W Resistor: 13.7 Ω 1% 1/2 W		X			-hp- 0757-0996 -hp- 0698-4998
Resistive Divider	Consisting of: Resistor: 40.2 Ω 1% 1/2 W Resistor: 10 Ω 1% 1/2 W		X			-hp- 0698-5022 -hp- 0757-0984
Resistive Divider	Consisting of: Resistor: 30 Ω 1% 1/4 W Resistor: 20 Ω 1% 1/4 W		X			-hp- 0698-7533 -hp- 0698-6296
Resistive Divider	Consisting of: Resistor: 100 k Ω 1% 1/8 W Resistor: 162 k Ω 1% 1/8 W		X			-hp- 0757-0465 -hp- 0757-0470
Termination	50 ohm Feedthrough 1%		X			-hp- 11048C
Thermal Converter	BNC Connectors		X			-hp- 11050A

SECTION II INSTALLATION

TABLE OF CONTENTS

Paragraph	Page
2-1. Introduction	2-1
2-3. Initial Inspection	2-1
2-5. Preparation For Use	2-1
2-6. Power Requirements	2-1
2-8. Line Voltage Selection	2-1
2-10. Power Cable	2-1
2-12. HP-IB Connections	2-1
2-15. 3325A Listen/Talk Address	2-2
2-17. HP-IB Description	2-3
2-19. Connecting Oven Option 001	2-3
2-21. Operating Environment	2-3
2-23. Cooling System	2-3
2-26. Bench Operation	2-3
2-28. Rack Mounting	2-3
2-30. Storage and Shipment	2-3
2-31. Environment	2-3
2-33. Instrument Identification	2-5
2-35. Packaging	2-5

LIST OF ILLUSTRATIONS

Figure	Page
2-1. Power Cables	2-2
2-2. HP-IB Connector	2-2
2-3. Rack Mount and Handle Kits	2-5

LIST OF TABLES

Table	Page
2-1. HP-IB Addresses	2-4

SECTION II INSTALLATION

2-1. INTRODUCTION.

2-2. This section contains instructions for installing and interfacing the Model 3325A Synthesizer/Function Generator. Included are initial inspection procedures, power and grounding requirements, line voltage selection, environmental requirements, installation instructions, HP-IB connection procedure, and instructions for repackaging for shipment.

2-3. INITIAL INSPECTION.

2-4. Inspect the shipping container for damage. If the shipping container or cushioning material is damaged, it should be kept until the contents of the shipment have been checked for completeness and the instrument has been checked mechanically and electrically. This instrument was carefully inspected both mechanically and electrically before shipment. It should be free of marks and scratches and in perfect electrical order upon receipt. Procedures for checking electrical performance are given in Section IV. If there is mechanical damage or defect or if the instrument does not pass the electrical performance test, notify the nearest Hewlett-Packard Sales and Service Office listed at the rear of this manual. If the shipping container is damaged or the cushioning material shows signs of stress, notify the carrier as well as the Hewlett-Packard office. Keep the shipping material for the carrier's inspection. The warranty statement is located in the front of this manual.

2-5. PREPARATION FOR USE.

2-6. Power Requirements.

2-7. The Model 3325A requires a power source of 100, 120, 220, or 240 V ac, +5%, -10%, 48 to 66 Hz single phase. Power consumption is 100 VA maximum.

2-8. Line Voltage Selection.



Before connecting ac power to this instrument, make sure it is set to the line voltage of the power source. Also ensure that the common connection of the power outlet is connected to a protective earth contact.

2-9. The line voltage selection switches are set at the factory to correspond to the line voltage option ordered. This information may be found on the rear panel.

Option	Line Voltage Selected
100	100 V
120	120 V
220	220 V
240	240 V

WARNING

The line voltage selection switches are located inside the top cover of the instrument. Line voltage selection should be done by trained service personnel only.

2-10. Power Cable.

2-11. In accordance with international safety standards, this instrument is equipped with a three-wire cable. When connected to an appropriate power line outlet, this cable grounds the instrument cabinet. The type of power cable shipped with each instrument depends on the country of destination. Refer to Figure 2-1 for the connector configuration and -hp- part numbers of the available power cables.

2-12. HP-IB Connections.

2-13. Interconnection data concerning the rear panel HP-IB connector is provided in Figure 2-2. This connector is compatible with the -hp- 10631 (A, B, or C) HP-IB cables. The lengths of these cables are as follows:

10631A	1 meter
10631B	2 meters
10631C	4 meters

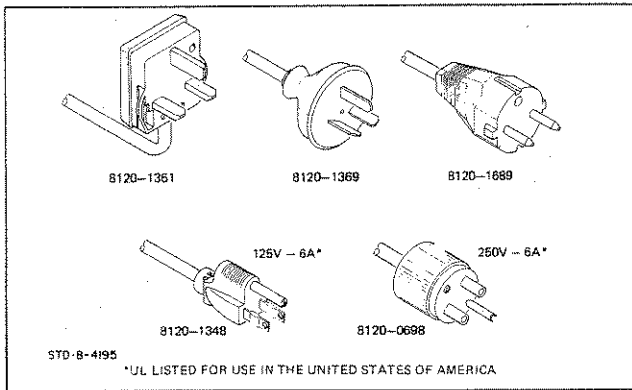


Figure 2-1. Power Cables.

Up to 15 instruments (including the controller) may be connected in an HP-IB system. The HP-IB cables have identical stacking connectors on both ends so that several cables can be connected to a single source. As a practical matter, avoid stacking more than three or four cables on any one connector. If the stack gets too large, the force on the stack can produce enough leverage to damage the connector mounting. Be sure that the connector screws are tightened firmly in place to keep it from working loose during use, and be sure to observe the

CAUTION of Figure 2-2.

2-14. Cable Length Restrictions. System components can be interconnected in virtually any configuration. However, to achieve reliable system performance, proper voltage levels and timing relationships must be maintained. If the system cable is too long, the lines cannot be driven properly and the system will fail to perform. The maximum length of cable that can be used to connect a group of instruments must not exceed 2 meters (6.5 ft.) times the number of instruments to be connected, or 20 meters (65.6 ft.), whichever is less.

2-15. 3325A Listen/Talk Address.

2-16. The 3325A is normally shipped from the factory with the listen address set to ASCII character 1; talk address Q. The 3325A address switches are located inside the top cover near the center of the instrument. The possible HP-IB addresses are shown in Table 2-1. The five switches (marked 1 through 5) are set according to the ASCII code address chosen. The 3325A may be set to a "listen only" condition by having the switch marked LON set to the "1" position.

PIN	LINE
1	DI01
2	DI02
3	DI03
4	DI04
13	DI05
14	DI06
15	DI07
16	DI08
5	EO1
17	REN
6	DAV
7	NRFD
8	NDAC
9	IFC
10	SRQ
11	ATN
12	SHIELD-CHASSIS GROUND
18	P/O TWISTED PAIR WITH PIN 6
19	P/O TWISTED PAIR WITH PIN 7
20	P/O TWISTED PAIR WITH PIN 8
21	P/O TWISTED PAIR WITH PIN 9
22	P/O TWISTED PAIR WITH PIN 10
23	P/O TWISTED PAIR WITH PIN 11
24	ISOLATED DIGITAL GROUND

LOCKSCREW 1390-0360 LONG MOUNTING STUD 0380-0643 SHORT MOUNTING STUD 0380-0644

6.5mm 4.9mm

THESE PINS ARE INTERNALLY GROUNDED

Figure 2-2. HP-IB Connector.

WARNING

Because the address switches are located inside the instrument, they should be set by trained service personnel only.

2-17. HP-IB Description.

2-18. A description of the HP-IB is provided in Section III of this manual. A study of this information is necessary if you are not familiar with the HP-IB concept. Additional information concerning the design criteria and operation of the bus is available in IEEE Standard 488-1978 "IEEE Standard Digital Interface for Programmable Instrumentation".

2-19. Connecting Oven Option 001.

2-20. In order to use the Oven Option 001, an external connection must be made between the rear panel 10 MHz OVEN OUTPUT and the REF IN connectors. A special connector for this purpose, -hp- Part No. 1250-1499, is supplied with instruments having Option 001.

2-21. OPERATING ENVIRONMENT.**WARNING**

To prevent potential electrical or fire hazard, do not expose equipment to rain or moisture.

2-22. In order for the 3325A to meet the specifications listed in Table 1-1, the operating environment must be within the following limits:

Temperature	0 to +55° C
Relative Humidity	95% at 40° C
Altitude	4600 meters (15,000 feet)

2-23. Cooling System.

2-24. The cooling fan intake and the exhaust vent are located in the rear panel. When operating the instrument, provide at least 75 mm (3 inches) of clearance at the rear, and at least 7 mm (¼ inch) on all sides of the instrument. Failure to allow adequate air circulation will result in excessive internal temperature, reducing instrument reliability.

2-25. It is imperative that the fan filter be inspected frequently and cleaned or replaced as necessary to permit the free flow of air through the instrument. To clean the

filter, remove the four nuts that secure the filter retainer. Remove the filter and flush with soapy water, rinse clean, and air dry.

2-26. Bench Operation.

2-27. The instrument has plastic feet attached to the bottom panel. The front feet contain foldaway tilt stands for convenience in bench operation. The tilt stand raises the front of the instrument for easier viewing of the control panel. The plastic feet are shaped to make full width modular instruments self-align when they are stacked. A front handle kit, -hp- part number 5061-0089 (Option 907), can be installed for ease of handling the instrument on the bench (see Figure 2-3). The kit is shipped with the instrument if Option 907 is also ordered. Otherwise, the front handle kit is available separately by its -hp- part number.

2-28. Rack Mounting.

2-29. The 3325A can be rack mounted in a rack having an EIA standard width of 482.6 mm (19 inches). The instrument can be rack mounted with or without a handle kit by use of the following items:

- Rack mounting without handles; use Rack Mount Flange Kit -hp- Part No. 5061-0077 (Option 908).
- Rack mounting with handles; use the combination Rack Mount Flange/Front Handle Kit -hp- Part No. 5061-0083 (Option 909).

NOTE

The Rack Mount Flange Kit of item a will not provide the space requirement for rack mounting when used with the bench handle assembly (-hp- part number 5060-9899, Option 907). To rack mount with handles, the combination kit of item b, (Option 909) must be used (see Figure 2-3). If either Option 908 or 909 is ordered, the corresponding kit is shipped with the instrument. Otherwise, both kits are available separately by their -hp- part numbers.

2-30. STORAGE AND SHIPMENT.**2-31. Environment.**


2-32. The instrument should be stored in a clean, dry environment. The following environmental limitations apply to both storage and shipment:

Temperature	-40° C to +75° C
Relative Humidity	95% at 40° C
Altitude	15,300 meters (50,000 feet)

Table 2-1. HP-IB Addresses.

ASCII Characters		Address Switches (Binary Code)	Equivalent Codes (To 5-Bit Binary Switches)		
Listen Address	Talk Address		Octal	Decimal	Hexadecimal
SP	@	0 0 0 0 0	00	00	00
!	A	0 0 0 0 1	01	01	01
"	B	0 0 0 1 0	02	02	02
#	C	0 0 0 1 1	03	03	03
\$	D	0 0 1 0 0	04	04	04
%	E	0 0 1 0 1	05	05	05
&	F	0 0 1 1 0	06	06	06
'	G	0 0 1 1 1	07	07	07
(H	0 1 0 0 0	10	08	08
)	I	0 1 0 0 1	11	09	09
*	J	0 1 0 1 0	12	10	0A
+	K	0 1 0 1 1	13	11	0B
,	L	0 1 1 0 0	14	12	0C
-	M	0 1 1 0 1	15	13	0D
.	N	0 1 1 1 0	16	14	0E
/	O	0 1 1 1 1	17	15	0F
0	P	1 0 0 0 0	20	16	10
1	Q	1 0 0 0 1	21	17	11
2	R	1 0 0 1 0	22	18	12
3	S	1 0 0 1 1	23	19	13
4	T	1 0 1 0 0	24	20	14
5	U	1 0 1 0 1	25	21	15
6	V	1 0 1 1 0	26	22	16
7	W	1 0 1 1 1	27	23	17
8	X	1 1 0 0 0	30	24	18
9	Y	1 1 0 0 1	31	25	19
:	Z	1 1 0 1 0	32	26	1A
;	[1 1 0 1 1	33	27	1B
<	\	1 1 1 0 0	34	28	1C
=]	1 1 1 0 1	35	29	1D
>	~	1 1 1 1 0	36	30	1E

Factory Selected Address →

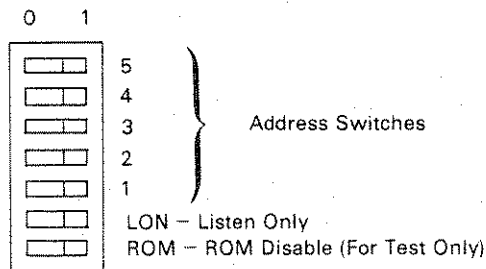

NOTE: The Equivalent Codes shown correspond only to the 5-bit binary switch code. These bits are the same for both listen and talk addresses, and the sixth and seventh bits determine whether the address is listen (01) or talk (10). Some controllers distinguish between listen and talk automatically, requiring only the 5-bit code equivalent to designate a device.

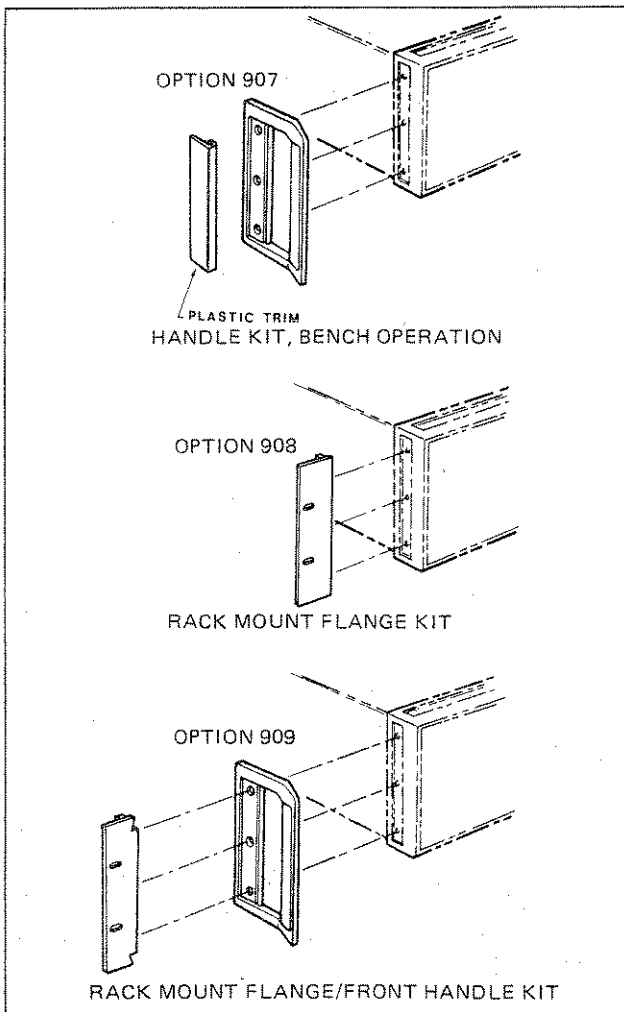


Figure 2-3. Rack Mount and Handle Kits.

2-33. Instrument Identification.

2-34. If the instrument is being returned to Hewlett-Packard for servicing, attach a tag indicating the type of service required, return address, model number, and full serial number. In any correspondence, refer to the instrument by model number and full serial number.

2-35. Packaging.

2-36. **Original Packaging.** If the original packaging has been retained, pack the instrument in the same manner as it was received. Be sure to seal the shipping container securely. Also, mark the container FRAGILE to assure careful handling.

2-37. **Other Packaging.** The following general instructions should be used for repackaging with commercially available materials.

a. Wrap the instrument in heavy paper or plastic. (If shipping to a Hewlett-Packard office or service center, attach a tag indicating the type of service required, return address, model number, and full serial number.)

b. Use a strong shipping container. A doublewall carton made of 250-pound test material is adequate.

c. Use enough shock-absorbing material (3-to-4 inch layer) around all sides of the instrument to provide firm cushion and prevent movement inside the container. Protect the control panel with cardboard.

d. Seal the shipping container securely.

e. Mark the shipping container FRAGILE to assure careful handling.

SECTION III

OPERATION

TABLE OF CONTENTS

Paragraph	Page
3-1. Introduction	3-1
3-3. Panel Features	3-3
3-5. Power/Warm-Up	3-3
3-8. Initial Conditions	3-3
3-10. Self Test	3-3
3-12. Front/Rear Signal Output	3-3
3-14. Sync Output	3-3
3-16. External Reference Input	3-4
3-18. 10MHz Oven Option 001	3-4
3-20. Manual Programming	3-4
3-22. Clear Display	3-4
3-24. Entry Errors	3-4
3-26. Function Selection	3-4
3-28. Frequency Entry	3-4
3-30. Frequency Limits	3-4
3-32. Frequency Display and Resolution	3-5
3-34. Auxiliary Output (Sine Function Only)	3-5
3-36. Amplitude Entry	3-5
3-39. Amplitude Calibration	3-5
3-41. High Voltage Output Option 002	3-6
3-43. DC Offset	3-6
3-46. Phase Entry	3-7
3-49. Frequency Sweep	3-7
3-55. Sweep Marker	3-9
3-58. Sweep X Drive Output	3-10
3-60. Sweep Z Blank Output	3-10
3-62. Amplitude Modulation	3-10
3-66. Phase Modulation	3-11
3-68. Modify Keys	3-11
3-70. Store and Recall	3-11
3-72. Operator's Checks	3-11
3-74. Self Test	3-11
3-76. Output Checks	3-11
3-78. Operator's Maintenance	3-12
3-81. HP-IB Operation	3-12
3-83. General HP-IB Description	3-13
3-88. Definition of HP-IB Terms and Concepts	3-13
3-89. Basic Device Communication Capability	3-14
3-91. Message Definitions	3-14
3-93. 3325A Response to Messages	3-14
3-95. HP-IB Work Sheet	3-14
3-97. HP-IB Addressing	3-14

3-100.	3325A Remote Programming	3-14
3-101.	3325A HP-IB Capabilities	3-14
3-103.	Developing an HP-IB Program	3-15
3-107.	Universal and Addressed Commands	3-17
3-109.	Placing the 3325A in Remote	3-17
3-111.	The 3325A Address	3-17
3-113.	3325A Data Message Formats	3-17
3-115.	Data Transfer Mode	3-20
3-118.	Programming Data Transfer Mode	3-21
3-120.	Programming Entry Parameters	3-21
3-122.	Programming Waveform Function	3-21
3-124.	Programming Binary (On or Off) Functions	3-22
3-126.	Programming Selection Functions	3-22
3-128.	Programming Execution Functions	3-22
3-130.	Programming Amplitude Units Conversion	3-23
3-132.	Programming Storage Registers	3-23
3-134.	Service Requests	3-23
3-136.	Serial Poll	3-23
3-138.	Status Byte	3-24
3-140.	Busy Flag	3-24
3-142.	Sweep Flag	3-24
3-144.	Masking or Enabling Service Requests	3-24
3-146.	Interrogating Program Errors	3-24
3-148.	Interrogating Entry Parameters	3-25
3-150.	Interrogating Function (Waveform)	3-25
3-152.	Interrogating Miscellaneous Parameters	3-26
3-154.	Using the Interrogate Capability	3-26
3-156.	3325A Programming Procedure	3-27
Appendix A. Meta Messages Block Diagrammed		A-1
Appendix B. Programming the Model 3325A with the 9825A Calculator		B-1

LIST OF ILLUSTRATIONS

Figure	Page
3-1. Front and Rear Panel Controls	3-2
3-2. Maximum DC Offset With AC Functions	3-8
3-3. Interface Connections and Bus Structure	3-13

LIST OF TABLES

Table	Page
3-1. Operating Information	3-1
3-2. Amplitude Limits of AC Functions	3-5
3-3. High Voltage Output Amplitudes (Option 002)	3-6
3-4. Maximum DC Offset with any AC Function	3-7
3-5. General Interface Management Lines	3-14
3-6. Definition of Meta Messages	3-15
3-7. 3325A Implementation of Messages	3-16
3-8. Interface Functions	3-16
3-9. Summary of 3325A Programming (ASCII)	3-18
3-10. Programming Codes	3-19
3-11. SRQ Mask/Enable Data	3-25

SECTION III OPERATION

3-1. INTRODUCTION.

3-2. This section of the manual contains instructions for manual operation and HP-IB (Hewlett-Packard In-

terface Bus) programming. The HP-IB information includes the basic concepts of the interface bus operation, with which you may already be familiar. Use Table 3-1 to locate the information you need for your particular situation.

Table 3-1. Operating Information.

Paragraph	Content	Paragraph	Content
3-3	PANEL FEATURES (Figure 1-1)	3-100	3325A REMOTE PROGRAMMING
3-5	POWER/WARMUP	3-101	3325A HP-IB Capabilities
3-8	INITIAL CONDITIONS		Table 3-8, Interface Functions
3-10	SELF TEST	3-103	Developing an HP-IB Program
3-12	FRONT/REAR SIGNAL OUTPUT	3-107	Universal and Addressed Commands
3-14	SYNC OUTPUT	3-109	Placing the 3325A in Remote
3-16	EXTERNAL REFERENCE INPUT	3-111	The 3325A Address
3-18	10 MHz OVEN OPTION 001		Table 3-9, Summary of 3325A Programming, ASCII Characters
3-20	MANUAL PROGRAMMING		Table 3-10, Programming Codes
3-22	Clear Display	3-113	3325A Data Message Formats
3-24	Entry Errors	3-115	Data Transfer Mode
3-26	Function Selection	3-118	Programming Data Transfer Mode
3-28	Frequency Entry	3-120	Programming Entry Parameters
3-30	Frequency Limits		Frequency
3-32	Frequency Display and Resolution		Amplitude
3-34	Auxiliary Output (Sine Function Only)		Offset
3-36	Amplitude Entry		Phase
	Table 3-2, Amplitude Limits of AC Functions		Sweep Start Frequency
3-39	Amplitude Calibration		Sweep Stop Frequency
3-41	High Voltage Output Option 002		Sweep Marker Frequency
	Table 3-3, High Voltage Output Amplitudes		Sweep Time
3-43	DC Offset	3-122	Programming Waveform Function
	Table 3-4 and Figure 3-2, Maximum DC Offset	3-124	Programming Binary (ON or OFF) Function
3-46	Phase Entry		High Voltage Output (Option 002)
3-49	Frequency Sweep		Amplitude Modulation
3-55	Sweep Marker		Phase Modulation
3-58	Sweep X Drive Output	3-126	Programming Selection Functions
3-60	Sweep Z Blank Output		Rear Output/Front Output
3-62	Amplitude Modulation		Linear Sweep/Logarithmic Sweep
3-66	Phase Modulation		Data Transfer Mode
3-68	Modify Keys	3-128	Programming Execution Functions
3-70	Store and Recall		Assign Zero Phase Reference
3-72	OPERATOR'S CHECKS		Perform Amplitude Calibration
3-74	Self Test		Start Single Sweep
3-76	Output Checks		Start Continuous Sweep
3-78	OPERATOR'S MAINTENANCE		Perform Self Test
3-81	HP-IB OPERATION	3-130	Programming Amplitude Units Conversion
3-83	General HP-IB Description	3-132	Programming Storage Registers
	Figure 3-3, Interface Connections and Bus Structure	3-134	Service Requests
	Table 3-5, General Interface Management Lines	3-136	Serial Poll
3-88	Definition of HP-IB Terms and Concepts	3-138	Status Byte
3-89	Basic Device Communication Capability	3-140	Busy Flag
3-91	Message Definitions	3-142	Sweep Flag
	Table 3-6, Definition of Meta Messages	3-144	Masking or Enabling Service Requests
3-93	3325A Response to Messages		Table 3-11, SRQ Mask/Enable Data
	Table 3-7, Implementation of Messages	3-146	Interrogating Program Errors
3-95	HP-IB Work Sheet	3-148	Interrogating Entry Parameters
3-97	HP-IB Addressing	3-150	Interrogating Function (Waveform)
		3-152	Interrogating Miscellaneous Parameters
		3-154	Using the Interrogate Capability
		3-156	3325A Programming Procedure


Appendices

A-3

B-3

META MESSAGES BLOCK DIAGRAMMED
PROGRAMMING THE MODEL 3325A with the
9825A CALCULATOR

- 8 DATA group. This group includes the numeric data keys, the data value suffix keys, the Store and Recall command keys, and the entry Clear key. When preceded by the blue prefix key, the keys in the left column control the modulation functions.
 - 9 MODIFY group. The horizontal arrow keys select the digit to be modified (indicated by a bright digit), and the vertical arrow keys increment or decrement that digit.
 - 10 UNITS annunciators. Display the units of volume represented by the numeric display. Entry annunciator indicates that an entry is in progress.
 - 11 FUNCTION group. These keys select the output signal function or dc only (see Paragraph 3-26).
 - 12 EXT REF annunciator is on if an external reference or the Option 001 internal 10 MHz oven reference is connected to the rear panel REF IN. Annunciator flashes if the 30 MHz internal reference is not phase locked to the external reference.
 - 13 MODULATION annunciator is on if either AM or Phase modulation is programmed.
 - 14 AMPTD CAL key. Automatically calibrates the amplitude and offset of the output signal (see Paragraph 3-39). When preceded by the blue prefix key, initiates a self test operation (see Paragraph 3-10).
- CAUTION**
The maximum peak voltage that can be safely applied between chassis and the outer conductor of any of the 3325A input or output signal connectors is ± 42 V.
- 15 SYNC OUT. A square wave sync signal is available at this connector and also at a rear panel connector, item 28. This signal is always in sync with the output signal cross-over point. (Zero volts or dc offset voltage, see Paragraph 3-14.) J2.
 - 16 AUX 21-60 MHz REAR annunciator. This annunciator is on when the rear panel AUX output is active (see Paragraph 3-34).
 - 17 REAR ONLY key. In standard instruments, switches signal output from front to rear panel and vice versa. Rear panel output is active when the annunciator in the center of the key is on. In instruments with High Voltage Output Option 002, this key switches from normal to high voltage output, and the annunciator indicates when the high voltage output is on. The key is labeled "40 Vpp, 40 mA, 0-1 MHz" for Option 002. In Option 002 instruments, no rear panel signal output is provided.
 - 18 SIGNAL output. Standard output impedance is 50 ohms. High Voltage Output Option 002 output impedance is nominally < 1 ohm at dc and < 10 ohms at 1 MHz. Load impedance must be at least 500 ohms. Standard and High Voltage amplifier outputs are fused. J1.
 - 19 10 MHz OVEN OUTPUT. This signal is present only in instruments with Option 001. To make use of the Oven Output, it must be connected to the REF IN connector, item 21. A special connector, -hp- Part No. 1250-1499, is supplied with Option 001 for this purpose. J3.
 - 20 AC POWER input connector. E1.
 - 21 REF IN. An external reference may be used to phase lock the internal 30 MHz reference (see Paragraph 3-16). J4.
 - 22 HP-IB connector. Remote control of the 3325A by means of an HP-IB system controller is accomplished through this connector. Part of W6.
 - 23 REF OUT. A 1 MHz signal from the 3325A reference circuits is available at this connector. J5.
 - 24 SIGNAL. The output signal is switched to this connector by the front panel REAR ONLY key, item 17. J6. (Instruments with Option 002 do not have rear panel signal output.)
- NOTE**
The rear panel signal output is inactive (no internal signal connection) if the instrument has the High Voltage Output Option 002 installed. Instructions are given in the Operating and Service Manual, Section VIII, Service Group M, for activating the rear panel signal output in one of two ways: 1) Placing the standard/high voltage output on the rear panel only, disconnecting the front panel signal output, or 2) Disabling the high voltage output and enabling the standard front/rear output configuration.
- If the standard instrument signal output is not terminated by an external 50-ohm load (a high impedance load, for example) undesirable distortion may result, particularly at higher frequencies. Similar conditions may result if the High Voltage Output (Option 002) is terminated by less than 500 ohms.
- 25 BLOWER, B1.
 - 26 PHASE MOD. Input connector for a phase modulating signal of ± 5 V maximum peak voltage (see Paragraph 3-66). J7.
 - 27 AMPTD MOD. Input connector for an amplitude modulating signal of ± 5 V maximum peak voltage (see Paragraph 3-62). J8.
 - 28 SYNC OUT. This output is identical to the output at the front panel sync connector, item 15. J10.
 - 29 AUX 21-60 MHz. A signal is available at this output when the sine wave frequency is programmed above 21 MHz (see Paragraph 3-34). J9.
 - 30 Z BLANK. A TTL compatible output is present during a sweep operation (see Paragraph 3-60). J11.
 - 31 X DRIVE. This output progresses from 0 V to +10 V during a sweep-up operation (see Paragraph 3-58). J12.
 - 32 MARKER. This TTL compatible output goes low at the selected marker frequency during a sweep up, and high at completion of the sweep (see Paragraph 3-55). J13.
 - 33 Power Transformer, T1.
 - 34 Line Fuse, F1.

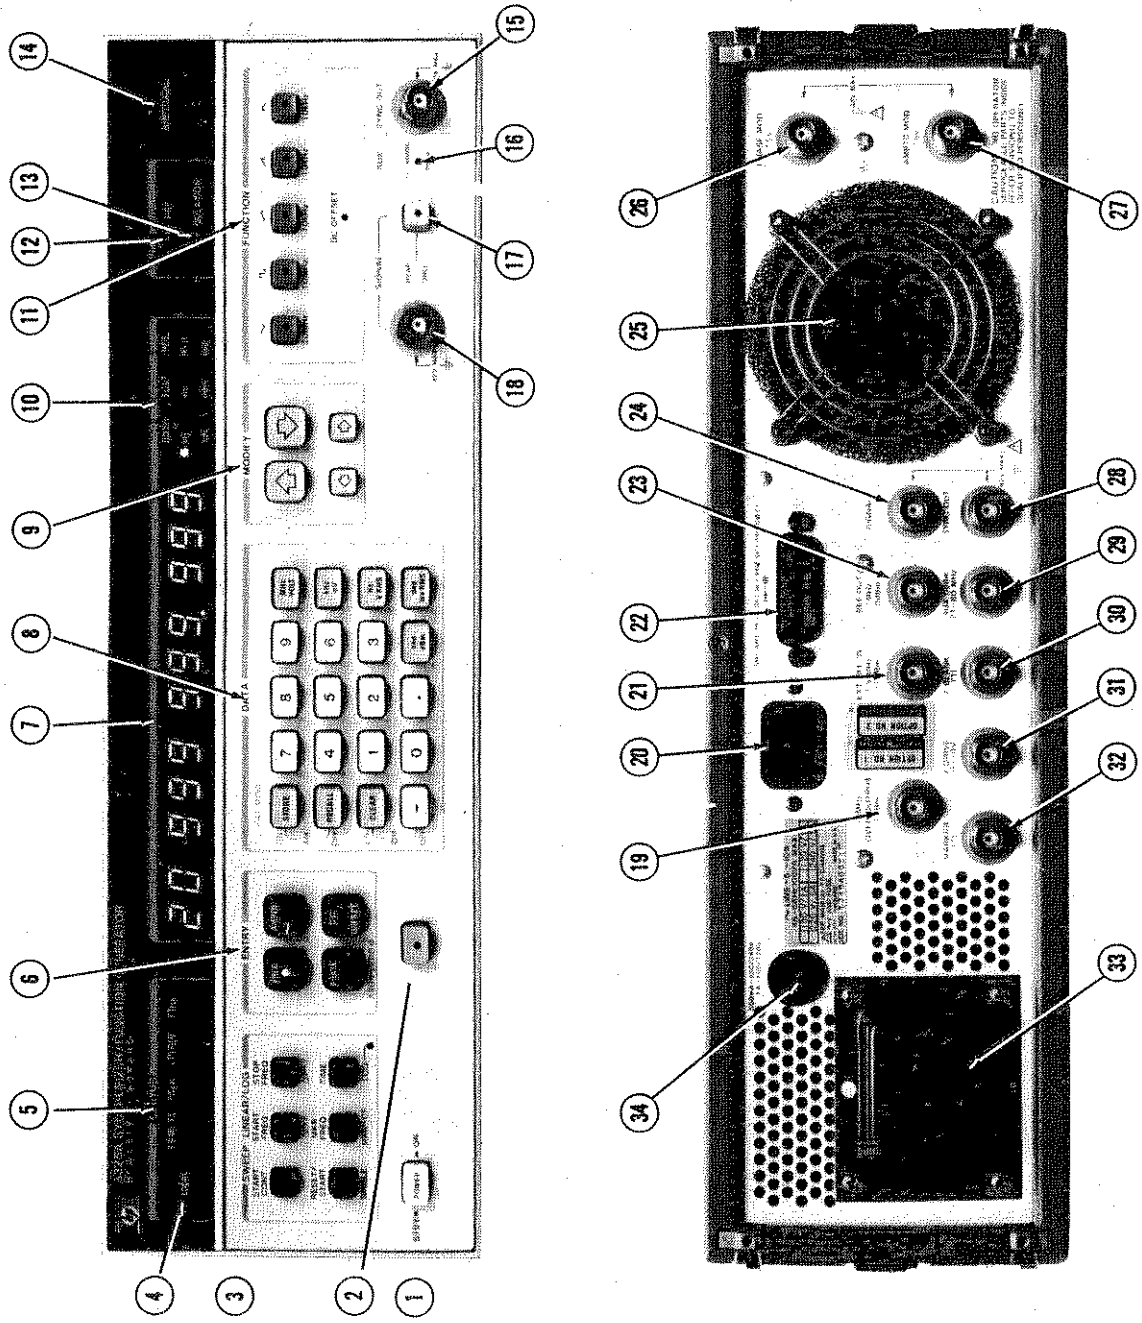

- 1 POWER STBY/ON Key. In the STBY position, power is applied to the Oven (Option 001), the HP-IB interface circuits that are external to the isolation barrier, and the High Voltage Output circuits (Option 002), in addition to the power supply circuits.
- 2 BLUE prefix key. This key must be pressed to select any of the key functions labeled in blue.
- 3 SWEEP key group. These are entry prefix keys for the sweep parameters, plus the sweep start keys. When preceded by the blue prefix key, the sweep parameter keys control sweep modification functions and linear/log selection.
- 4 LOCAL key. Returns 3325A from remote to front panel control unless Local Lockout has been programmed. When preceded by the blue prefix key, this key causes the 3325A HP-IB address to be displayed in decimal code.
- 5 STATUS annunciator group. These annunciators indicate the 3325A HP-IB status: Remote; Addressed to Talk; Addressed to Listen; Request Service (SRQ).
- 6 ENTRY group. Prefix keys for programming signal parameters.
- 7 ALPHANUMERIC display. Displays the value of the parameter selected, error codes, failure modes, HP-IB address, amplitude and phase modulation state.

Figure 3-1. 3325A Front and Rear Panels.

NOTE

The HP-IB is Hewlett-Packard Company's implementation of IEEE Standard 488-1978.

3-3. PANEL FEATURES.

3-4. Figure 3-1 identifies and describes the functions of the front and rear panel controls, indicators, and connectors.

3-5. POWER/WARM-UP.

3-6. The Model 3325A requires a power source of 100, 120, 220, or 240 Vac, +5% -10%, 48 to 66 Hz single phase. The selection of line voltage and fuse is described in Paragraph 2-8 and Figure 2-1.

3-7. The 3325A POWER switch has two positions, STBY and ON. Power is applied to some circuits at any time the instrument is connected to the ac power source. If the instrument has the Oven Assembly Option 001 installed, it is important that it remain connected to the power source to maintain a constant oven temperature, eliminating the need for a long warm-up period. If an instrument with the Oven Assembly has been disconnected from ac power no longer than 24 hours, a 15-minute warmup period is sufficient to bring the reference frequency to within $\pm 1 \times 10^{-7}$ of final value.

3-8. INITIAL CONDITIONS.

3-9. After the POWER switch has been set to ON, the instrument status will be as follows:

Function	Sine
Frequency	1000 Hz
Amplitude	1 mV p-p
Phase	0 deg
DC Offset	0 V
Front Signal Output	
Sweep	Linear
Start Frequency	1 MHz
Stop Frequency	10 MHz
Marker Frequency	5 MHz
Time	1 sec

NOTES

1. If the display reads OSC FAIL the frequency synthesis circuits are not operating properly.
2. If A-CAL FAIL appears in the display momentarily after turn-on, any one of the three AMPTD CAL tests could be incorrect. Perform a SELF TEST operation to identify the failure.
3. If either of the above conditions occurs, refer the instrument to qualified service personnel for repair.

3-10. SELF TEST.

3-11. The self test operation is initiated by pressing the blue prefix key, then the SELF TEST key (AMPTD CAL). This test uses the control, ROM, and control clock circuits to perform the following checks:

- LED check: Turns on all LED's for about 2 seconds
- Check 1: Tests AMPTD CAL of the sine wave
- Check 2: Tests AMPTD CAL of the square wave
- Check 3: Tests AMPTD CAL of the triangle wave

Following each check the display indicates either PASS or FAIL for approximately one second. If all tests pass, this indicates that approximately 60% of all circuits are operating properly.

3-12. FRONT/REAR SIGNAL OUTPUT.



The maximum peak voltage that can be safely applied between chassis and the outer conductor of any of the 3325A input or output signal connectors is ± 42 V.

3-13. The standard Model 3325A provides selectable front or rear panel 50-ohm signal outputs. The rear panel signal output is selected by pressing the REAR ONLY key. The lighted indicator in the center of this key denotes that the signal output is at the rear panel.

NOTE

The rear panel SIGNAL output is not present on instruments equipped with the High Voltage Output Option 002.

3-14. SYNC OUTPUT.

3-15. A square wave sync output is provided at BNC connectors on both the front and rear panels. This sync signal is always in phase with the output signal, with the sync transition occurring at the signal zero crossing, or when the signal crosses the dc offset voltage. The output impedance of either front or rear panel sync output is approximately 50 ohms. When connected to a 50-ohm coaxial cable that is terminated by a 50 ohm resistive load, the sync signal levels are as follows:

- Low Level = < 0.2 V
- High level = > 1.2 V

NOTE

If a sync output is connected to a 50-ohm coaxial cable that is terminated by a high impedance load (≥ 1 megohm) the voltage levels are approximately twice the values given above. However, the improper ter-

mination of the 50-ohm system will cause ringing at the positive and negative transitions of the sync signal.

3-16. EXTERNAL REFERENCE INPUT.

3-17. The 3325A may be operated with an external reference to control the standard 30 MHz internal reference oscillator frequency. The external reference level must be greater than 0 dBm (50 ohms), and the frequency must be within 10 PPM of 10 MHz or a sub-multiple thereof down to 1 MHz (10, 5, 3.33, 2.5, or 1 MHz). The front panel EXT REF annunciator will light to indicate that an external reference is being used. The internal reference oscillator is phase locked to the external reference, and a phase lock detector circuit causes the EXT REF light to flash if synchronization is lost.

3-18. 10 MHz OVEN OPTION 001.

3-19. Option 001 is a temperature stabilized 10 MHz oscillator which provides improved frequency stability (see specifications in Table 1-1). The output from this oscillator is at the rear panel 10 MHz OVEN OUTPUT connector. This output must be connected to the EXT REF input. A special connector, -hp- Part No. 1250-1499, is provided with Option 001 for this purpose.

3-20. MANUAL PROGRAMMING.

3-21. The following paragraphs describe the procedures for operating the 3325A from the front panel. Also included are the limits for each parameter.

3-22. Clear Display.


3-23. Pressing the CLEAR key (in the left column of the DATA group) clears the display to zero. This key is useful when an error is made while entering data.

3-24. Entry Errors.

3-25. The word "Error" will appear in the display for approximately one second when an error in programming occurs. The incorrect entry will not be accepted.

ASCII Numeric	Error
1	Entry parameter out of bounds (for example, Freq \geq 61 MHz)
2	Invalid delimiter
3	Frequency too large for function (for example, Function = Triangle, Freq \geq 11 kHz)
4	Sweep time too small or too large
5	Offset incompatible with amplitude, or amplitude incompatible with offset
6	Sweep frequency too large for function; Sweep bandwidth too small; Start frequency too small (log sweep); Start frequency greater than stop frequency (log sweep)
7	Unrecognizable mnemonic received
8	Unrecognizable data character received
9	Option does not exist (High Voltage or Rear/Front)

3-26. Function Selection.

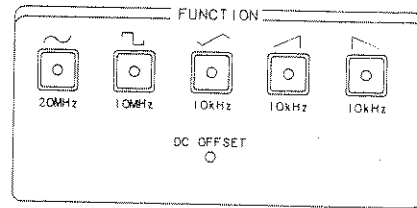


3-27. Any of the five functions may be selected by pressing the appropriate FUNCTION key. A light in the center of the key indicates the present function. Pressing the same key the second time removes the ac signal, setting the output to zero unless a dc offset has been programmed (see Paragraph 3-43). When the ac signal is removed in this way, the instrument automatically displays dc offset, and the dc offset entry key light comes on. The ac signal can be restored by pressing the FUNCTION key again. The output signal for each function is centered about zero volts unless a dc offset has been programmed.

NOTE

The standard instrument signal output must be terminated by an external 50-ohm load or sine wave distortion and square wave overshoot may result, particularly at higher frequencies.

3-28. Frequency Entry.

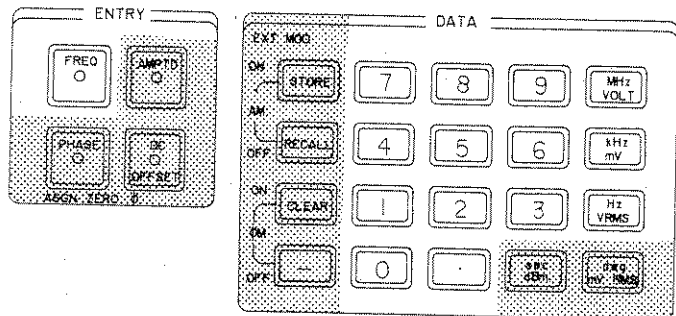

NOTE

A lighted indicator in the center of any entry key denotes it as the active entry parameter. For example, if the FREQ entry key indicator is on, it is not necessary to press that key before entering data.

3-29. Enter frequency by first pressing the FREQ ENTRY key, then the numerical data, followed by the data suffix (delimiter) key (Hz, kHz, MHz). Numerical data must be entered most significant digit first, entering the decimal in the proper place. The frequency parameter is stored in the 3325A when the delimiter key is pressed.

3-30. Frequency Limits.

3-31. The minimum frequency for all functions is 1 μ Hz. The nominal maximum frequency for each function is shown below the function select key on the front

Table 3-2. Amplitude Limits of AC Functions.

Function	Peak-to-Peak		rms		dBm (50 Ω)	
	Max.	Min.	Max.	Min.	Max.	Min.
Sine	10 V	1 mV	3.536 V	0.354 mV	+23.98	-56.02
Square	10 V	1 mV	5.000 V	0.5 mV	+26.99	-53.01
Triangle	10 V	1 mV	2.888 V	0.289 mV	+22.22	-57.78
± Ramp	10 V	1 mV	2.888 V	0.289 mV	+22.22	-57.78

panel. However, because of the overrange capability of the 3325A, the maximum frequency for each function is as shown below:

Sine wave	20 999 999.999 Hz
Square wave	10 999 999.999 Hz
Triangle	10 999.999 999 Hz
Positive slope ramp	10 999.999 999 Hz
Negative slope ramp	10 999.999 999 Hz

3-32. Frequency Display and Resolution.

3-33. Frequency is always displayed in Hz, even though the entry may have been made in kHz or MHz. For example, an entry of 1.2 MHz is displayed as 1 200 000.0 Hz. Non-significant zeroes to the right of the first digit following the decimal point are not displayed except during a “modify” condition (see Paragraph 3-68). The maximum resolution is 1 μHz for frequencies up to and including 99 999.999 999 Hz, and 1 mHz for frequencies of 100 000.000 Hz and higher.


3-34. Auxiliary Output (Sine Function Only).

3-35. A rear panel auxiliary output can be used for frequencies above 19 MHz to a maximum of 60 999 999.999 Hz. The output level is a nominal 0 dBm into 50 ohms. The output automatically switches to the AUX output when frequencies of 21 000 000.000 Hz or higher are programmed. For this reason, the AUX output is labeled “21–60 MHz”. Frequencies between 19 MHz and 21 MHz can be obtained at the AUX output only by first entering 21 MHz or higher, then entering the desired frequency. For example, if the desired frequency is 19.5 MHz, first enter “FREQ 21 MHz”, then “19.5 MHz”. Then, if a front panel SIGNAL output of 19.5 MHz (or any frequency between 19 MHz and 21 MHz) is desired, enter any frequency 19 MHz or lower, then enter 19.5 MHz.

NOTE

Only one signal output is active at one time. A lighted “21-60 MHz Rear” annunciator indicates that the rear panel AUX, 0 dBm, 21-60 MHz output is active. A lighted “Signal, Rear Only” annunciator indicates that the rear panel signal output is active. Neither light on, indicates the front panel signal output is active.


3-36. Amplitude Entry.

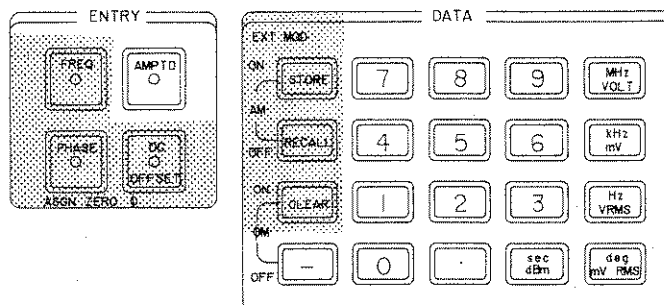

3-37. Amplitude is entered and displayed with 4-digit resolution. Press the AMPTD ENTRY key, then the numerical data, followed by the V, mV, Vrms, mVrms, or dBm key. The V and mV keys enter peak-to-peak value of ac functions. Maximum and minimum amplitudes for each function are shown in Table 3-2.

3-38. The 3325A will convert an amplitude value between peak-to-peak, rms, or dBm for any function. For example, if a sine wave amplitude of 10 V p-p has been entered, press the Vrms or mVrms key to display the same amplitude as 3.536 Vrms, or press the dBm key to display the value as (+)23.98 dBm.

3-39. Amplitude Calibration.

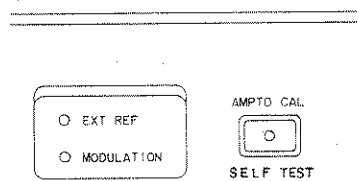


3-40. The 3325A will calibrate the output signal when the AMPTD CAL key is pressed. The output goes to less than 4 mV p-p while the calibration is in process. An amplitude and offset calibration is performed automatically whenever the function is switched and at instrument turn-on.

NOTE

If A-CAL FAIL appears in the display momentarily after an AMPTD CAL operation, the instrument should be referred to qualified service personnel for repair.

3-41. High Voltage Output Option 002.

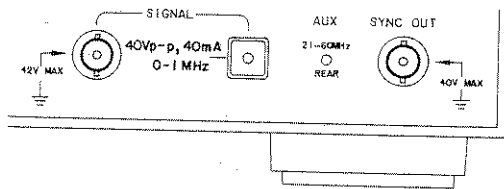

3-42. The high voltage output is selected by pressing the key in the lower right corner of the front panel. This option provides a maximum output of 40 V p-p into a high impedance. The load resistance must be greater than 500 ohms or distortion will result, particularly at higher frequencies. To assure square wave overshoot < 5% of peak-to-peak output, the total capacitance connected to the output should be < 500 pF. The same entry procedures and display features apply as in the standard operation. Maximum and minimum amplitudes are shown in Table 3-3. Maximum frequency for sine and square wave functions is 1 MHz (10 kHz for triangle and ramps).

NOTE

The rear panel signal output is inactive (no internal signal connection) if the instrument has the High Voltage Output Option 002 installed. Instructions are given in the Operating and Service Manual, Section VIII, Service Group M, for activating the rear panel signal output in one of two ways: 1) Placing the standard/high voltage output on the rear panel only, disconnecting the front panel signal output, or 2) Disabling the high voltage output and enabling the standard front/rear output configuration.

3-43. DC Offset.

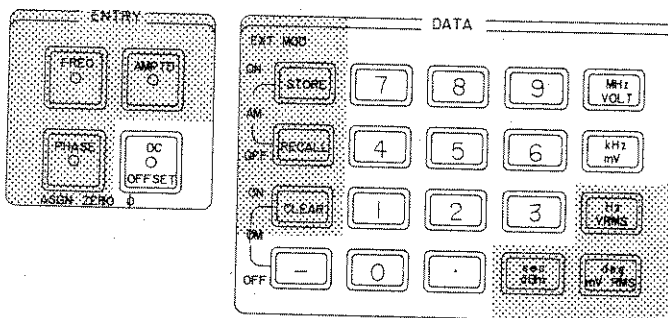


Table 3-3. High Voltage Output Amplitudes (Option 002).

Function	Peak-to-Peak		rms	
	Max.	Min.	Max.	Min.
Sine	40 V	4 mV	14.14 V	1.42 mV
Square	40 V	4 mV	20.0 V	2.0 mV
Triangle	40 V	4 mV	11.55 V	1.16 mV
± Ramp	40 V	4 mV	11.55 V	1.16 mV

3-44. Offset Only, No AC Function. When no ac function is present, the dc voltage output may be programmed from 0mV to ±5V, with 4 digit resolution. When no ac function is present, the DC OFFSET entry prefix is automatically selected. It is necessary merely to enter the numerical data followed by the V or mV delimiter. The rms keys cannot be used to enter offset.

NOTE

When the High Voltage Output is selected (Option 002), minimum amplitude for dc only (no ac function) is 0.01 mV and maximum is 20.0 V.


3-45. Offset with AC Function. When dc offset is to be added to any ac function, there are minimum and maximum offset limits which must be observed. These limits are affected by the ac voltage and the resulting attenuator settings, which are shown in Table 3-4: Figure 3-2 is a set of graphs which show the approximate maximum dc offset permissible for a given ac peak-to-peak voltage. The following equation may be used to determine maximum offset voltage.

$$\text{Maximum dc offset} = \frac{5}{A} - \frac{\text{Amptd}}{2}$$

Where A = Attenuator factor (from Table 3-4)
Amptd = Amplitude in V p-p of the ac function

NOTES

1. If an attempt is made to enter a dc offset that is too great for the amplitude already programmed, "Error 5" will appear in the display momentarily, and the dc offset entry will not be accepted.
2. After a dc offset has been entered, if the amplitude (ac) is then increased beyond the level where the amplitude and offset are compatible, "Error 5" will appear in the display momentarily, and the ac amplitude entry will not be accepted.

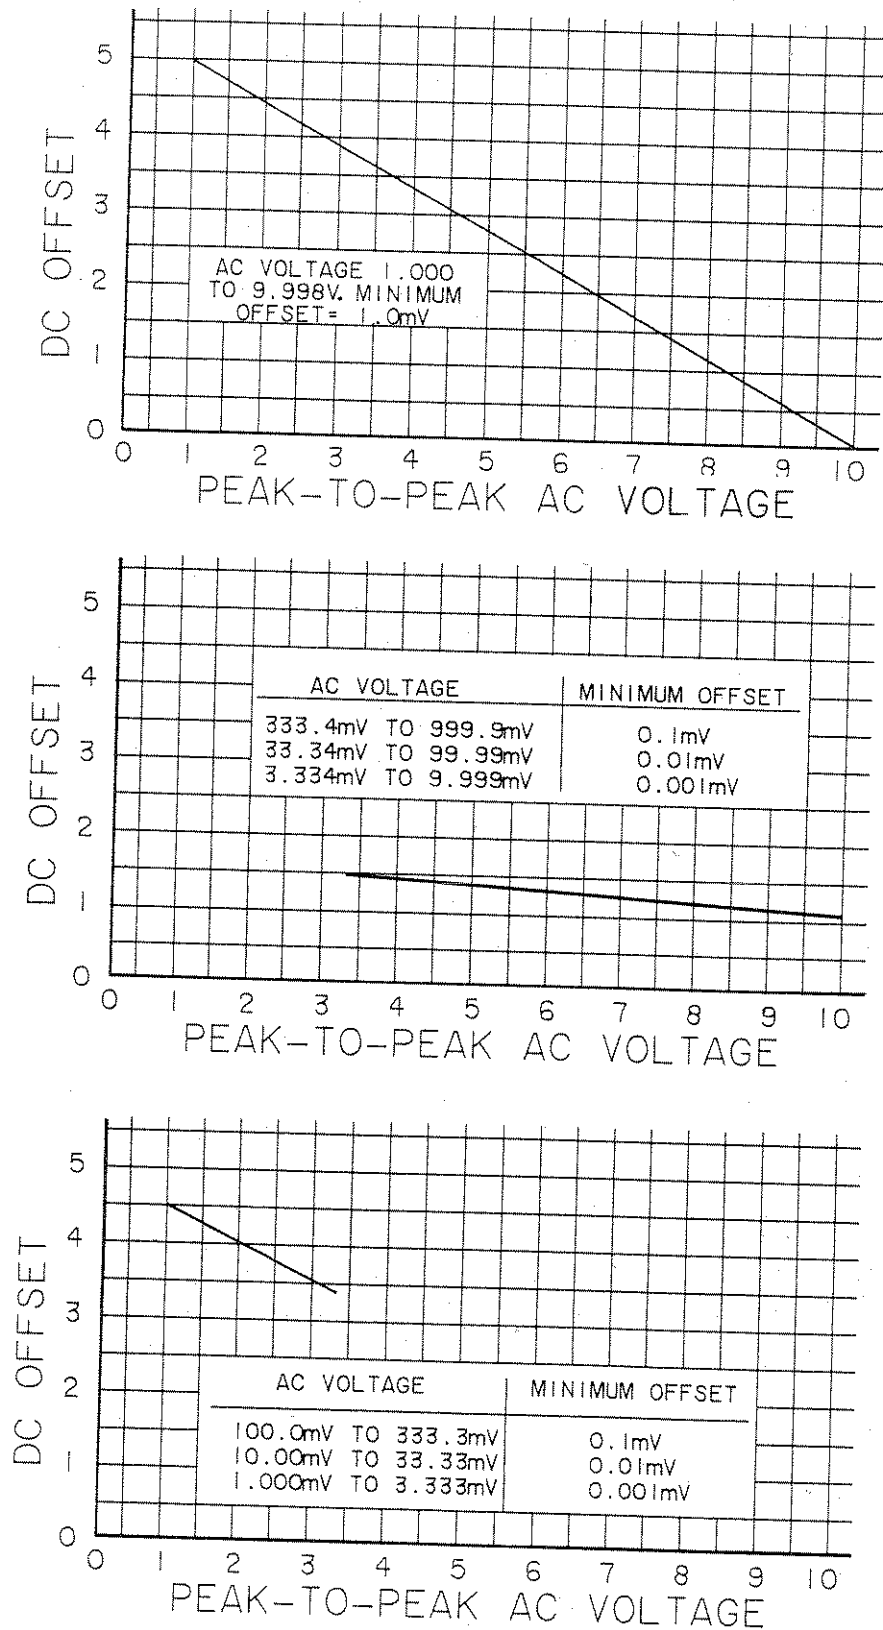


3325A-30

Figure 3-2. Maximum DC Offset With AC Functions.

NOTE

The Marker Frequency must be lower than Stop Frequency by a sufficient amount to permit the Marker pulse width to be approximately 400 microseconds. See Paragraph 3-55.


To change any of the sweep parameters, press the appropriate SWEEP entry key, then enter the desired data. To select LOG sweep, press the blue prefix key and then the LOG (TIME) key. The log indicator should light. The sweep mode is linear unless this light is on.




3-51. Linear Sweep. In linear mode, either CONTINUOUS or SINGLE sweep may be used. Single sweep is from START to STOP frequency, and either START or STOP may be the higher frequency. To begin a single sweep:

Press "RESET/START" key to set output and display to the start frequency selected and reset the X Drive ramp.

Press "RESET/START" key again to start the sweep.



The output frequency sweeps to the STOP frequency selected and remains there. This frequency appears in the display. Continuous sweep is up-down-up, etc., and begins when the "START CONT" key is pressed. Continuous sweep may be stopped by pressing the "START CONT" key again, or by pressing "START SINGLE", "FREQ ENTRY", or "PHASE ENTRY". The display will indicate the frequency at which the sweep stopped. The sweep will stop while any other parameter is being changed, then will restart. Pressing "AMPTD CAL", "SELF TEST", "ASSIGN ZERO 0", or changing the function will also stop continuous sweep.



3-52. Log Sweep. In either single or continuous log sweep mode, the stop frequency must be higher than the start frequency, and sweep is up only. (Continuous sweep is start to stop, start to stop, etc.) The minimum bandwidth for log sweep is one decade. Single log sweep is a line-segmented log approximation in one-tenth decade seg-

ments, and continuous log sweep is a two-segment log approximation.

NOTE

Because of the computation time required by the control circuits in log sweep, the actual stop frequency (which is displayed at the end of a single sweep) will be higher than the selected stop frequency, but always within 0.25%. The error decreases as sweep time is increased.

3-53. Sweep Time. The maximum time per sweep (up or down) for all sweep modes is 99.99 seconds, with .01 second resolution for times ≥ 1 second, and .001 second resolution for times < 1 second. Minimum times are as follows:

Linear sweep, single or continuous...	0.010 s
Log sweep	
Single.....	2.000 s
Continuous.....	0.100 s

NOTE

In single log sweep, the sweep time is increased by the processing time required between segments. The time increase (in seconds) is approximately equal to

$$.045 \left(10 \log \frac{\text{stop frequency}}{\text{start frequency}} \right)$$

3-54. Sweep Bandwidth. The maximum sweep bandwidth is the full frequency range for the function selected, except that in log sweep, the minimum frequency is 1 Hz. The minimum bandwidth for log sweep is one decade. Minimum bandwidth for each function (linear sweep) is as follows:

Sine.....	(10 mHz/s) \times (sweep time)
Square.....	(5 mHz/s) \times (sweep time)
Triangle.....	(0.5 mHz/s) \times (sweep time)
Ramps.....	(1 mHz/s) \times (sweep time)

For sweep bandwidths of less than 100 times the minimum, Bandwidth selected should be an integral multiple of the minimum. In linear sweep mode the sweep bandwidth may be multiplied or divided by two by pressing the blue prefix key and then " $\Delta f \times 2$ " or " $\Delta f \div 2$ ". These bandwidth modification keys do not operate in log sweep mode.

3-55. Sweep Marker.

3-56. The marker frequency may be set to any point within the sweep band up to within approximately 400 microseconds of the stop frequency. If the marker frequency is set beyond this point, the stop frequency will automatically be increased so that the marker pulse is

approximately 400 microseconds wide. The following equation may be used to determine the approximate maximum marker frequency:

$$\text{Max. marker freq.} = \text{stop freq.} - \frac{.0004 \times \text{bandwidth}}{\text{sweep time}}$$

The rear panel MARKER output is at TTL compatible voltage levels. It is High at the start of a sweep up, goes Low at the selected marker frequency, then High again at the stop frequency. No marker output is present during sweep down or during a log sweep. Set the marker frequency by pressing the "MKR FREQ" key and entering the numerical data and the frequency suffix.

3-57. The sweep band can be moved up or down to center on the marker frequency by pressing the blue prefix key and then the MKR → CF(MKR FREQ) key. This does not change the sweep bandwidth unless either the new upper or lower limit would be beyond the frequency limit for the present function.

3-58. Sweep X Drive Output.

3-59. The rear panel X DRIVE output is as follows:

Linear sweep:

Single: 0 V at start, increasing linearly to > +10 V at stop, whether the sweep is up or down. Remains at essentially this voltage until reset prior to the start of another sweep. (Voltage will drift downward less than 10 mV/s.)

Continuous: Increases linearly from 0 V to > +10 V during sweep up, then goes to 0 V at beginning of sweep down and remains at 0 V during sweep down.

Log sweep: Starts at 0 V and increases to > +10 V with the sweep segments.

NOTE

The X DRIVE output has a nominal voltage of +10.5 V at the end of a sweep. This final voltage is specified to be greater than 10.0 V to ensure compatibility with oscilloscopes having a horizontal sensitivity of 10.0 V for full-screen deflection.

X DRIVE output voltage is linear with time in both linear and log sweep modes.

3-60. Sweep Z Blank Output.

3-61. The Z BLANK output voltages are TTL compatible, and the output logic levels are as follows:

Linear sweep:

Single: Goes LOW at start of sweep, HIGH at stop, whether the sweep is up or down. Remains until start of next sweep.

Continuous: LOW during sweep up, HIGH during sweep down.

Log sweep: Goes LOW at start frequency, HIGH at stop. In single sweep, remains HIGH until start of next sweep. In continuous sweep, is HIGH momentarily at stop frequency.


When the Z BLANK output is low, it is capable of sinking current through a relay or other device. The maximum ratings are:

Maximum current sink: 200 mA

Allowable voltage range: 0 V to +45 V dc

Maximum power (voltage at output x current): 1 W

3-62. Amplitude Modulation.

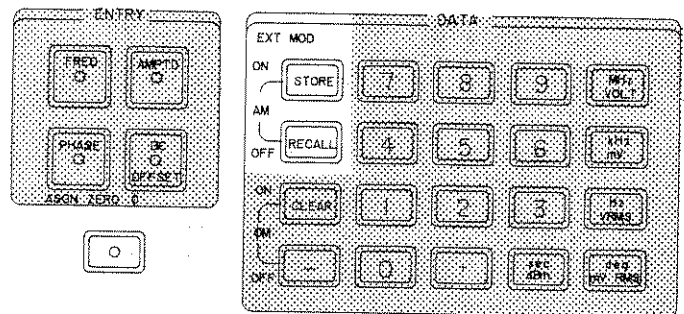


3-63. To program amplitude modulation, press the blue prefix key, then press the "AM ON" (STORE) key. To remove the modulation, press the blue key, then "AM OFF" (RECALL). The display shows "A ON" or "A OFF" momentarily to indicate the status of the amplitude modulation. The status of phase modulation (P ON or P OFF) is displayed at the same time. The modulation input must be connected to the rear panel AMPTD MOD input. The impedance of this input is 20 kΩ (10 kΩ when AM is OFF).

3-64. When amplitude modulation is programmed, the amplitude of the output signal (with no modulation) is halved; however, the display still indicates the programmed amplitude. Then, when the output (carrier) is modulated 100%, the maximum amplitude of the modulated output equals the programmed amplitude. A modulation input of approximately 5 V peak results in 100% modulation. Modulation frequency may be 0 to 50 kHz. If amplitude modulation is ON when 3325A functions other than sine wave are selected, the output may be gated, depending on the level of the modulation input. Amplitude modulation should be used only with the sine wave function, and the modulation input should not exceed ±10 V peak.

3-65. A dc voltage may be applied to the AMPTD MOD input to control the 3325A output level, or a pulse may be used to gate the output. Approximately +5 V cuts off the output signal, while approximately -5 V doubles the output. (Maximum output is 10 V p-p.) DC or pulse inputs should not exceed ±5 V peak.

3-66. Phase Modulation.

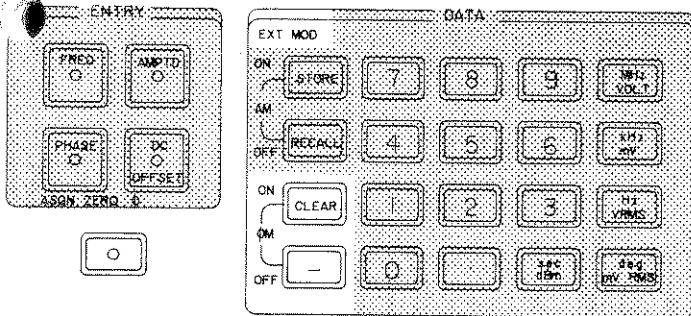

NOTE

Any phase information stored is invalid when recalled because the instrument performs an amplitude calibration on RECALL. Phase relationship between the output signal and the reference is not maintained when AMPTD CAL occurs.

3-67. To program phase modulation, press the blue prefix key, the the “ØM ON” (CLEAR) key, and to remove phase modulation, press the blue key, then “ØM OFF” (-). The phase modulation signal at the rear panel PHASE MOD input may be up to ±10 V peak. The input impedance is 10 kΩ. The modulating signal frequency may be dc to 5 kHz. An input of ±5 V results in the following approximate phase deviation (±170° per volt for sine function):

3325A Function	Phase Deviation
Sine	±850°
Square	±425°
Triangle	±42.5°
± Ramp	±85°

3-72. OPERATOR'S CHECKS.

3-73. The following checks provide the operator with a means of determining whether the instrument is operational. They are not intended to verify any specifications. If the instrument fails any of these checks, it should be referred to qualified service personnel for repair.


3-74. Self Test.

3-75. Press the blue prefix key, then SELF TEST (AMPTD CAL). All the front panel display and annunciator LED's should light for approximately two seconds, then the instrument performs an automatic calibration of the sine, square, and triangle functions and the display indicates momentarily whether each test-passed or failed. The dc offset is also checked in these tests.

NOTE

If the display reads OSC FAIL at any time, the frequency synthesis circuits are not functioning properly. Refer the instrument to qualified service personnel for repair.

3-68. Modify Keys.



3-69. The numerical data of any parameter may be changed by use of the MODIFY keys. First press the prefix key of the parameter to be modified, placing the information in the display. Next, press the ← or → key to move the bright digit cursor to the digit you want to modify. Then press the ↑ or ↓ key momentarily

to increase or decrease the value of that digit by 1. If the modify key is held, the digit will continue to increment or decrement after a slight delay. As the modified digit passes 9 (incrementing) or 0 (decrementing) the digit to its left will increment or decrement.

to increase or decrease the value of that digit by 1. If the modify key is held, the digit will continue to increment or decrement after a slight delay. As the modified digit passes 9 (incrementing) or 0 (decrementing) the digit to its left will increment or decrement.

3-70. Store and Recall.

3-71. An entire program may be stored in any one of 10 registers by pressing the “STORE 0-9” key, then the register number. This stores all the information that is in the current program memory. Other programs may then be entered. All stored information is lost when power is removed from these circuits by setting the POWER switch to STBY or disconnecting ac power from the instrument.

3-76. Output Checks.

3-77. An oscilloscope (-hp- 1740A or equivalent) is required for these checks. Connect the 3325A output through a 50-ohm feedthru termination (-hp- 11048C) to the oscilloscope input (input dc coupled), or set the 1740A input switch to 50 ohms.

FUNCTIONS

a. Make the following 3325A keyboard selections:

FUNCTION Sine
 FREQUENCY 2 kHz
 AMPLITUDE 10 V p-p

b. Set the oscilloscope controls as follows:

Vertical 5 V/div
 Horizontal 0.5 ms/div
 Trigger Auto

c. Adjust oscilloscope controls for a stable display, which should show a sine wave approximately two divisions peak-to-peak and one cycle per division.

d. Select square wave, triangle, positive slope ramp, and negative slope ramp and verify that each function indicates the same frequency and peak-to-peak amplitude.

AMPLITUDE AND DC OFFSET

e. Set the 3325A as follows:

FUNCTION.....Square
 FREQUENCY.....2 kHz
 AMPLITUDE.....10 V p-p

f. Set the oscilloscope controls as follows:

Vertical.....2 V/div
 Horizontal.....0.5 ms/div
 Trigger.....Auto

g. Oscilloscope display should show one square wave per division, 5 divisions peak-to-peak vertical. This checks the output with no attenuation. Actual display will depend greatly upon the accuracy of the oscilloscope amplifiers and display.

h. Change 3325A amplitude to 1 V p-p, and change oscilloscope vertical to .2 V/div. Oscilloscope display should again be 5 divisions peak-to-peak. This checks the +3 attenuator section.

i. Change 3325A amplitude to 500 mV p-p, and change oscilloscope vertical to .1 V/div. Oscilloscope display should be 5 divisions peak-to-peak. This checks the +10 attenuator section.

j. Change 3325A amplitude to 50 mV p-p, and change oscilloscope vertical to .01 V/div. The square wave display should be 5 divisions peak-to-peak. This checks the +100 attenuator section.

k. Press the 3325A SQUARE WAVE FUNCTION key to remove the square wave output. The indicator in the DC OFFSET Entry key should light and the 3325A display should show 0.0 mV.

l. Set the oscilloscope vertical control to 2 V/div. Ground the input and set the trace to the center line. Set input to dc coupled.

m. Enter 5 V offset in the 3325A. The oscilloscope trace should be 2.5 divisions above the center line. Enter -5 V offset in the 3325A. The oscilloscope trace should go to 2.5 divisions below the center line.

n. Enter 0 V offset in the 3325A. Trace should be on the center line.

FREQUENCY

o. Set the 3325A as follows:

FUNCTION.....Sine
 FREQUENCY.....100 Hz
 AMPLITUDE.....10 V p-p

p. Set the oscilloscope controls as follows:

Vertical.....2 V/div
 Horizontal.....1 ms/div

q. Oscilloscope display should show one cycle of sine wave, which should be free of any apparent irregularities.

r. Enter 20 MHz in the 3325A. Change oscilloscope horizontal to .05 μ s/div. Oscilloscope should display one cycle of sine wave per division.

HIGH VOLTAGE OUTPUT (OPTION 002)

s. Remove the 50-ohm feedthru termination between the 3325A output and the oscilloscope input. Press the key in the lower right corner of the 3325A front panel to select the High Voltage output.

t. Set the 3325A as follows:

FUNCTION.....Sine
 FREQUENCY.....2 kHz
 AMPLITUDE.....40 V p-p

u. Set the oscilloscope controls as follows:

Vertical.....10 V/div
 Horizontal.....0.5 ms/div

v. The oscilloscope display should show a sine wave four divisions peak-to-peak, one cycle per division. This checks the high voltage output amplifier.

3-78. OPERATOR'S MAINTENANCE.

3-79. Maintenance by the operator is limited to cleaning or replacing the rear panel fan filter, or replacing the ac line fuse on the rear panel. Generally, if the ac line fuse requires replacement there is a failure within the instrument, which should be referred to qualified service personnel. Disconnect the ac line cord before replacing the fuse. Be sure to use the correct replacement fuse:

Nominal Line Voltage	Fuse	-hp- Part No.
100/120 V	1 A	2110-0001
220/240 V	0.5 A	2110-0012

3-80. The fan filter should be inspected frequently and cleaned or replaced as necessary to allow free flow of air. To remove the filter, disconnect ac power from the instrument and remove the four nuts that secure the filter retainer. Remove the filter and wash thoroughly with soapy water, rinse clean, and air dry.

3-81. HP-IB OPERATION.

3-82. The Model 3325A is remotely controlled by means of the Hewlett-Packard Interface Bus (HP-IB).

The following information gives a general description of the HP-IB and defines the terms, concepts, and messages used in an HP-IB system. It also lists the capabilities and requirements for programming the 3325A. Program examples using a specific Hewlett-Packard calculator as the system controller may be found in the Supplemental Programming Information, Appendix 3-A at the rear of this section.

NOTE

HP-IB is Hewlett-Packard Company's implementation of IEEE Standard 488-1978, "Standard Digital Interface for Programmable Instrumentation."

3-83. General HP-IB Description.

3-84. The HP-IB is a parallel bus of 16 active signal lines grouped into three sets according to function, to interconnect up to 15 instruments. Figure 3-3 is a diagram of the interface connections and bus structure.

3-85. Eight signal lines form the first set and are termed "data" lines. The data lines carry coded messages which represent addresses, program data, measurements, and status bytes. The same data lines are used for input and

output messages in bit-parallel, byte-serial form. Normally, a seven-bit ASCII code represents each piece (byte) of data, leaving the eighth bit available for parity checking.

3-86. Data transfer is controlled by means of an interlocked "handshake" technique which permits data transfer (asynchronously) at the rate of the slowest device participating in that particular conversation. The three data byte transfer control lines which implement the handshake form the second set of lines.

3-87. The remaining five general interface management lines form the third set and are used in such ways as activating all the connected devices at once, clearing the interface, etc. Table 3-5 defines each of the management lines.

3-88. Definition of HP-IB Terms and Concepts.

Byte - A unit of information consisting of eight binary digits (bits).

Device - Any unit that is compatible with the IEEE Standard 488-1978.

Device Dependent - 1. An action a device performs in response to information sent on the HP-IB. The action is characteristic of an individual device and may vary from device to device. 2. The data required to communicate with a particular device.

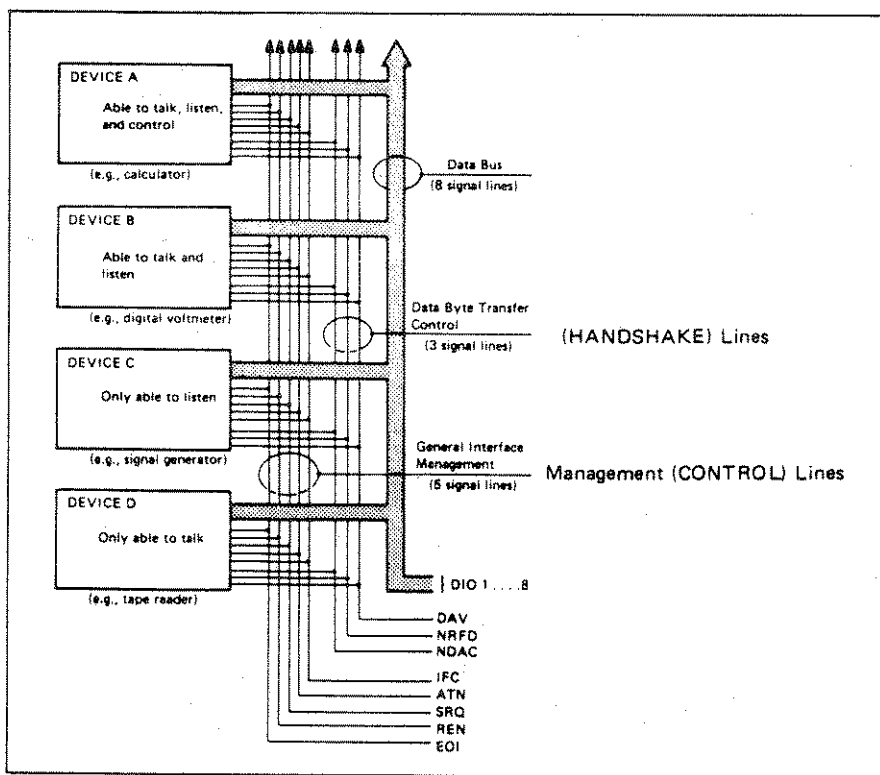


Figure 3-3. Interface Connections and Bus Structure.

Table 3-5. General Interface Management Lines.

Name	Mnemonic	Description
Attention	ATN	Enables a device to interpret data on the bus as a controller command (command mode) or data transfer (Data Mode).
Interface Clear	IFC	Initializes the HP-IB system to an idle state (no activity on the bus.)
Service Request	SRQ	Alerts the controller to a need for communication.
Remote Enable	REN	Places instruments under remote program control.
End Or Identify	EOI	Indicates last data transmission during a data transfer sequence; used with ATN to poll devices for their status.

Operator - The person that operates either the system or any device in the system.

Address - The characters sent by a controller to specify which device will send information on the bus and which device(s) will receive information. A device may also have its address fixed so that it may only receive information (listen only) or only send information (talk only).

Polling - Polling is a means by which a controller can identify a device that needs interaction with it. The controller may poll devices for their operational condition one at a time, which is termed a serial poll, or as groups of devices simultaneously, which is termed a parallel poll.

3-89. Basic Device Communication Capability.

3-90. Devices which communicate along the interface bus fall into three basic categories.

Talkers - Devices which send information on the bus when they have been addressed.

Listeners - Devices which receive information sent on the bus when they have been addressed.

Controllers - Devices that can specify the talker and listener(s) for an information transfer. The controller can be an active controller or a system controller. The active controller is defined as the current controlling device on the bus. The system controller can take control of the bus even if it is not the active controller. Each system can have only one system controller, even if several controllers have system control capability.

3-91. Message Definitions.

3-92. Information is transferred on the HP-IB from one device to one or more other devices in quantities

called "messages". Some of the messages consist of two basic parts, the address portion and the information portion. Others are general messages to all devices. Messages can be classified into twelve types, which are referred to as "meta messages". These are defined in Table 3-6. A block diagram presentation of meta messages and their implementation will be found in Appendix A-3 at the rear of this section.

NOTE

The meta message in itself is not a program code or an HP-IB command. It is only intended as a tool to translate a program written as an algorithm into the controller's code.

3-93. 3325A Response to Messages.

3-94. The 3325A is capable of implementing only those messages indicated in Table 3-7. In order for those messages to be implemented, certain bus actions are required, which are shown in the Interface Functions column.

3-95. HP-IB Work Sheet.

3-96. A work sheet is provided at the end of this section for listing the address and message capabilities of each instrument in your HP-IB system. When this sheet is filled out, it will provide a summary of the system capabilities.

3-97. HP-IB Addressing.

3-98. Certain messages require that a specific talker and listener be designated. Each instrument on the bus has its own distinctive listen and/or talk address which distinguishes it from other devices. The 3325A receives programming instructions when addressed to listen. When addressed to talk, it will respond to the instructions it received prior to being addressed to talk, such as an interrogation or serial poll.

3-99. Addressing usually takes the form of "universal unlisten, device talk, device(s) listen". The universal unlisten command removes all listeners from the bus, allowing only the listener(s) designated by the device(s) listen parameter to receive information. The information is sent by the talker designated by the device talk parameter. The system controller may designate itself as either talker or listener.

3-100. 3325A REMOTE PROGRAMMING.

3-101. 3325A HP-IB Capabilities.

3-102. Table 3-8 lists the HP-IB capabilities of the 3325A, which are compatible with IEEE Standard 488-1978.

Table 3-6. Definition of Meta Messages.

Message	Definition	Message	Definition
Data	The actual information (binary bytes) which is sent from a talker to one or more listeners. The information or data can be in a numeric form or a string of characters.	Status Byte	A byte that represents the status of a single device. One bit indicates whether the device sent the required service message and the remaining 7 bits indicate operational conditions defined by the device. This byte is sent from the talking device in response to a "Serial Poll" operation performed by a controller.
Trigger	The trigger message causes the listening device(s) to perform a device-dependent action.	Status Bit	A byte that represents the operational conditions of a group of devices on the bus. Each device responds on a particular bit of the byte thus identifying a device dependent condition. This bit is typically sent by devices in response to a parallel poll operation.
Clear	A clear message will cause a device(s) to return to a pre-defined device-dependent state.	Pass Control	The status bit message can also be used by a controller to specify the particular bit and logic level that a device will respond with when a parallel poll operation is performed. Thus, more than one device may respond on the same bit.
Remote	The remote message causes the listening device(s) to switch from local front panel control, to remote program control. This message remains in effect so that devices subsequently addressed to listen will go into remote operation.	Abort	This message transfers the bus management responsibilities from the active controller to another controller.
Local	This message clears the remote message from the listening device(s) and returns the device(s) to local front panel control.		The system controller sends the abort message to unconditionally assume control of the bus from the active controller. The message will terminate all bus communications but does not implement the clear message.
Local Lockout	The local lockout message is implemented to prevent the device operator from manually inhibiting remote program control.		
Clear Lockout and Set Local	This message causes all devices to be removed from the local lockout mode and revert to local. It will also clear the remote message for all devices.		
Require Service	A device can send this message at any time to signify that it needs some type of interaction with the controller. The message is cleared by the device's status byte message if it no longer requires service.		

3-103. Developing an HP-IB Program.

3-104. Basically, the 3325A is programmed remotely in the same manner as it is programmed manually. The sequence in which the various parameters are programmed is not important. At the end of this section (III) there is a summary of the HP-IB Programming Codes. This chart may be removed from the manual and/or copied to be used as a programming reference.

NOTE

It may be necessary to refer to some paragraphs on manual operation for descriptions of certain signals and requirements.

3-105. Several steps are needed to develop an HP-IB program.

a. Completely define the operation(s) the system is required to perform.

b. Write the program in flowchart or algorithm form. (An algorithm may be defined as a fixed step-by-step procedure for finding a solution to a problem.) Use the key words for meta messages shown in Table 3-6 in developing the program. The twelve key words are repeated here for reference.

- Data
- *Trigger
- Clear
- Remote
- Local
- Local Lockout
- Clear Lockout and Set Local
- Require Service

Table 3-7. 3325A Implementation of Messages.

Message	Implementation*	Interface Functions**		3325A Response
		Sender	Receiver	
Data	SR	T, SH	L ⁿ , AH	Will send or receive as instructed
Trigger	NA	T, SH	L ⁿ , AH	None
Clear-ID	R	C, SH	DC ⁿ , L, AH	Device Clear sets 3325A to initial turn-on conditions. See Para. 3-8.
Clear-All	R	C, SH	DC ^h , AH	
Remote	R	C _s , SH	RL ⁿ , L, AH RL, AH	Goes to Remote. Can be set to Local by LOCAL key.
Local	R	C _s , SH	RL ⁿ , L, AH	Goes to Local.
Local Lockout	R	C, SH	RL, AH	Goes to Remote. Cannot be set to Local by LOCAL key.
Clear Lockout and Set Local	R	C _s	RL	Goes to Local from Local Lockout.
Require Service	S	SR ⁿ	C	Sets SRQ True.
Status Byte	S	SR ⁿ , T, SH	L ⁿ , AH	Sends byte which indicates if service required and reason.
Status Bit	NA	pp ^h	C	None
Pass Control	NA	C _A , SH	C _B , T, AH	None
Abort	R	C _s		Unaddress

*S = Send Only
 R = Receive Only
 SR = Send and Receive
 NA = Not Applicable

**SH = Source Handshake
 AH = Acceptor Handshake
 T = Talker (includes TE = Extended Talker)
 L = Listener (includes LE = Extended Listener)
 SR = Service Request
 RL = Remote/Local
 PP = Parallel Poll
 DC = Device Clear
 DT = Device Trigger
 C = Any Controller
 C_N = A specific controller (for example, C_A, C_B)
 C_s = The System Controller
 X^h = Indicates message can be sent to/by one or more devices simultaneously

Status Byte
 *Status Bit
 *Pass Control
 Abort

*Not implemented by the 3325A

NOTE

The meta message in itself is not a program code or an HP-IB command. It is only intended as a tool to translate a program written as an algorithm into the controller's code.

Table 3-8. Interface Functions.

Code	Function
SH1	Source handshake capability
AH1	Acceptor handshake capability
T6	Basic talker; Serial Poll; Unaddressed to talk if addressed to listen
L3	Basic listener; Listen Only; Unaddressed to listen if addressed to talk
SR1	Service Request capability
RL1	Remote/Local capability
PP0	No parallel poll capability
DC1	Device clear capability
DT0	No device trigger capability
CD	No controller capability
E1	Open collector bus drivers

c. Define the operation in program codes that the instrument can use. Each instrument has its own set of program codes which are ASCII characters. The 3325A program codes are shown beginning with Paragraph 3-120 or Table 3-9.

d. Convert the program into the controller's language. The conversion information is supplied with each controller. For example, the -hp- 9825A Calculator Extended I/O Manual provides a chart for program code conversion.

NOTE

Examples for controlling the 3325A with a specific Hewlett-Packard calculator are provided in the Supplemental Programming Information, Appendix B-3 at the rear of this section.

3-106. Block diagrams and explanations of the meta messages that apply to the 3325A are shown in Appendix A-3 at the rear of this section.

3-107. Universal and Addressed Commands.

3-108. The 3325A will respond to the following universal and addressed commands, which are sent in the command mode (ATN true).

Mnemonic	Command	ASCII Code
Universal:		
*DCL	Device Clear	DC4
LLO	Local Lockout	DC1
MLA	My Listen Address	(selectable)
MTA	My Talk Address	(selectable)
SPD	Serial Poll Disable	EM
SPE	Serial Poll Enable	CAN
UNL	Unlisten	?
UNT	Untalk	-
Addressed:		
GTL	Go to Local	SOH
*SDC	Selected Device Clear	EOT

*DCL and SDC commands set the 3325A to its initial turn-on conditions (see Paragraph 3-8) and cause an AMPTD CAL operation. Any data in the HP-IB input buffer is lost. The storage registers, SRQ masking, and the status byte are not affected.

3-109. Placing the 3325A in Remote.

3-110. The 3325A will go to Remote when ATN is true, REN is true, and it receives its listen address.

3-111. The 3325A Address.

3-112. The 3325A address is normally set at the factory to:

	ASCII Character	5-Bit Octal	(5-Bit Octal Equivalent) Decimal	Hexadecimal
Listen	I	21	17	11
Talk	Q	21	17	11

The 3325A can be made to display its address in decimal code by pressing the blue prefix key and the BUS ADRS (LOCAL) key.

NOTES

1. All programming is shown in ASCII code.

2. Table 3-9 is a summary of the 3325A program data messages and program times. Table 3-10 lists program codes in binary, octal, decimal, and hexadecimal. At the end of this section (III) there is also a summary of the HP-IB programming codes. This chart may be removed from the manual and/or copied to be used as a programming reference.

3. The following front panel key actions cannot be remotely programmed:

- Modify group
- Sweep bandwidth × 2
- Sweep bandwidth ÷ 2
- Set sweep center frequency to marker frequency
- Display bus address
- Clear display

4. The 3325A must be set to REMOTE and addressed to LISTEN before it will accept device dependent data messages.

3-113. 3325A Data Message Formats.

3-114. The following are valid programming strings (data messages) for the 3325A:

- Mnemonic, Data, Delimiter, EOS
- Mnemonic, Data, EOS
- Mnemonic, EOS
- I, Mnemonic, EOS

Where I is the ASCII character I and EOS is the end-of-string character, which is required for Data Transfer Mode 2 (see following paragraphs). Valid EOS characters are:

- LF = Line Feed = 12 octal
- * = Asterisk = 52 octal

Table 3-9. Summary of 3325A Programming (ASCII Characters).**

Parameter or Operation	Mnemonics ASCII Code	Data	ASCII Code Delimiters	Approximate Programming Time*
Data Transfer Mode Data Mode 1 Data Mode 2	= MD = MD	1 2	NA	MD = 4.5 ms
Function	= FU	0 = DC Only 1 = Sine 2 = Square 3 = Triangle 4 = Positive Ramp 5 = Negative Ramp	NA	FU = 1500 ms
Frequency	= FR	≤ 11 Digits and Decimal	HZ = Hertz KH = Kilohertz MH = Megahertz	FR = 7.0 ms Each digit or decimal = 2.8 ms HZ, KH, or MH = 12.5 ms
Amplitude	= AM	≤ 4 Digits and Decimal. Also - sign if negative dBm. + sign is valid but not required.	VO = Volts (p-p) MV = Millivolts (p-p) VR = Volts rms MR = Millivolts rms DB = dBm	AM = 6.8 ms Each digit, decimal or decimal = 2.8 ms VO or MV = 90 ms VR or MR = 130 ms DB = 250 ms
DC Offset	= OF	≤ 4 Digits and Decimal. Also - sign if negative dc offset. + sign is valid but not required.	VO = Volts MV = Millivolts	OF = 6.8 ms Each digit, decimal, or - sign = 2.8 ms VO or MV = 82 ms
Phase	= PH	≤ 4 Digits - minus sign	DE = Degrees	PH = 5 ms; DE = 28 ms Each digit and - sign = 2.8 ms
Sweep Start Frequency Sweep Stop Frequency Sweep Marker Frequency	= ST = SP = MF	≤ 11 Digits and Decimal	HZ = Hertz KH = Kilohertz MH = Megahertz	ST, SP, or MF = 7.0 ms Each digit or decimal = 2.8 ms HZ, KH, or MH = 10.3 ms
Sweep Time	= TI	≤ 4 Digits and Decimal	SE = Seconds	TI = 5.5 ms; SE = 7.0 ms Each digit and decimal = 2.8 ms
Sweep Mode Linear Logarithmic	= SM	1 2	NA	SM = 4.5 ms
Rear or Front Panel Output Front Panel Rear Panel	= RF	1 2	NA	RF = 44.5 ms
Store Program Recall Program	= SR = RE	1 Digit, 0-9	NA	SR = 11 ms; RE = 1700 ms
Execution Functions Assign Zero Phase Perform Auto-Cal Start Single Sweep Start Continuous Sweep Perform Self-Test	= AP = AC = SS = SC = TE	NA NA	NA NA	AP = 5.2 ms AC = 1500 ms SS = 300 ms SC = 300 ms TE = 10,000 ms
Interrogate Program Error	= IER	NA	NA	IER = 11.5 ms
Interrogate Entry Parameters Frequency Amplitude Offset Phase Sweep Start Frequency Sweep Stop Frequency Sweep Marker Frequency Sweep Time	= IFR = IAM = IOF = IPH = IST = ISP = IMF = ITI	NA	NA	IFR = 10 ms IAM = 9.8 ms IOF = 9.8 ms IPH = 8 ms IST = 10 ms ISP = 10 ms IMF = 10 ms ITI = 8.5 ms
Interrogate Function	= IFU	NA	NA	IFU = 1603 ms
Mask Service Requests	= MS	See Para. 3-144	NA	MS = 4.5 ms
Binary (ON/OFF) Functions High Voltage Output Amplitude Modulation Phase Modulation	= HV = MA = MP	OFF = 0 ON = 1	NA	HV = 48 ms MA = 7.0 ms MP = 7.0 ms

*Program times are in addition to the data transfer time of 225 to 250 μs per byte.

**See Note 2 following Paragraph 3-112.

Table 3-10. Programming Codes.

Instruction	ASCII Characters	Binary Code	Octal Code	Decimal Code	Hexadecimal Code
Entry Frequency	F	1 0 0 0 1 1 1 0	106	70	46
	R	1 0 1 0 0 1 1 0	122	82	52
Amplitude	A	1 0 0 0 0 0 1	101	65	41
	M	1 0 0 1 1 0 1	115	77	4D
Offset	O	1 0 0 1 1 1 1 1	117	79	4F
	F	1 0 0 0 1 1 1 0	106	70	46
Phase	P	1 0 1 0 0 0 0	120	80	50
	H	1 0 0 1 0 0 0	110	72	48
Sweep Start Frequency	S	1 0 1 0 0 1 1	123	83	53
	T	1 0 1 0 1 0 0	124	84	54
Stop Frequency	S	1 0 1 0 0 1 1	123	83	53
	P	1 0 1 0 0 0 0	120	80	50
Marker Frequency	M	1 0 0 1 1 0 1	115	77	4D
	F	1 0 0 0 1 1 1 0	106	70	46
Time	T	1 0 1 0 1 0 0	124	84	54
	I	1 0 0 1 0 0 1	111	73	49
Start Continuous	S	1 0 1 0 0 1 1	123	83	53
	C	1 0 0 0 0 1 1	103	67	43
Start Single (must be sent twice)	S	1 0 1 0 0 1 1	123	83	53
	S	1 0 1 0 0 1 1	123	83	53
Sweep Mode	S	1 0 1 0 0 1 1	123	83	53
	M	1 0 0 1 1 0 1	115	77	4D
Numerical Data	0	0 1 1 1 0 0 0 0	060	48	30
	1	0 1 1 1 0 0 0 1	061	49	31
	2	0 1 1 1 0 0 1 0	062	50	32
	3	0 1 1 1 0 0 1 1	063	51	33
	4	0 1 1 1 0 1 0 0	064	52	34
	5	0 1 1 1 0 1 0 1	065	53	35
	6	0 1 1 1 0 1 1 0	066	54	36
	7	0 1 1 1 0 1 1 1	067	55	37
	8	0 1 1 1 1 0 0 0	070	56	38
	9	0 1 1 1 1 0 0 1	071	57	39
	.(decimal)	.	0 1 0 1 1 1 1 0	056	46
-(minus)	-	0 1 0 1 1 0 1	055	45	2D
Data Suffix (Delimiter) Hertz	H	1 0 0 1 0 0 0	110	72	48
	Z	1 0 1 1 0 1 0	132	90	5A
Kilohertz	K	1 0 0 1 0 1 1	113	75	4B
	H	1 0 0 1 0 0 0	110	72	48
Megahertz	M	1 0 0 1 1 0 1	115	77	4D
	H	1 0 0 1 0 0 0	110	72	4A
Volts (p-p or dc)	V	1 0 1 0 1 1 1 0	126	86	56
	O	1 0 0 1 1 1 1	117	79	4F
Millivolts (p-p or dc)	M	1 0 0 1 1 0 1	115	77	4D
	V	1 0 1 0 1 1 0	126	86	56
Volts rms	V	1 0 1 0 1 1 0	126	86	56
	R	1 0 1 0 0 1 0	122	82	52
Millivolts rms	M	1 0 0 1 1 0 1	115	77	4D
	R	1 0 1 0 0 1 0	122	82	52
dBm	D	1 0 0 0 1 0 0	104	68	44
	B	1 0 0 0 0 1 0	102	66	42
Degrees	D	1 0 0 0 1 0 0	104	68	44
	E	1 0 0 0 1 0 1	105	69	45
Seconds	S	1 0 1 0 0 1 1	123	83	53
	E	1 0 0 0 1 0 1	105	69	45
Store	S	1 0 1 0 0 1 1	123	83	53
	R	1 0 1 0 0 1 0	122	82	52
Recall	R	1 0 1 0 0 1 0	122	82	52
	E	1 0 0 0 1 0 1	105	69	45

Table 3-10. Programming Codes (Cont'd).

Instruction	ASCII Characters	Binary Code	Octal Code	Decimal Code	Hexadecimal Code
High Voltage Output	H	1 0 0 1 0 0 0	110	72	48
	V	1 0 1 0 1 1 0	126	86	56
Modulation-Amplitude	M	1 0 0 1 1 0 1	115	77	4D
	A	1 0 0 0 0 0 1	101	65	41
Modulation-Phase	M	1 0 0 1 1 0 1	115	77	4D
	P	1 0 1 0 0 0 0	120	80	50
Rear or Front Output	R	1 0 1 0 0 1 0	122	82	52
	F	1 0 0 0 1 1 0	106	70	46
Data Transfer Mode	M	1 0 0 1 1 0 1	115	77	4D
	D	1 0 0 0 1 0 0	104	68	44
Assign Zero Phase Reference	A	1 0 0 0 0 0 1	101	65	41
	P	1 0 1 0 0 0 0	120	80	50
Perform Auto Cal.	A	1 0 0 0 0 0 1	101	65	41
	C	1 0 0 0 0 1 1	103	67	43
Perform Self Test	T	1 0 1 0 1 0 0	124	84	54
	E	1 0 0 0 1 0 1	105	69	45
Mask SRQ	M	1 0 0 1 1 0 1	115	77	4D
	S	1 0 1 0 0 1 1	123	83	53
Interrogate (Parameter)	I	1 0 0 1 0 0 1	111	73	49
Interrogate Error	I	1 0 0 1 0 0 1	111	73	49
	E	1 0 0 0 1 0 1	105	69	45
	R	1 0 1 0 0 1 0	122	82	52
EOS (End of String) Line Feed Asterisk	LF	0 0 0 1 0 1 0	12	10	A
	*	0 1 0 1 0 1 0	52	42	2A

All spaces (40 octal), carriage returns (15 octal), commas (54 octal), and all lower case alphabets are ignored by the 3325A.

NOTE

A program string may program one parameter or all parameters. For example, the string "FU2FR10KHAM3V0" programs the following:

FU2 = Square wave function
FR10KH = 10 kHz
AM3V0 = 3 V p-p

The EOS character should follow the complete string, or a maximum of 48 characters (see Paragraphs 3-115 through 3-118).

3-115. Data Transfer Mode.

3-116. The 3325A accepts data from the HP-IB in either of two modes. If speed of communication is a critical factor on your HP-IB system, Mode 2 is preferable. The characteristics of the two modes are:

Data Mode 1. The 3325A turns on in Data Mode 1. In this mode, each device dependent character (byte) is processed when received.

Line feeds and Asterisks (EOS characters) are ignored. No other device dependent data communications are permitted on the bus until the entire 3325A program string has been accepted and all but the last character processed.

Data Mode 2. Device dependent characters are accepted and stored in an internal buffer and not processed until the EOS character is received or the buffer is filled (48 bytes). Consequently, other communications on the bus are permitted after the program string has been accepted (at the rate of approximately 150 to 200 microseconds per character). If the program string contains 48 characters or more, the 3325A will hold up the bus while it processes the 48 characters before accepting and storing the rest of the string. Because the instrument turns on in Data Mode 1, Mode 2 must be programmed remotely. It will then remain in Mode 2 until Mode 1 is programmed or until the POWER switch is set to STBY.

3-117. While the 3325A is processing data it will accept and respond to universal commands. For this reason, when operating in Mode 2, the controller can send a program string (48 characters or less) to the 3325A, and

while this data is being processed the controller can unaddress the 3325A to listen and then communicate with another device. However, if the string is more than 48 characters, the bus will be held up until the first 48 characters have been processed and the remaining characters accepted. In order for the bus to be used during 3325A processing time for communication between other devices, a program string greater than 48 characters should be divided and an EOS character sent after (or at a convenient place before) the 48th byte. The remaining program can then constitute a second string. While the 3325A is processing input information, a "Busy" flag is set in the status byte (see Paragraph 3-136). This flag can be used to determine when the 3325A has finished processing.

NOTE

The 3325A will handshake bus communications even though the POWER switch is set to STBY. This will not interfere with the operation of the bus unless it was set to STBY while addressed to talk. Before it is set to STBY, make sure it is not addressed to talk, or else disconnect the HP-IB cable from the 3325A. The addressed to talk condition can be cleared by an IFC command, even when the 3325A is in Standby.

3-118. Programming Data Transfer Mode.

3-119. Instructions for programming Data Transfer Mode are included in Paragraph 3-126.

3-120. Programming Entry Parameters.

3-121. The 3325A entry parameters are:

- Frequency
- Amplitude
- Offset
- Phase
- Sweep Start Frequency
- Sweep Stop Frequency
- Sweep Marker Frequency
- Sweep Time

The programming syntax for these parameters is:

Mnemonic, Data, Delimiter, EOS

NOTE

All program codes are shown in ASCII characters.

Valid mnemonics:

- FR = Frequency
- AM = Amplitude
- OF = Offset

- PH = Phase
- ST = Sweep Start Frequency
- SP = Sweep Stop Frequency
- MF = Sweep Marker Frequency
- TI = Sweep Time

Valid data:

0 thru 9 = ASCII numerics (if too many digits are sent, the extra digits will be ignored or rounded)

+ = ASCII plus sign (plus sign is accepted but not required)

- = ASCII minus sign (minus sign will be ignored if sent for parameters that cannot be negative)

. = ASCII decimal (floating decimal entries not valid)

Valid delimiters:

- HZ = Hertz
- KH = Kilohertz
- MH = Megahertz
- VO = Volts (peak-to-peak or dc)
- MV = Millivolts (peak-to-peak or dc)
- VR = Volts rms
- MR = Millivolts rms
- DB = dBm
- DE = Degrees
- SE = Seconds

NOTE

When operating in Data Mode 1, an EOS character is not required. When in Mode 2, the EOS character should not be sent until the end of the program string (or after 48 bytes; see Paragraph 3-117).

3-122. Programming Waveform Function.

3-123. The selectable functions are:

- DC only
- Sine wave
- Square wave
- Triangle wave
- Positive Slope Ramp
- Negative Slope Ramp

The programming syntax for selecting function is:

Mnemonic, Data, EOS

Valid mnemonic:

FU = Function

Valid data:

- 0 = Function off (dc only)
- 1 = Sine
- 2 = Square
- 3 = Triangle
- 4 = Positive Slope Ramp
- 5 = Negative Slope Ramp

3-124. Programming Binary (On or Off) Functions.

3-125. The programmable binary functions are:

- High Voltage Output (Option 002)
- Amplitude Modulation
- Phase Modulation

The programming syntax for binary functions is:

Mnemonic, Data, EOS

Valid mnemonics:

- HV = High Voltage Output (If the 3325A receives the HV mnemonic but does not have the high voltage option, SRQ (if enabled) and an error code will be generated. See Paragraph 3-134.)
- MA = Modulation - Amplitude
- MP = Modulation - Phase

Valid data:

- 0 = Off
- 1 = On

NOTE

The rear panel signal output is inactive (no internal signal connection) if the instrument has the High Voltage Output Option 002 installed. Instructions are given in the Operating and Service Manual, Section VIII, Service Group M, for activating the rear panel signal output in one of two ways: 1) Placing the standard/high voltage output on the rear panel only, disconnecting the front panel signal output, or 2) Disabling the high voltage output and enabling the standard front/rear output configuration.

3-126. Programming Selection Functions.**NOTE**

The selection functions are similar to binary functions, but instead of ON or OFF states, selection is made between two mutually exclusive operations.

3-127. The programmable selection functions are:

- Rear Output/Front Output
- Linear Sweep/Logarithmic Sweep
- Data Transfer Mode

The programming syntax for the selection functions is:

Mnemonic, Data, EOS

Valid mnemonics:

- RF = Rear or Front Output
- SM = Sweep Mode
- MD = Data Transfer Mode

Valid data for RF is:

- 1 = Select Rear Output
- 2 = Select Front Output (If the 3325A receives the RF mnemonic but does not have rear output capability (Option 002, for example) SRQ (if enabled) and an error code will be generated. See Paragraph 3-134.)

Valid data for SM is:

- 1 = Linear Sweep (The 3325A turns on in Linear Sweep function. This function need not be programmed except to change from Linear to Log Sweep or to return to Linear.)
- 2 = Logarithmic Sweep

Valid data for MD is:

- 1 = Data Mode 1 (The 3325A turns on in Data Mode 1. This function need not be programmed if it is desired to remain in Data Mode 1.)
- 2 = Data Mode 2

3-128. Programming Execution Functions.

3-129. The programmable execution functions are:

- Assign Zero Phase Reference
- Perform Amplitude Calibration
- Start Single Sweep
- Start Continuous Sweep
- Perform Self Test

The programming syntax for execution functions is:

Mnemonic, EOS

Valid mnemonics:

- AP = Assign Zero Phase Reference
- AC = Perform Amplitude Calibration
- SS = Start Single Sweep

SC = Start Continuous Sweep
TE = Perform Self Test

NOTES

1. The Start Single mnemonic must be sent twice (SSSS). The first SS sets the output (and display) to the start frequency, and the second SS starts the sweep.

2. While the 3325A is in Continuous Sweep mode, if it receives the mnemonics SC, SS, FR, PH, AC, AP, or TE, it will stop sweeping. It must receive SC again in order to resume continuous sweeping; or if a single sweep is to be programmed, SSSS is required.

3. The "Busy" flag (bit 7 in the status byte, see Paragraph 3-138) will be "1" for the duration of a Self Test operation. After Self Test, the 3325A returns to the previously programmed conditions, except that if a sweep was in progress the sweep will remain stopped.

3-130. Programming Amplitude Units Conversion.

3-131. The programming syntax for converting amplitude units (Vp-p, Vrms, dBm) is:

Mnemonic, Delimiter, EOS

Mnemonic = AM = Amplitude

Delimiter = The units to which you want to convert:

VO = Vp-p
MV = mVp-p
VR = Vrms
MR = mVrms
DB = dBm

Example: If amplitude was programmed in Vp-p, it may be converted to dBm by programming "AMDB". If amplitude was the last parameter programmed and is shown in the display, only the delimiter "DB" needs to be programmed.

3-132. Programming Storage Registers.

3-133. The data that will be stored includes the current program of Entry Parameters, Function (Waveform), Binary Functions, and Selection Functions. The storage register functions are:

Store Data in Register N
Recall Data from Register N

The programming syntax for storage register functions is:

Mnemonic, Data, EOS

Valid mnemonics:

SR = Store
RE = Recall

Valid data:

0 thru 9 = ASCII numerics specifying register number

NOTES

1. If no data has been stored in a register, the recall command for that register will be ignored.

2. An amplitude calibration is performed when a register is recalled.

3. The numeric value for the phase is stored, but the phase of the output is not changed when the register is recalled. (Phase may need to be reprogrammed.)

4. DCL (Device Clear) and SDC (Selected Device Clear) commands do not affect the storage registers.

3-134. Service Requests.

3-135. The 3325A will set the SRQ line true for any of the following reasons, if enabled by the SRQ mask (see Paragraph 3-144):

Program String Error
Sweep Started or Sweep Stopped
System Failure (Possible component problem)
Failed Self Test
Failed Amplitude Calibration
External Reference Unlocked
Main Oscillator Unlocked

3-136. Serial Poll.

3-137. When the system controller determines that the SRQ line is true, it may conduct either a Serial Poll or a Parallel Poll to determine which device(s) initiated the Service Request, and the reason(s) for the request. The 3325A responds to a Serial Poll, which is conducted in the following manner:

Controller places ATN true (command mode)
Controller sends Serial Poll Enable (SPE) on lines DIO1-8 (ASCII CAN, binary code ×0011000)

Controller sends 3325A Talk address, controller Listen address
 Controller places ATN false (data mode)
 3325A responds by sending status byte on DIO1-8
 Controller places ATN true (after each device has been polled)
 Controller sends Serial Poll Disable (SPD) on DIO1-8 (ASCII EM, binary code ×0011001)


Serial Poll Disable clears the SRQ message originated by the 3325A, resetting bits 0 through 3 and bit 6 in the status byte.

NOTE

Some of the above Serial Poll operations are performed automatically by some controllers in response to certain programming statements. Refer to the programming instructions for your particular controller.

3-138. Status Byte.

3-139. A status byte consists of one 8-bit byte on the HP-IB data lines. A "1" in bit 6 indicates that the 3325A did request service (placed SRQ true), and a "0" in bit 6 indicates that it did not request service. The 3325A status byte contains the following information:

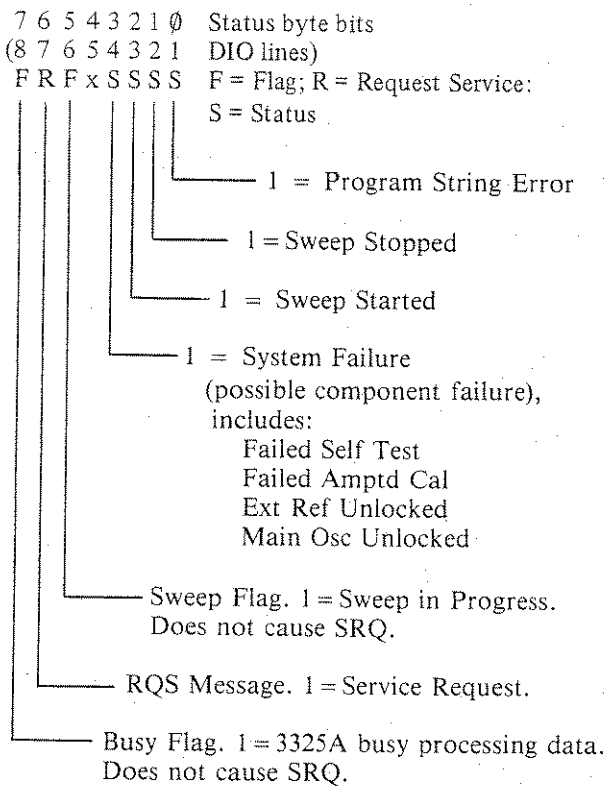

3-140. Busy Flag.

3-141. The Busy Flag (status byte bit 7) is high (1) while the 3325A is processing data. This bit can be monitored

by the controller to determine when the 3325A is ready for more data.

3-142. Sweep Flag.

3-143. The Sweep Flag (bit 5 of the status byte) is high (1) while the 3325A is in the process of sweeping. This bit can be monitored by the controller to determine when the end of a sweep occurs.

3-144. Masking or Enabling Service Requests.

3-145. Bits 3 through 0 in the status byte can be masked so that the corresponding conditions will not cause a service request. However, a "1" will still appear in the status byte if the condition exists, and can be cleared only by a serial poll. At instrument turn-on all SRQ conditions are masked. The programming syntax for masking and enabling SRQ conditions is:

Mnemonic, Data, EOS

Mnemonic = MS

Valid Data is shown in Table 3-11.

3-146. Interrogating Program Errors.

3-147. The "Program Error" service request may result from the following Errors:

ASCII Numeric	Error
1	Entry parameter out of bounds (for example, Freq ≥ 61 MHz)
2	Invalid delimiter
3	Frequency too large for function (for example, Function = Triangle, Freq ≥ 11 kHz)
4	Sweep time too small or too large
5	Offset incompatible with amplitude, or amplitude incompatible with offset
6	Sweep frequency too large for function; Sweep bandwidth too small; Start frequency too small (log sweep); Start frequency greater than stop frequency (log sweep)
7	Unrecognizable mnemonic received
8	Unrecognizable data character received
9	Option does not exist (High Voltage or Rear/Front)

Table 3-11. SRQ Mask/Enable Data.

ASCII Character	Bits 3 thru 0	System Fail Bit 3	Sweep Start Bit 2	Sweep Stop Bit 1	Program Error Bit 0
@	*0000	Mask	Mask	Mask	Mask
A	0001	Mask	Mask	Mask	Enable
B	0010	Mask	Mask	Enable	Mask
C	0011	Mask	Mask	Enable	Enable
D	0100	Mask	Enable	Mask	Mask
E	0101	Mask	Enable	Mask	Enable
F	0110	Mask	Enable	Enable	Mask
G	0111	Mask	Enable	Enable	Enable
H	1000	Enable	Mask	Mask	Mask
I	1001	Enable	Mask	Mask	Enable
J	1010	Enable	Mask	Enable	Mask
K	1011	Enable	Mask	Enable	Enable
L	1100	Enable	Enable	Mask	Mask
M	1101	Enable	Enable	Mask	Enable
N	1110	Enable	Enable	Enable	Mask
O	1111	Enable	Enable	Enable	Enable

*Initial turn-on conditions

The programming syntax for interrogating error is:

Mnemonic, EOS

Mnemonic = IER

After receiving IER, the 3325A will send back the following the next time it is addressed to talk:

Mnemonic, Data, CR (ASCII carriage return), LF & EOI (ASCII line feed with EOI sent simultaneously)

Mnemonic = ER

Data = The ASCII numeric corresponding to the first error that occurred (see list above).

If no error occurred, the code returned is 0. When more than one error has occurred, only the code for the first error will be returned. After interrogation, the error code is set to zero until the next error occurs.

3-148. Interrogating Entry Parameters.

3-149. Each entry parameter can be interrogated by the controller to determine its value. The programming syntax for interrogating entry parameters is:

I, Mnemonic, EOI

I = the ASCII character I and indicates interrogation desired.

Valid mnemonics (parameter to be interrogated):

- FR = Frequency
- AM = Amplitude
- OF = Offset

PH = Phase

ST = Sweep Start Frequency

SP = Sweep Stop Frequency

MF = Sweep Marker Frequency

TI = Sweep Time

After receiving a parameter interrogation, the 3325A will send back the following the next time it is addressed to talk:

Mnemonic, Data, Delimiter, CR (ASCII Carriage Return), LF & EOI (ASCII Line Feed with EOI sent simultaneously)

Mnemonic = The mnemonic of the parameter being interrogated

Data = 11 digits of ASCII numerics equal to the value of the specified parameter plus decimal point. If the value is negative, the first digit is a minus sign.

Delimiter = The data suffix mnemonic denoting the parameter value (see Paragraph 3-120)

NOTE

Only one parameter can be interrogated by each interrogation message.

3-150. Interrogating Function (Waveform).

3-151. The 3325A may be interrogated by the controller to determine the current function programmed. The programming syntax for interrogating function is:

I, Mnemonic, EOS

I = The ASCII character I and indicates interrogation desired

Mnemonic = FU = Function

After receiving IFU, the 3325A will send back the following the next time it is addressed to talk:

Mnemonic, Data, CR (ASCII Carriage Return), LF & EOI (ASCII Line Feed with EOI sent simultaneously)

Mnemonic = FU

Data = One ASCII numeric indicating function as follows:

- 0 = DC Only (Offset)
- 1 = Sine
- 2 = Square
- 3 = Triangle
- 4 = Positive Slope Ramp
- 5 = Negative Slope Ramp

3-152. Interrogating Miscellaneous Parameters.

3-153. The other parameters shown below can be interrogated by the controller to determine their present state. The programming syntax is:

I, Mnemonic, EOS

I = The ASCII character I and indicates interrogation desired

Valid Mnemonics (parameter to be interrogated):

- SM = Sweep Mode
- RF = Rear or Front Output*
- HV = High Voltage Output*
- MA = Amplitude Modulation
- MP = Phase Modulation

*Rear/Front output and High Voltage Output (Option 002) are mutually exclusive. If either RF or HV is interrogated, the mnemonic and data returned will indicate the actual capability of the instrument and its state. For example, if the High Voltage option is present and OFF, HV0 will be returned in response to either IRF or IHV.

After receiving an interrogation, the 3325A will send back the following the next time it is addressed to talk:

Mnemonic, Data, CR (ASCII Carriage Return), LF & EOI (ASCII Line Feed with EOI sent simultaneously)

Mnemonic = The mnemonic of the parameter being interrogated

Data = 1 ASCII digit specifying the state of the parameter. This is the same digit that would be used to program the parameter to that state.

3-154. Using the Interrogate Capability.

3-155. When the 3325A is changed from local to remote operation or vice versa, it retains its currently programmed state until this program is changed by the operator or controller. This feature can be useful in setting up a program string for HP-IB programming. For example, using the 3325A in local, the operator can determine experimentally the parameters required to perform the operation or test desired. Then the 3325A can be placed in remote and its function and entry parameters interrogated. Each item can be stored by the controller and then combined to form the 3325A program string to be incorporated into the total HP-IB program.


3-156. 3325A Programming Procedure.

3-157. The following examples are given to illustrate the basic procedure for developing a program. Program examples are shown in Appendix B-3, using the -hp-Model 9825A Calculator as the system controller. Appendix A-3 diagrams the required messages.

Example 1:

Address controller to talk,
3325A to listen

Send Program Data

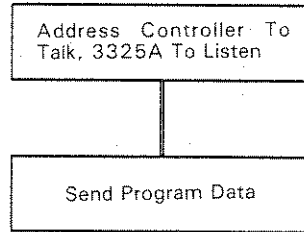

Example 2:


Address controller to talk,
3325A to listen

Send Program Data

Check for Require Service message


If yes, determine reason from 3325A Status Byte

Take corrective action if necessary

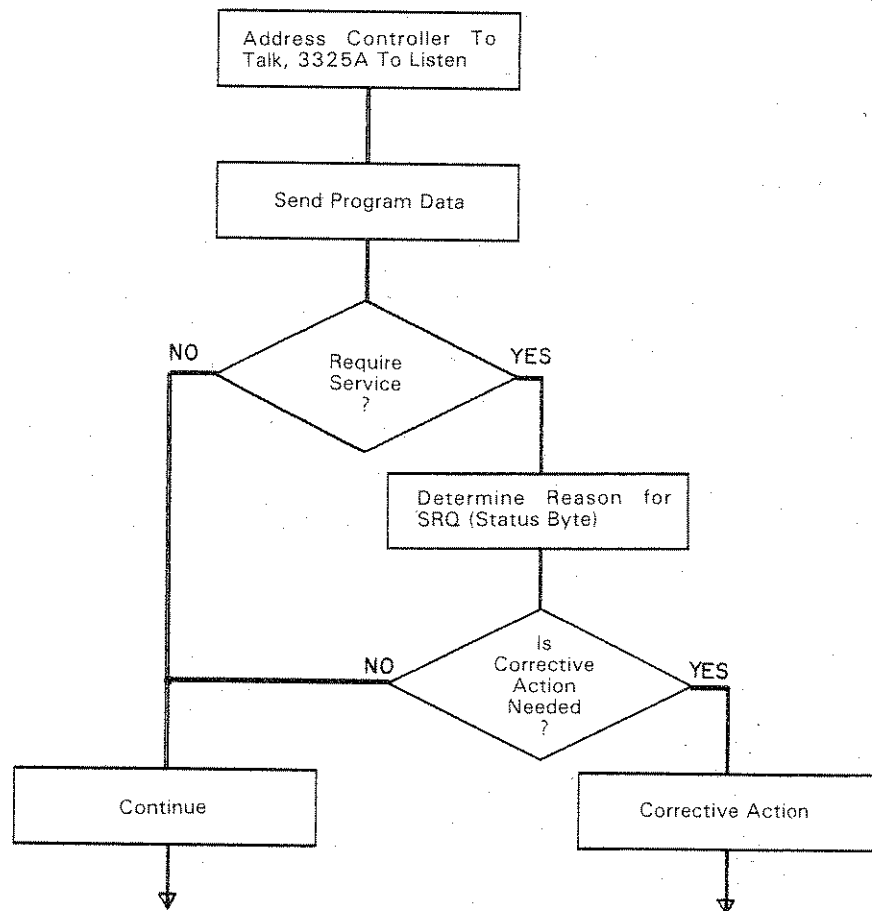


APPENDIX A SECTION III META MESSAGES BLOCK DIAGRAMMED

DATA MESSAGE — The Data message is the actual information that is sent from a talker to one or more listeners. This action requires the controller to first enter the command mode to set up the talker and listener(s) for the transfer of data. The information is then transferred in the data mode.

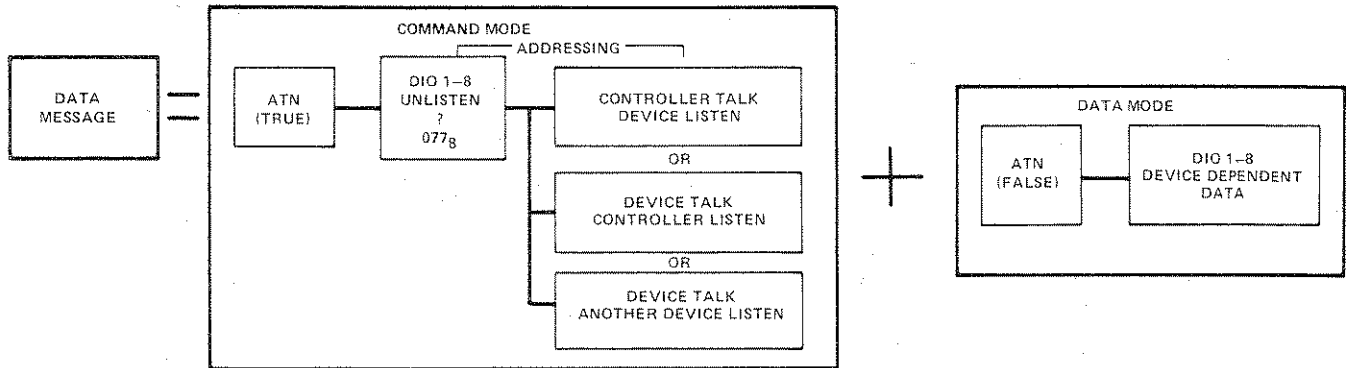


TRIGGER — The Trigger message causes all addressed instruments with this capability to execute some predefined function simultaneously.


The 3325A does not have Trigger capability.

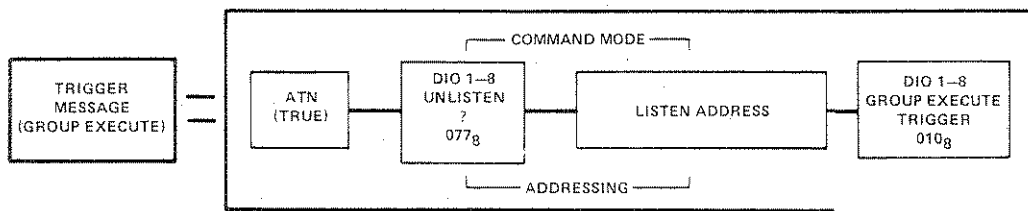


REN MUST BE TRUE BEFORE EXECUTING THE TRIGGER MESSAGE.

CLEAR — The Clear message may be implemented for addressed devices or for all devices on the bus capable of responding. In both cases the controller places the bus in the command mode to execute the message.

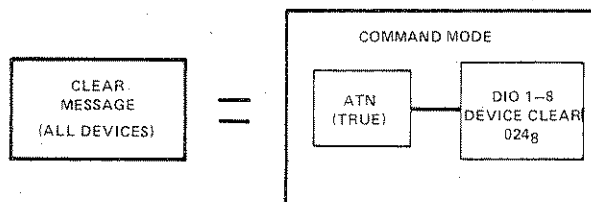


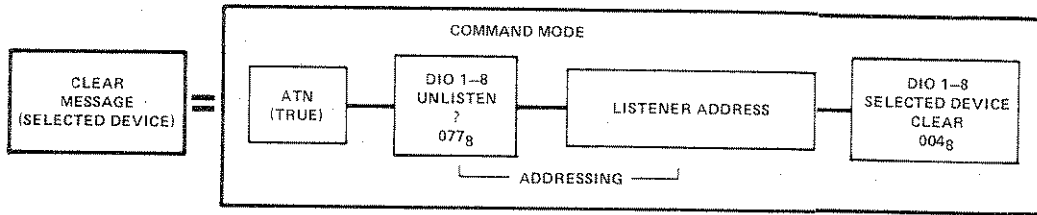


REMOTE — Only the system controller can place the device into the Remote operating condition. To implement the Remote message, the controller must set the REN line true. The HP-IB is then in the Remote Enable mode. The controller then sends the listen addresses of those devices that are to be placed in the Remote operating condition. Some instruments have been designed to enter the Remote mode as soon as REN is true.

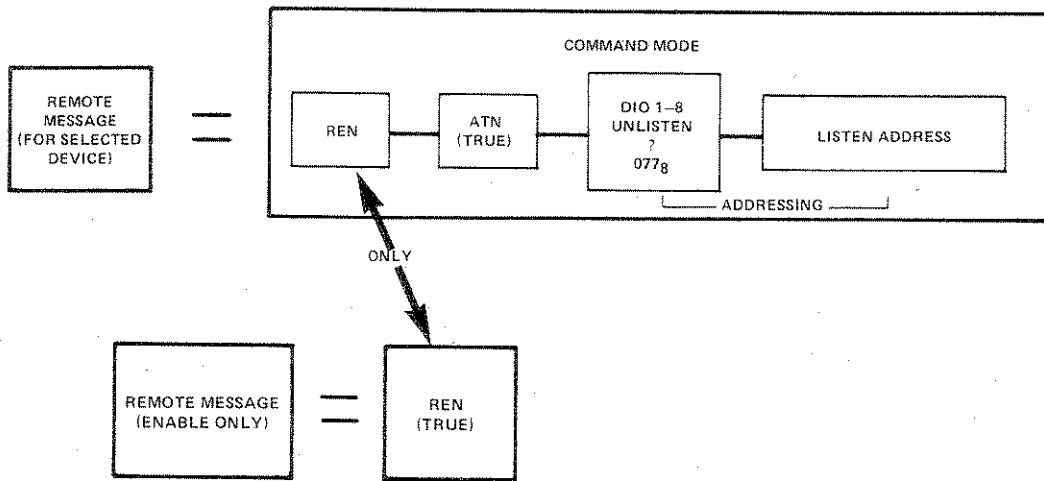

LOCAL — The Local message will remove addressed devices from the Remote operating mode to local (front panel) control. The controller must place the HP-IB into the command mode and address to listen all devices that are to be returned to local. The Local message does not remove the HP-IB from the Remote mode, only the listening devices.

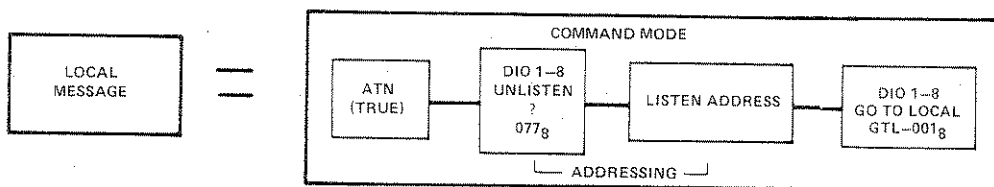


LOCAL LOCKOUT — The Local Lockout message prevents the operator from placing the instrument into local control from the front panel. The controller must be in the command mode to send the Local Lockout message.

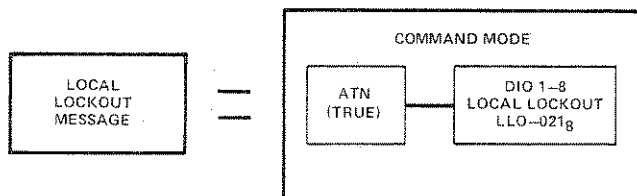


REN MUST BE TRUE BEFORE EXECUTING THE LOCAL LOCKOUT MESSAGE.

CLEAR LOCKOUT AND SET LOCAL — This message removes all devices from the Local Lockout mode and causes them to revert to local control. Because the REN line is set false, the HP-IB is in the local mode.

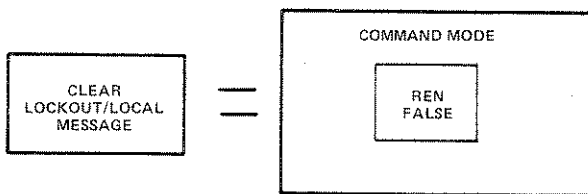


REQUIRE SERVICE — The Require Service message is implemented by a device setting the SRQ line true. The Require Service message and, therefore, the SRQ line is held true until a poll is conducted by the controller to determine the cause of the request for service, or until the device no longer needs service.



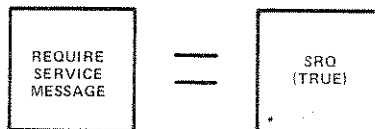


*REFER TO THE STATUS BYTE MESSAGE FOR THE SPECIFICATIONS REQUIRED TO FORCE SRQ FALSE.


STATUS BYTE — The Status Byte message represents the operational status of a single instrument during a Serial Poll. A controller usually Serial Polls devices in response to a Require Service message. The controller requests device status from one device at a time. The status information byte (8 bits) sent by the device will tell whether that device needed service and why. A device will stop requesting service upon being Serial Polled, or if it no longer needs service. The controller initiates the message by placing the bus into the command mode, sending the Serial Poll Enable command, and addressing the specific devices to be polled, one at a time. The device then sends its Status Byte and clears the SRQ line provided the cause for the require Service message is no longer present. The controller then places the bus in the command mode to terminate the message with a Serial Poll Disable command.

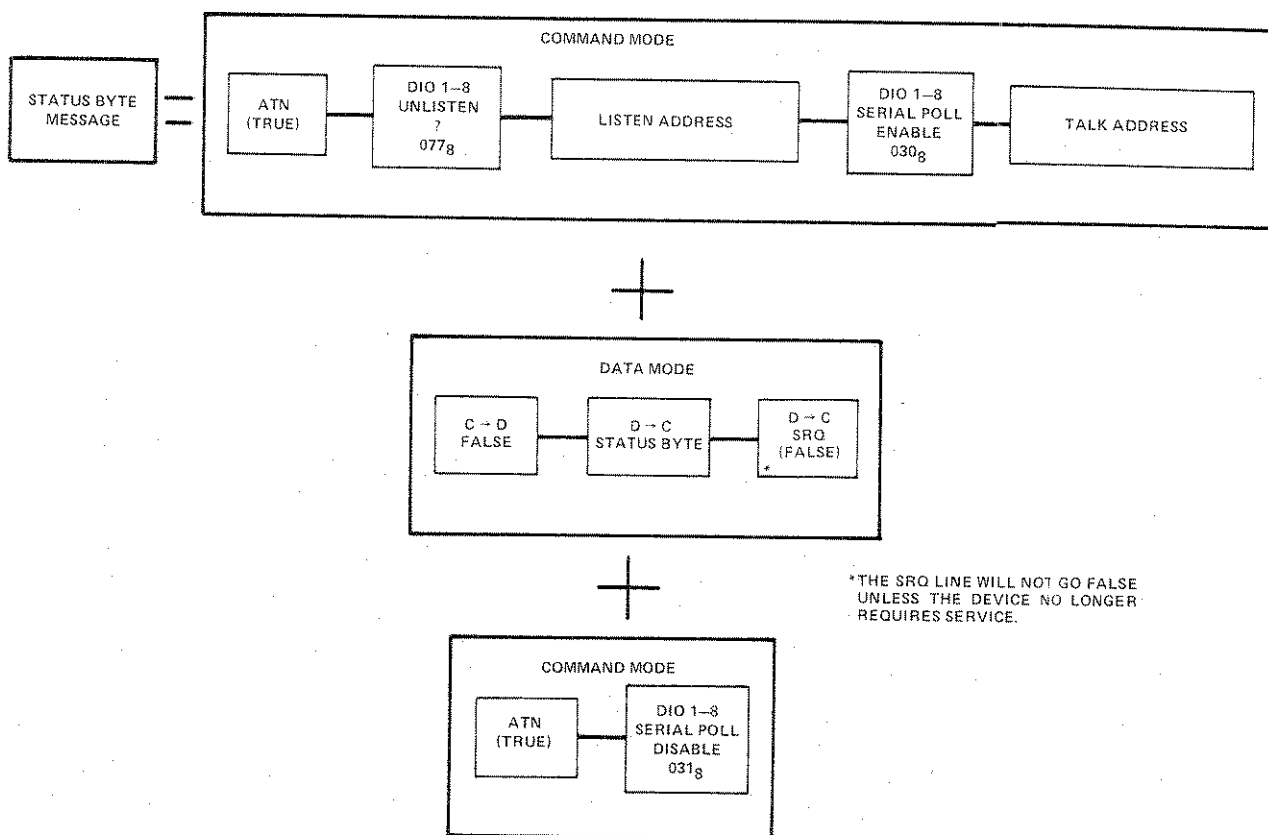

STATUS BIT — The Status Bit message is sent by a device to the controller to indicate its operational status in response to a Parallel Poll. Parallel Polling consists of the controller requesting one bit of status from each device simultaneously. The Parallel Poll may consist of three types of operations: Configuring, Polling, and Unconfiguring. In Configuring, the controller assigns each device a logic level and bit (on the bus data lines) for a poll response. During polling, each device responds on its assigned data line with the appropriate logic level. In Unconfiguring, the controller negates the bit and level assignments for all or selected devices. Several devices may be assigned to the same bit and level, causing their response bits to be logically ORed or ANDED.

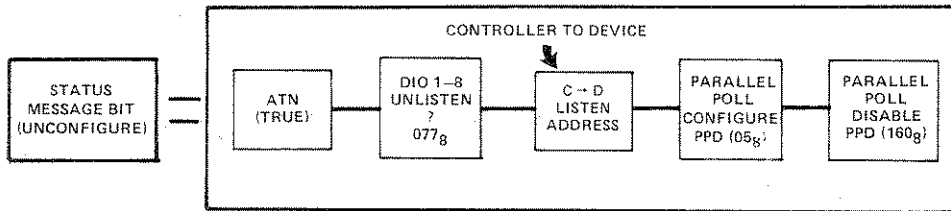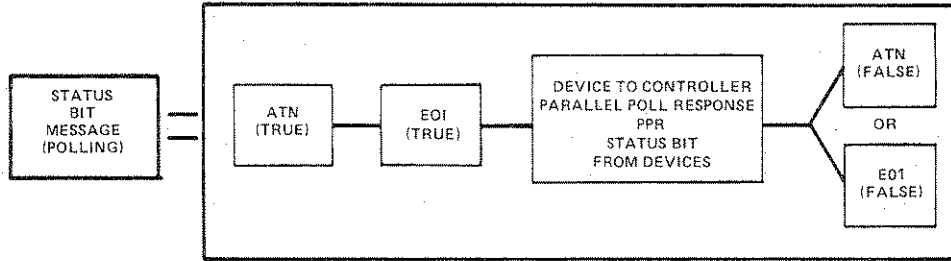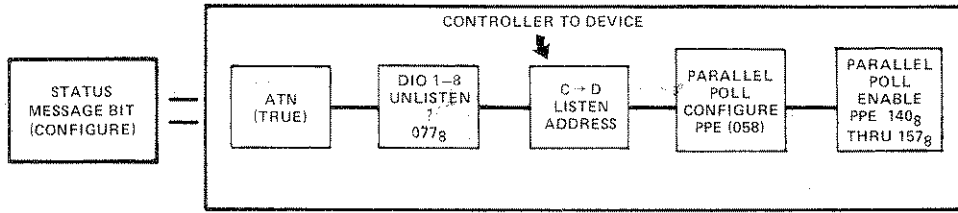


OR

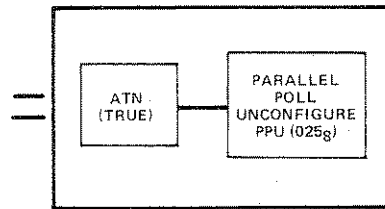

PPE ASSIGNS THE LOGIC LEVEL AND DATA LINE OF A DEVICE(S) RESPONSE. 140₈ THRU 147₈ ASSIGN THE LOW (TRUE) LEVEL AND 150₈ THRU 1507₈ ASSIGNS THE HIGH (FALSE) LEVEL. 140₈ AND 150₈ ASSIGNS BIT 2° (DATA LINE 1), 141₈ AND 157₈ WHICH ASSIGN BIT 2⁷ AND IS THE LAST POSSIBLE ASSIGNMENT.

The 3325A does not respond to Parallel Poll.


PASS CONTROL — The Pass Control message transfers bus management responsibilities from the active controller to another controller. In order to pass control, the active controller must enter the command mode, send the talk address, and the HP-IB characters for talk control.

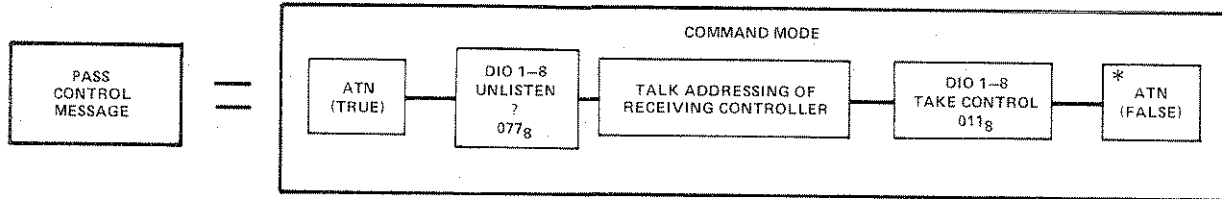

*THE RECEIVING CONTROLLER TAKES CONTROL AT THIS TIME.

The 3325A does not respond to the Pass Control message.

ABORT —The system Controller implements the Abort Message to regain control of the HP-IB from the active controller.

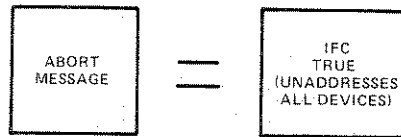


**APPENDIX B
SECTION III
PROGRAMMING THE MODEL 3325A
with the
MODEL 9825A CALCULATOR**

The following basic examples are provided to assist the operator in developing programs for the Model 3325A in an HP-IB system which uses the -hp- Model 9825A Calculator as the system controller. The calculator must be equipped with a General I/O ROM and an HP-IB Interface set to select code 7. The calculator (controller) normally holds the REN line true, unless the "lcl 7" (local) command is sent. REN may be returned to the true state by the "rem 7" (remote) command.

Example 1: This is a basic program statement which accomplishes the following:

- Address the controller to talk
- Address the 3325A to listen
- Sent Program Data:
 - Function: Sine
 - Frequency: 5 kHz
 - Amplitude: 3 Vp-p
 - Offset: +1.5 V

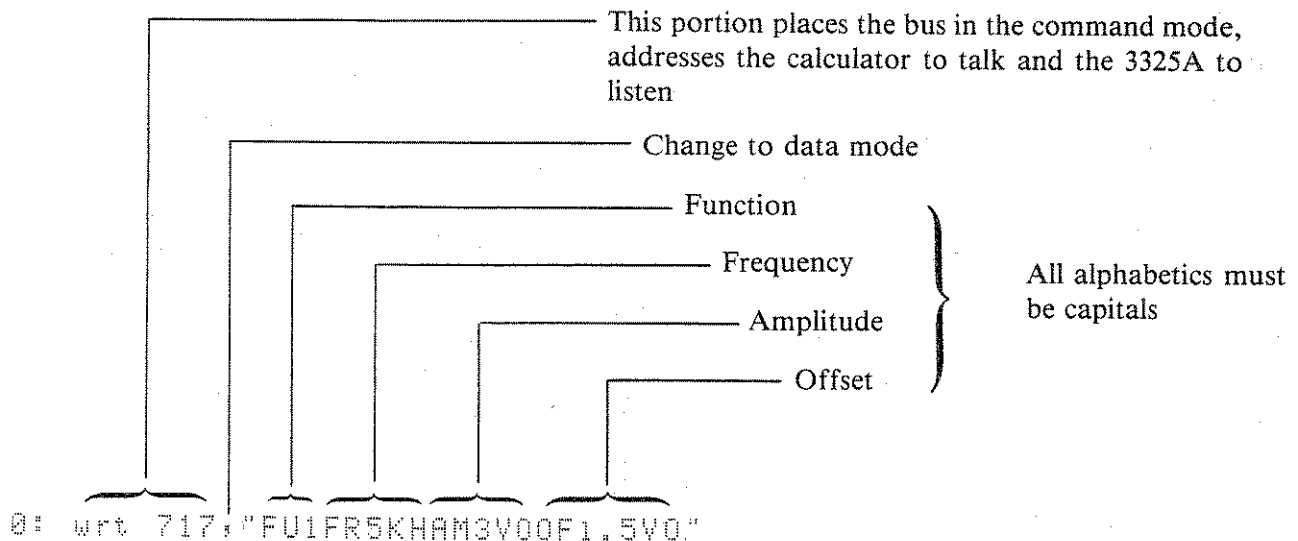


The last parameter programmed can be changed without sending the parameter mnemonic. For example, following the program string above, the offset (OF) may be changed to 1 V by sending "1V0".

Example: 2: This program sets up sweep parameters and initiates a single sweep.

Address the controller to talk
 Address the 3325A to listen
 Send Program Data:
 Function: Sine
 Amplitude: 3 Vrms
 Start Frequency: 1 kHz
 Stop Frequency: 10 kHz
 Marker Frequency: 5 kHz
 Sweep Time: 2 seconds
 Start Single Sweep

NOTE

To start a single sweep the mnemonic "SS" must be sent twice. The first "SS" sets the 3325A to the Start frequency, and the second "SS" starts the sweep.

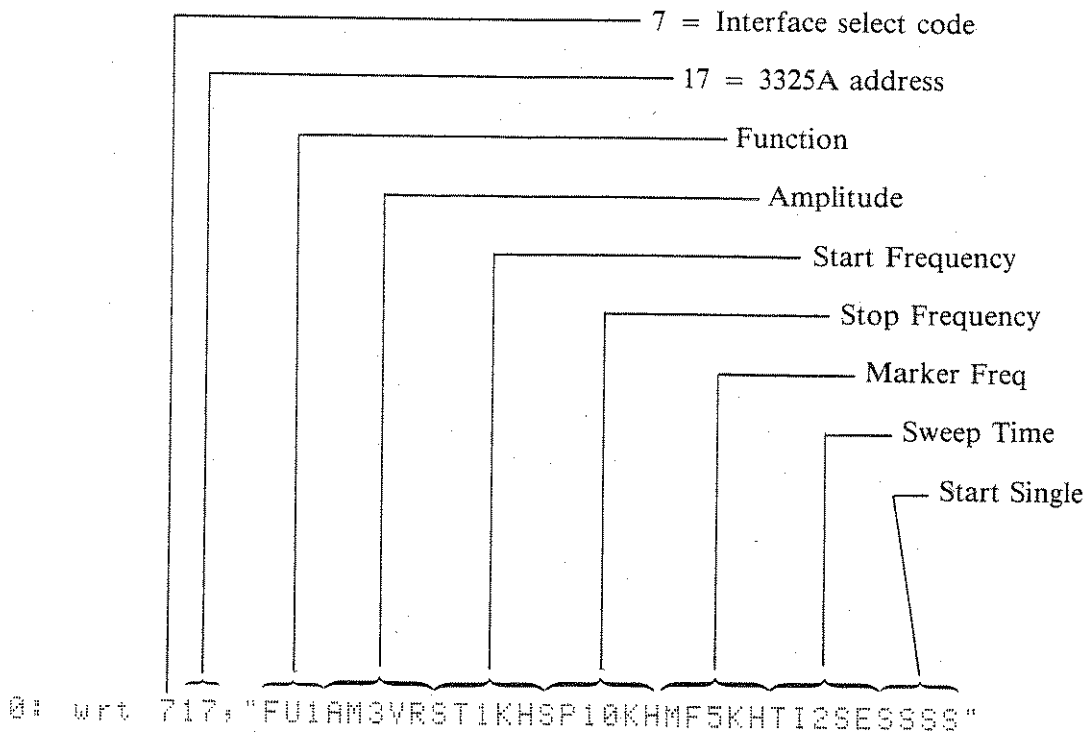

Example 3: This example checks the "Require Service" status of the 3325A and if it did request service, determines the reason.

```

    ①
0: wrt 717,"MSDF
  U3AM3VOST1KHSP1 ②
  5KHM5KHTI58ESC
1: wait 1000 ③
2: rds(717)+6 ④
3: if bit(6,6)=1 ⑤
  :prt "Request
  Service";esb 5
4: dep "PROCEED
  WITH PROGRAM"; ⑥
  stop
5: if bit(0,6)=1 ⑦
  :prt "Program
  Error";wrt 717,
  "IER";red 717,E
6: if E=1;prt
  "Parameter out
  of Bounds"
7: if E=2;prt
  "Invalid Delimi
  ter"
8: if E=3;prt
  "Frea too large
  for Function"
9: if E=4;prt
  "Sweep Time
  Invalid"
10: if E=5;prt
  "Offset & Amptd
  Incompatible"
11: if E=6;prt ⑧
  "Sweep Paramete
  r Error"
12: if E=7;prt
  "Unrecognizable
  Mnemonic"
13: if E=8;prt
  "Unrecognizable
  Data Char"
14: if E=9;prt
  "Option Does
  Not Exist"
  
```

1. Enables all service request conditions.

2. Program data contains an error. Stop frequency (SP15KH) is too large for triangle function (FU3).

3. Wait statement allows time for sweep to start before reading status.

4. Read status byte from the 3325A and place in the calculator variable "S".

5 If bit 6 of the status byte = 1, the 3325A did request service. Go to subroutine to determine the reason.

6. Programming continues at this point if the 3325A did not request service or upon returning from the subroutine.

7. If service request resulted from a program string error, interrogate the 3325A to determine the error code and place in the calculator variable "E".

8. Determine the nature of the program error.

```

15: if bit(1,
    3)=1:prt "Sweep
    Stopped"
16: if bit(2,
    3)=1:prt "Sweep
    Started"
17: if bit(3,
    3)=1:prt "System
    Failure"
18: if bit(5,
    3)=1:prt "Sweep
    In Progress"
19: if bit(7,
    3)=1:prt "Busy"
20: ret

```

9. Determine other reason for service request and if "Sweeping" or "Busy" flags were true.

10. Return from subroutine.

11. Printer records the results of the serial poll.

12. If the program string were corrected to make all data valid, this printout would result from the above program.

```

Request Service
Program Error
Sweep Parameter
Error

```

```

Request Service
Sweep Started
Sweeping

```

Example 4: The 3325A can be set up manually to the optimum parameters needed for the test to be performed, then the calculator can interrogate the 3325A to determine and record these parameters. This example program interrogates:

Function: IFU
 Frequency: IFR
 Amplitude: IAM
 DC Offset: IOF

```

0: wrt 717,"IFU"
  :red 717,W:fxd
  :6
1: prt "Function
  =":W

```

Line 0 Write statement interrogates Function; read statement addresses 3325A to talk, calculator to listen, and places data in variable W; "fxd 6" fixes six decimal places.

Line 1 Because only numerical data can be placed in the variables, print statements may include in quotes the parameter interrogated.

```

2: wrt 717,"IFR"
 ired 717;F
3: prt "Freuenc
y =" ;F;"Hz"
4: wrt 717,"IAM"
 ired 717;A
5: prt "Amplitud
e =" ;A
6: wrt 717,"IOF"
 ired 717;O
7: prt "Offset
 =" ;O;"V"
    
```

Lines 2 - 7 Other parameters are interrogated. Amplitude data acquired by this program does not indicate the units programmed. Frequency is always returned in Hz and DC Offset in Volts.

```

Function =
      1.000000
Frequency =
      1000.000000
Hz
Amplitude =
      22.310000
Offset =
      0.001000
V
    
```

— This printout results from the above program.

If the calculator is equipped with a String Variable ROM, the interrogate program may be changed to the following. Because string variables accept both alpha and numeric characters, the resulting printout includes the mnemonics and delimiters (units).

```

0: dim W#[50],
  F#[50],A#[50],
  O#[50]
1: wrt 717,"IFU"
 ired 717;W#;
  prt W#
2: wrt 717,"IFR"
 ired 717;F#;
  prt F#
3: wrt 717,"IAM"
 ired 717;A#;
  prt A#
4: wrt 717,"IOF"
 ired 717;O#;
  prt O#
    
```

1. Dimension a string variable for each parameter you want to interrogate. The dimension number (in brackets) is the number of spaces assigned to the variable.
2. This printout results when string variables are used.

```

FU1
FR000001000.000HZ
AM000000022.310DE
OF000000.001000VO
    
```

Example 5: The 3325A can be made to sweep amplitude (in steps) if a for/next statement is used in the calculator program. It is recommended that the upper and lower amplitude limits selected be on the same range because irregularities in the sweep will occur if the attenuator relays are switched.

```

0: wrt 717,"FU1F
  R1KHOF0VOAM3VO"
1: for I=3 to
  10 by .1:wrt
  717,I,"VO"
2: next I
3: for I=10 to
  3 by -.1:wrt
  717,I,"VO"
4: next I
5: goto 1

```

Line 0 DC Offset (OF0VO) is programmed to zero because any offset would be incompatible with the 10 V maximum amplitude of this sweep.

Line 1 The sweep limits (3 to 10) are on the same range. The sweep increment is in .1 V steps. Because amplitude was the last parameter programmed, the write statement does not require the "AM" mnemonic.

Line 2 The calculator returns to Line 1 until I = 10, then proceeds to Line 3.

Line 3 The sweep decrement is also in .1 V steps.

Line 5 Return to Line 1 to continue sweeping.

The sweep speed is determined by calculator and 3325A data transfer and processing times. If a slower sweep time is desired, wait statements may be added before the "next I" statements.

**MODEL 3325A
SYNTHESIZER/FUNCTION GENERATOR
HP-IB PROGRAMMING CODE
(ASCII Characters)**

<u>F</u> unction			<u>H</u> igh <u>V</u> oltage Output
DC only	0		On 1
Sine	1		Off 0
Square	2		
Triangle	3		Amplitude Modulation - <u>MA</u>
Positive Ramp	4		On 1
Negative Ramp	5		Off 0
<u>F</u> requency			Phase Modulation - <u>MP</u>
Hz	HZ		On 1
kHz	KH		Off 0
MHz	MH		
<u>A</u> mplitude			Data
Volts p-p	VO		0 0
mVp-p	MV		1 1
Vrms	VR		2 2
mVrms	MR		3 3
dBm	DB		4 4
			5 5
DC <u>O</u> ffset			6 6
Volts	VO		7 7
mV	MV		8 8
			9 9
<u>P</u> Hase			-(Decimal)
Degrees	DE		
Sweep <u>S</u> Tart Frequency			Interrogate Operations
Sweep <u>S</u> to <u>P</u> Frequency			Function IFU
Sweep <u>M</u> arker <u>F</u> requency			Frequency IFR
Sweep <u>T</u> ime			Amplitude IAM
Seconds	SE		Offset IOF
			Phase IPH
<u>S</u> weep <u>M</u> ode			Swp Start Freq IST
Linear	1		Swp Stop Freq ISP
Logarithmic	2		Swp Mkr Freq IMF
			Sweep Time ITI
<u>S</u> to <u>R</u> e Program			Sweep Mode ISM
	0 - 9		Rear/Front Out IRF
<u>R</u> ecall Program			High Volt Out IHV
	0 - 9		Error IER
<u>R</u> ear or <u>F</u> ront Panel Output			Program Mode IMD
Front	1		Amptd Mode IMA
Rear	2		Phase Mode IMP
Execution Functions			Error Codes (See Paragraph 3-146)
Assign Zero <u>P</u> hase			1. Entry parameter out of bounds
Perform <u>A</u> mp <u>t</u> d <u>C</u> al			2. Invalid delimiter
<u>S</u> tart <u>S</u> ingle*			3. Frequency too large for function
<u>S</u> tart <u>C</u> ontinuous			4. Sweep time too small or too large
Perform Self <u>T</u> est			5. Offset and amplitude incompatible
			6. Sweep frequency or bandwidth error
			7. Unrecognizable mnemonic
			8. Unrecognizable data character
			9. Option does not exist

*Start Single code must be sent twice "SSSS". The first "SS" resets the sweep to start conditions and the second "SS" starts the sweep.

SECTION IV

PERFORMANCE TESTS

TABLE OF CONTENTS

Paragraph	Page
4-1. Introduction	4-1
4-3. Calculator-Controlled Test	4-1
4-5. Operational Verification	4-1
4-8. Required Test Equipment	4-1
4-10. Self Test	4-1
4-12. Sine Wave Verification	4-1
4-14. Square Wave Verification	4-2
4-16. Triangle and Ramp Verification	4-3
4-18. Amplitude Flatness Check	4-3
4-20. Sync Output Check	4-4
4-22. Frequency Accuracy	4-4
4-24. Output Level and Attenuator Check	4-4
4-26. Harmonic Distortion Test	4-5
4-28. Close-In Spurious Signal Test	4-6
4-30. HP-IB Interface Test	4-6

LIST OF ILLUSTRATIONS

LIST OF TABLES

Figure	Page	Table	Page
4-1. Harmonic Distortion Verification (High Voltage Output)	4-5	4-1. Test Equipment Required for Operational Verification	4-2

SECTION IV PERFORMANCE TESTS

4-1. INTRODUCTION.

4-2. This section contains tests which are in-cabinet procedures to determine whether the instrument is operating properly. In the Operating and Service Manual two sets of procedures are provided:

a. Operational Verification procedures which are recommended for incoming inspection and general after-repair tests.

b. Performance Tests which compare the instrument operation to the specifications listed in Table 1-1. The Operating Supplement contains only the Operational Verification Procedures.

4-3. CALCULATOR-CONTROLLED TEST.

4-4. The only calculator-controlled test in these procedures tests the HP-IB interface circuits for proper operation. All input and output lines are tested. The program used for this test is written specifically for the -hp- Model 9825A Calculator but may be adapted to other controllers. The calculator prints the test results. This test is recommended for both the Operational Verification Checks and the Performance Tests.

4-5. OPERATIONAL VERIFICATION.

4-6. The following procedures are recommended for incoming inspection and for testing the instrument after repair. Additional tests to be performed following repair of certain circuits are indicated in Section VIII. An Operational Verification Record is located at the end of this section. For ease of recording the test data at various times, copies of the blank Operational Verification Record may be made without written permission from Hewlett-Packard.

4-7. Operational Verification includes the following procedures:

Par. No.	Test
4-10	Self Test
4-12	Sine Wave Verification
4-14	Square Wave Verification
4-16	Triangle and Ramp Verification
4-18	Amplitude Flatness Check
4-20	Sync Output Check
4-22	Frequency Accuracy
4-24	Output Level and Attenuator Check
4-26	Harmonic Distortion Test
4-28	Close-in Spurious Signal Test
4-30	HP-IB Interface Test

4-8. Required Test Equipment.

4-9. A list of test equipment required for the Operational Verification procedures is given in Table 4-1. Any equipment that satisfies the critical specifications given in the table may be substituted for the recommended model.

4-10. Self Test.

4-11. This test uses the control, ROM, and control clock circuits to verify operation of these and other circuits. The following front panel indications result from this test.

LED check: Turns on all LED's for about two seconds

The following messages are displayed for about one second:

OSC FAIL - displayed only if the VCO is not controlled (displayed continuously after test)

PASS or FAIL 1 - tests AMPTD CAL of sine wave

PASS or FAIL 2 - tests AMPTD CAL of square wave

PASS or FAIL 3 - tests AMPTD CAL of triangle

Press the blue entry prefix key, then press SELF TEST (AMPTD CAL) key. All LED's should light, and the display should not indicate any failures.

4-12. Sine Wave Verification.

4-13. This procedure visually checks the sine wave output for the correct frequency and any visible irregularities.

Equipment Required: Oscilloscope (-hp- Model 1740A)

a. Connect the 3325A signal output to the oscilloscope vertical input. If the oscilloscope is an -hp- Model 1740A, set the input switch to the 50-ohm position. If your oscilloscope does not have a 50-ohm input, use a 50-ohm load (-hp- Model 11048C 50-ohm Feed-thru Termination) at the input.

b. Set the 3325A as follows:

High Voltage Output (Option 002) Off
 Function Sine
 Frequency 20 MHz
 Amplitude 10 V p-p

Table 4-1. Test Equipment Required for Operational Verification.

Instrument	Critical Specifications	Recommended Model
Oscilloscope	Vertical: Bandwidth: dc to 100 MHz Deflection: 1 V to 5 V/div Horizontal: Sweep: .05 μ s to 1 s/div External Sweep Input	-hp- 1740A
Electronic Counter	Frequency measurement to 20 MHz Accuracy: ± 2 counts Resolution: 8 digits	-hp- 5328A with Opt. 040 or 041
DC Digital Voltmeter	Ranges: 0.1 V to 100 V Resolution: 6 digits Accuracy: $\pm 0.1\%$	-hp- 3455A
50-ohm load	Accuracy: $\pm 0.2\%$ Power Rating: 1 W	-hp- 11048C
High Frequency Spectrum Analyzer	Frequency Range: 1 MHz to 80 MHz Amplitude Accuracy: ± 0.5 dB Noise: > 70 dB below reference	-hp- 141T/8552B/8553B/ 8566A/8568A
Low frequency Spectrum Analyzer	Frequency Range: 100 Hz to 50 kHz Amplitude Range: 2 mV to 20 V Noise: > 80 dB below input reference or -140 dBv	-hp- 3580A/3585A
Resistor	56.2 Ω 1/8W 1.0%	-hp- 0757-0395
Adapter	BNC female-to-dual banana plug	-hp- 1250-2277
Calculator	HP-IB Control Capability	-hp- 9825A with 98034A Interface, General I/O ROM, Extended I/O ROM
Resistor	470 Ω 2W 5%	-hp- 0698-3634

- c. Set the oscilloscope vertical control to 2 V/div, horizontal to .05 μ s/div.
- d. The oscilloscope should display one cycle per division, approximately five divisions peak-to-peak.
- e. Change 3325A frequency to 1 MHz.
- f. Change oscilloscope horizontal control to .1 μ s/div.
- g. The oscilloscope should display one sine wave having no visible irregularities.
- High Voltage Output (Option 002)
- h. Set the oscilloscope vertical control to 5 V/div.
- i. Set the oscilloscope input switch to 1 M Ω dc coupled position (or disconnect external 50-ohm load).
- j. Press 3325A High Voltage Output key (lower right corner of front panel).
- k. Change 3325A amplitude to 40 V p-p. The oscilloscope should display one sine wave approximately eight divisions peak-to-peak having no visible irregularities.
- l. Press the High Voltage Output key again to turn the option off.

4-14. Square Wave Verification.

4-15. This procedure checks the square wave output for frequency, rise time, and aberrations.

Equipment Required: Oscilloscope (-hp- Model 1740A)

a. Connect the 3325A signal output to the oscilloscope vertical input. If the oscilloscope is an -hp- Model 1740A, set the input switch to the 50-ohm position. If your oscilloscope does not have a 50-ohm input, use a 50-ohm load (-hp- Model 11048C 50-ohm Feedthru Termination) at the input.

b. Set the 3325A as follows:

High Voltage Output (Option 002) Off
 Function Square
 Frequency 1 MHz
 Amplitude 10 V p-p

c. Set the oscilloscope vertical control to 2 V/div, horizontal to .2 μ s/div. The oscilloscope should display two square waves, approximately five divisions peak-to-peak.

d. Switch the oscilloscope vertical control to 1 V/div, so that the aberrations (overshoot and ringing) can be measured. Aberration excursion should be less than 500 mV ($\frac{1}{2}$ div.).

e. Repeat Step d at 2 kHz and .1 ms/div.

f. Adjust the oscilloscope vertical and horizontal controls so that the square wave rise time between the 10% and 90% points can be measured. Rise time should be less than 20 nanoseconds.

4-16. Triangle and Ramp Verification.

4-17. This procedure checks the triangle and ramp output signals for frequency, shape, and ramp retrace time.

Equipment Required: Oscilloscope (-hp- Model 1740A)

a. Connect the 3325A signal output to the oscilloscope vertical input. If the oscilloscope is an -hp- Model 1740A, set the input switch to the 50-ohm position. If your oscilloscope does not have a 50-ohm input, use a 50-ohm load (-hp- Model 11048C 50-ohm Feedthru Termination) at the input.

b. Set the 3325A as follows:

High Voltage Output (Option 002) Off
 Function Triangle
 Frequency 10 kHz
 Amplitude 10 V p-p

c. Set the oscilloscope vertical control to 2 V/div, horizontal to .1 ms/div. The oscilloscope should display one triangle wave per division, approximately five divisions peak-to-peak.

d. Change the 3325A function to positive slope ramp. The display should be one ramp per division, approximately five divisions peak-to-peak.

e. Change 3325A function to negative slope ramp. The display should be one ramp per division, approximately five divisions peak-to-peak.

f. Change the oscilloscope horizontal and vertical controls so that the ramp retrace time from the 90% to 10% points can be measured. Retrace time should be less than 3 μ s.

g. Change 3325A function to positive slope ramp and repeat Step f.

h. Change 3325A function to triangle.

i. Set oscilloscope vertical control to 2 V/div, horizontal to 10 μ s/div. The oscilloscope should display one triangle wave with no visible irregularities in either slope.

4-18. Amplitude Flatness Check.

4-19. This procedure provides a visual check of the sine wave amplitude flatness.

Equipment Required: Oscilloscope (-hp- Model 1740A)

a. Connect the 3325A signal output to the oscilloscope vertical input. If the oscilloscope is an -hp- Model 1740A, set the input switch to the 50-ohm position. If your oscilloscope does not have a 50-ohm input, use a 50-ohm load (-hp- Model 11048C 50-ohm Feedthru Termination) at the input.

b. Set the 3325A as follows:

High Voltage Output (Option 002) Off
 Function Sine
 Frequency 2 kHz
 Amplitude 10 V p-p
 Sweep Start Freq 0 Hz
 Sweep Stop Freq 20 MHz
 Sweep Marker Freq 5 MHz
 Sweep Time 01 sec

c. Connect the 3325A X-Drive output to the oscilloscope's channel B input. Connect the 3325A signal output to the oscilloscope's channel A input.

* d. Set the oscilloscope as follows:

Display A vs B
 Channel A Sensitivity 1V/div
 (uncal - adjust for full vertical deflection)
 Channel B Sensitivity 0.5V/div
 (uncal - adjust for full horizontal sweep)

* Settings may vary from one oscilloscope to another. Note that whichever scope is used, it should be operated in a "X-Y" mode, with the 3325A X-Drive output driving the horizontal (X) sweep and the signal output driving the scope's vertical (Y) channel.

- e. Press the 3325A START CONT key.
- f. The oscilloscope display should show a sweep that is essentially flat, dropping no more than 3.5%. Any D.C. variations should be ignored, taking the peak-to-peak reading for flatness comparison.

4-20. Sync Output Check.

4-21. This test verifies the sync output signal levels.

Equipment Required: Oscilloscope (-hp- Model 1740A)

- a. Connect the 3325A sync output to the oscilloscope vertical input. If the oscilloscope is an -hp- Model 1740A, set the input switch to the 50-ohm position. If your oscilloscope does not have a 50-ohm input, use a 50-ohm load (-hp- Model 11048C 50-ohm Feedthru Termination) at the input.
- b. Set the 3325A function to sine, frequency to 20 MHz.
- c. Adjust the oscilloscope controls to measure the high and low voltage levels of the sine square wave. The high level should be greater than +1.2 V and the low level should be less than +0.2 V.

4-22. Frequency Accuracy.

4-23. This test compares the accuracy of the 3325A output signal to the specification in Table 1-1: $\pm 5 \times 10^{-6}$ of selected frequency.

Equipment Required: Electronic Counter (-hp- Model 5328A, calibrated within three months or with an accurate 10 MHz external reference input)

- a. Connect the 3325A signal output to the electronic counter channel A input with a 50 Ω load. Allow 3325A and counter to warm up for 20 minutes.
- b. Set the 3325A output as follows:

Function	Sine
Frequency	20 MHz
Amplitude	0.99 V P-P
DC Offset	0 V

- c. Set the counter to count the frequency of the A input with 0.1Hz resolution, and adjust for stable triggering. Electronic counter should indicate 20 000 000.0Hz ± 100 Hz.
- d. Change 3325A function to square wave. Frequency automatically changes to 10 MHz. Electronic counter should indicate 10 000 000.0 Hz ± 50 Hz.
- e. Change 3325A function to triangle. Frequency automatically changes to 10kHz. Move the counter input to

the sync output of the 3325A. Set the counter to average 1000 periods. Electronic counter should indicate 100 000.00ns ± 0.5 ns.

- f. Change 3325A function to positive slope ramp. Electronic counter should indicate 100,000 ns $\pm .5$ ns.

4-24. Output Level and Attenuator Check.

4-25. This procedure checks the output level and the attenuator by using the "dc only" function.

Equipment Required:

- DC Digital Voltmeter (-hp- Model 3455A)
- 50-ohm Feedthru Termination (-hp- Model 11048C)

- a. Connect the 3325A signal output through a 50-ohm feedthru termination to a dc digital voltmeter input.
- b. If the instrument has High Voltage Output Option 002, make sure the High Voltage Output is Off (High Voltage indicator light in the center of the "SIGNAL" key in the lower right corner of the front panel if Off).
- c. Press whichever function key is presently active, indicated by a lighted indicator in the center of the key. This removes the ac output. The indicator in the center of the DC OFFSET key should light.
- d. Set the 3325A dc offset to -5 V, then press the AMPTD CAL key.
- e. The dc digital voltmeter reading should be -4.980V to -5.020V.
- f. Change 3325A dc offset to (+)5 V. Digital voltmeter reading should be +4.980 V to +5.020 V.
- g. Change 3325A dc offset to the following voltages. The voltmeter readings should be within the tolerances shown.

DC Offset	Tolerances
± 1.499 V	± 1.49300 to 1.50499 V
± 499.9 mV	± 0.49790 to 0.50190 V
± 149.9 mV	± 0.14930 to 0.15050 V
± 49.99 mV	± 0.04979 to 0.05019 V
± 14.99 mV	± 0.01493 to 0.01505 V
± 4.999 mV	± 0.004979 to 0.005019 V
± 1.499 mV	± 0.001479 to 0.001519 V

High Voltage Output Option 002 DC Offset

- h. Remove the 50-ohm feedthru termination and connect the 3325A output directly to the digital voltmeter input.

i. Press the "SIGNAL" key in the lower right corner of the 3325A front panel to select High Voltage Output (Option 002). Lighted indicator in the center of this key indicates High Voltage Output is on.

j. Set 3325A dc offset to 20 V. Digital voltmeter reading should be +19.775 V to +20.225 V.

k. Set 3325A dc offset to -20 V. Digital voltmeter reading should be -19.775 V to -20.225 V.

4-26. Harmonic Distortion Test.

4-27. This procedure tests the harmonic distortion of the 3325A sine wave output against the following specifications from Table 1-1.

Harmonic Distortion (relative to fundamental)

Fundamental Frequency	No Harmonic Greater Than
0.1 Hz to 50 kHz	- 65 dB
50 kHz to 200 kHz	- 60 dB
200 kHz to 2 MHz	- 40 dB
2 MHz to 15 MHz	- 30 dB
15 MHz to 20 MHz	- 25 dB

a. Set the 3325A output as follows:

High Voltage Output (Option 002) Off
 Function Sine
 Frequency 20 MHz
 Amplitude 999mVp-p

b. Connect the 3325A signal output to the high frequency spectrum analyzer's 50 ohm input.

c. Set the spectrum analyzer controls to display the fundamental and at least four harmonics. Verify that all harmonics are 25dB below the fundamental.

d. Set the 3325A to the following frequencies and verify that all harmonics are below the specified levels, relative to the fundamental.

15 MHz	- 30 dB
2 MHz	- 40 dB
200 kHz	- 60 dB

e. Disconnect the 3325A from the high frequency spectrum analyzer and connect it to the low frequency spectrum analyzer's 50 ohm input.

f. Set the 3325A frequency to 50kHz and the amplitude to 9.99mVp-p.

g. Set the spectrum analyzer controls to display the fundamental and at least three harmonics. (It may be necessary to decrease the analyzer's video bandwidth to separate the harmonics from the noise floor.) Verify that all harmonics are at least 65dB below the fundamental.

Equipment Required:

High Frequency Spectrum Analyzer (-hp- Model 141T/8552B/8553B/8566A/8568A)

Low Frequency Spectrum Analyzer (-hp- Model 3580A/ 3585A)

50-ohm Feedthru Termination (-hp- Model 11048C)

Resistor 470Ω 2W 5% (-hp- 0698-3634)

Resistor 56.2Ω 1/8W 1% (-hp- 0757-0395)

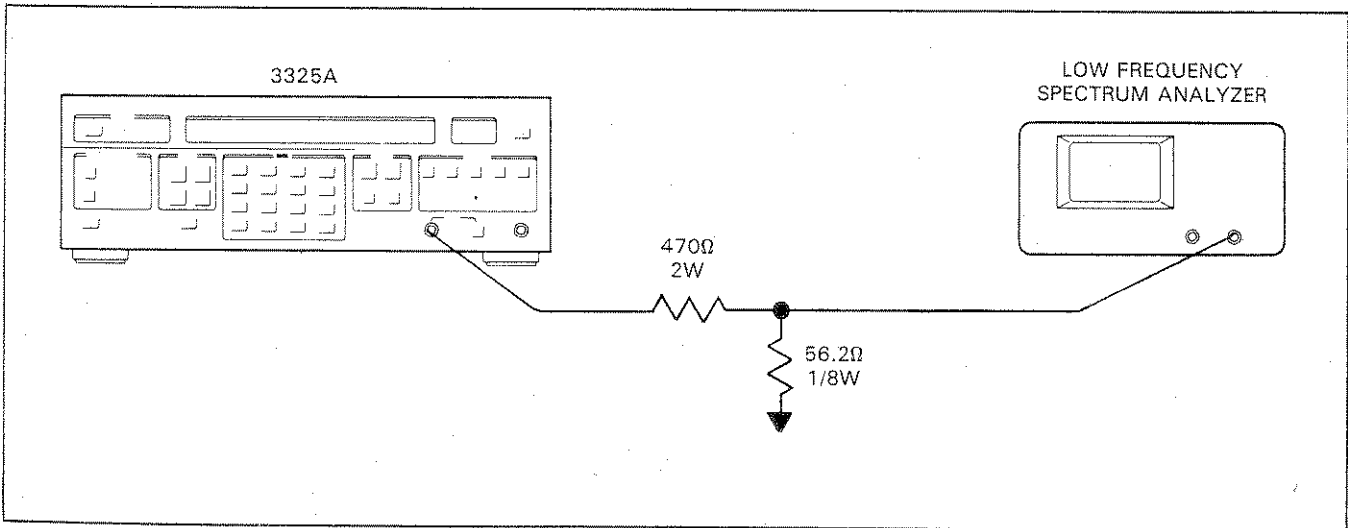


Figure 4-1. Harmonic Distortion Verification (High Voltage Output).

h. Set the 3325A to the following frequencies and verify that all harmonics are 65dB below the fundamental.

- 10kHz
- 1kHz
- 100Hz

High Voltage Output (Option 2)

i. Connect the 3325A signal output to the low frequency spectrum analyzer's 50Ω input. (See Figure 4-1.)

j. Press the "high voltage output" key on the 3325A. Set the amplitude to 40Vp-p and the frequency to 100Hz.

k. Set the spectrum analyzer controls to display the fundamental and at least three harmonics. Verify that all harmonics are 65dB below the fundamental.

l. Set the 3325A to the following frequencies and verify that their harmonics are below the specified levels, relative to the fundamental.

- 10kHz -65dB
- 200kHz -60dB
- 1MHz -40dB

m. Press the high voltage output key to deactivate the high voltage output.

4-28. Close-In Spurious Signal Test.

4-29. This procedure tests the sine wave output for spurious signals which may be generated by the 3325A frequency synthesis circuits. The spurious signals must be more than 70 dB lower than the fundamental signal.

Equipment Required: Spectrum Analyzer (-hp-3585A/8566A/8568A)

a. Set the 3325A as follows:

- High Voltage Output (Option 002) Off
- Function Sine

- Frequency 20.001MHz
- Amplitude -2.99dBm
- DC Offset 0 V

b. Connect the 3325A signal output to the spectrum analyzer's 50 ohm input.

c. Set the spectrum analyzer controls for a center frequency of 20.001MHz, a resolution bandwidth of 30Hz, a 100Hz/div frequency span, with the fundamental referenced to the top of the display graticule.

d. Set the spectrum analyzer center frequency to 20.002, 20.003, and 20.004MHz, verifying in each case that all spurious signals are more than 70dB below the fundamental.

4-30. HP-IB Interface Test.

4-31. The following calculator program tests the operation of the 3325A HP-IB interface circuits. The program is written for an -hp- Model 9825A calculator but may be adapted for other controllers.

Equipment Required:

- hp- Model 9825A Calculator equipped with:
- 98034A HP-IB Interface (set to select code 7)
- Any combination of ROM's that includes a General I/O ROM and an Extended I/O ROM

a. Connect the calculator interface cable to the 3325A rear panel HP-IB connector. It is recommended that no other equipment be connected to this HP-IB during this test.

b. Enter the program into the calculator.

c. Press RUN. Tests 4 through 7 in this program require the operator to press CONTINUE if the test passes, or 1 CONTINUE if the test fails. If the Test 4 question (SRQ LIGHT ON?, 1 = NO) does not appear in the calculator display within 30 seconds after start of the program (RUN), the 3325A and calculator are not interfacing properly. The calculator may display an error indication that will identify the problem. If not, the 3325A HP-IB circuits are probably not operating correctly.

Instrument Returns To Known Conditions After Self Test

Test 1 – Did Frequency Go To 1000 Hz?

Test 2 – Interrogate Frequency

Test 3 – Interrogate Amplitude


Test 4 – Test SRQ Circuits

Test 5 – Test Talk Circuits

Test 6 – Test Listen Circuits

Test 7 – Test Remote Circuits

PROGRAM FLOWCHART

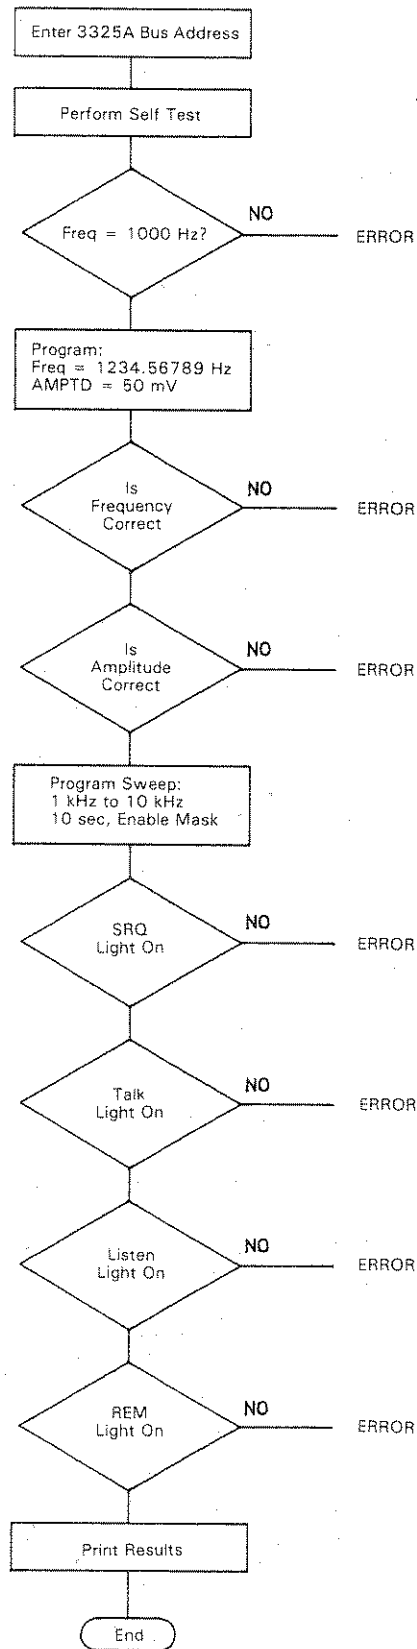

```

0: fmt fcsu;0+r1+r2+r3+r4+r5+r6+r7
1: prt "*****"
2: prt "3325A"
3: prt "HP-IB TEST"
4: prt "*****"
5: beed;ent "3325A BUS ADDRESS?;cont=717";A
6: if f1=13;717+A
7: clr A _____ Clear the 3325A to Turn-on State
8: rem 7 _____ Set HP-IB Remote Enable (Select Code 7)
9:
10: "TEST 1":
11: wrt A;"TE" _____ Perform Self Test
12: wrt A;"IFR" _____ Interrogate Frequency
13: red A;F _____ Read 3325A Frequency
14: if F#1000;1+r1 _____ Compare Frequency to 1000 Hz
15:
16: "TEST 2,3 SETUP":
17: wrt A;"FR1234.567890HZ AM50MV" _____ Set Freq to 1234.567890 Hz, Amptd to 50mV
18: wrt A;"SR3" _____ Store Settings in Register 3
19: clr A _____ Clear the 3325A
20: wrt A;"RE3" _____ Recall Settings in Register 3
21:
22: "TEST 2":
23: wrt A;"IFR" _____ Interrogate Frequency
24: red A;G _____ Read Frequency
25: if G#1234.56789;1+r2 _____ Compare to Frequency Stored
26:
27: "TEST3":
28: wrt A;"IAM" _____ Interrogate Amplitude
29: red A;H _____ Read Amplitude
30: if H#.05;1+r3 _____ Compare to Amplitude Stored
31:

```

```

32: "TEST 4":
33: wrt A,"STIKH SP10KH SM1 TI10SE MEF 9999"Lin Sweep 1-10kHz, Enable SRQ Mask
34: cli 7;lcl 7 _____Clear Interface, Interface to Local
35: beep!ent "SRQ LIGHT ON?,1=NO",r4 _____Did 3325A Initiate SRQ?
36:
37: "TEST 5":
38: rds(A)+S _____Read Status into Variable 5
39: ren 7 _____Set Remote Enable
40: red A;S _____Read from the 3325A
41: beep!ent "TALK LIGHT ON?,1=NO",r5 _____Did 3325A respond to Talk Command?
42:
43: "TEST6":
44: wrt A;lcl 7 _____Write to the 3325A, Interface to Local
45: beep!ent "LISTEN LIGHT ON?,1=NO",r6 _____Did 3325A respond to Listen Command?
46:
47: "TEST 7":
48: ren 7;wrt A;lcl 7 _____Remote Interface, Write to 3325A,
Clear Interface
49: beep!ent "REMOTE LIGHT ON?,1=NO",r7 _____Did the 3325A Respond to Remote?
50:
51: spc !prt "*****"
52: prt "TEST RESULTS:"
53: spc !1+1!fxd 0
54: if r1=0!prt "TEST",I," PASS"
55: if r1=1!prt "TEST",I," FAIL"
56: if (I+1+I)<=7!jmp -2
57: prt "*****"!epc 3
58: ent "Repeat test?,1=Yes",C!if C=1!eto 0 _____Self Contained Program may be
59: end _____Linked or Used as a Subroutine
*24986
    
```

Variables used in this Test Program:

- A Address of 3325A (defaults to 717)
- F Frequency read from 3325A in test #1
- G Frequency read from 3325A in test #2
- H Amplitude read from 3325A in test #3
- I Counter used to print test results
- r1-r7 Test results (0 = Pass, 1 = Fail)
- S Status read from 3325A in test #5

Samples of Program Printouts:

```

*****
3325A
HP-IB TEST
*****

*****
TEST RESULTS:

TEST          1
TEST PASS
TEST          2
TEST PASS
TEST          3
TEST PASS
TEST          4
TEST          FAIL
TEST          5
TEST PASS
TEST          6
TEST PASS
TEST          7
TEST PASS
*****

```

```

*****
3325A
HP-IB TEST
*****

*****
TEST RESULTS:

TEST          1
TEST PASS
TEST          2
TEST PASS
TEST          3
TEST PASS
TEST          4
TEST PASS
TEST          5
TEST PASS
TEST          6
TEST PASS
TEST          7
TEST PASS
*****

```

OPERATIONAL VERIFICATION RECORD

Hewlett-Packard
 Model 3325A
 Synthesizer/Function Generator
 Serial No. _____

Tested by _____

Date _____

Par. 4-10	Self Test	Passed _____
Par. 4-12	Sine Wave Verification	
Step d	20 MHz: Frequency and Amplitude	Passed _____
Step g	Signal Purity	Passed _____
	High Voltage Output (1 MHz)	Passed _____
Par. 4-14	Square Wave Verification	
Step c	Frequency and Amplitude	Passed _____
Steps d & e	Abberations	Passed _____
Step f	Rise Time	Passed _____
Par. 4-16	Triangle and Ramp Verification	
Step c	Triangle Freq. and Amptd.	Passed _____
Step d	+ Ramp Freq. and Amptd.	Passed _____
Step e	- Ramp Freq. and Amptd.	Passed _____
Step f	- Ramp Retrace Time	Passed _____
Step g	+ Ramp Retrace Time	Passed _____
Step i	Triangle Linearity	Passed _____
Par. 4-18	Amplitude Flatness	Passed _____
	Spec	
Par. 4-20	Sync Output Check	High _____ > +1.2 V
		Low _____ < 0.2 V
Par. 4-22	Frequency Accuracy	Spec.
Step c	Sine, 20 MHz	_____ ± 100 Hz
Step d	Square, 10 MHz	_____ ± 50 Hz
Step e	Triangle, 10 kHz (100,000 ns)	_____ ± .5 ns
Step f	Ramp, 10 kHz (100,000 ns)	_____ ± .5 ns

Operational Verification

Par. 4-24 Output Level and Attenuator Check
 (DC Offset Only)

Entry	Min.	Max.
- 5 V	- 4.980 V _____	- 5.020 V
(+) 5 V	+ 4.980 V _____	+ 5.020 V
* (±) 1.499V	(±) 1.49300V _____	(±) 1.50499V
499.9 mV	+ 0.49790 V _____	+ 0.50190 V
149.9 mV	+ 0.14930 V _____	+ 0.15050 V
49.99 mV	+ 0.04979 V _____	+ 0.05019 V
14.99 mV	+ 0.01493 V _____	+ 0.01505 V
4.999 mV	+ 0.04979 V _____	+ 0.005019 V
1.499 mV	+ 0.001479 V _____	+ 0.001519 V

* All entries and limits are ±

High Voltage Output (Option 002)

20 V	+ 19.775 V _____	+ 20.225 V
- 20 V	- 19.775 V _____	- 20.225 V

Par. 4-26 Harmonic Distortion

	All Harmonics Below:
20 MHz	_____ - 25 dB
15 MHz	_____ - 30 dB
2 MHz	_____ - 40 dB
200 kHz	_____ - 60 dB
50 kHz	_____ - 65 dB
10 kHz	_____ - 65 dB
1 kHz	_____ - 65 dB
100 Hz	_____ - 65 dB
High Voltage Output (Option 002)	
100 Hz	_____ - 65 dB
10 kHz	_____ - 65 dB
200 kHz	_____ - 60 dB
1 MHz	_____ - 40 dB

Par. 4-28 Close-In Spurious Signal Test Passed _____

Par. 4-30 HP-IB Check Passed _____