

Valuetronics International, Inc.

1-800-552-8258

**MASTER COPY**

---

## Programmer's Guide

© Copyright Hewlett-Packard Company 1993, 1994

All Rights Reserved.

Reproduction, adaptation, or translation without prior written permission is prohibited, except as allowed under the copyright laws.

#### Printing History

HP Part Number  
04155-90110

First edition, February 1994

Second edition, December 1994

Printed in Japan

MS-DOS® is U.S. registered trademark of Microsoft Corporation.

Lotus 1-2-3 is U.S. registered trademark of Lotus Development Corporation.

PageMaker is a trademark of Aldus Corporation.

#### Product Warranty

This Hewlett-Packard product is warranted against defects in material and workmanship for a period of one year from date of shipment. During the warranty period, Hewlett-Packard will, at its option, either repair or replace products which prove to be defective.

For warranty service or repair, this product must be returned to a service facility designated by Hewlett-Packard. Buyer shall prepay shipping charges to Hewlett-Packard and Hewlett-Packard shall pay shipping charges to return the product to Buyer. However, Buyer shall pay all shipping charges, duties, and taxes for products returned to Hewlett-Packard from another country.

Hewlett-Packard warrants that its software and firmware designated by Hewlett-Packard for use with an instrument will execute its programming instructions when properly installed on that instrument. Hewlett-Packard does not warrant that the operation of the instrument, or software, or firmware will be uninterrupted or error free.

#### Limitation of Warranty

The foregoing warranty shall not apply to defects resulting from improper or inadequate maintenance by Buyer, Buyer-supplied software or interfacing, unauthorized modifications or misuse, operation outside of the environment specifications for the products, or improper site preparation or maintenance.

No other warranty is expressed or implied. Hewlett-Packard specifically disclaims the implied warranties of merchantability and fitness for a particular purpose.

#### Exclusive Remedies

The remedies provided herein are the Buyer's sole and exclusive remedies. Hewlett-Packard shall not be liable for any direct, indirect, special, incidental, or consequential damages, whether based on contract, tort, or any other legal theory.

#### Assistance

Product maintenance agreements and other customer assistance agreements are available for Hewlett-Packard products.

For any assistance, contact your nearest Hewlett-Packard Sales Office.

#### Certification

Hewlett-Packard Company certifies that this product met its published specifications at the time of shipment (from the factory). Hewlett-Packard further certifies that its calibration measurements are traceable to the **National Institute of Standards and Technology (NIST)**, to the extent allowed by the Institute's calibration facility, and to the calibration facilities of other International Standards Organization members.

## Programming Overview

The HP 4155A/56A can be *fully* controlled from an external computer or by using built-in HP Instrument BASIC (IBASIC) controller. IBASIC is a programming environment that allows full control of HP 4155A/56A without using an external computer.

To fully control the HP 4155A/56A, you execute programs that contain SCPI commands. SCPI means Standard Commands for Programmable Instruments. SCPI is the default program language of the HP 4155A/56A, and can control all functions of the HP 4155A/56A. These programs can be run from IBASIC or an external computer.

The HP 4155A/56A has two command modes:

- *HP 4155/56 command mode* is the default mode of HP 4155A/56A. You use this mode in *all* cases, *except* when directly running an HP 4145A/B program. In this mode, you can use a program that contains SCPI commands, which allow you to control *all* functions of the HP 4155A/56A.
- *HP 4145 syntax command mode*, which allows you to execute HP 4145A/B programs on the HP 4155A/56A directly with little or no modification. In this command mode, you *cannot* control all functions of HP 4155A/56A.



### How to Migrate HP 4145A/B Programs

*HP 4145A/B Auto Sequence Program (ASP) programs* run on the HP 4145A/B built-in programming environment and allow *basic* control of HP 4145A/B without using an external computer. To run the ASP programs on the HP 4155A/56A, you do one of the following and execute the program in the *HP 4155/56 command mode*:

- Create a program that performs the same operations as the desired ASP program by using the IBASIC editor typing aid softkeys to enter commands that correspond to each ASP command. This program can run on IBASIC only, *not* on an external computer. Refer to "Creating ASP-like IBASIC Programs" in Chapter 1 for details.
- Create a program using SCPI commands that performs same operations as the desired ASP program. This program can run on IBASIC or on an external computer. Refer to "Programming Example for HP 4145 Users" in Chapter 4 for details.

*HP 4145A/B HP-IB programs* run on an external computer and allow *full* control of the HP 4145A/B. To run these programs on the HP 4155A/56A, do one of the following:

- Directly run the HP 4145A/B program on the HP 4155A/56A with little or no modification. You must run this program in the *HP 4145 syntax command mode* from IBASIC or an external computer. Refer to Chapter 5 for details.
- Create a program using SCPI commands that performs same operations as the HP 4145A/B program. You must run this program in *HP 4155/56 command mode* from IBASIC or an external computer.

---

## In This Manual

This manual describes how to control the HP 4155A/4156A by using HP-IB commands from an external computer or built-in HP Instrument BASIC.

This manual consists of the following chapters:

- Using HP Instrument BASIC
- Reference: HP Instrument BASIC
- Getting Started on Programming the HP 4155A/4156A
- HP 4155A/4156A SCPI Programming
- Running HP 4145A/B Program Directly on HP 4155A/4156A
- Sample Application Programs
- Manual Changes Depending on ROM Version

Refer to the HP 4155A/4156A *HP-IB Command Reference* for detailed syntax of each command.

See the HP 4155A/4156A *User's Task Guide* and *User's Dictionary Reference* for information about HP 4155A/4156A itself.

### Text Conventions.

The following text conventions are used in this manual:

<b>Front-panel key</b>	Represents a key physically located on HP 4155A/4156A.
<b>Softkey</b>	Represents a softkey that appears on screen of HP 4155A/4156A.
<b>Screen Text</b>	Represents text displayed on HP 4155A/4156A.
<i>Italic</i>	Refers to a related document, or is used for emphasis.

---

## Contents

<b>1. Using HP Instrument BASIC</b>	
Before Operating IBASIC . . . . .	1-3
To Switch Screen Mode . . . . .	1-4
Front Panel . . . . .	1-4
External Keyboard . . . . .	1-4
To Use the Help Function . . . . .	1-5
Creating and Executing a Simple IBASIC Program . . . . .	1-7
Step 1. Editing . . . . .	1-7
Step 2. Exiting from Editor . . . . .	1-9
Step 3. Executing Program . . . . .	1-9
Modifying Program by using Editor Functions . . . . .	1-10
Step 1. Inserting Lines . . . . .	1-11
Step 2. Deleting a Line . . . . .	1-12
Step 3. Renumbering . . . . .	1-13
Step 4. Inserting Characters . . . . .	1-14
Step 5. Recalling Deleted Line . . . . .	1-15
Step 6. Indenting . . . . .	1-15
Saving and Getting a Program . . . . .	1-16
Step 1. Saving a Program . . . . .	1-17
Step 2. Listing Contents of Diskette . . . . .	1-17
Step 3. Clearing a Program . . . . .	1-18
Step 4. Getting a Program . . . . .	1-18
Summary of Softkeys and Keyboard Operations for Editor . . . . .	1-19
Other Basic Features of IBASIC . . . . .	1-20
Branching/Repeating . . . . .	1-21
Subprograms and COM Blocks . . . . .	1-22
IBASIC Basic Operation Tasks . . . . .	1-24
To Execute HP Instrument BASIC Commands . . . . .	1-25
To Execute Program . . . . .	1-25
Front Panel . . . . .	1-25
External Keyboard . . . . .	1-25
To List Files . . . . .	1-26
To Retrieve Program . . . . .	1-27
To Save Program . . . . .	1-28
IBASIC Editor Tasks . . . . .	1-29
To Start the Editor . . . . .	1-30

**Change 1**

To Quit the Editor . . . . .	1-30
To Move the Cursor . . . . .	1-31
To Insert Characters . . . . .	1-31
To Delete Character . . . . .	1-32
To Insert Line . . . . .	1-32
To Delete Line . . . . .	1-33
To Scroll Pages . . . . .	1-33
To Recall Most Recently Deleted Line . . . . .	1-34
Control from External Computer . . . . .	1-35
To Download a Program to HP 4155A/4156A . . . . .	1-36
Example . . . . .	1-36
To Upload a Program from HP 4155A/4156A . . . . .	1-38
Example . . . . .	1-38
To Control State of HP 4155A/4156A Program . . . . .	1-40
Example . . . . .	1-40
Creating ASP-like IBASIC Programs . . . . .	1-41
Step 1. Creating Programs by using the Typing Aid . . . . .	
Softkeys . . . . .	1-41
Step 2. Executing the Program . . . . .	1-43
Step 3. Creating a Longer Program . . . . .	1-43
Programming Tips . . . . .	1-45
Example ASP Program . . . . .	1-45
Corresponding IBASIC Program. . . . .	1-45
Reading HP 4155/56 Data to IBASIC Variables . . . . .	1-46
Auto Scaling . . . . .	1-47
HP 4145 ASP and HP 4155A/4156A Corresponding . . . . .	
Keywords . . . . .	1-48
<b>2. Reference: HP Instrument BASIC</b>	
IBASIC Screen . . . . .	2-3
All IBASIC Screen . . . . .	2-4
IBASIC Output Area . . . . .	2-4
Command Entry Line . . . . .	2-4
System Message and Display Line . . . . .	2-4
Blue Key & Green Key Shift Status . . . . .	2-5
Execution Status . . . . .	2-5
IBASIC Status Screen . . . . .	2-6
Keys for IBASIC . . . . .	2-7
Front-panel Keys for IBASIC . . . . .	2-8
PAGE CONTROL key group . . . . .	2-8
MARKER/CURSOR key group . . . . .	2-8

MEASUREMENT key group . . . . .	2-9
IBASIC key group . . . . .	2-9
ENTRY key group . . . . .	2-10
Other Keys . . . . .	2-10
Primary Softkeys in Idle, Pause, Run, or Input?	
execution status . . . . .	2-11
Step . . . . .	2-11
Conti-nue . . . . .	2-11
RUN . . . . .	2-11
Pause . . . . .	2-11
Stop . . . . .	2-11
ClearI/O . . . . .	2-11
Reset . . . . .	2-11
Secondary Softkeys in Idle or Pause execution status . .	2-12
CAT . . . . .	2-12
SAVE "" . . . . .	2-12
RE-SAVE "" . . . . .	2-12
GET "" . . . . .	2-13
PURGE "" . . . . .	2-13
EDIT . . . . .	2-13
REN umber . . . . .	2-13
Secondary Softkeys in Run or Input? execution status .	2-13
Primary Softkeys in Edit execution status . . . . .	2-14
Backspace . . . . .	2-14
Insertline . . . . .	2-14
Deleteline . . . . .	2-14
Re-number . . . . .	2-14
Indent . . . . .	2-14
Scratch . . . . .	2-14
Endedit . . . . .	2-14
Secondary Softkeys in Edit execution status . . . . .	2-15
GETSETUP . . . . .	2-15
SINGLE . . . . .	2-15

Change 1

STANDBY	2-15
STRESS	2-16
AUTOSCALE	2-16
SAVEDATA	2-16
READDATAVARIABL	2-16
DEFINEUSERVARIABL	2-16
PRINT/PLOT	2-16
CURVEPLOT	2-16
OUTPUT@Hp415x	2-17
ENTER@Hp415x	2-17
PAUSE	2-17
DISP	2-17
INPUT	2-17
IF THENELSEEND IF	2-17
WHILEEND WHILE	2-18
FORNEXT	2-18
External Keyboard	2-19
Esc	2-19
F1 through F8	2-19
Shift + F1 through F7	2-19
F9	2-19
F11	2-19
Shift + F11	2-19
F12	2-20
Print Screen	2-20
Scroll Lock	2-20
Shift + Scroll Lock	2-20
Pause	2-20
Shift + Pause	2-20
Insert	2-20
Shift + Insert	2-20
Delete	2-20
Shift + Delete	2-20
Ctrl + Delete	2-21
Home	2-21

Shift + Home	2-21
End	2-21
Shift + End	2-21
Page Up	2-21
Shift + Page Up	2-21
Page Down	2-22
Shift + Page Down	2-22
▲	2-22
Shift + ▲	2-22
Alt + ▲	2-22
▼	2-22
Shift + ▼	2-22
Alt + ▼	2-22
◀, ▶	2-23
Shift + ◀	2-23
Shift + ▶	2-23
Backspace	2-23
Alt + D	2-23
Alt + I	2-23
Ctrl + U	2-23
Ctrl + P	2-23
Ctrl + G	2-24
HP 4155A/4156A Specific IBASIC Keywords	2-25
Available I/O Resources for IBASIC	2-27
CRT Display	2-28
HP-IB Interfaces	2-28
Serial Interface	2-29
Built-in Diskette Drive	2-30
ASP-like Commands	2-31
EXECUTE	2-31
Syntax	2-31
<i>directive</i>	2-31
GET SETUP Directive	2-32
Directive syntax	2-32
Directive parameter	2-32
Example	2-32
SINGLE Directive	2-32
Directive syntax	2-32
Example	2-32
STANDBY directive	2-33
Directive syntax	2-33

## Change 1

Directive parameter . . . . .	2-33
Example . . . . .	2-33
STRESS Directive . . . . .	2-33
Directive syntax . . . . .	2-33
Example . . . . .	2-33
AUTO-SCALE Directive . . . . .	2-34
Directive syntax . . . . .	2-34
Example . . . . .	2-34
SAVE DATA Directive . . . . .	2-34
Directive syntax . . . . .	2-34
Directive parameter . . . . .	2-34
Example . . . . .	2-34
READ DATA VARIABLE Directive . . . . .	2-35
Directive syntax . . . . .	2-35
Directive parameter . . . . .	2-35
Example . . . . .	2-35
DEFINE USER VARIABLE Directive . . . . .	2-36
Directive syntax . . . . .	2-36
Directive parameter . . . . .	2-36
Example . . . . .	2-36
PRINT/PLOT Directive . . . . .	2-37
Directive syntax . . . . .	2-37
Example . . . . .	2-37
CURVE PLOT Directive . . . . .	2-37
Directive syntax . . . . .	2-37
Example . . . . .	2-37
<b>3. Getting Started on Programming the HP 4155A/4156A</b>	
Creating a Simple Measurement Program . . . . .	3-3
Before Creating a Program . . . . .	3-4
Step 1. Getting the Setup File and Making a Measurement . . . . .	3-4
Step 2. Changing the Sweep Setup Parameters . . . . .	3-8
Step 3. Changing the Display Setup Parameters . . . . .	3-10
Step 4. Saving All Measurement Results to a Diskette. . . . .	3-12
Step 5. Printing the Measurement Results . . . . .	3-14
Programming for Data Extraction . . . . .	3-16
Reading HP 4155/56 Setup Data . . . . .	3-16
Reading HP 4155/56 Measurement Data . . . . .	3-17
Transferring Specific HP 4155/56 Data to a File . . . . .	3-18
Complete Example Program for Vth Measurement . . . . .	3-21

Example Application Setup for Vth Measurement . . . . .	3-23
<b>4. HP 4155A/4156A SCPI Programming</b>	
SCPI Programming Basics . . . . .	4-3
Preparation before Controlling the HP 4155A/56A via HP-IB . . . . .	4-4
SCPI Command Hierarchy . . . . .	4-5
To Control HP 4155A/56A by HP BASIC Programming . . . . .	4-6
Example . . . . .	4-7
Programming: Measurement Setup . . . . .	4-8
To Set or Change HP 4155/56 Setup Data Values . . . . .	4-9
Example . . . . .	4-10
To Read HP 4155/56 Setup Data Values . . . . .	4-11
Example . . . . .	4-11
Programming: Measurement Execution . . . . .	4-12
To Execute a Sweep or Sampling Measurement . . . . .	4-13
Example . . . . .	4-13
To Force Stress . . . . .	4-15
Example . . . . .	4-15
To Start the Knob Sweep Function . . . . .	4-17
Example . . . . .	4-17
To Control Standby Units . . . . .	4-18
Example . . . . .	4-18
Programming: File Operation . . . . .	4-20
To Store Setup Data to Diskette or Internal Memory . . . . .	4-21
Example . . . . .	4-21
To Store Measurement Data to Diskette or Internal Memory . . . . .	4-22
Example . . . . .	4-22
To Load Setup Data from Diskette or Internal Memory . . . . .	4-23
Example . . . . .	4-23
To Load Measurement Data from Diskette or Internal Memory . . . . .	4-24
Example . . . . .	4-24
Programming: Data Transfer . . . . .	4-25
To Read HP 4155/56 Measurement Data . . . . .	4-26
Example . . . . .	4-26
To Transfer Data to HP 4155A/4156A (Using User Variable) . . . . .	4-27
Example . . . . .	4-28
Programming: Print/Plot Operation . . . . .	4-31

**Change 1**

To Output Setup Data to Printer/Plotter . . . . .	4-33
Example . . . . .	4-34
To Output Graphics Result Data to Printer/Plotter . . . . .	4-37
Example . . . . .	4-37
To Output List Results Data to Printer/Plotter . . . . .	4-40
Example . . . . .	4-40
To Dump Screen Image to Printer/Plotter . . . . .	4-43
Example . . . . .	4-43
To Save Hardcopy Image to Diskette . . . . .	4-46
Example . . . . .	4-46
Other Programming Tips . . . . .	4-48
Disabling Instrument Screen Update to Improve Speed . . . . .	4-48
Auto-loading of Files . . . . .	4-49
Programming Example for HP 4145 Users . . . . .	4-50
<b>5. Running HP 4145A/B Program Directly on HP 4155A/4156A</b>	
Non-supported Commands . . . . .	5-3
Considerations about Differences . . . . .	5-4
Spot Measurement . . . . .	5-4
Sweep Steps in Logarithmic Step Mode . . . . .	5-4
Terminator . . . . .	5-5
<b>6. Sample Application Programs</b>	
Flash EEPROM Test . . . . .	6-3
Program Overview . . . . .	6-4
Stress_loop . . . . .	6-8
Vth_meas . . . . .	6-9
Program Customization . . . . .	6-10
Program Listing . . . . .	6-14
Time Dependent Dielectric Breakdown (TDDB) . . . . .	6-20
Application Overview . . . . .	6-20
Customization . . . . .	6-21
Electromigration . . . . .	6-22
Application Overview . . . . .	6-22
Customization . . . . .	6-23

**Change 1**

**7. Manual Changes Depending on ROM Version**

Change 1 . . . . .	7-3
Timing Considerations . . . . .	7-3
Data Length Considerations . . . . .	7-6

**Index**

---

## Figures

2-1. All IBASIC Screen . . . . .	2-4
2-2. IBASIC Status Screen . . . . .	2-6
6-1. Device Connection (NOR Type) . . . . .	6-4
6-2. Device Connection (NAND Type) . . . . .	6-5
6-3. Device Connection . . . . .	6-20
6-4. Device Connection . . . . .	6-22

---

## Tables

1-1. Branch and Repeat Keywords of IBASIC . . . . .	1-21
1-2. Corresponding HP 4145 ASP and HP 4155A/4156A Keywords . . . . .	1-48
2-1. Available I/O Interfaces and Select Code . . . . .	2-27
4-1. :PAGE Subsystem Commands for Measurement Setup . . . . .	4-9
4-2. Corresponding HP 4145 ASP and HP 4155A/56A SCPI Commands . . . . .	4-51
6-1. Selector's State in Each Phase . . . . .	6-4
6-2. Selector's State in Each Phase . . . . .	6-5

---

1

---

Using HP Instrument  
BASIC

---

## Using HP Instrument BASIC

HP Instrument BASIC (IBASIC) is a system controller built into your HP 4155A/4156A. By using IBASIC, you can run a program to control the HP 4155A/4156A and other instruments (connected via interfaces of HP 4155A/4156A) without using an external computer.

IBASIC is a subset of HP BASIC. Programs created by IBASIC can run on an HP BASIC controller with little or no modification.

This chapter consists of the following ten sections.

The following six sections provide step-by-step instructions to operate IBASIC by using examples. You can learn the basics of IBASIC programming and operations. If you are not familiar with IBASIC, we recommend to read through these sections first.

- Before Operating IBASIC
- Creating and Executing a Simple IBASIC Program
- Modifying Program by using Editor Functions
- Saving and Getting a Program
- Summary of Softkeys and Keyboard Operations for Editor
- Other Basic Features of IBASIC

The following three sections are a task oriented reference for IBASIC. You can quickly find the desired IBASIC task.

- IBASIC Basic Operation Tasks
- IBASIC Editor Tasks
- Control from External Computer

The following section introduces how to easily create a program by using the typing aid softkeys in the IBASIC editor. This method of creating a program is similar to using the ASP environment on the HP 4145A/B semiconductor parameter analyzer.

- Creating ASP-like IBASIC Programs

---

## Before Operating IBASIC

HP 4155A/4156A provides the following three screen modes for operating IBASIC.

- |                            |                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |
|----------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| “All IBASIC”<br>screen     | Entire screen including softkeys is used for IBASIC, so no instrument page is displayed.<br><br>You can execute programs, but no instrument page appears in this mode.                                                                                                                                                                                                                                                                                             |
| “IBASIC Status”<br>screen  | Softkeys and bottom two lines are used for IBASIC. Rest of screen is for instrument page.<br><br>In this mode, you can start the IBASIC editor. The displayed softkeys are for IBASIC operation. You can execute IBASIC commands interactively. Characters you type are displayed at the bottom of the screen.                                                                                                                                                     |
| “All Instrument”<br>screen | . This is regular instrument screen and the default display mode at power on. Entire screen is for instrument page, and all softkeys are for interactive use of instrument. In this mode, you <i>cannot</i> use the IBASIC editor. Only the front-panel keys of IBASIC key group and <b>Ctrl</b> + <b>U</b> (Run) and <b>Ctrl</b> + <b>P</b> (Pause) on external keyboard are available to execute or pause program for HP Instrument BASIC from this screen mode. |

For details about HP Instrument BASIC screens, refer to “IBASIC Screen” in Chapter 2.

Using HP Instrument BASIC  
**Before Operating IBASIC**

---

## To Switch Screen Mode

To switch the screen mode, repeat the following operation until the desired screen is displayed.


Front Panel

1. Press **Display** of IBASIC key group.

External Keyboard

1. Press **Ctrl** + **G**.

This operation toggles screen display as follows:

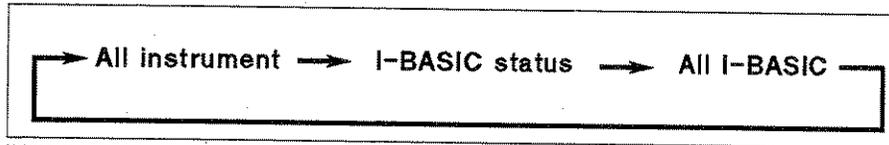

PG02003 12/00

---

## To Use the Help Function

By using the built-in help function of the HP 4155A/4156A, you can easily get information (name, syntax, and description) about programming commands, and can enter the desired command into the program without typing.

To start the help function for the programming commands, press **Help** key while you are in the IBASIC editor.

In the help function, the programming commands are divided into the following three categories, which you can access by secondary softkeys.

Softkey	Category
<b>IBASIC</b>	IBASIC commands.
<b>PAGE IMAGE COMMAND</b>	SCPI commands specific for HP 4155A/4156A. These are the help commands associated with the instrument setup pages that begin with <b>:PAGE</b> .
<b>SCPI COMMAND</b>	Standard SCPI commands.

The upper part of the help screen displays a list of the command names. The lower part displays a description of the selected (by field pointer) command.

Using HP Instrument BASIC

### Before Operating IBASIC

#### To Move the Field Pointer.

To move the field pointer, refer to the following table:

Rotary knob or Arrow keys	Basically, you move the field pointer by using the rotary knob or arrow keys.
PAGE CONTROL keys	Field pointer moves to first PAGE IMAGE command that is associated with the pressed key. PAGE CONTROL keys are <b>Chan</b> , <b>Meas</b> , <b>Display</b> , <b>Graph/List</b> , <b>Stress</b> , and <b>System</b> .
MEASUREMENT keys <b>Get</b> , <b>Save</b>	Field pointer moves to the PAGE IMAGE command that is associated with the pressed key. MEASUREMENT keys are <b>Single</b> , <b>Repeat</b> , and <b>Append</b> . Field pointer moves to the associated SCPI command.
Alphabetical keys	Field pointer moves to next command that has a keyword that begins with same letter as the pressed key.  If you are in the PAGE IMAGE command category, search is only within the instrument <i>page group</i> of the currently selected command.

#### To Search for a Command.

To search for a command:

1. Press **SEARCH** secondary softkey.
2. Type in command string that you want to search for, then press **Enter**

#### To Enter a Command into the Editor.

The command specified by the field pointer is displayed on the entry line. If you press **Enter**, the command is entered into the editor.

If command specified by the field pointer is a PAGE IMAGE or SCPI command, first select the **OUTPUT @Hp415x** secondary softkey. The entry line becomes **OUTPUT @Hp415x;"command"**, where *command* is command specified by field pointer. Then, press **Enter**.

**OUTPUT @Hp415x;"command"** is entered into the editor.

---

## Creating and Executing a Simple IBASIC Program

In this section, let's try to create and execute a simple program.

Before creating a program in the IBASIC editor, first change the screen display mode to IBASIC Status screen mode or All IBASIC screen mode by pressing IBASIC **Display** key as described in "To Switch Screen Mode". In following sections, the All IBASIC screen display mode is used.

---

### Step 1. Editing

Select **EDIT** secondary softkey or type EDIT, then press **Enter**.

10 \_

**To start the editor at a specific program line or label**

Type **EDIT *linenum*** or **EDIT *label***.

For example, if you type **EDIT 30**, the cursor appears at line 30. If you do not specify a line number or label, the cursor will appear at line 10.

The following program prints the numbers from 1 to 10. Type as follows:

```
10 FOR I=1 TO 10
20 PRINT I
30 NEXT I
40 END
```

Using HP Instrument BASIC

### Creating and Executing a Simple IBASIC Program

#### Always Insert Mode

Editor is always in insert mode, and *cannot* be changed to overwrite mode. If you mistyped, use **Backspace** to move back a character, or move cursor using arrow key **←**, then use **Delete** to delete a character. Then type correct characters.

#### Program End

In IBASIC, **END** must be at end of main program. In above example, line 40 is the last line of the program.

---

## Step 2. Exiting from Editor

Select **End edit** primary softkey to exit from the editor.

---

## Step 3. Executing Program

To execute the program, press **Run** of the IBASIC key group, select **RUN** primary softkey, or type RUN and press **Enter**. The following should be displayed on the screen:

```
1
2
:
9
10
```

**If an error message appears**

If an error message appears, you probably mistyped. The error message indicates the line number where the error occurs. You need to modify the line.

---

## Modifying Program by using Editor Functions

In this section, you can learn the following editor functions:

1. Inserting lines
2. Deleting a line
3. Renumbering
4. Inserting characters
5. Recalling deleted line
6. Indenting
7. Changing line numbers

---

## Step 1. Inserting Lines

Type EDIT 20, then press **Enter**. Cursor appears at line 20.

```
10  FOR I=1 TO 10
20  PRINT I
30  NEXT I
40  END
```

Select **Insert line** or press **Insert** to insert a line above line 20.

```
10  FOR I=1 TO 10
11
20  PRINT I
30  NEXT I
40  END
```

Type as follows:

```
10  FOR I=1 TO 10
11  PRINT I^2
12
20  PRINT I
30  NEXT I
40  END
```

$I^2$  means the second power of I. The above program increments I from 1 to 10, and displays second power of I and I for each step.

Select **End edit** to exit editor, then press **Run** to execute the program. The following is displayed:

```
1
1
4
2
9
3
:
81
9
100
10
```

Using HP Instrument BASIC

### Modifying Program by using Editor Functions

---

## Step 2. Deleting a Line

Type EDIT 20 to start editor at line 20.

```
10 FOR I=1 TO 10
11 PRINT I^2
20 PRINT I
30 NEXT I
40 END
```

Then, select **Delete line** or press **(Shift)+(Delete)** to delete line 20. The result is as follows:

```
10 FOR I=1 TO 10
11 PRINT I^2
30 NEXT I
40 END
```

The above program increments I from 1 to 10, and displays the second power of I at each step.

If you exit editor and execute the program, the following is displayed:

```
1
4
9
:
81
100
```

---

### Step 3. Renumbering

In above example, line numbers are not in equal increments. To change the line number increment to 10, select **Re-number** softkey. Line numbers will be changed as follows:

```
10  FOR I=1 TO 10
20  PRINT I^2
30  NEXT I
40  END
```

If you use the **Re-number** softkey, the renumbering is always as follows: first line is 10 and the increment is 10.

If you desire other numbering, you need to exit the editor, and use the **REN** command. For example, if you want first line number to be 100 and increment to be 20, type as follows:

```
REN 100, 20 Enter
```

Using HP Instrument BASIC

### Modifying Program by using Editor Functions

---

## Step 4. Inserting Characters

Type EDIT 20, then press **Enter**.

```
10 FOR I=1 TO 10
20 PRINT I^2
30 NEXT I
40 END
```

Move the cursor by using **▶** key.

```
10 FOR I=1 TO 10
20 PRINT I^2
30 NEXT I
40 END
```

Then type I, as follows:

```
10 FOR I=1 TO 10
20 PRINT I, I^2
30 NEXT I
40 END
```

Above program increments I from 1 to 10, and displays I and the second power of I on one line at each step. Exit editor, then execute the program. The following is displayed:

```
1          1
2          4
3          9
.          .
.          .
9          81
10         100
```

Using HP Instrument BASIC  
Modifying Program by using Editor Functions

---

## Step 5. Recalling Deleted Line

To restore the most recently deleted line, press **Recall** front-panel key.

---

## Step 6. Indenting

Move to desired line, then select **Indent** to indent the line. Indenting makes the program flow easier to understand.

```
10  FOR I=1 TO 10
20      PRINT I,I^2
30  NEXT I
40  END
```

---

## Saving and Getting a Program

The created program can be saved to a diskette. So, you can get the saved program from the diskette, then execute it.

In this section, you can learn the following file operation tasks:

1. Saving a Program
2. Listing Contents of Diskette
3. Clearing a Program
4. Getting a Program

---

## Step 1. Saving a Program

Insert a diskette into the built-in drive. Then, type SAVE "*filename*", then press **Enter**. For this example, we will type SAVE "PROG1".

---

## Step 2. Listing Contents of Diskette

Type CAT to list contents of the diskette.

If you are using an MS-DOS format diskette, the display is similar to the following example:

```
DIRECTORY : \:INTERNAL,4
LABEL: HP4156
FORMAT: DOS
AVAILABLE SPACE :      5692
      FILE      NUM  REC      MODIFIED
FILE NAME      TYPE  RECS  LEN  DATE  TIME PERMISSION
=====
PROG1          DOS      65    1 27-Jun-94 14:30 RW-RW-RW-
```

### Filer

You can also check the contents of the diskette by using the filer (SYSTEM: FILER page) of the HP 4155A/4156A. But you *cannot* save and get the IBASIC programs by using the filer.

Using HP Instrument BASIC  
**Saving and Getting a Program**

---

### Step 3. Clearing a Program

To clear the program, enter the editor, then select **Scratch** softkey. Then, select **Yes** secondary softkey.

Existing program will be cleared, and following is displayed:

```
10 COM @Hp415x
20 ASSIGN @Hp415x TO 800
30 !
9990 END
```

COM @Hp415x and ASSIGN @Hp415x TO 800 are used to control the HP 4155A/4156A. For details, please refer to "Step 1. Getting the Setup File and Making a Measurement" in Chapter 3, and refer to "Subprograms and COM Blocks".

---

### Step 4. Getting a Program

Type GET "PROG1", then press **Enter**. When the LED turns off, enter the editor if you want to display the program.

---

## Summary of Softkeys and Keyboard Operations for Editor

### Front-panel keys

Arrow keys (←, →, ↑, ↓)	Move the cursor
<b>Delete</b>	Delete character
<b>Recall</b>	Recall most recently deleted line

### External Keyboard

<b>Esc</b>	Exit editor
<b>F1</b> to <b>F8</b>	Primary softkeys
<b>Shift</b> + <b>F1</b> to <b>F7</b>	Secondary softkeys
<b>F9</b>	Toggle screen mode
<b>F11</b>	Clear to end
<b>Insert</b>	Insert line
<b>Delete</b>	Delete character at cursor
<b>Shift</b> + <b>Delete</b>	Delete line
<b>Home</b>	Beginning of line
<b>End</b>	End of line
<b>Page Up</b> or <b>Page Down</b>	Scroll pages

### Primary Softkeys

<b>Back space</b>	Delete character before cursor
<b>Insert line</b>	Insert line
<b>Delete line</b>	Delete line
<b>Re-number</b>	Renumber the lines
<b>Indent</b>	Indent the line
<b>Scratch</b>	Clear program
<b>End edit</b>	Exit editor

---

## Other Basic Features of IBASIC

This section describes the following:

- Branching/Repeating
- Subprograms and COM Blocks

---

## Branching/Repeating

Table 1-1. Branch and Repeat Keywords of IBASIC

IBASIC Keyword	Function
FOR, NEXT	Repeat specified number of times.
IF THEN, ELSE, END IF	Branch.
WHILE, END WHILE	Repeat until specified condition is <i>false</i> .
REPEAT, UNTIL	Repeat until specified condition is <i>true</i> .

Following program tests 1000 devices, and judges them pass or fail.

```

1  COM Data(1:1000)
2  DIM Id(1:1000)
10 EXECUTE ("GETSETUP 'SAMPL.MES'")
20 FOR I=1 TO 1000
30   EXECUTE ("SINGLE")
40   EXECUTE ("READDATAVAR 'Id'")
50   IF Id(I)<1E-6 THEN
60     PRINT "FAIL LOWER"
70     Data(I)=1
80   ELSE
90     IF Id(I)>1E-4 THEN
100      PRINT "FAIL HIGHER"
110      Data(I)=2
120     ELSE
130      PRINT "PASS"
140      Data(I)=0
150     END IF
160   END IF
170 NEXT I
180 CALL Save_data
190 END
200 !
210 SUB Save_data
220 COM Data(*)
230 CREATE "data_file",1
240 ASSIGN @File TO "data_file";FORMAT ON
250 OUTPUT @File;Data(*)
260 ASSIGN @File TO *
270 SUBEND

```

Using HP Instrument BASIC

### Other Basic Features of IBASIC

---

## Subprograms and COM Blocks

One of the most powerful constructs available is the subprogram. A subprogram has its own "context" or state that is distinct from the main program and all other subprograms. There are several benefits of subprograms.

- The subprogram allows you to take advantage of the "top-down design" method of programming.
- You can remove all subtasks from the overall logic flow of the main program.
- You can debug the program by testing each subprogram independently.
- The subprograms can be used to reduce the overall size of the program.
- Libraries of commonly used subprograms can be assembled for widespread use.

Refer to the example program in the previous section. Line 180 calls a subprogram to store data into a DOS file.

```

:
160   END IF
170 NEXT I
180 CALL Save_data
190 END
200 !
210 SUB Save_data
220 COM Data(*)
230 CREATE "data_file",1
240 ASSIGN @File TO "data_file";FORMAT ON
250 OUTPUT @File;Data(*)
260 ASSIGN @File TO *
270 SUBEND
```

## **COM Blocks.**

COM blocks are used by the subprogram to communicate with the main program or with other subprograms.

If you create subprograms and want to use common variables between main program and subprograms, you should use COM blocks.

Refer to the above example.

In the main program, line 1 declares that the `Data` array will be a COM array. Then, the main program assigns values to this array. Line 220 specifies that the subprogram `Save_data` will also use the `Data` array. So, `Data` array of main program can be operated on in the `Save_data` subprogram.

---

## IBASIC Basic Operation Tasks

This section describes the following basic operations to use HP Instrument BASIC.

- Executing HP Instrument BASIC commands
- Executing program
- Listing files
- Retrieving program
- Saving program

---

## To Execute HP Instrument BASIC Commands

1. Confirm your HP 4155A/4156A is in the following status:
  - a program is not executing.
  - another command is not executing.
  - Editor is not running.
  - the screen is "All IBASIC" screen or "IBASIC Status" screen. For "All Instrument" screen, **Run** and **Pause** front-panel keys and **Ctrl+U** (Run) and **Ctrl+P** (Pause) on external keyboard are available.
2. Type in commands by using front-panel keys in the ENTRY key group or external keyboard.
3. Press **Enter** front-panel key or **Enter** key on external keyboard.

---

## To Execute Program

Front Panel

1. Press **Run** front-panel key in the IBASIC key group.

External Keyboard

1. Press **Ctrl+U** on external keyboard.

Using HP Instrument BASIC  
**IBASIC Basic Operation Tasks**

---

## To List Files

1. Confirm your HP 4155A/4156A is in the following status:
  - the screen is "All IBASIC" screen.
  - a program is not executing.
  - another command is not executing.
  - Editor is not running.
2. Insert a 3.5 inch diskette (that contains the files you want to list) into the built-in diskette drive.
3. Select **CAT** secondary softkey, then press **Enter** front-panel key.

The file names on diskette are listed on the screen.

---

## To Retrieve Program

1. Confirm your HP 4155A/4156A is in the following status:
  - the screen is "All IBASIC" screen or "IBASIC Status" screen.
  - a program is not executing.
  - another command is not executing.
  - Editor is not running.
2. Insert the 3.5 inch diskette (that contains the program you want to retrieve) into the built-in diskette drive.
3. Select **GET ""** secondary softkey.
4. Type in file name to be retrieved. Typed name is inserted after first " .
5. Press **Enter** front-panel key, or **Enter** key on external keyboard.

### **External disk drive**

An external disk drive cannot be connected to HP 4155A/4156A. For using a disk drive connected to external controller, see "Control from External Computer".

Using HP Instrument BASIC  
**IBASIC Basic Operation Tasks**

---

## To Save Program

1. Confirm your HP 4155A/4156A is in the following status:
  - the screen is "All IBASIC" screen or "IBASIC Status" screen.
  - a program is not executing.
  - another command is not executing.
  - Editor is not running.
2. Insert a 3.5 inch diskette into the built-in diskette drive.
3. Select **SAVE** "" secondary softkey.
4. Type in name of file to which you want to save program.

If the file already exists on the diskette, **SAVE** cannot be used. If you want to overwrite an existing file, select **RE-SAVE** secondary softkey instead of **SAVE** secondary softkey in the previous step.

5. Press **Enter** front-panel key or **Enter** key on the external keyboard.

### External disk drive

An external disk drive cannot be connected to HP 4155A/4156A. For using a disk drive connected to external controller, see "Control from External Computer".

---

## IBASIC Editor Tasks

This section describes the following tasks to use built-in editor of HP Instrument BASIC.

- Starting the editor
- Quitting the editor
- Moving the cursor
- Inserting characters
- Deleting character
- Inserting line
- Deleting line
- Scrolling pages
- Recalling most recently deleted line

Using HP Instrument BASIC

## IBASIC Editor Tasks

---

### To Start the Editor

1. Confirm the screen is "All IBASIC" screen or "IBASIC Status" screen.
2. Select **EDIT** secondary softkey.
3. Press **Enter** front-panel key or **Enter** key on the external keyboard.

If you want to start the editor to edit a specific program line, type in the line number or label of the program line, then press **Enter** front-panel key. The editor starts, and cursor is displayed on specified line.

4. If a program is loaded into the HP 4155A/4156A, the program is displayed.  
If no program is loaded, 10 is automatically displayed and rest of screen is empty.

If you start the editor from the "IBASIC Status" screen, the screen switches to "All IBASIC" screen, and the editor starts.

---

### To Quit the Editor




1. Select **End edit** primary softkey.

If you started the editor from the "IBASIC Status" screen, the screen returns from "All IBASIC" screen to the "IBASIC Status" screen after you quit the editor.

---

## To Move the Cursor

To move the cursor, use the following keys.

Direction	Front-panel	Keyboard
Up	 of MARKER/CURSORS group Rotate rotary knob counter-clockwise	
Down	 of MARKER/CURSORS group Rotate rotary knob clockwise	
Right	 of ENTRY group  of MARKER/CURSORS group	 
Left	 of ENTRY group  of MARKER/CURSORS group	 
Beginning of Line	 +  of MARKER/CURSORS group	 
End of Line	 +  of MARKER/CURSORS group	 

---

## To Insert Characters

1. Move the cursor to character you want to insert before.
  2. Characters you type will be automatically inserted.
  3. After you insert characters, you must select the  key to enter the line with inserted characters into the program.
- Editor is always in insert mode, and cannot be changed to overwrite mode.

Using HP Instrument BASIC

### IBASIC Editor Tasks

## To Delete Character

1. Move the cursor to character you want to delete.
2. Press key according to the following table:

Front-panel	Keyboard
<b>Delete</b> of ENTRY group	<b>Delete</b>

3. After you delete characters, you must select the **Enter** key to enter the line with deleted characters into the program.

## To Insert Line

1. Move the cursor to the line that you want to insert a new line before.
2. Press key or softkey according to following table:

Front-panel	Keyboard
<b>Insert line</b> primary softkey	<b>(Shift) + (Insert)</b>
	<b>(Alt) + (I)</b>

3. After you type in a new line, you must select the **Enter** key to enter the new line into the program.

---

## To Delete Line

1. Move the cursor to line you want to delete.
2. Press key or softkey according to the following table:

Front-panel	Keyboard
Delete line primary softkey	Shift + Delete Alt + D

---

## To Scroll Pages

To scroll the editor by one-half screen, use the following keys:

Direction	Front-panel	Keyboard
Up	n.a.	Page Up
Down	n.a.	Page Down

Using HP Instrument BASIC  
**IBASIC Editor Tasks**

---

## To Recall Most Recently Deleted Line

To display the line most recently deleted line, use the following keys.

Front-panel	Keyboard
<b>Recall</b>	<b>Shift + Page Up</b>

If you want to enter the line into the program, you must select the **Enter** key.

---

## Control from External Computer

This section describes how to control the HP 4155A/4156A from a program that is running on an external computer:

- Downloading a program to HP 4155A/4156A.
- Uploading a program from HP 4155A/4156A.
- Controlling execution of a HP 4155A/4156A program.

Before executing a program on external computer to control HP 4155A/4156A, do as follows:

1. Set the "HP 4155A/4156A is" field on the SYSTEM: MISCELLANEOUS page to NOT SYSTEM CONTROLLER.
2. Connect an HP-IB cable from the external computer to the HP-IB connector on rear panel of HP 4155A/4156A.

Using HP Instrument BASIC

### Control from External Computer

---

## To Download a Program to HP 4155A/4156A

To download a program from the external computer to HP 4155A/4156A, you need to use the :PROG:SELected]:DEFine command.

#### Example

The following is an example of an HP BASIC program (running on external computer) that reads an HP Instrument BASIC program file (from a disk drive connected to external computer) and downloads it to HP 4156A.

```

10  OPTION BASE 1
20  !
30  DIM Line$[1024]
40  !
50  ASSIGN @Hp4156 TO 717
60  !
70  OUTPUT @Hp4156;"PROG:DEL:ALL" ! Clears program in HP 4156A
80  File_name$="prog"
90  ASSIGN @File TO File_name$ ! Opens file and assigns data path
100 OUTPUT @Hp4156;"PROG:DEF #0" ! Sends header to 4156A
110 ON ERROR GOTO Done
120 LOOP
130   Line$=""
140   ENTER @File;Line$ ! Reads one program line
150   OUTPUT @Hp4156;Line$ ! Downloads line to HP 4156A
160 END LOOP
170 Done: !
180 OFF ERROR
190 OUTPUT @Hp4156;Line$
200 OUTPUT @Hp4156;" " END
210 ASSIGN @File TO *
220 END

```

Using HP Instrument BASIC  
**Control from External Computer**

<b>Line Number</b>	<b>Description</b>
50	assigns I/O path to control HP 4155A/4156A.
70	deletes existing HP Instrument BASIC program in HP 4155A/4156A.
80	name of file (in disk drive of external computer) that contains desired HP Instrument BASIC program
90	opens file and assigns data path
100	#0 indicates that an indefinite length of parameters (program lines) will be downloaded
110 to 180	reads program lines from the file and downloads them until EOF.
210	closes file.

Using HP Instrument BASIC  
**Control from External Computer**

---

## To Upload a Program from HP 4155A/4156A

To upload a program from the HP 4155A/4156A to external computer, you need to use the :PROG:am[:SElected]:DEFine? command.

Example

The following is an example of an HP BASIC program (running on external computer) that uploads an HP Instrument BASIC program from HP 4156A and stores the program on a disk drive that is connected to external computer.

```

10  OPTION BASE 1
20  !
30  DIM Num_dig$(2)
40  INTEGER Byte
50  !
60  ASSIGN @Hp4156 TO 717
70  !
80  OUTPUT @Hp4156;":PROG:DEF?"
90  ENTER @Hp4156 USING "%,2A";Num_dig$
100 PRINT Num_dig$
110 !
120 Byte=VAL(Num_dig$(2))
130 !
140 ALLOCATE Data_byt$(Byte)
150 !
160 FOR I=1 TO Byte
170   ENTER @Hp4156 USING "#,A";Data_byt$(I;1) ! Enter length of program
180 NEXT I
190 !
200 D=VAL(Data_byt$)
210 PRINT D
220 ALLOCATE Prog$(D)
230 PRINTER IS CRT;WIDTH D
240 ENTER @Hp4156 USING "-K";Prog$           ! Enter the program into Prog$
250 PRINT Prog$
260 ENTER @Hp4156;B$
270 PRINT B$
280 !
290 CREATE "prog",1
300 ASSIGN @File TO "prog";FORMAT ON
310 OUTPUT @File;Prog$
320 ASSIGN @File TO *
330 !
340 END

```

Using HP Instrument BASIC  
Control from External Computer

Line Number	Description
60	Assigns I/O path to control HP 4155A/4156A.
80	Sends :PROGm[:SElect]:DEFine? query command.
90	Reads first two characters of response. These two bytes indicate how many bytes are used to specify length of program.
160 to 180	Reads the bytes that specify length of program.
200	Calculates length of program.
220	Allocates string variables for program.
240	Reads program.
280	Reads terminator.
290	Creates file "prog"
300	Assigns I/O path to "prog"
310	Stores program into "prog" file.
320	Closes file.

Using HP Instrument BASIC  
**Control from External Computer**

---

## To Control State of HP 4155A/4156A Program

:PROGrama[:SElected].STATE command from external computer can control HP Instrument BASIC program in the HP 4155A/4156A as follows:

Example

- To run the program:  
    OUTPUT @Hp4155;":PROGrama[:SElected]:STATE RUN"
- To continue the program:  
    OUTPUT @Hp4155;":PROGrama[:SElected]:STATE CONT"
- To stop the program:  
    OUTPUT @Hp4155;":PROGrama[:SElected]:STATE STOP"
- To pause the program:  
    OUTPUT @Hp4155;":PROGrama[:SElected]:STATE PAUSE"

---

## Creating ASP-like IBASIC Programs

In the IBASIC editor of the HP 4155A/4156A, there are several typing aid softkeys that allow you to easily create a program.

When you press the softkey, the corresponding IBASIC command is entered into the program, so you do not have to type it, but you may need to type in some parameters.

For HP 4145A/B users, this environment is very familiar because it is similar to the Auto Sequence Program (ASP) programming environment of the HP 4145A/B. For most of the HP 4145 ASP commands, the IBASIC editor has a softkey to enter a corresponding IBASIC command.

These programs can run in IBASIC *only*, not on an external computer.

---

### Step 1. Creating Programs by using the Typing Aid Softkeys

In the IBASIC editor, you can easily create programs that perform the same operations as a desired HP 4145 ASP program by using the typing aid softkeys. These are secondary softkeys. To display more softkeys, select **More** softkey.

For the ASP program shown below, let's create the corresponding IBASIC program:

! ASP Program:	Corresponding IBASIC Program:
!	
1 GET P ICBVBE	10 EXECUTE ("GETSETUP 'ICBVBE.PRO'")
2 SINGLE	20 EXECUTE ("SINGLE")
3 SAVE D BV1	30 EXECUTE ("SAVEDATA 'BV1.DAT'")
	40 END

1. Select the **GET SETUP** secondary softkey. The following appears:

```
10 EXECUTE ("GETSETUP ")
```

Using HP Instrument BASIC

### Creating ASP-like IBASIC Programs

You need to specify a filename in this command.

At bottom of screen, **enter** `fileName[,msus]` is displayed, where `msus` means the mass storage unit specifier. You can specify `,DISK` or `,MEMORY`. Default is `,DISK`.

2. Type a setup file name.

```
10 EXECUTE ("GETSETUP 'ICVBE.PRO'")
```

File name must be in single quotations ( ' ' ). Then press **Enter**.

3. Select **SINGLE** secondary softkey.

```
10 EXECUTE ("GETSETUP 'ICVBE.PRO'")
20 EXECUTE ("SINGLE")
30
```

4. Select **SAVEDATA** secondary softkey.

```
10 EXECUTE ("GETSETUP 'ICVBE.PRO'")
20 EXECUTE ("SINGLE")
30 EXECUTE ("SAVEDATA ")
```

5. Specify file name to which you want to save the measurement setup and result data.

```
10 EXECUTE ("GETSETUP 'ICVBE.PRO'")
20 EXECUTE ("SINGLE")
30 EXECUTE ("SAVEDATA 'BV1.DAT'")
40 END
```

Finally, type **END** as above.

#### Setup File

In `EXECUTE ("GETSETUP ")`, you can specify a `.PRO` or `.MES` file:

- `.PRO` files are setup files created by the HP 4145B. The HP 4155A/4156A can read `.PRO` files.
- `.MES` files are setup files created by the HP 4155A/4156A.

In `EXECUTE ("SAVEDATA ")`, you specify a `.DAT` file, which is a file for storing the setup and measurement result data.

---

## Step 2. Executing the Program

To execute the program, exit editor, then press **Run**.

The HP 4155A/4156A gets the setup file from the diskette, performs measurement, then saves setup and results to specified file on the diskette. However, in All IBASIC mode, no graphics results are displayed. To display results graphically, the display mode must be All Instrument mode or IBASIC Status mode.

To execute the program and display the results graphically, change the display mode to All Instrument or IBASIC Status mode, then press **Run**.

---

## Step 3. Creating a Longer Program

In the program below, the left side is an ASP program example from the HP 4145B manual.

The right side shows a program that was created by using the typing aid softkeys to enter the ASP-like commands (of the HP 4155A/4156A) that correspond to the original ASP commands. These softkeys allow you to easily create a program that runs on the HP 4155A/4156A and performs the same operations as the original ASP program.

1	GET P ICBVBE	10	EXECUTE ("GETSETUP 'ICBVBE.PRO'")
2	SINGLE	20	EXECUTE ("SINGLE")
3	WAIT 3	30	WAIT 3
4	GET P HFE1	40	EXECUTE ("GETSETUP 'HFE1.PRO'")
5	SINGLE	50	EXECUTE ("SINGLE")
6	WAIT 3	60	WAIT 3
7	GET P VCESAT	70	EXECUTE ("GETSETUP 'VCESAT.PRO'")
8	SINGLE	80	EXECUTE ("SINGLE")
9	WAIT 3	90	WAIT 3
10	GET P COLR	100	EXECUTE ("GETSETUP 'COLR.PRO'")
11	SINGLE	110	EXECUTE ("SINGLE")
12	WAIT 3	120	WAIT 3
13	PAUSE	130	PAUSE
14	GET P NPN1	140	EXECUTE ("GETSETUP 'NPN1.PRO'")

Using HP Instrument BASIC

### Creating ASP-like IBASIC Programs

```
15 SINGLE
16 PAUSE
17 PLOT 100,100,7000,7000
18 GET P BV
19 SINGLE
20 PLOT 100,100,7000,7000
21 PAUSE
22 SINGLE
23 CPLOT 100,100,7000,7000
150 EXECUTE ("SINGLE")
160 PAUSE
170 EXECUTE ("PRINTPLOT")
180 EXECUTE ("GETSETUP 'BV.PRO'")
190 EXECUTE ("SINGLE")
200 EXECUTE ("PRINTPLOT")
210 PAUSE
220 EXECUTE ("SINGLE")
230 EXECUTE ("CURVEPLOT")
240 END
```

#### Print/Plot

EXECUTE ("PRINTPLOT") prints/plots the information of the present instrument page, not the IBASIC screen. If present page is GRAPH/LIST: GRAPHICS page, the graph is printed/plotted.

EXECUTE ("CURVEPLOT") changes to the GRAPH/LIST: GRAPHICS page, then prints/plots the graph.

You need to set the desired settings on the SYSTEM: PRINT/PLOT SETUP page before EXECUTE ("PRINTPLOT") and EXECUTE ("CURVEPLOT") are performed.

---

## Programming Tips

This section describes features and tips of IBASIC programs in relation to ASP programs. Some examples use an example measurement setup file named "VTH.MES". Before executing these examples, you need to save setup data to a file named "VTH.MES" on the diskette. For an example setup, see "Example Application Setup for Vth Measurement" in Chapter 3.

### File Name Variables.

You can specify a string variable for the file name in `SAVEDATA` as follows:

```
Filename$="DATA1.DAT"
EXECUTE ("SAVEDATA Filename$")
```

This feature allows you to create a more simple program as follows.

Example ASP Program

Following ASP program gets a setup file, makes measurements, and saves results to following files: VTH1, VTH2, ... VTH10. Program is 21 lines.

```
1  GET P  VTH
2  SINGLE
3  SAVE D VTH1
4  SINGLE
5  SAVE D VTH2
6  SINGLE
7  SAVE D VTH3
  :
21 SAVE D VTH10
```

Corresponding IBASIC Program.

The following HP Instrument BASIC (IBASIC) program does the same operation as the above ASP program. The program is simplified by using a filename variable `Filename$` and the `FOR NEXT` keyword.

```
10  EXECUTE ("GETSETUP 'VTH.PRO'")
20  FOR I=1 TO 10
30      EXECUTE ("SINGLE")
40      Filename$="VTH"&VAL$(I)&".DAT"
50      EXECUTE ("SAVEDATA Filename$")
60  NEXT I
```

In line 40, the `Filename$` is defined. For example, `Filename$="VTH1.DAT"` when `I=1`. So, the 21-line ASP program can be converted to a 6-line IBASIC program.

Using HP Instrument BASIC  
Creating ASP-like IBASIC Programs

---

## Reading HP 4155/56 Data to IBASIC Variables

You can transfer read-out function values or data variable values (output data, measurement data, and user function values) from the HP 4155/56 to HP Instrument BASIC (IBASIC) variables.

### Transferring Multiple Data.

You can transfer multiple data (such as sweep measurement data) to an array variable of IBASIC by using EXECUTE ("READDATAVAR ") as follows:

```
EXECUTE ("READDATAVAR 'ID', Id_data")
```

The above example transfers the drain current data ID of a sweep measurement to the array variable previously defined as Id\_data.

Following example program gets VTH.MES setup file, performs measurement, then transfers ID data to an array. In this example, the array Id\_data is defined in line 10, and it has elements 1 to 51.

```
10 DIM Id_data(1:51)
20 EXECUTE ("GETSETUP 'VTH.MES'")
30 EXECUTE ("SINGLE")
40 EXECUTE ("READDATAVAR 'ID', Id_data")
50 FOR I=1 TO 51
60   PRINT "Id(";I;)"=";Id_data(I);"A"
70 NEXT I
80 END
```

Result with example measurement data is as follows:

```
Id( 1)= 0.00031 A
Id( 2)= 0.00282 A
Id( 3)= 0.00514 A
Id( 4)= 0.01017 A
  :
Id( 51)= 0.08274 A
```

### Transferring a Single Data.

In the following example, a single data is to transferred to a variable. For example, VTH is a single data point calculated by a user function that was defined by the user.

```
EXECUTE ("READDATAVAR 'VTH', Vthdata")
```

Using HP Instrument BASIC  
Creating ASP-like IBASIC Programs

In following example, EXECUTE ("READDATAVAR") is used to transfer the VTH value to the IBASIC variable Vthdata. And for example, VTH.MES is a setup file that includes auto analysis setup to extract a threshold voltage VTH.

```
10 EXECUTE ("GETSETUP 'VTH.MES'")
20 EXECUTE ("SINGLE")
30 EXECUTE ("READDATAVAR 'VTH',Vthdata")
40 PRINT "Vthdata =";Vthdata;"V"
50 END
```

Result will be for example:

```
Vthdata = 1.2345 V
```

You can also specify a read out function as the item to be transferred:

```
EXECUTE ("READDATAVAR '@MX',Vthdata")
```

@MX is the read out function that reads X-axis value of point where marker is located.

---

## Auto Scaling

Auto scaling can be done by using the following:

```
EXECUTE ("AUTOSCALE").
```

In the following example, the image dumps will be scaled for best fit to the printer or plotter even if the measurement results vary greatly.

```
10 EXECUTE ("GETSETUP 'VTH.MES'")
11 FOR I=1 TO 100
20   EXECUTE ("SINGLE")
30   EXECUTE ("AUTOSCALE")
40   EXECUTE ("PRINTPLOT")
41 NEXT I
50 END
```

Using HP Instrument BASIC  
**Creating ASP-like IBASIC Programs**

---

## HP 4145 ASP and HP 4155A/4156A Corresponding Keywords

Following shows HP 4145A/B's ASP keywords and corresponding HP 4155A/4156A keywords. In IBASIC editor, there are typing aid softkeys to help you quickly enter the related HP 4155A/4156A keyword, which must be used in the EXECUTE( ) directive:

**Table 1-2. Corresponding HP 4145 ASP and HP 4155A/4156A Keywords**

4145A/B	4155A/4156A	Function	Remark
GET P	GETSETUP	Gets setup .MES or .PRO file	
SINGLE	SINGLE	Initiates single measurement	
SAVE D	SAVEDATA	Saves data to .DAT file	
PLOT	PRINTPLOT	Prints/plots present instrument page.	
CPLLOT	CURVEPLOT	Prints/plots measurement graph.	
PRINT	PRINTPLOT	Prints/plots present instrument page.	
PAUSE			Use BASIC keyword PAUSE
WAIT			Use BASIC keyword WAIT
PAGE			Set in the Print/Plot setup
	STANDBY	Sets Standby status on or off	
	STRESS	Initiates stress force	
	AUTOSCALE	Scales dump for best fit.	
	READDATAVAR	Gets data variable from 4155A/56A	
	DEFUSERVAR	Defines user variable	

For WAIT and PAUSE of HP 4145's ASP, there are no related typing aid softkeys. You type in the IBASIC keywords (WAIT and PAUSE).

For more information about IBASIC Keywords, use help functions described in the next chapter or refer to the *HP Instrument BASIC Users Handbook*.

---

Reference:  
HP Instrument BASIC

---

## Reference: HP Instrument BASIC

This chapter provides following reference information for HP Instrument BASIC:

- IBASIC Screen
- Front-panel keys
- External Keyboard
- Softkeys for Operating IBASIC
- Softkeys for IBASIC Editor
- HP 4155A/4156A Specific IBASIC Commands
- Available I/O Resources
- ASP-like Commands


---

## IBASIC Screen

HP 4155A/4156A provides the following three screen modes for operating IBASIC.

- |                            |                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
|----------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| “All IBASIC”<br>screen     | Entire screen including softkeys is used for IBASIC, so no instrument page is displayed.<br><br>You can execute programs, but no instrument page appears in this mode.                                                                                                                                                                                                                                                                               |
| “IBASIC Status”<br>screen  | Softkeys and bottom two lines are used for IBASIC. Rest of screen is for instrument page.<br><br>In this mode, you can start the IBASIC editor. The displayed softkeys are for IBASIC operation. You can execute IBASIC commands interactively. Characters you type are displayed at the bottom of the screen.                                                                                                                                       |
| “All Instrument”<br>screen | .This is regular instrument screen and the default display mode at power on. Entire screen is for instrument page, and all softkeys are for interactive use of instrument. In this mode, you <i>cannot</i> use the IBASIC editor. Only the front-panel keys of IBASIC key group and <b>Ctrl</b> + <b>U</b> (Run) and <b>Ctrl</b> + <b>P</b> (Pause) on external keyboard are available to execute or pause program for IBASIC from this screen mode. |

**Display** front-panel key or **Ctrl**+**G** (or **F9**) on external keyboard are used to toggle the screen display mode as shown in the following figure:

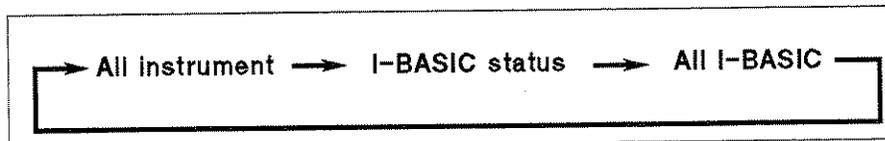


PG02003 12/02/00

Reference: HP Instrument BASIC  
**IBASIC Screen**

---

## All IBASIC Screen

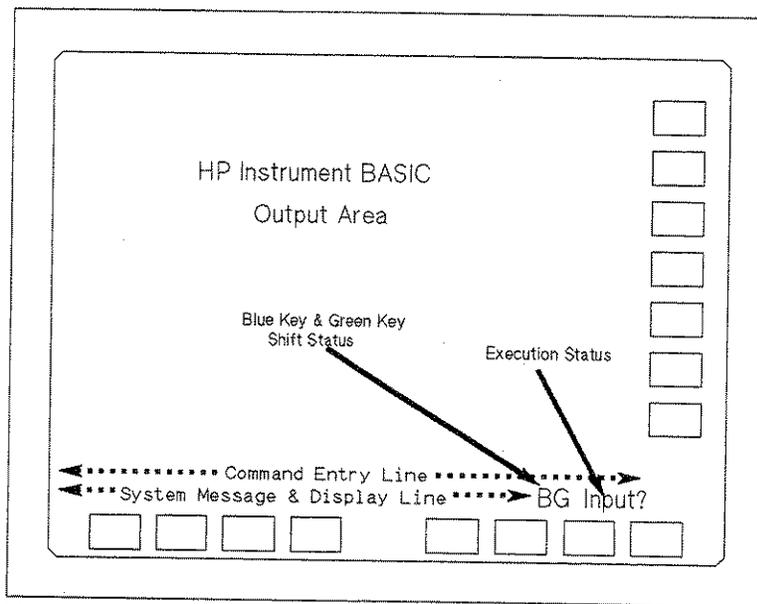

PG02001 120x80

**Figure 2-1. All IBASIC Screen**

For the "All IBASIC" screen, the entire screen including softkeys is used for IBASIC. The following describes each part of this screen:

IBASIC Output Area

CRT output commands of IBASIC (such as **PRINT** and **OUTPUT 1**;) display characters in this area. This area has 24 lines and 60 columns.

Command Entry Line

IBASIC command you type is displayed on this line. The length of this line is 60 characters.

System Message and Display Line

For displaying IBASIC error messages and other system messages, and **DISP** and **INPUT** commands of IBASIC.

Reference: HP Instrument BASIC

**IBASIC Screen****Blue Key & Green Key  
Shift Status**

This field displays the shift status of ENTRY front-panel keys. The shift status is controlled by using the blue and green front-panel keys:

The following statuses are displayed:

- Non-shift status: B, b, or G is not displayed. You can enter numeric values.
- Uppercase shift status: B is displayed, G is not displayed. You can enter uppercase alphabet characters.
- Lowercase shift status: b is displayed. G is not displayed. You can enter lowercase alphabet characters.
- Non-alphanumeric status: G is displayed. You can enter one non-alphanumeric character. So, you must press green key before entering each alphanumeric character.

Basically, you can change between these states as follows:

- To toggle between non-shift and shift status: press blue key,
- To toggle between uppercase and lowercase shift status: press green key, then blue key.
- To enter one non-alphanumeric character: press green key, then character.

**Execution Status**


This field displays the execution status of IBASIC:

<b>Idle</b>	IBASIC program is stopped. IBASIC commands can be executed.
<b>Run</b>	IBASIC program or command is being executed.
<b>Pause</b>	IBASIC program is paused.
<b>Input?</b>	IBASIC program is waiting for input from front-panel keys or external keyboard.
<b>Edit</b>	IBASIC editor is running.

Reference: HP Instrument BASIC  
**IBASIC Screen**

---

## IBASIC Status Screen

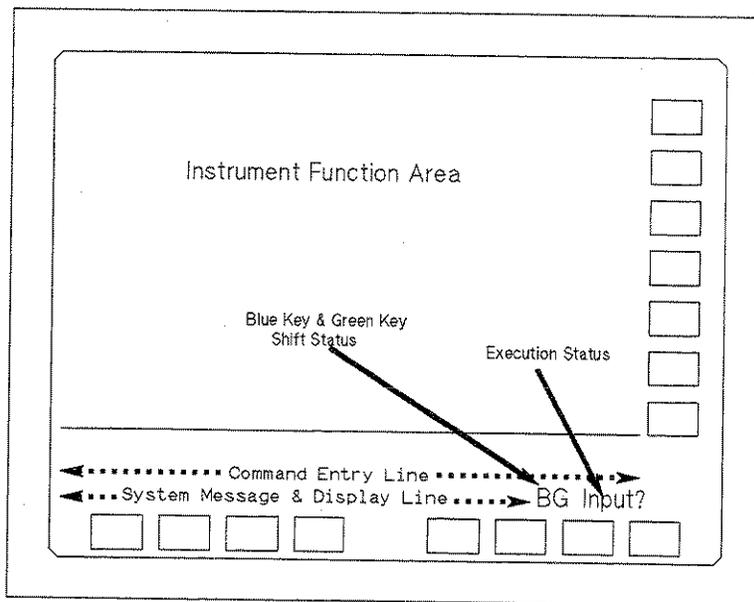

**Figure 2-2. IBASIC Status Screen**

For the "IBASIC Status" screen, the two bottom lines are used to display the status of IBASIC. These two lines are the same as in "All IBASIC" screen. Refer to "All IBASIC Screen". Also, the softkeys are for IBASIC.

The other part of the screen is the normal 4155A/4156A screen. This is useful if you want to view a graph of the measurement results while executing IBASIC program.

---

## Keys for IBASIC

This section provides information about the following keys for IBASIC:

- Front-panel Keys
- Primary Softkeys
- Secondary Softkeys
- External Keyboard Keys

Reference: HP Instrument BASIC

### Keys for IBASIC

---

## Front-panel Keys for IBASIC

- PAGE CONTROL key group
- In “IBASIC Status” screen:  
Changes to “All Instrument” screen and displays the specified page.
  - In “All IBASIC” screen:  
All front-panel keys in this group are *ignored*.
- MARKER/CURSOR key group
- In “IBASIC Status” screen:  
When you operate MARKER/CURSOR front-panel keys, the screen changes to “All Instrument” screen and function of operated key is executed.
  - In all IBASIC screen:
    - Rotary Knob
      - When the editor is running, the rotary knob moves the cursor vertically in the edit area.
      - When the editor is not running, the rotary knob scrolls the IBASIC output area.
    - 
      - When the editor is running, these keys move the cursor vertically.
      - When the editor is not running, these keys scroll the IBASIC output area.
    -  Moves the cursor horizontally on the IBASIC Editor or Command Entry line.
- If you hold down the **Fast** key, the arrow keys move the cursor faster.

Reference: HP Instrument BASIC  
**Keys for IBASIC**

MEASUREMENT key group • In "IBASIC Status" screen:

- Single**, **Repeat**, **Append** Changes the displayed page to GRAPH/LIST: GRAPHICS or GRAPH/LIST: LIST page and executes the measurement.
- Standby** Toggles the operation state of the standby channels between the standby state and the idle state.
- Stop** Stops the measurement or stress forcing.
- Stress** Changes the displayed page to the STRESS: STRESS FORCE page and starts to force stress.
- Short**, **Medium**, **Long** Changes the measurement integration time.


• In "All IBASIC" screen:

- Standby** Toggles the operation state of the standby channels between the standby state and the idle state.
  - Stop** Stops the measurement or stress forcing.
- Other front-panel keys in this group are ignored.

IBASIC key group

The following front-panel keys of IBASIC key group are available to control IBASIC in any display mode.

- Run** Executes IBASIC program that is loaded into internal memory of HP 4155A/4156A.
- Pause** Pauses program execution until CONT command is executed or **Continue** primary softkey is pressed. If the program is modified while paused, RUN command must be used to restart program execution.
- Display** Toggles the display mode in the following sequence.

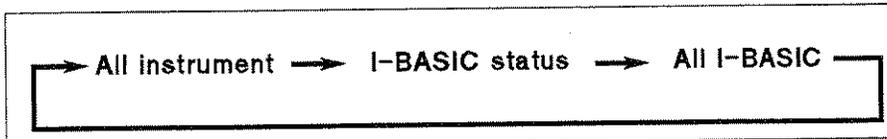

PG22003 12/92

Reference: HP Instrument BASIC

### Keys for IBASIC

#### ENTRY key group

**Recall ↓**

- When the editor is running, this key displays the last deleted line. To enter this displayed line as part of the program, press **Enter** front-panel key.
- When the editor is not running, this key cycles through the 10 commands that were most recently entered on the Command Entry line.

**Recall ↑**

- When the editor is running, this key is same as **Recall ↓**.
- When the editor is not running, this key is same as **Recall ↓**, but cycles through commands in opposite order.

**Save**, **Get**

These keys are ignored.

Other front-panel keys in ENTRY group are available to enter characters on the Command Entry line or Editor. For the usage of the blue and green front-panel keys to enter characters, see "All IBASIC Screen".

#### Other Keys

**Help**

Displays information about IBASIC. And can be used to select and enter SCPI and IBASIC commands into Editor or Command Entry line.

**Plot/Print**

If present screen is "All IBASIC", dumps "All IBASIC" screen image to the printer or plotter.

If present screen is "IBASIC Status", prints/plots instrument part of screen.

Reference: HP Instrument BASIC

**Keys for IBASIC**

---

## Primary Softkeys in Idle, Pause, Run, or Input? execution status

This section describes the primary softkeys that are displayed during the Idle, Pause, Run, or Input? execution status.

Refer to "Primary Softkeys in Edit execution status" for primary softkeys that are displayed when the editor is running.

**Step**

1. Executes the paused program line of paused program or the first program line of stopped (idle) program.
2. Displays next program line on system message line of the screen.
3. Pauses program again.

**Conti-  
nue**

Starts execution of paused program from paused program line.

**RUN**

Starts program execution immediately from first program line.

**Pause**

Pauses program execution immediately. And displays line at which execution was paused.

**Stop**

Stops program execution after current line executes.

**Clear  
I/O**

Stops I/O operation of program.

**Reset**

Stops program execution immediately.

Reference: HP Instrument BASIC

### Keys for IBASIC


---

## Secondary Softkeys in Idle or Pause execution status

This section describes the secondary softkeys that are displayed during the Idle or Pause execution status

For the secondary softkeys that are displayed during the Run or Input? status, refer to "Secondary Softkeys in Run or Input? execution status".

For the secondary softkeys that are displayed when the editor is running, refer to "Secondary Softkeys in Edit execution status"



CAT

Clears the Command Entry line, and types in CAT .

To list file names on the disk, press **Enter**.



SAVE ""


1. Clears the Command Entry line.

2. Types in SAVE " " .

3. Positions the cursor after first " .

To save program to diskette, type name of file to which you want to save program, then press **Enter**.

If file already exists on diskette, program will not be saved.



RE-SAVE ""

1. Clears the Command Entry line.

2. Types in RE-SAVE " " .

3. Positions the cursor after first " .

To save program to diskette, type name of file to which you want to save program, then press **Enter**.

If file already exists on diskette, file will be overwritten, so previous data in file is lost.

Reference: HP Instrument BASIC  
**Keys for IBASIC**

**GET** " " "

1. Clears the Command Entry line.
2. Types in GET " " " .
3. Positions the cursor after first " .

To get a program from diskette, type name of file to get, then press **Enter**.

**PURGE** " "

1. Clears the Command Entry line.
2. Types in PURGE " " .
3. Positions the cursor after first " .

To delete a file from diskette, type in the file name to be deleted, then press **Enter**.

**EDIT**

Clears the Command Entry line and types in EDIT. To start the editor, press **Enter** front-panel key.

**REN**  
umber

Clears the Command Entry line and types in REN.

To re-number lines of a program, type in appropriate parameters, then press **Enter**. For more details about REN command, refer to the *HP Instrument BASIC User's Handbook*.

---

## Secondary Softkeys in Run or Input? execution status

When the execution status is Run or Input?, user-defined softkeys, which are defined by using ON KEY command in the program, are displayed in the secondary softkey area.

Reference: HP Instrument BASIC

### Keys for IBASIC

---

## Primary Softkeys in Edit execution status

This section describes the primary softkeys that are displayed when the IBASIC editor is running (Edit execution status is displayed).

**Back  
space**

Deletes the character before the cursor.

**Insert  
line**

Inserts a line between the cursor line and the previous line.

**Delete  
line**

Deletes the cursor line.

**Re-  
number**

Changes the program line numbers so that first line is 10 and line number increment is 10.

**Indent**

Indents so that all program lines begin at the same position.

**Scratch**

Clears the program and all variables not in COM. Before clearing, **YES** and **NO** secondary softkeys are displayed for confirmation.

**End  
edit**

Exits the editor.

---

## Secondary Softkeys in Edit execution status

This section describes the secondary softkeys that are displayed when the IBASIC editor is running (Edit execution status is displayed).

These softkeys help you enter program commands. For commands that require you to type in some parameters, these softkeys display the command. You must enter the parameters, then you must press **(Enter)** key to enter the command into the program. For commands that do not have parameters, the commands are entered directly into the program. Commands are entered at the cursor line.

For the EXECUTE command, refer to "EXECUTE" for details.

For secondary softkeys that are displayed during Idle or Pause execution status, refer to "Secondary Softkeys in Idle or Pause execution status".

For secondary softkeys that are displayed during Run or Input? execution status, refer to "Secondary Softkeys in Run or Input? execution status".

In Edit execution status, there are three pages of secondary softkeys. To move to next page, press **MORE** secondary softkey.

**GET  
SETUP**

1. Displays the following program line for loading a setup file:

```
EXECUTE("GETSETUP ")
```

2. Positions cursor at second double quotes. You enter the file name to be loaded, then select **(Enter)** key.

**SINGLE**

Enters the following program line for triggering a single measurement:

```
EXECUTE("SINGLE")
```

**STANDBY**

1. Displays the following program line for changing the operation state of the standby channels:

```
EXECUTE("STANDBY ")
```

2. Positions the cursor at the second double quote. You enter ON or OFF, then select **(Enter)** key.

Reference: HP Instrument BASIC

### Keys for IBASIC

#### STRESS

Enters the following program line for triggering stress force:

```
EXECUTE("STRESS")
```

#### AUTO SCALE

Enters the following program line for autoscaling:

```
EXECUTE("AUTOSCALE")
```

#### SAVE DATA

1. Displays the following program line for saving measurement data to a file:

```
EXECUTE("SAVEDATA ")
```

2. Positions the cursor at the second double quote. You enter file name to which you want to save measurement data, then select **Enter** key.

#### READ DATA VARIABLE

1. Displays the following program line for reading the values of an HP 4155A/4156A data variable, then storing the values into an IBASIC program variable:

```
EXECUTE("READDATAVAR ,")
```

2. Positions the cursor at the comma. You enter names of HP 4155A/4156A data variable and IBASIC program variable, then select **Enter** key.

#### DEFINE USER VARIABLE

1. Displays the following program line for defining a user variable:

```
EXECUTE("DEFUSERVAR , , ,")
```

2. Positions the cursor at the first comma. You enter the user variable name, number of data, name of IBASIC program variable that contains desired data, and user variable unit, then select **Enter** key.

#### PRINT/ PLOT

Enters following program line for printing/plotting the instrument window:

```
EXECUTE("PRINTPLOT")
```

#### CURVE PLOT

Enters following program line for printing/plotting a graphics plot of measurement results:

```
EXECUTE("CURVEPLOT")
```

Reference: HP Instrument BASIC

**Keys for IBASIC****OUTPUT  
@Hp415x**

1. Displays the following program line for outputting a command to the HP 4155A/4156A:

```
OUTPUT @Hp415x;""
```

2. Positions the cursor at the second double quotes. You enter desired command, then select **Enter** key.

**ENTER  
@Hp415x**

1. Displays the following program line for entering data from the HP 4155A/4156A:

```
ENTER @Hp415x;
```

2. Positions the cursor after the semicolon. You enter desired variable, then select **Enter** key.

**PAUSE**

Enters the following program line for pausing a program:

```
PAUSE
```

**DISP**

1. Displays the following program line for displaying a message:

```
DISP ""
```

2. Positions the cursor at the second double quotes. You enter the message that you want to display, then select **Enter** key.

**INPUT**

1. Displays the following program line for assigning keyboard input to program variable:

```
INPUT "",
```

2. Positions the cursor at the second double quote. Enter string that you want to be displayed on CRT, and name of variable in which you want to store keyboard input, then select **Enter** key.

**IF THEN  
ELSE  
END IF**

1. Displays the following program lines for conditional branching:

```
IF THEN  
ELSE  
END IF
```

2. Positions the cursor before THEN. Fill in as desired, then select **Enter** key.

Reference: HP Instrument BASIC

**Keys for IBASIC**

```
WHILE  
END WHI  
LE
```

1. Displays the following program lines for defining a loop:

```
WHILE  
END WHILE
```

2. Positions the cursor after WHILE. Fill in as desired, then select **Enter** key.

```
FOR  
NEXT
```

1. Displays the following program lines for defining a loop:

```
FOR = TO STEP  
NEXT
```

2. Positions the cursor at =. Fill in as desired, then select **Enter** key.

Reference: HP Instrument BASIC  
**Keys for IBASIC**

---


## External Keyboard

You can connect an external keyboard to the HP 4155A/4156A and use to enter text.

Also, you can use the keyboard for other tasks as described in this chapter.

In this section, the notation "**KeyA** + **KeyB**" means to hold down **KeyA** and press **KeyB**.

<b>Esc</b>	Exits the editor
<b>F1</b> through <b>F8</b>	Primary softkeys      Corresponds to the primary softkeys.
<b>Shift</b> + <b>F1</b> through <b>F7</b>	Secondary softkeys      Corresponds to the secondary softkeys.
<b>F9</b>	Screen mode      Toggles the screen mode as follows:

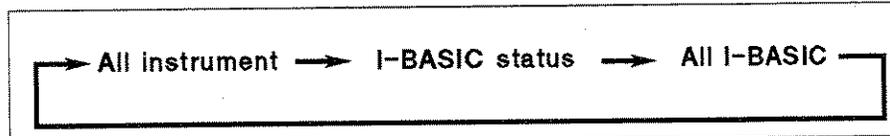

PG02003 120/27

Same as **Ctrl** + **G**.

<b>F11</b>	Clear to end      Deletes characters from cursor to end of line.
	Same as <b>Ctrl</b> + <b>Delete</b>

<b>Shift</b> + <b>F11</b>	Clear line      When editor is running, same as <b>F11</b> . When editor is not running, deletes characters on the Command Entry line.
---------------------------	-------------------------------------------------------------------------------------------------------------------------------------------

Reference: HP Instrument BASIC

**Keys for IBASIC**

<b>F12</b>	Clear display	Clears the display for IBASIC. When the editor is running, exits from the editor, and clears the display for IBASIC.
<b>Print Screen</b>	Clear I/O	Stops I/O operation of program.
<b>Scroll Lock</b>	Stop	Stops program execution after executing the current line. Same as <b>Shift</b> + <b>Pause</b> .
<b>Shift</b> + <b>Scroll Lock</b>	Reset	Stops program execution immediately.
<b>Pause</b>	Pause	Pauses program execution until <b>CONT</b> is executed or <b>Continue</b> primary softkey is pressed. If the program is modified while paused, <b>RUN</b> must be used to restart program execution.  Same as <b>Ctrl</b> + <b>P</b> .
<b>Shift</b> + <b>Pause</b>	Stop	Stops program execution after executing the current line. Same as <b>Scroll Lock</b> .
<b>Insert</b>	Insert	When the editor is running, opens a new line before the current line. When the editor is not running, inserts text at the cursor (press <b>Insert</b> again to end insert mode).  Same as <b>Alt</b> + <b>I</b> .
<b>Shift</b> + <b>Insert</b>	Insert	Same as <b>Insert</b> .
<b>Delete</b>	Delete	Deletes character at the cursor.
<b>Shift</b> + <b>Delete</b>	Delete line	When the editor is running, deletes the current line. When the editor is not running, deletes character at cursor.  Same as <b>Alt</b> + <b>D</b> .

Reference: HP Instrument BASIC

**Keys for IBASIC**

<b>Ctrl</b> + <b>Delete</b>	Clear to end Same as <b>F11</b> .	Deletes characters from cursor to end of line.
<b>Home</b>	Beginning of line Same as <b>Shift</b> + <b>←</b> .	Moves the cursor to beginning of the line.
<b>Shift</b> + <b>Home</b>	Page move	When the editor is running, same as <b>Page Up</b> . Also, same as <b>Shift</b> + <b>▲</b> . When the editor is not running, jumps to the top of the IBASIC output area. Also, same as <b>Shift</b> + <b>▼</b> .
<b>End</b>	End of line Same as <b>Shift</b> + <b>→</b> .	Moves cursor to end of line.
<b>Shift</b> + <b>End</b>	Page move	When the editor is running, same as <b>Page Down</b> . Also, same as <b>Shift</b> + <b>▼</b> . When the editor is not running, jumps to the bottom of the IBASIC output area. Same as <b>Shift</b> + <b>▲</b> .
<b>Page Up</b>	Page move	When the editor is running, moves the cursor one-half display page toward the beginning of the program. Same as <b>Shift</b> + <b>Home</b> . Same as <b>Shift</b> + <b>▲</b> . When the editor is not running, moves display down one page.
<b>Shift</b> + <b>Page Up</b>	Recall	When the editor is running, displays last deleted line. To enter line into program, press <b>Enter</b> . When the editor is not running, cycles through the 10 commands that were most recently entered on the Command Entry line.

Reference: HP Instrument BASIC

**Keys for IBASIC**

<b>Page Down</b>	Page move	When the editor is running, moves the cursor one-half display page toward the end of the program. Same as <b>Shift</b> + <b>End</b> . Same as <b>Shift</b> + <b>▼</b> . When the editor is not running, moves display up one page.
<b>Shift</b> + <b>Page Down</b>	Recall backward	When the editor is running, same as <b>Shift</b> + <b>Page Up</b> . When the editor is not running, cycles through the 10 commands that were most recently entered on the Command Entry line in reverse order of <b>Shift</b> + <b>Page Up</b> .
<b>▲</b>	Previous line	When the editor is running, moves cursor up one line. When the editor is not running, display on the IBASIC output area moves one line toward the end.
<b>Shift</b> + <b>▲</b>	Page move	When the editor is running, same as <b>Page Up</b> . Also, same as <b>Shift</b> + <b>Home</b> . When the editor is not running, jumps to the bottom of the IBASIC output area. Same as <b>Shift</b> + <b>End</b> .
<b>Alt</b> + <b>▲</b>	Recall backward	When the editor is running, same as <b>Shift</b> + <b>Page Up</b> . When the editor is not running, same as <b>Shift</b> + <b>Page Down</b> .
<b>▼</b>	Next line	When the editor is running, cursor moves down one line. When editor is not running, display on IBASIC output area moves one line toward beginning.
<b>Shift</b> + <b>▼</b>	Page move	When the editor is running, same as <b>Page Down</b> . Also, same as <b>Shift</b> + <b>End</b> . When the editor is not running, jumps to the top of the IBASIC output area. Same as <b>Shift</b> + <b>Home</b> .
<b>Alt</b> + <b>▼</b>	Recall	Same as <b>Shift</b> + <b>Page Up</b> .

Reference: HP Instrument BASIC

**Keys for IBASIC**

<b>←</b> <b>→</b>	Move cursor	Moves the cursor one character in indicated direction.
<b>Shift</b> + <b>←</b>	Beginning of line	Moves the cursor to beginning of line. Same as <b>Home</b> .
<b>Shift</b> + <b>→</b>	End of line	Moves the cursor to end of line. Same as <b>End</b> .
<b>Backspace</b>	Backspace	When the editor is running, deletes the character before cursor. When the editor is not running, deletes the character before cursor (if mode is insert mode). If mode is not insert mode, moves cursor to left by one cursor.
<b>Alt</b> + <b>D</b>	Delete line	When the editor is running, deletes the current line. When the editor is not running, deletes the character at the cursor. Same as <b>Shift</b> + <b>Delete</b> .
<b>Alt</b> + <b>I</b>	Insert line	When the editor is running, opens a new line before the current line. When the editor is not running, inserts text at the cursor (press <b>Insert</b> again to end insert mode). Same as <b>Insert</b> .
<b>Ctrl</b> + <b>U</b>	Run	Executes the program.
<b>Ctrl</b> + <b>P</b>	Pause	Pauses program execution until <b>CONT</b> is executed or <b>Continue</b> primary softkey is pressed. If the program is modified while paused, <b>RUN</b> must be used to restart program execution. Same as <b>Pause</b> .

Reference: HP Instrument BASIC

**Keys for IBASIC**

**Ctrl**+**G**

Screen mode      Toggles the screen mode as follows:

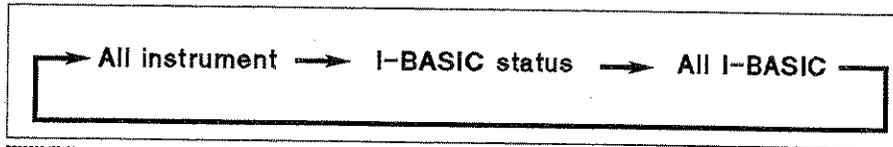


FIG2003 120x60

Same as **F9**

---

## HP 4155A/4156A Specific IBASIC Keywords

The following keywords are not standard IBASIC keywords, or are standard keywords, but with a difference. These keywords are specific to HP 4155A/4156A.

- EXECUTE** Not standard IBASIC keyword. Refer to “ASP-like Commands” for details.
- ON KEY** Standard IBASIC keyword, except the range of *key selector* is 1 to 7.  
1 to 7 of *key selector* corresponds to secondary softkeys 1 to 7, respectively.
- PEN** Standard IBASIC keyword, except the range of *pen selector* is 7. The following table shows the corresponding color for each *pen selector*.

<i>pen selector</i>	<b>Color</b>
1	color defined for Foreground on SYSTEM: COLOR SETUP page.
2	color defined for Y1 Axis on SYSTEM: COLOR SETUP page.
3	color defined for Y2 Axis on SYSTEM: COLOR SETUP page.
4	color defined for Marker/Cursor/Line on SYSTEM: COLOR SETUP page.
5	color defined for Active Mkr/Csr/Line on SYSTEM: COLOR SETUP page.
6	color defined for Advisory on SYSTEM: COLOR SETUP page.
7	color defined for Title on SYSTEM: COLOR SETUP page.

Reference: HP Instrument BASIC

**HP 4155A/4156A Specific IBASIC Keywords**

The following IBASIC keywords are not implemented in HP 4155A/4156A's Instrument BASIC.

- ALPHA ON/OFF
- AREA
- CLIP
- CONTROL
- DUMP
- EDGE
- FILL
- FRAME
- GESCAPE
- GLOAD
- GRAPHICS
- GRID
- GSTORE
- LINE TYPE
- PLOTTER IS
- POLYGON
- POLYLINE
- RATIO
- RECTANGLE
- SET PEN
- SHOW
- STATUS
- VIEWPORT
- WINDOW

---

## Available I/O Resources for IBASIC

This section provides information about available I/O resources for IBASIC of HP 4155A/4156A.

The following I/O resources are available for IBASIC.

- CRT Display
- External keyboard and front-panel keyboard
- HP-IB Interface on rear panel
- Internal pseudo HP-IB Interface (to control HP 4155A/4156A itself)
- Serial Interface
- Built-in Disk Drive (no select code)

Table 2-1 shows available I/O interfaces and their select codes.

**Table 2-1. Available I/O Interfaces and Select Code**

Select Code	Interface
1	CRT
2	External and front-panel keyboard
7	HP-IB Interface on rear panel
8	Internal pseudo HP-IB Interface
9	Serial Interface

Reference: HP Instrument BASIC

### Available I/O Resources for IBASIC

---

## CRT Display

IBASIC can display text or graphics on the CRT display of the HP 4155A/4156A.

### **Text display.**

Text can be displayed in the IBASIC output area of "All IBASIC" screen.

### **Graphics display.**

In "All IBASIC" screen, you can display a graphical plot.

The x and y coordinate values are as follows:

- lower left corner of screen: (0,0)
- upper right corner of screen: (545,400).

---

## HP-IB Interfaces

- Internal pseudo HP-IB

By using select code 8, you can control HP 4155A/4156A via internal pseudo HP-IB interface. The HP-IB address of HP 4155A/4156A has no meaning, so you can use any address (0 through 30).

- HP-IB on rear panel

You can access HP-IB interface on rear panel by using select code 7.

Reference: HP Instrument BASIC  
Available I/O Resources for IBASIC

---

## Serial Interface

You can access serial interface on rear panel by using select code 9.

### Receiving data

To receive data from serial interface successfully, be sure to do the following:

- Use **ASSIGN** IBASIC command to open I/O path. Refer to the following example:

```
ASSIGN @Serial TO 9  
ENTER @Serial;A$
```

Do not use **ENTER 9;A\$** because every time it is executed, the I/O path is opened, which may cause errors.

- If you receive multiple lines of data (such as by a loop of **ENTER** statements), make sure no other operation or statement occurs between receptions. It may cause an overrun error. If overrun error is caused, use a slower baud rate for receiving.

Reference: HP Instrument BASIC

**Available I/O Resources for IBASIC**

---

## Built-in Diskette Drive

If you specify optional volume specifier when accessing the built-in diskette drive, the volume specifier must be ":INTERNAL,4".

**Available diskettes.**

You can use the following types of 3.5 inch diskettes:

- 2HD 1.44 MB
- 2DD 720 KB

Diskette must be formatted as LIF or the following DOS format:

- 80 tracks/side
- 18 sectors/track (2HD)  
9 sectors/track (2DD)
- 512 bytes/sector

---

## ASP-like Commands

EXECUTE is an IBASIC keyword for executing function directives, which allow you to easily create simple programs in a way similar to creating Auto Sequence Programs (ASP) on the HP 4145A/B Semiconductor Parameter Analyzer.

### Compatibility Consideration

EXECUTE is *not* a standard IBASIC or HP BASIC keyword. So, if you use this keyword in your program, it will *not* execute on another IBASIC or HP BASIC system.

---

## EXECUTE

Keyboard Executable	Yes
Programmable	Yes
In an IF ... THEN ...	Yes

This keyword can execute the function directives that are described on the following pages.

Syntax                    **EXECUTE** ("directive\_keyword [ ,parameter ]")

*directive*                Some directives require parameters. There must be one or more spaces between *directive\_keyword* and *parameter*.

The following pages describe the *directives* that can be used in the EXECUTE command.

Reference: HP Instrument BASIC

### ASP-like Commands

## GET SETUP Directive

This directive loads the specified HP 4155A/4156A setup file.

Directive syntax

```
GETSETUP file_name [ ,DISK|MEMORY ]
```

Directive parameter

Parameter	Type	Explanation
<i>file_name</i>	string	name of setup file with extension (.MES or .STR) to be loaded. You must enclose the name with single quotes or double-double quotes.
DISK	character	(default) loads setup data from internal diskette.
MEMORY	character	loads setup data from internal memory.

Example

```
EXECUTE("GETSETUP 'SWEEP.MES'")
EXECUTE("GETSETUP ""SWEEP.MES""")
EXECUTE("GETSETUP File$,DISK")
EXECUTE("GETSETUP 'MEM1.MES',MEMORY")
```

## SINGLE Directive

This directive executes measurement.

Directive syntax

```
SINGLE
```

Example

```
EXECUTE("SINGLE")
```

Reference: HP Instrument BASIC  
**ASP-like Commands**

---

## STANDBY directive

This directive changes STBY ON channels to standby state or idle state.

Directive syntax

STANDBY ON|OFF

Directive parameter

Parameter	Type	Explanation
ON	character	changes STBY ON channels from idle state to standby state.
OFF	character	changes STBY ON channels from standby state to idle state.

Example

EXECUTE("STANDBY ON")

EXECUTE("STANDBY OFF")

---

## STRESS Directive

This directive forces stress.

Directive syntax

STRESS

Example

EXECUTE("STRESS")

Reference: HP Instrument BASIC

**ASP-like Commands**

---

**AUTO-SCALE Directive**

This directive changes page to GRAPH/LIST: GRAPHICS and executes auto-scaling function.

Directive syntax            **AUTOSCALE**

Example                      **EXECUTE("AUTOSCALE")**

---

**SAVE DATA Directive**

This directive stores measurement data file to internal diskette or internal memory.

Directive syntax            **SAVEDATA *file\_name* [ ,DISK|MEMORY ]**

Directive parameter

Parameter	Type	Explanation
<i>file_name</i>	string	name of measurement data file with extension (.DAT) to be stored. You must enclose the name with single quotes or double-double quotes.
DISK	character	(default) stores measurement data to internal diskette.
MEMORY	character	stores measurement data to internal memory.

Example

```
EXECUTE("SAVEDATA 'SWEEP.DAT'")
EXECUTE("SAVEDATA ""SWEEP.DAT""")
EXECUTE("SAVEDATA File$,DISK")
EXECUTE("SAVEDATA 'MEM1.DAT',MEMORY")
```

Reference: HP Instrument BASIC  
ASP-like Commands

---

## READ DATA VARIABLE Directive

This directive gets values of specified HP 4155A/4156A data variable, and stores the values in an IBASIC variable.

Directive syntax      `READDATAVAR data_variable_name, ibasic_variable_name)`

Directive parameter

Parameter	Type	Explanation
<i>data_variable_name</i>	string	name of the data variable of HP 4155A/4156A. You must enclose the name with single quotes or double-double quotes. Name is case sensitive.
<i>ibasic_variable_name</i>	string	name of numeric variable or numeric array of IBASIC program. <i>ibasic_variable_name</i> is not case sensitive.

Example

```
EXECUTE("READDATAVAR 'V1',V")
```

```
EXECUTE("READDATAVAR ""V1"",v")
```

Reference: HP Instrument BASIC

**ASP-like Commands**

---

**DEFINE USER VARIABLE Directive**

This directive defines an HP 4155A/4156A user variable, and transfers values from an IBASIC variable to the user variable.

Directive syntax

```
DEFUSERVAR user_variable_name, no_of_points, ibasic_variable_name
[ , unit ]
```

Directive parameter

Parameter	Type	Explanation
<i>user_variable_name</i>	string	user variable name that you want to define. You must enclose the name with single quotes or double-double quotes.
<i>no_of_points</i>	numeric	number of data for the user variable
<i>ibasic_variable_name</i>	string	name of numeric variable or numeric array of IBASIC program. The data in this variable will be transferred to the user variable.
<i>unit</i>	string	unit of user variable. You must enclose the unit with single quotes or double-double quotes.

Example

```
EXECUTE("DEFUSERVAR 'U_var',101,Vth,'V'")
```

Reference: HP Instrument BASIC  
**ASP-like Commands**

---

## PRINT/PLOT Directive

This directive prints/plots the information of the present instrument page, not the IBASIC screen. If present page is GRAPH/LIST: GRAPHICS page, the graph is printed/plotted.

Directive syntax	<code>PRINTPLOT</code>
Example	<code>EXECUTE("PRINTPLOT")</code>

---


## CURVE PLOT Directive

This directive changes to GRAPH/LIST: GRAPHICS page, then prints/plots the graph.

Directive syntax	<code>CURVEPLOT</code>
Example	<code>EXECUTE("CURVEPLOT")</code>

Reference: HP Instrument BASIC

**ASP-like Commands**



---

Getting Started on  
Programming the HP  
4155A/4156A

---

## Getting Started on Programming the HP 4155A/4156A

This chapter provides step-by-step tutorials for programming to control the HP 4155A/4156A along with programming examples.

This chapter consists of the following sections:

- **Creating a Simple Measurement Program**

This section introduces how to create a measurement program.

- **Programming for Data Extraction**

This section provides the programming tutorials for data extraction.

- **Complete Example Program for Vth Measurement**

This section shows complete example program based on the parts described in the other sections.

- **Example Application Setup for Vth Measurement**

This section describes an example application setup that you should save to the file named `VTH.MES` on diskette before executing program examples (that use `VTH.MES`) described in this chapter.

In addition to this chapter, Chapter 6 provides some application examples which are helpful to increase your understanding.

---

## Creating a Simple Measurement Program

This section introduces how to create a measurement program.

A simple measurement program created by using built-in IBASIC controller is provided as an example and you learn step-by-step how to create a measurement program.

This section consists of the following:

1. Getting a setup file and making a measurement
2. Changing the sweep setup parameters
3. Changing the display setup parameters
4. Saving the measurement results to a diskette
5. Printing the measurement results

Getting Started on Programming the HP 4155A/4156A

### Creating a Simple Measurement Program

---

## Before Creating a Program

This section assumes that you have already saved a measurement setup file for Vth measurement to diskette.

Before starting this section, prepare the diskette and save the measurement setup (described in "Example Application Setup for Vth Measurement") to the file named "VTH.MES" on the diskette.

---

## Step 1. Getting the Setup File and Making a Measurement

In this step, you can create a program to get a setup file from the diskette and execute a measurement.

1. Press IBASIC **Display** key until screen display mode is All IBASIC mode.
2. Select **EDIT** softkey, then press **Enter** key to start the IBASIC editor
3. If there is an existing program, save it if necessary.
4. Delete existing program and assign I/O path to control HP 4155A/56A.

Type **SCRATCH**, then **Enter**. Or select **Scratch** primary softkey to delete the program.

Existing program is deleted and the following program lines are entered automatically. These lines are for assigning HP 4155A/56A control I/O path.

```
10 CDM @Hp415x
20 ASSIGN @Hp415x TO 800
30 !
9990 END
```

Getting Started on Programming the HP 4155A/4156A  
**Creating a Simple Measurement Program**

Line number	Description
10	Declares COM so that subprograms can access the I/O path (that is assigned in line 20) for controlling the HP 4155A/56A. Refer to the <i>HP Instrument BASIC Users Handbook</i> for details.
20	Assigns the I/O path for controlling the HP 4155A/56A. 800 means built-in IBASIC controller.

#### To ASSIGN I/O path

- Built-in IBASIC controller

Specify select code 8. For the HP-IB address, you can use *any* number between 0 to 31. Refer to the following example:

```
10 ASSIGN @Hp4155 TO 800
```

- HP BASIC on an external computer

Specify the select code of the external computer. And specify the HP-IB address that you entered into the HP-IB ADDRESS field on the SYSTEM: MISCELLANEOUS page. In the following example, the select code of the external computer is 7 and HP-IB address of HP 4155A/56A is 17:

```
10 ASSIGN @Hp4155 TO 717
```

5. Select **OUTPUT @Hp415x** secondary softkey.

The following characters are automatically entered:

```
30 OUTPUT @Hp415x; ""
```

Do not press **Enter** yet.

6. Use the help function to find the command for getting a setup file:
  - a. Press **Help**.
  - b. Press **Get**.

Getting Started on Programming the HP 4155A/4156A

### Creating a Simple Measurement Program

The cursor in help window automatically jumps to the command (:MMEM:LOAD:STAT) for getting a setup file.

7. Press **Enter** to insert the command into the program line.

Now line 30 is as follows:

```
30 OUTPUT @Hp415x;":MMEM:LOAD:STAT"
```

8. Type in the command parameters as in following example:

```
30 OUTPUT @Hp415x;":MMEM:LOAD:STAT 0,'VTH.MES','DISK'"
```

Parameter	Description
0	No meaning (dummy parameter).
'VTH.MES'	File name to be loaded.
'DISK'	Source mass storage is diskette.

Then press **Enter**. Then select the **Insert line** softkey.

9. Select **OUTPUT @Hp415x** secondary softkey.

```
40 OUTPUT @Hp415x;""
```

10. Press **Help**, then press **Single**, **Append**, or **Repeat** to find the command for executing a measurement.

Execution Key	Command
<b>Single</b>	:PAGE:SCON:MEAS:SING
<b>Append</b>	:PAGE:SCON:MEAS:APP
<b>Repeat</b>	:PAGE:SCON:MEAS:REP

11. Press **Enter** to insert the found command into the program line.

```
10 COM @Hp415x
20 ASSIGN @Hp415x TO 800
30 OUTPUT @Hp415x;":MMEM:LOAD:STAT 0,'VTH.MES','DISK'"
40 OUTPUT @Hp415x;":PAGE:SCON:MEAS:SING"
9990 END
```

Then press **Enter**

Getting Started on Programming the HP 4155A/4156A  
**Creating a Simple Measurement Program**

12. Press **End edit** to exit from the editor.

Now you have created a measurement program.

To execute the program, do as follows:

1. Press IBASIC **Display** key until screen display mode is All Instrument or IBASIC Status mode. This allows you to monitor the measurement on GRAPH/LIST: GRAPHICS page.
2. Press **Run** front-panel key. The measurement program is executed.

#### **Controlling from External Computer**

You must do as follows before controlling HP 4155A/4156A from an external computer:

1. Connect the HP-IB interface of external computer to HP-IB interface on rear panel of HP 4155A/4156A.
2. Set the HP 4155A/56A is field on the SYSTEM: MISCELLANEOUS page to NOT SYSTEM CONTROLLER.
3. Enter the HP-IB address of your HP 4155A/4156A into the HP-IB ADDRESS field.

Getting Started on Programming the HP 4155A/4156A

## Creating a Simple Measurement Program

### Step 2. Changing the Sweep Setup Parameters

Modify measurement program created in previous step so that you can enter new sweep start and stop values while program is running:

1. Press IBASIC **Display** key until the screen display mode is All IBASIC mode.
2. Select **EDIT** softkey, then press **Enter** key to start the IBASIC editor
3. Insert program lines that allow you to enter the sweep start and stop values from the keyboard during program running.
  - a. Move the cursor to program line 30.
  - b. Select **Insert line** primary softkey.
  - c. Type the following program lines:

```
21 !
22 INPUT "Sweep Start (V)?",Start_v
23 INPUT "Sweep Stop (V)?",Stop_v
24 !
```

4. If you do not know the SCPI commands for changing the sweep start and stop parameters, do as follows:
  - a. Press IBASIC **Display** key until screen display mode is All Instrument mode.
  - b. Press **Meas** to change to MEASURE: SWEEP SETUP page.
  - c. Move the field pointer to the parameter that you want to change.
  - d. Press **Help** key. The corresponding command is displayed at the bottom of the help window:

Command	Description
:PAGE:MEAS:SWE:VAR1:STAR	VAR1 sweep start
:PAGE:MEAS:SWE:VAR1:STOP	VAR1 sweep stop

You need to remember the commands, so that you can enter them in the next step.

- e. Select the **EXIT HELP** softkey.

**Creating a Simple Measurement Program**

5. Press IBASIC **Display** key until screen display mode is All IBASIC mode. Then, do the following to insert the program lines for changing the sweep start and stop values.
  - a. Move the cursor to the program line 40.
  - b. Select **Insert line** primary softkey.
  - c. Select the **OUTPUT @Hp415x** softkey.
  - d. Type in the SCPI command. Or you can use the help function to enter the command. For the help function, see "To Use the Help Function" in Chapter 1.

After you finish, the program lines should look as follows:

```
31 OUTPUT @Hp415x;":PAGE:MEAS:SWE:VAR1:STAR";Start_v
32 OUTPUT @Hp415x;":PAGE:MEAS:SWE:VAR1:STOP";Stop_v
```

Now the program is as follows:

```
10 COM @Hp415x
20 ASSIGN @Hp415x TO 800
21 !
22 INPUT "Sweep Start (V)?",Start_v
23 INPUT "Sweep Stop (V)?",Stop_v
24 !
30 OUTPUT @Hp415x;":MMEM:LOAD:STAT 0,'VTH.MES','DISK'"
31 OUTPUT @Hp415x;":PAGE:MEAS:SWE:VAR1:STAR";Start_v
32 OUTPUT @Hp415x;":PAGE:MEAS:SWE:VAR1:STOP";Stop_v
40 OUTPUT @Hp415x;":PAGE:SCON:MEAS:SING"
9990 END
```

6. Select **End edit** to exit from the editor.
7. Press IBASIC **Display** key until screen display mode is IBASIC Status mode.
8. Press **Run** to execute the program.
9. **Sweep Start (V)?** is displayed on the display line. Enter the desired sweep start voltage.
10. **Sweep Stop (V)?** is displayed on the display line. Enter the desired sweep stop voltage.

Getting Started on Programming the HP 4155A/4156A  
**Creating a Simple Measurement Program**

---

### Step 3. Changing the Display Setup Parameters

In this step, change X-axis range of display setup parameters to match the sweep start and stop values.

1. Press IBASIC **Display** key until screen display mode is All IBASIC mode.
2. Select **EDIT** softkey, then press **Enter** key to start the IBASIC editor
3. If you do not know the SCPI commands for changing the X-axis parameters, do as follows:
  - a. Press IBASIC **Display** key until screen display mode is All Instrument mode.
  - b. Press PAGE CONTROL **Display** key to change to DISPLAY: DISPLAY SETUP page.
  - c. Move the field pointer to the parameter that you want to change.
  - d. Press **Help** key. The corresponding commands are displayed at the bottom of the help window. You need to remember the commands, so that you can enter them in the next step.

Command	Description
:PAGE:DISP:SET:GRAP:X:MIN	minimum value of X-axis
:PAGE:DISP:SET:GRAP:X:MAX	maximum value of X-axis

- 
- 
- 
- 
- e. Select the **EXIT HELP** softkey.

## Getting Started on Programming the HP 4155A/4156A

## Creating a Simple Measurement Program

4. Press IBASIC **Display** key until screen display mode is All IBASIC mode. Then, do the following to insert the program lines for changing the X-axis display parameters:
  - a. Move the cursor to the program line 40.
  - b. Select **Insert line** primary softkey.
  - c. Select the **OUTPUT @Hp415x** softkey.
  - d. Type in the SCPI command. Or you can use the help function to enter the command. For the help function, see "To Use the Help Function" in Chapter 1. After you finish, the program lines should look as follows:

```

33 OUTPUT @Hp415x;":PAGE:DISP:SET:GRAP:X:MIN";Start_v
34 OUTPUT @Hp415x;":PAGE:DISP:SET:GRAP:X:MAX";Stop_v

```

Now the program is as follows:

```

10 COM @Hp415x
20 ASSIGN @Hp415x TO 800
21 !
22 INPUT "Sweep Start (V)?",Start_v
23 INPUT "Sweep Stop (V)?",Stop_v
24 !
30 OUTPUT @Hp415x;":MMEM:LOAD:STAT 0,'VTH.MES','DISK'"
31 OUTPUT @Hp415x;":PAGE:MEAS:SWE:VAR1:STAR";Start_v
32 OUTPUT @Hp415x;":PAGE:MEAS:SWE:VAR1:STOP";Stop_v
33 OUTPUT @Hp415x;":PAGE:DISP:SET:GRAP:X:MIN";Start_v
34 OUTPUT @Hp415x;":PAGE:DISP:SET:GRAP:X:MAX";Stop_v
40 OUTPUT @Hp415x;":PAGE:SCON:MEAS:SING"
9990 END

```

5. Select **End edit** to exit from the editor.
6. Press IBASIC **Display** key until screen mode is IBASIC Status mode.
7. Press **Run** to execute the program.
8. Enter the desired sweep start and stop values as prompted. The minimum and maximum X-axis values of the graph will be the same as these entered values.

Getting Started on Programming the HP 4155A/4156A

### Creating a Simple Measurement Program

## Step 4. Saving All Measurement Results to a Diskette.

In this step, add program lines that save the setup data and measurement results to the diskette.

1. Press IBASIC **Display** key until screen display mode is All IBASIC mode.
2. Select **EDIT** softkey, then press **Enter** key to start the IBASIC editor
3. Move the cursor to program line 9990.
4. Select **Insert line** primary softkey.
5. Insert the following program lines, which wait until the measurement is completed.

```
50 OUTPUT @Hp415x;"*OPC?"
60 ENTER @Hp415x;Complete
```

When measurement is completed, HP 4155A/56A returns 1 to the **Complete** variable.

6. Insert the following program line, which saves the measurement setup and results to a file named VTH.DAT:

```
70 OUTPUT @Hp415x;"MMEM:STOR:TRAC DEF,'VTH.DAT'"
```

Now the program is as follows:

```
10 COM @Hp415x
20 ASSIGN @Hp415x TO 800
21 !
22 INPUT "Sweep Start (V)?",Start_v
23 INPUT "Sweep Stop (V)?",Stop_v
24 !
30 OUTPUT @Hp415x;"MMEM:LOAD:STAT 0,'VTH.MES','DISK'"
31 OUTPUT @Hp415x;"PAGE:MEAS:SWE:VAR1:STAR";Start_v
32 OUTPUT @Hp415x;"PAGE:MEAS:SWE:VAR1:STOP";Stop_v
33 OUTPUT @Hp415x;"PAGE:DISP:SET:GRAP:X:MIN";Start_v
34 OUTPUT @Hp415x;"PAGE:DISP:SET:GRAP:X:MAX";Stop_v
40 OUTPUT @Hp415x;"PAGE:SCON:MEAS:SING"
50 OUTPUT @Hp415x;"*OPC?"
60 ENTER @Hp415x;Complete
70 OUTPUT @Hp415x;"MMEM:STOR:TRAC DEF,'VTH.DAT'"
9990 END
```

7. Select **End edit** to exit from the editor.

Getting Started on Programming the HP 4155A/4156A

**Creating a Simple Measurement Program**

8. Press IBASIC **Display** key until screen display mode changes to IBASIC Status mode.
9. Press **Run** to execute the program.

The measurement setup and results are automatically saved to the diskette after measurement is performed.

Getting Started on Programming the HP 4155A/4156A

### Creating a Simple Measurement Program

---

## Step 5. Printing the Measurement Results

### Printing from IBASIC

If you use built-in IBASIC controller to control HP 4155A/4156A, you do not need to prepare before controlling HP 4155A/4156A because built-in IBASIC controller is always connected to HP 4155A/4156A via internal HP-IB.

However, to *print/plot* from built-in IBASIC controller, set "HP 4155A/56A is" field on the SYSTEM: MISCELLANEOUS page to SYSTEM CONTROLLER.

In this step, add program lines that print the measurement results.

1. Press **Display** key until screen display mode is All IBASIC mode.
2. Select **EDIT** softkey, then press **Enter** key to start the IBASIC editor
3. Move the cursor to the program line 70.
4. Select **Insert line** primary softkey.
5. Insert the following program lines, which print a screen dump of the results:

```
61 OUTPUT @Hp415x;":HCOP:SDUM"  
62 DISP "Printing"  
63 OUTPUT @Hp415x;":*OPC?"  
64 ENTER @Hp415x;Complete  
65 DISP "Done"
```

:HCOP immediately initiates the plot or print according to the current setup. After printing is finished, HP 4155A/56A returns 1 to the **Complete** variable, then "Done" is displayed on the screen.

Now the program is as follows:

Getting Started on Programming the HP 4155A/4156A  
**Creating a Simple Measurement Program**

```
10 COM @Hp415x
20 ASSIGN @Hp415x TO 800
21 !
22 INPUT "Sweep Start (V)?",Start_v
23 INPUT "Sweep Stop (V)?",Stop_v
24 !
30 OUTPUT @Hp415x;":MMEM:LOAD:STAT 0,'VTH.MES', 'DISK'"
31 OUTPUT @Hp415x;":PAGE:MEAS:SWE:VAR1:STAR";Start_v
32 OUTPUT @Hp415x;":PAGE:MEAS:SWE:VAR1:STOP";Stop_v
33 OUTPUT @Hp415x;":PAGE:DISP:SET:GRAP:X:MIN";Start_v
34 OUTPUT @Hp415x;":PAGE:DISP:SET:GRAP:X:MAX";Stop_v
40 OUTPUT @Hp415x;":PAGE:SCON:MEAS:SING"
50 OUTPUT @Hp415x;"*OPC?"
60 ENTER @Hp415x;Complete
61 OUTPUT @Hp415x;":HCOP:SDUM"
62 DISP "Printing"
63 OUTPUT @Hp415x;"*OPC?"
64 ENTER @Hp415x;Complete
65 DISP "Done"
70 OUTPUT @Hp415x;":MMEM:STOR:TRAC DEF,'VTH.DAT'"
9990 END
```

---

## Programming for Data Extraction

This section provides the following programming tutorials for data extraction:

- Reading HP 4155/56 setup data
- Reading values of data variables (measurement results)
- Transferring data into a file

---

### Reading HP 4155/56 Setup Data

To read setup data from HP 4155/56 into an IBASIC variable, use the query form of the corresponding setting command. To make the query form of a command, simply add a question mark (?) to the end of the command.

Refer to the following program lines of example program:

```
60   OUTPUT @Hp415x;":PAGE:MEAS:SWE:VAR1:STAR?"
70   ENTER @Hp415x;Vd_start
80   OUTPUT @Hp415x;":PAGE:MEAS:SWE:VAR1:STOP?"
90   ENTER @Hp415x;Vd_stop
100  OUTPUT @Hp415x;":DISP:ALL BAS"
110  CLEAR SCREEN
120  PRINT TABXY(1,1);"Vd START=";Vd_start;"(V)"
130  PRINT TABXY(1,2);"Vd STOP =" ;Vd_stop;"(V)"
```

- Line 60            This query command tells the HP 4155A/56A to put the VAR1 start value in its output buffer.
- :PAGE:MEAS:SWE:VAR1:STAR is the command for setting the VAR1 start value. By adding ?, the command becomes the query command for reading the VAR1 start value.
- Line 70            This gets the start value from the output buffer, then enters it in the Vd\_start variable.
- Line 80 to 90     These lines tell the HP 4155A/56 to put VAR1 stop value in its output buffer, then the value is entered into the Vd\_stop variable.

---

## Reading HP 4155/56 Measurement Data

To read read-out function values or data variable values (output data, measurement data, and user function values) from HP 4155/56 to IBASIC variables, use the `:DATA?` command.

Refer to the following program lines in the example program:

```
410   OUTPUT @Hp415x;":PAGE:SCON:MEAS:SING"  
420   OUTPUT @Hp415x;":*OPC?"  
430   ENTER @Hp415x;Complete  
440   OUTPUT @Hp415x;":DATA? 'VTH'"  
450   ENTER @Hp415x;Vth
```

Line 410 Execute single measurement.

Line 420 to 430 Wait for measurement completion.

Line 440 Send `:DATA?` query command to read the result value of user function "VTH".

Line 450 Store the result value into `Vth` variable.

### NOTE

Be aware that data variable names, such as user functions and user variables, are *case sensitive*. For example, if you set up user function name `VTH` on the CHANNEL: USER FUNCTION DEFINITION page, then to read it, you must use `:DATA? 'VTH'`, not `:DATA? 'Vth'`.

---

## Transferring Specific HP 4155/56 Data to a File

To transfer data from the HP 4155A/56A to a file, do as follows:

1. Create a data file.

You can create three types of data files: DOS, LIF ASCII, or BDAT as follows:

```
CREATE "data_file",1           ! Creates a DOS file.
```

```
CREATE ASCII "ascii_file",100 ! Creates a LIF ASCII file.
```

```
CREATE BDAT "binary_file",100 ! Creates a BDAT file.
```

DOS files are compatible with MS-DOS, which are easy to transfer to PCs and other computers.

LIF ASCII files are compatible with HP computers that support this file type, so this type is best if you are transferring files among HP computers that support this file type.

BDAT (binary data) files provide more flexibility (can specify both number of records and record length) and faster transfer rate. But BDAT files cannot be interchanged with as many other systems.

The first parameter of each statement specifies the file name to create.

The second parameter specifies number of records to allocate for the file as follows:

DOS                    Second parameter specifies how many records are to be *initially* allocated for the file. A DOS file system automatically allocates additional space for the file as new data is written to it, so you can always specify 1 for this parameter.

LIF ASCII            Second parameter specifies *total* number of records to allocate for the file, so you must specify a sufficient number of records. The length of one record is 256 bytes.

For example, the following statement would create a file with 100 records (each record is 256 bytes):

```
CREATE ASCII "file",100
```

Getting Started on Programming the HP 4155A/4156A

### Programming for Data Extraction

```

460 .   OUTPUT @File;Vth
      .
630 .   UNTIL Stop$="S" OR Stop$="s"

```

The above program repeats appending Vth variable value to a DOS file in ASCII format.

In addition to numeric data, array data and string data can be stored to a file as in following examples:

- Array data:

```

1 .   DIM Vth(1:100)
      .
340 .   INPUT "Enter file name to store data",File$
350 .   CREATE File$,1
360 .   ASSIGN @File TO File$;FORMAT ON
      .
390 .   FOR I=1 TO 100
      .
440 .       OUTPUT @Hp415x;":DATA? 'VTH'"
450 .       ENTER @Hp415x;Vth(I)
460 .   NEXT I
470 .   OUTPUT @File;Vth(*)
      .

```

- String data:

```

10 .   DIM Data$[10](1:100)
20 .   CREATE "DATAFILE",1
30 .   ASSIGN @File TO "DATAFILE";FORMAT ON
40 .   FOR I=1 TO 100
50 .       Data$(I)="ABC"
60 .   NEXT I
70 .   OUTPUT @File;Data$(*)
      .

```

#### 4. Close the I/O path.

To close an I/O path to a file, ASSIGN the path name to an \* (asterisk) as in the following example:

```

340 .   INPUT "Enter file name to store data",File$
350 .   CREATE File$,1
360 .   ASSIGN @File TO File$;FORMAT ON
      .
460 .   OUTPUT @File;Vth
      .
590 .   ASSIGN @File TO *

```

In this program, line 590 closes the I/O path that was opened by line 360.

**BDAT**                      Second parameter specifies *total* number of records to allocate for the file, so you must specify a sufficient number of records. You can specify a record length by using an optional third parameter (default length is 256 bytes).

For example, the following statement creates a file with 7 records (each record is 128 bytes):

```
CREATE BDAT "B_file",7,128
```

The following statement creates a file with 7 records (each record is 256 bytes):

```
CREATE BDAT "B_file",7
```

## 2. Open an I/O path for transferring data into the file.

To open an I/O path to the file, assign an I/O path name to the file by using an ASSIGN statement as in the following example:

```
340 INPUT "Enter file name to store data",File$
350 CREATE File$,1
360 ASSIGN @File TO File$;FORMAT ON
```

Line 350 creates a DOS file, then line 360 opens an I/O path to the file.

For DOS and BDAT files, ASSIGN statement can also specify the following:

**FORMAT ON**                      ASCII data representations are used. Specify this if you need to transport data between IBASIC and other machines.

**FORMAT OFF**                      IBASIC internal data representations are used. Specify this if you need a faster transfer rate and space efficiency.

## 3. Store data into the file.

To store data into a file, use OUTPUT and ENTER statements as in the following examples:

```
340 INPUT "Enter file name to store data",File$
350 CREATE File$,1
360 ASSIGN @File TO File$;FORMAT ON
:
390 REPEAT
:
440 OUTPUT @Hp415x;":DATA? 'VTH'"
450 ENTER @Hp415x;Vth
```

---

## Complete Example Program for Vth Measurement

The example program shown below uses the measurement setup file described in "Example Application Setup for Vth Measurement". This is a complete example program based on the parts described in the previous sections.

```

10     COM @Hp415x
20     ASSIGN @Hp415x TO 800
30     OUTPUT @Hp415x;"MMEM:LOAD:STAT 0,'VTH.MES','DISK'"
40     !
50     ! Read and Disp. Measurement Conditions
60     OUTPUT @Hp415x;"PAGE:MEAS:SWE:VAR1:STAR?"
70     ENTER @Hp415x;Vd_start
80     OUTPUT @Hp415x;"PAGE:MEAS:SWE:VAR1:STOP?"
90     ENTER @Hp415x;Vd_stop
100    OUTPUT @Hp415x;"DISP:ALL BAS"
110    CLEAR SCREEN
120    PRINT TABXY(1,1);"Vd START=";Vd_start;"(V)"
130    PRINT TABXY(1,2);"Vd STOP =";Vd_stop;"(V)"
140    !
150    ! Parameter Change
160    Change$="n"
170    Change:    !
180    INPUT "Change these parameters? (y/n default=n)",Change$
190    SELECT Change$
200    CASE "Y","y"
210        INPUT "New Vd START (V)?",Vd_start
220        INPUT "New Vd STOP (V)?",Vd_stop
230        OUTPUT @Hp415x;"PAGE:MEAS:SWE:VAR1:STAR";Vd_start
240        OUTPUT @Hp415x;"PAGE:MEAS:SWE:VAR1:STOP";Vd_stop
250        PRINT TABXY(1,1);"Vd START=";Vd_start;"(V)"
260        PRINT TABXY(1,2);"Vd STOP=";Vd_stop;"(V)"
270    CASE "N","n"
280        GOTO Store_file
290    CASE ELSE
300        GOTO Change
310    END SELECT
320    !
330    Store_file:    !
340    INPUT "Enter file name to store data",File$
350    CREATE File$,1
360    ASSIGN @File TO File$;FORMAT ON
370    !
380    No_of_data=0
390    REPEAT

```

Getting Started on Programming the HP 4155A/4156A  
Complete Example Program for Vth Measurement

```
400 OUTPUT @Hp415x;":DISP:ALL BST"
410 OUTPUT @Hp415x;":PAGE:SCON:MEAS:SING"
420 OUTPUT @Hp415x;":*OPC?"
430 ENTER @Hp415x;Complete
440 OUTPUT @Hp415x;":DATA? 'VTH'"
450 ENTER @Hp415x;Vth
460 OUTPUT @File;Vth
470 No_of_data=No_of_data+1
480 OUTPUT @Hp415x;":DISP:ALL BASIC"
490 PRINT TABXY(1,10);"Last measured Vth =";Vth;"(V)
500 PRINT TABXY(1,11);"Total number of die tested=";No_of_data
510 Stop_query:INPUT "Continue to next die or Stop test? (c/s)",Stop$
520 SELECT Stop$
530 CASE "C","c"
540     DISP "Move to the next die, then press [Continue]"
550     PAUSE
560     DISP ""
570 CASE "S","s"
580     PRINT TABXY(1,24);"Test Stopped!!"
590     ASSIGN @File TO *
600 CASE ELSE
610     GOTO Stop_query
620 END SELECT
630 UNTIL Stop$="S" OR Stop$="s"
640 END
```

## Example Application Setup for Vth Measurement

This section describes an example application setup that you should save to the file named **VTH.MES** on diskette before executing program examples (that use **VTH.MES**) described previously in this chapter.

A frequently used method of measuring  $V_{th}$  is to synchronously sweep the exact same voltage to gate and drain, and measure the characteristics in the saturation region.

The theoretical value of drain current in the saturation region is calculated as follows:

$$I_d = \beta * (V_g - V_{th})^2$$

Where  $\beta$  is the gain factor, which is  $-1/2 * (\mu\epsilon_{ox} W/L) * t_{ox}$ . Therefore, if you take the square root of both sides of the equation:

$$\sqrt{I_d} = \sqrt{\beta} * (V_g - V_{th})$$

$\sqrt{I_d}$  is proportional to  $V_g$ , and the slope is  $\sqrt{\beta}$ . At the point where  $\sqrt{I_d}$  is equal 0,  $V_{th}$  is equal to  $V_g$ . So, to know  $V_{th}$ , we need to find that point.

The measurement conditions are as follows:

- Channel Definition

<b>Measurement Mode</b>	Sweep
-------------------------	-------

UNIT	VNAME	INAME	MODE	FCTN
SMU1	Vd	Id	V	VAR1'
SMU2	Vg	Ig	V	VAR1
SMU3	Vs	Is	COMMON	CONST
SMU4	Vsb	Isb	V	CONST

Getting Started on Programming the HP 4155A/4156A  
**Example Application Setup for Vth Measurement**

• Sweep Setup

	<b>VAR1</b>
<b>UNIT</b>	SMU2
<b>NAME</b>	Vg
<b>SWEEP MODE</b>	Single
<b>LIN/LOG</b>	LINEAR
<b>START</b>	0.0000 V
<b>STOP</b>	5.000 V
<b>STEP</b>	100.0 mV
<b>NO OF STEP</b>	51
<b>COMPLIANCE</b>	100.0 mA
<b>POWER COMP</b>	OFF

	<b>VAR1'</b>
<b>UNIT</b>	SMU1
<b>NAME</b>	Vd
<b>OFFSET</b>	0.0000 V
<b>RATIO</b>	1.000
<b>COMPLIANCE</b>	100.00 mA
<b>POWER COMP</b>	OFF

Getting Started on Programming the HP 4155A/4156A  
**Example Application Setup for Vth Measurement**

	CONSTANT
<b>UNIT</b>	SMU4
<b>NAME</b>	Vsb
<b>MODE</b>	V
<b>SOURCE</b>	0.0000 V
<b>COMPLIANCE</b>	100.00 mA

By this setup, Id-Vg characteristics can be measured. On the CHANNELS: USER FUNCTION DEFINITION page shown in the following table, we defined the square root of Id (SQRTId), and the differential coefficient (GRAD) of SQRTId versus Vg.

Also, we defined VTH and BETA by using Read Out Functions. VTH is @L1X (X-intercept of line 1) and BETA is @L1G^2 (slope of line 1 to second power). Line 1 is drawn according to DISPLAY: ANALYSIS SETUP page, which is described later.

NAME	UNIT	DEFINITION
SQRTId		SQRT(Id)
GRAD		DIFF(SQRTId,Vg)
VTH	V	@L1X
BETA		@L1G^2

As shown in the following tables, we set the DISPLAY: DISPLAY SETUP page to plot two curves: SQRTId versus Vg, and GRAD versus Vg. And VTH and BETA will be displayed in the data variables display area.

Getting Started on Programming the HP 4155A/4156A

**Example Application Setup for Vth Measurement**

	X-axis	Y1-axis	Y2-axis
<b>NAME</b>	Vg	SQRTId	GRAD
<b>SCALE</b>	LINEAR	LINEAR	LINEAR
<b>MIN</b>	0 V	0	0
<b>MAX</b>	5 V	200 m	80 m

GRID	LINE PARAMETER	DATA VARIABLES
ON	ON	VTH BETA

The auto analysis functions are defined on DISPLAY: ANALYSIS SETUP page as shown below. A tangent line (line 1) is drawn to "SQRTId versus Vg" curve (Y1) at point where GRAD is maximum. VTH is the X-intercept of this line. Also, the marker is moved to point where GRAD is maximum.

\*LINE1: [TANGENT] line on [Y1] at a point where  
[GRAD] = [MAX(GRAD)]

If you execute a single measurement, the two curves are drawn. Right after the measurement, a tangent line is drawn as specified in DISPLAY: ANALYSIS SETUP page, and resulting VTH and BETA values are displayed.

---

**HP 4155A/4156A SCPI  
Programming**

---

## HP 4155A/4156A SCPI Programming

Standard Commands for Programmable Instruments (SCPI) is a universal programming language for electronic test and measurement instruments, and based on IEEE 488.1 and IEEE488.2.

This chapter describes how to create programs that contain SCPI commands to control the HP 4155A/56A. These programs can be run from an external computer or from the built-in HP Instrument BASIC (IBASIC) controller.

This chapter explains the following programming tasks along with programming examples:

- SCPI Programming Basics
- Measurement Setup
- Measurement Execution
- File Operation
- Data Transfer
- Print/Plot Operation
- Other Programming Tips
- Example for HP 4145 Users

If you are not familiar with HP 4155A/4156A programming, Chapter 3 provides step-by-step tutorials for programming and helps you to understand quickly.

In addition to this chapter, "Example Application Setup for Vth Measurement" in Chapter 3 provides some application examples which are helpful to increase your understanding.

---

## SCPI Programming Basics

This section provides the following basic tasks to control and program the HP 4155A/4156A:

- Preparation before controlling the HP 4155A/56A via HP-IB
- SCPI Command Hierarchy
- To control HP 4155A/4156A by HP BASIC programming

---

## Preparation before Controlling the HP 4155A/56A via HP-IB

SCPI programs to control the HP 4155A/4156A via HP-IB can be run from an external computer or from the built-in HP Instrument BASIC (IBASIC) controller.

To run these programs, the HP 4155A/56A must be set to *HP 4155A/56A command mode*, which is the default mode.

The HP 4155A/56A has two command modes: HP 4155A/56A command mode (default) and HP 4145 syntax command mode.

You use the HP 4145 syntax command mode if you need to execute HP 4145A/B programs on the HP 4155A/56A. For information about this, refer to Chapter 5.

### **Controlling from External Computer.**

You must do as follows before controlling HP 4155A/4156A from an external computer:

1. Connect the HP-IB interface of external computer to HP-IB interface on rear panel of HP 4155A/4156A.
2. Set the HP 4155A/56A *is* field on the SYSTEM: MISCELLANEOUS page to NOT SYSTEM CONTROLLER.
3. Enter the HP-IB address of your HP 4155A/4156A into the HP-IB ADDRESS field.

### **Controlling from built-in IBASIC controller.**

If you use built-in IBASIC controller to control HP 4155A/4156A, you do not need to prepare before controlling HP 4155A/4156A because built-in IBASIC controller is always connected to HP 4155A/4156A via internal HP-IB.

However, to *print/plot* from built-in IBASIC controller, set "HP 4155A/56A *is*" field on the SYSTEM: MISCELLANEOUS page to SYSTEM CONTROLLER.

---

## SCPI Command Hierarchy

SCPI commands use a hierarchical structure for subsystem commands similar to the file system.

For example, in `:PAGE:MEASURE:SWEEP` command, the hierarchy is as follows:

<b>PAGE</b>	root
<b>MEASURE</b>	sub-level 1
<b>SWEEP</b>	sub-level 2

The colon at the beginning of the command means root.  
The colons between two command keywords means moving down to a lower level.

### Using a Semicolon to Reduce Typing

A semicolon enables two commands to be sent on the same line.

For example, `:PAGE:MEAS:VAR1:START 0;STOP 5` is the same as the following two commands:

```
:PAGE:MEAS:VAR1:START 0  
:PAGE:MEAS:VAR1:STOP 5
```

So, using a semicolon reduces typing and simplifies the program.

A command terminator (such as a `<newline>`) resets the path to root.

## To Control HP 4155A/56A by HP BASIC Programming

1. Assign I/O path for controlling HP 4155A/4156A.

Use ASSIGN command to assign I/O path:

- Built-in IBASIC

Specify select code 8. For the HP-IB address, you can use *any* number between 0 to 31. Refer to the following example:

```
10 ASSIGN @Hp4155 TO 800
```

- HP BASIC on an external computer

Specify the select code of the external computer. And specify the HP-IB address that you entered into the HP-IB ADDRESS field on the SYSTEM: MISCELLANEOUS page. In the following example, the select code of the external computer is 7 and HP-IB address of HP 4155A/56A is 17:

```
10 ASSIGN @Hp4155 TO 717
```

2. Use OUTPUT command to send commands to HP 4155A/56A.
3. Use ENTER command to get query response from HP 4155A/56A.

HP 4155A/4156A SCPI Programming  
SCPI Programming Basics

## Example

The following is the example program to control HP 4155A/4156A:

```
10  DIM I3(1:501)
20  !
30  ASSIGN @Hp4155 TO 717
40  !
50  OUTPUT @Hp4155;"*RST"
60  !
70  OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'SWP.MES','DISK'"
80  !
90  OUTPUT @Hp4155;":PAGE:SCON:SING"
100 OUTPUT @Hp4155;"*OPC?"
110 ENTER @Hp4155;Complete
120 !
130 OUTPUT @Hp4155;"FORM:DATA ASC"
140 OUTPUT @Hp4155;":DATA? 'I3'"
150 ENTER @Hp4155;I3(*)
160 !
170 END
```

Line Number	Description
30	Assigns I/O path to control HP 4155A/4156A.
50	Resets HP 4155A/4156A by sending *RST command.
70	Loads measurement setup data from diskette file SWP.MES.
90 to 110	Executes measurement
130 to 150	Gets the measurement data

---

## Programming: Measurement Setup

To set up a measurement, you can use SCPI commands to set the setup pages of HP 4155A/4156A the same way that you can by interactive operation.

Basically, there are the following three ways to set up a measurement via SCPI programming:

- Load the measurement setup data from diskette or internal memory.

Load the measurement setup data by SCPI programming. The data was previously defined and stored to a diskette file or internal memory interactively or by SCPI programming.

- Load the measurement setup data, then change some of the settings.

Load the measurement setup data from diskette or internal memory, then change desired settings by SCPI programming.

- Set all settings.

Set all settings for measurement setup by SCPI programming.

This section describes the following tasks:

- To set or change setup data values.
- To read setup data values

To load previously defined measurement setup data, refer to "Programming: File Operation".

---

## To Set or Change HP 4155/56 Setup Data Values

1. Send :PAGE subsystem commands that correspond to the setup data values that you want to change or set.

There is a command subsystem for each setup page as shown in Table 4-1. Each command subsystem has commands for setting the setup data of the corresponding setup page.

**Table 4-1. :PAGE Subsystem Commands for Measurement Setup**

Setup Page	Command Subsystem
CHANNELS: CHANNEL DEFINITION	:PAGE:CHANnels[:CDEFinition]
CHANNELS: USER FUNCTION DEFINITION	:PAGE:CHANnels:UFUNction
CHANNELS: USER VARIABLE DEFINITION	:PAGE:CHANnels:UVARiable
MEASURE: SWEEP SETUP	:PAGE:MEASure[:SWEep]
MEASURE: SAMPLING SETUP	:PAGE:MEASure:SAMPLing
MEASURE: PGU SETUP	:PAGE:MEASure:PGUSetup
MEASURE: MEASURE SETUP	:PAGE:MEASure:MSETup
MEASURE: OUTPUT SEQUENCE	:PAGE:MEASure:OSEquence
DISPLAY: DISPLAY SETUP	:PAGE:DISPlay[:SETup]
DISPLAY: ANALYSIS SETUP	:PAGE:DISPlay:ANALysis
STRESS: CHANNEL DEFINITION	:PAGE:STRes[:CDEFinition]
STRESS: STRESS SETUP	:PAGE:STRes:SETup

HP 4155A/4156A SCPI Programming  
**Programming: Measurement Setup**

Example

To load measurement setup data, then change the sweep start and stop values:

```
10  ASSIGN @Hp4155 TO 800
20  !
30  OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'SWP.MES','DISK'"
40  !
50  Swp_start=1
60  Swp_stop=10
70  !
80  OUTPUT @Hp4155;":PAGE:MEAS:VAR1:STAR";Swp_start
90  OUTPUT @Hp4155;":PAGE:MEAS:VAR1:STOP";Swp_stop
100 !
110 END
```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A.
30	Loads measurement setup data from diskette file <b>SWP.MES</b> .
80	Changes start value of VAR1.
90	Changes stop value of VAR1.

---

## To Read HP 4155/56 Setup Data Values

To read setup data from HP 4155/56 into an IBASIC variable, do as follows:

1. Send :PAGE subsystem query command that corresponds to setup data that you want to read.

### Example

To load measurement setup data, then read the sweep start and stop values:

```
10  ASSIGN @Hp4155 TO 717
20  !
30  OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'SWP.MES','DISK'"
40  !
50  OUTPUT @Hp4155;":PAGE:MEAS:VAR1:STAR?"
60  ENTER @Hp4155;Swp_start
70  OUTPUT @Hp4155;":PAGE:MEAS:VAR1:STOP?"
80  ENTER @Hp4155;Swp_stop
90  !
100 PRINT "Sweep-start=";Swp_start,"Sweep-stop=";Swp_stop
110 !
120 END
```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A.
30	Loads measurement setup data from diskette file <b>SWP.MES</b> .
50 to 60	Reads start value of VAR1.
70 to 80	Reads stop value of VAR1.

---

## Programming: Measurement Execution

To execute a measurement, you can use :PAGE:SCONtrol subsystem commands.

This section describes the following tasks:

- To execute a sweep or sampling measurement
- To force stress
- To start the knob sweep function
- To control standby units

---

## To Execute a Sweep or Sampling Measurement

1. Send `:PAGE:SCONtrol[:MEASurement]:SINGle` command to HP 4155A/4156A.
  - If you would like to repeat measurements, send `:PAGE:SCONtrol[:MEASurement]:REPeat` command instead of `:PAGE:SCONtrol[:MEASurement]:SINGle` command.
  - If you would like to append measurement, send `:PAGE:SCONtrol[:MEASurement]:APPend` command instead of `:PAGE:SCONtrol[:MEASurement]:SINGle` command.

### Example

#### Example 1.

To execute a sweep or sampling measurement after loading the measurement setup data:

```
10  ASSIGN @Hp4155 TO 717
20  !
30  OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'SWP.MES'"
40  OUTPUT @Hp4155;":PAGE:SCON:SING"
50  !
60  END
```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A.
30	Loads measurement setup data from diskette file <code>SWP.MES</code> .
40	Executes measurement.

## HP 4155A/4156A SCPI Programming

**Programming: Measurement Execution****Example 2.**

To load two measurement setups from diskette and store them into internal memory, then execute the measurements sequentially:

```

10  ASSIGN @Hp4155 TO 717
20  !
30  OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'MEAS1.MES','DISK'"
40  OUTPUT @Hp4155;":MMEM:STOR:STAT 0,'MEM1.MES','MEMORY'"
50  OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'MEAS2.MES','DISK'"
60  OUTPUT @Hp4155;":MMEM:STOR:STAT 0,'MEM2.MES','MEMORY'"
70  !
80  FOR I=1 TO 5
90      OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'MEM1.MES','MEMORY'"
100     OUTPUT @Hp4155;":PAGE:SCON:SING"
110     OUTPUT @Hp4155;":*OPC?"
120     ENTER @Hp4155;Complete
130     DISP "Analyze manually then press [Continue]"
140     PAUSE
150     !
160     OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'MEM2.MES','MEMORY'"
170     OUTPUT @Hp4155;":PAGE:SCON:SING"
180     OUTPUT @Hp4155;":*OPC?"
190     ENTER @Hp4155;Complete
200     DISP "Analyze manually and then press [Continue]"
210     PAUSE
220     !
230     IF I<5 THEN
240         DISP "Move to the next TEG and then press [Continue]"
250         PAUSE
260     END IF
270     !
280 NEXT I
290 !
300 END

```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A.
30 to 60	Loads two measurement setups from diskette, then stores them into internal memory.
90 to 120	Executes first measurement, then waits for measurement completion.
160 to 190	Executes second measurement, then waits for measurement completion.

---

## To Force Stress

1. Send `:PAGE:SCONtrol:STress[:START]` command to HP 4155A/4156A.

Example

### Example 1.

To force stress after loading the stress setup data:

```
10  ASSIGN @Hp4155 TO 717
20  !
30  OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'STRS.STR'"
40  OUTPUT @Hp4155;":PAGE:SCON:STR"
50  !
60  END
```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A.
30	Loads stress setup data from diskette file <code>STRS.STR</code> .
40	Executes stress forcing.

## HP 4155A/4156A SCPI Programming

**Programming: Measurement Execution****Example 2.**

To force stress, then execute sweep measurement:

```
10  ASSIGN @Hp4155 TO 717
20  !
30  OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'STRS.STR'"
40  OUTPUT @Hp4155;":PAGE:SCON:STR"
50  OUTPUT @Hp4155;":*OPC?"
60  ENTER @Hp4155;Complete
70  !
80  OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'SWP.MES'"
90  OUTPUT @Hp4155;":PAGE:SCON:SING"
100 !
110 END
```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A.
30	Loads stress setup data from diskette file <b>STRS.STR</b> .
40	Executes stress forcing.
50 to 60	Waits until stress forcing is completed.
80	Loads measurement setup data from diskette file <b>SWP.MES</b> .
90	Executes sweep measurement.

---

## To Start the Knob Sweep Function

1. Send :PAGE:SCONtrol:KSWEEP[:START] command

Example

To start the knob sweep function:

```
10  ASSIGN @Hp4155 TO 717
20  !
30  OUTPUT @Hp4155;":MMEM:LOAD:STAT 0, 'MEM1.MES', 'MEMORY'"
40  OUTPUT @Hp4155;":PAGE:SCON:KSW"
50  !
60  END
```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A.
30	Loads sweep setup data from internal memory file <b>MEM1</b> .
40	Starts knob sweep function.

HP 4155A/4156A SCPI Programming  
**Programming: Measurement Execution**

---

## To Control Standby Units

To change the standby units from the idle state to the standby state:

1. Send `:PAGE:SCONtrol:STANdby ON`.

You cannot change which units are standby units after you execute this command. Standby units are units for which `STBY` is set to `ON` in the `CHANNELS: CHANNELS DEFINITION` page.

To change the standby units from the standby state to the idle state.

1. Send `:PAGE:SCONtrol:STANdby OFF` to stop standby units.

### Example

To set standby units to standby state (so standby value will be output before and after measurements), then after final measurement, change standby units to idle state:

```

10  ASSIGN @Hp4155 TO 717
20  !
30  OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'SWP1.MES','DISK'"
40  OUTPUT @Hp4155;":PAGE:SCON:STAN ON"
50  OUTPUT @Hp4155;":PAGE:SCON:SING"
60  OUTPUT @Hp4155;":*OPC?"
70  ENTER @Hp4155;Complete
80  OUTPUT @Hp4155;":MMEM:STOR:TRAC DEF,'MEAS1.DAT','DISK'"
90  !
100 OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'SWP2.MES','DISK'"
110 OUTPUT @Hp4155;":PAGE:SCON:SING"
120 OUTPUT @Hp4155;":*OPC?"
130 ENTER @Hp4155;Complete
140 OUTPUT @Hp4155;":PAGE:SCON:STAN OFF"
150 OUTPUT @Hp4155;":MMEM:STOR:TRAC DEF,'MEAS2.DAT','DISK'"
160 END

```

HP 4155A/4156A SCPI Programming  
**Programming: Measurement Execution**

<b>Line Number</b>	<b>Description</b>
10	Assigns I/O path to control HP 4155A/4156A.
30	Loads measurement setup data from diskette file <b>SWP1.MES</b> .
40	The standby units specified in setup data start to output the standby value.
50	Executes measurement.
60 to 70	Waits for completion of measurement. After measurement, standby units output the standby value.
80	Stores measurement data onto a diskette.
100	Loads another measurement setup data from diskette file <b>SWP2.MES</b> . This setup data cannot change which units are the standby units.
110	Executes measurement.
120 to 130	Waits for completion of measurement. After measurement, standby units output the standby value.
140	Standby units stop standby output and change to idle state.
150	Stores measurement data onto a diskette.

---

## Programming: File Operation

This section describes how to use SCPI commands to move data to and from the internal memory or diskette memory of HP 4155A/4156A.

This section covers the following basic file operations:

- To store setup data to diskette or internal memory
- To store measurement data to diskette or internal memory
- To load setup data from diskette or internal memory
- To load measurement data from diskette or internal memory

---

## To Store Setup Data to Diskette or Internal Memory

1. Send `:MMEMory:STORe:STATe` command to HP 4155A/4156A.
  - a. Specify the first parameter to be 0. This parameter has no meaning for HP 4155A/4156A, but is necessary for SCPI compatibility.
  - b. Specify the second parameter:
    - For diskette:  
File name with extension: `.MES` for measurement setup data or `.STR` for stress setup data.
    - For internal memory:  
Internal memory name (`MEM1`, `MEM2`, `MEM3`, or `MEM4`) with extension: `.MES` for measurement setup data or `.STR` for stress setup data.
  - c. Specify the third parameter:
    - For diskette (default): `DISK`
    - For internal memory: `MEMORY`

### Example

To store measurement setup data to a diskette file:

```

10      !
20      ASSIGN @Hp4155 TO 717
30      !
40      OUTPUT @Hp4155;":MMEM:STOR:STAT 0,'SWP.MES','DISK'"
50      !
60      END

```

Line Number	Description
20	Assigns I/O path to control HP 4155A/4156A.
40	Stores measurement setup data to diskette file <code>SWP.MES</code> .

HP 4155A/4156A SCPI Programming  
**Programming: File Operation**

---

## To Store Measurement Data to Diskette or Internal Memory

1. Send :MMEmory:STORe:TRACe command to HP 4155A/4156A.
  - a. Specify the first parameter to be DEFault. This parameter has no meaning for HP 4155A/4156A, but is necessary for SCPI compatibility.
  - b. Specify the second parameter:
    - For diskette:  
File name with extension .DAT
    - For internal memory:  
Internal memory name (MEM1, MEM2, MEM3, or MEM4) with extension .DAT.
  - c. Specify the third parameter:
    - For diskette (default): DISK
    - For internal memory: MEMORY

Example

To store measurement data to a diskette file:

```

10      !
20      ASSIGN @Hp4155 TO 717
30      !
40      OUTPUT @Hp4155;":MME:STOR:TRAC DEF,'SWP.DAT','DISK'"
50      !
60      END

```

Line Number	Description
20	Assigns I/O path to control HP 4155A/4156A.
40	Stores measurement data to diskette file SWP.DAT.

---

## To Load Setup Data from Diskette or Internal Memory

1. Send `:MMEemory:LOAD:STATe` command to HP 4155A/4156A.
  - a. Specify the first parameter to be 0. This parameter has no meaning for HP 4155A/4156A, but is necessary for SCPI compatibility.
  - b. Specify the second parameter:
    - From diskette:  
File name with extension: `.MES` for measurement setup data or `.STR` for stress setup data.
    - From internal memory:  
Internal memory name (`MEM1`, `MEM2`, `MEM3`, or `MEM4`) with extension: `.MES` for measurement setup data or `.STR` for stress setup data.
  - c. Specify the third parameter:
    - From diskette (default): `DISK`
    - From internal memory: `MEMORY`

### Example

To load measurement setup data from a diskette file:

```

10  !
20  ASSIGN @Hp4155 TO 717
30  !
40  OUTPUT @Hp4155;":MMEemory:LOAD:STAT 0,'SWP.MES','DISK'"
50  !
60  END

```

Line Number	Description
20	Assigns I/O path to control HP 4155A/4156A.
40	Loads measurement setup data from diskette file <code>SWP.MES</code> .

HP 4155A/4156A SCPI Programming

**Programming: File Operation**

---

## To Load Measurement Data from Diskette or Internal Memory

1. Send `:MMEMory:LOAD:TRACe` command to HP 4155A/4156A.
  - a. Specify the first parameter to be `DEFault`. This file has no meaning for HP 4155A/4156A, but is necessary for SCPI compatibility.
  - b. Specify the second parameter:
    - From diskette:  
File name with extension `.DAT`
    - From internal memory:  
Internal memory name (`MEM1`, `MEM2`, `MEM3`, or `MEM4`) with extension `.DAT`.
  - c. Specify the third parameter:
    - From diskette (default): `DISK`
    - From internal memory: `MEMORY`

Example

To load measurement data from a diskette file:

```

10      !
20      ASSIGN @Hp4155 TO 717
30      !
40      OUTPUT @Hp4155;":MMEM:LOAD:TRAC DEF, 'SWP.DAT', 'DISK'"
50      !
60      END

```

Line Number	Description
20	Assigns I/O path to control HP 4155A/4156A.
40	Loads measurement data from diskette file <code>SWP.DAT</code> .

---

## Programming: Data Transfer

This section describes the data transfer between a program and HP 4155A/4156A.

The following programming tasks are described in this section:

- To read measurement data from HP 4155A/4156A
- To transfer data to HP 4155A/4156A

HP 4155A/4156A SCPI Programming

**Programming: Data Transfer**

---

## To Read HP 4155/56 Measurement Data

1. Send :DATA? query command to get data variable values (output data, measurement data, user function values) or read-out function values from HP 4155/56 to IBASIC variables.

Example

**Example 1.**

To get measurement data, then store it in a data array:

```

10  DIM I3(1:501)
20  !
30  ASSIGN @Hp4155 TO 717
40  !
50  OUTPUT @Hp4155;":FORM:DATA ASC"
60  !
70  OUTPUT @Hp4155;":DATA? 'I3'"
80  ENTER @Hp4155;I3(*)
90  !
100 END

```

Line Number	Description
30	Assigns I/O path to control HP 4155A/4156A.
50	Specifies ASCII data transfer format.
70 to 80	Gets the values of data variable I3.

**Example 2.**

To get slope of LINE1 for Y2 axis curve on GRAPH/LIST: GRAPHICS page:

```

10  ASSIGN @Hp4155 TO 717
20  !
30  OUTPUT @Hp4155;":DATA? '@L1G2'"
40  ENTER @Hp4155;Slope
50  !
60  PRINT Slope
70  END

```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A.
30 to 40	Gets slope of LINE1 for Y2 axis curve on GRAPH/LIST: GRAPHICS page.

---

## To Transfer Data to HP 4155A/4156A (Using User Variable)

To transfer a user variable to HP 4155A/4156A, use DATA|TRACe subsystem commands. A user variable consists of a name, unit, and numeric data.

Transferred user variable data can be used like other data variables in HP 4155A/4156A. You can perform calculations between measurement results and transferred data, plot transferred data on GRAPH/LIST: GRAPHICS page, or list transferred data on GRAPH/LIST: LIST page.

To transfer numeric data to the HP 4155A/4156A:

1. Define the data transfer format by using :FORMat[:DATA] command.
  - For ASCII data transfer format, send :FORM ASC.
  - For REAL 64-bit length data transfer format, send :FORM REAL, 64.
  - For REAL 32-bit length data transfer format, send :FORM REAL, 32.
2. For REAL data transfer format, define byte order by using :FORMat:BORDer command.
  - For normal order, send :FORM:BORD NORM.
  - For swapped order, send :FORM:BORD SWAP.
3. Define name of the user variable, unit (optional), and number of numeric data by using the :PAGE:CHANnels:UVARiable:DEFine command.

You can also define these parameters by using the :DATA:DEFine and :DATA:UNIT command.

If user variable is already defined, you do not have to perform this step.

4. Transfer data by using :DATA|:TRACe[:DATA] command.

## HP 4155A/4156A SCPI Programming

**Programming: Data Transfer**

Example

**Example 1.**

To transfer data array by using ASCII data transfer format:

```
10  DIM Uvar1(1:5)
20  !
30  ASSIGN @Hp4155 TO 717
40  !
50  Uvar1(1)=1.0
60  Uvar1(2)=1.1
70  Uvar1(3)=1.2
80  Uvar1(4)=1.3
90  Uvar1(5)=1.4
100 !
110 OUTPUT @Hp4155;":FORM:DATA ASC"
120 OUTPUT @Hp4155;":PAGE:CHAN:UVAR:DEF 'UVAR1','V',5"
130 OUTPUT @Hp4155;":TRAC 'UVAR1','";Uvar1(*)
140 !
150  END
```

Line Number	Description
30	Assigns I/O path to control HP 4155A/4156A.
110	Specifies ASCII data transfer format.
120	Defines user variable.
130	Transfers user variable.

**Example 2.**

To transfer data array by using REAL 64-bit data transfer format:

```

10  DIM Uvar1(1:101)
20  INTEGER I
30  !
40  ASSIGN @Hp4155 TO 717
50  ASSIGN @Form_off TO 717;FORMAT OFF
60  !
70  FOR I=1 TO 101
80    Uvar1(I)=SQRT(I)
90  NEXT I
100 !
110 OUTPUT @Hp4155;":FORM REAL,64"
120 OUTPUT @Hp4155;":FORM:BORD NORM"
130 OUTPUT @Hp4155;":PAGE:CHAN:UVAR:DEF 'UVAR1','',101"
140 OUTPUT @Hp4155;":TRAC 'UVAR1',#0";
150 OUTPUT @Form_off;Uvar1(*),END
160 !
170 END

```

Line Number	Description
40	Assigns I/O path to control HP 4155A/4156A.
50	Assigns I/O path to transfer data.
110 to 120	Specifies REAL 64 bit data transfer format.
130	Defines a user variable.
140 to 150	Transfers user variable.

## HP 4155A/4156A SCPI Programming

**Programming: Data Transfer****Example 3.**

To transfer data, then display plot of transferred data and measurement results:

```

10  DIM Uvar1(1:101)
20  !
30  ASSIGN @Hp4155 TO 717
40  !
50  FOR I=1 TO 101
60    Uvar1(I)=SQRT(I)
70  NEXT I
80  !
90  OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'SWP.MES'"
100 OUTPUT @Hp4155;":PAGE:SCON:SING"
110 OUTPUT @Hp4155;":*OPC?"
120 ENTER @Hp4155;Complete
130 !
140 OUTPUT @Hp4155;":FORM ASC"
150 OUTPUT @Hp4155;":DATA:DEF 'UVAR1',101"
160 OUTPUT @Hp4155;":DATA:UNIT 'UVAR1','V'"
170 OUTPUT @Hp4155;":DATA 'UVAR1','";Uvar1(*)"
180 !
190 OUTPUT @Hp4155;":PAGE:DISP:GRAP:Y2:NAME 'UVAR1'"
200 OUTPUT @Hp4155;":PAGE:GLIS"
210 END

```

Line Number	Description
30	Assigns I/O path to control HP 4155A/4156A.
90	Loads measurement setup data from diskette file SWP.MES.
100	Executes measurement.
110 to 120	Waits for measurement completion.
140	Specifies ASCII data transfer format.
150	Defines user variable.
160	Defines unit of user variable.
170	Transfers user variable.
190	Sets user variable to Y2 axis of graph.
200	Displays GRAPH/LIST: GRAPHICS page.

---

## Programming: Print/Plot Operation

For the print/plot operation, you can use :HCOPY subsystem commands.

This section describes the following tasks:

- To output setup data to printer/plotter
- To output graphics result data to printer/plotter
- To output list result data to printer/plotter
- To dump screen image to printer/plotter
- To save hardcopy image to diskette

Before performing above tasks, the following print or plot settings must be set interactively or by remote commands.

We recommend that you save the following settings in a file, then load it before printing or plotting.

- Interface information

Interface	Setting Parameter	Command
HP-IB	printer address	:SYST:COMM:GPIB:RDEV:ADDR
Serial	baud rate (reception)	:SYST:COMM:SER:BAUD
	parity scheme (reception)	:SYST:COMM:SER:PAR
	stop bits (reception)	:SYST:COMM:SER:SBIT
	software pacing scheme (reception)	:SYST:COMM:SER:PACE
	baud rate (transmission)	:SYST:COMM:SER:TRAN:BAUD
	parity scheme (transmission)	:SYST:COMM:SER:TRAN:PAR
	stop bits (transmission)	:SYST:COMM:SER:TRAN:SBIT
	software pacing scheme (transmission)	:SYST:COMM:SER:TRAN:PACE

HP 4155A/4156A SCPI Programming  
**Programming: Print/Plot Operation**

- Printer information

Setting Parameter	Command
color or not	:HCOP:DEV:COL
control language	:HCOP:DEV:LANG
resolution (PCL)	:HCOP:DEV:RES
destination	:HCOP:DEST

- Output Items

Item	Command
Title of the print or plot out	:HCOP:ITEM:ANN:STAT
User defined comment for page group	:HCOP:ITEM:ANN2:STAT
Present date and time of the built-in clock	:HCOP:ITEM:TDST:STAT
Page number of the print or plot out	:HCOP:ITEM:PNUM:STAT
User defined comment for print or plot out	:HCOP:ITEM:LAB:STAT
Graphics plot curve	:HCOP:ITEM:TRAC:STAT
Frame and grid	:HCOP:ITEM:TRAC:GRAT:STAT
Marker, cursor, and data variable coordinate fields, and line parameters (gradients and intercepts)	:HCOP:ITEM:TEXT:STAT
Names, units, and scale of the graph axis	:HCOP:ITEM:TEXT2:STAT

- For built-in IBASIC only

To print from built-in IBASIC, set "HP 4155A/56A is" field on the SYSTEM: MISCELLANEOUS page to SYSTEM CONTROLLER.

---

## To Output Setup Data to Printer/Plotter

1. If you want to output print/plot comment, enter comment by using :HCOPY:ITEM:LABel:TEXT command.
2. Specify the range of setup data to print/plot by sending :HCOPY:OPAGe command.
  - To print/plot present *page* setup data, send :HCOPY:OPAGe CURRent
  - To print/plot present *page group* setup data, send :HCOPY:OPAGe GRoup
  - To print/plot *all* setup data, send :HCOPY:OPAGe ALL
3. Display the page that you want to print/plot by using the appropriate command:

Page	Command
CHANNELS: CHANNEL DEFINITION	:PAGE:CHAN
CHANNELS: USER FUNCTION DEFINITION	:PAGE:CHAN:UFUN
CHANNELS: USER VARIABLE DEFINITION	:PAGE:CHAN:UVAR
MEASURE: SWEEP SETUP	:PAGE:MEAS
MEASURE: SAMPLING SETUP	:PAGE:MEAS:SAMP
MEASURE: PGU SETUP	:PAGE:MEAS:PGUS
MEASURE: MEASURE SETUP	:PAGE:MEAS:MSET
MEASURE: OUTPUT SEQUENCE	:PAGE:MEAS:OSEQ
DISPLAY: DISPLAY SETUP	:PAGE:DISP
DISPLAY: ANALYSIS SETUP	:PAGE:DISP:ANAL
STRESS: CHANNEL DEFINITION	:PAGE:STR
STRESS: STRESS SETUP	:PAGE:STR:SET
STRESS: STRESS FORCE	:PAGE:STR:FORC

HP 4155A/4156A SCPI Programming  
**Programming: Print/Plot Operation**

If you print/plot from built-in IBASIC, change display mode to All Instrument or IBASIC Status by sending :DISPlay[:WINDow]:ALlLocation command.

4. Print/plot the setup data by sending :HCOPy command.

If you print/plot from an external computer, pass Active Controller capability to HP 4155A/4156A after sending :HCOPy command because HP 4155A/4156A requires Active Controller capability to print.

Refer to the following example.

Example

The following two examples load a sweep setup file, then print setup data of the MEASURE: SWEEP SETUP page:

**Example 1.**

From an external computer:

```

10  ASSIGN @Hp4155 TO 717
20  CONTROL 7,3;21
30  !
40  OUTPUT @Hp4155;"*RST"
50  OUTPUT @Hp4155;"*PCB 21"
60  !
70  OUTPUT @Hp4155;"MMEM:LOAD:STAT 0,'SWP.MES'"
80  OUTPUT @Hp4155;"HCOP:ITEM:PNUM:STAT OFF"
90  OUTPUT @Hp4155;"HCOP:ITEM:LAB:TEXT 'This is an example'"
100 OUTPUT @Hp4155;"HCOP:DEST RDEV"
110 OUTPUT @Hp4155;"HCOP:OPAG CURR"
120 !
130 OUTPUT @Hp4155;"PAGE:MEAS"
140 !
150 OUTPUT @Hp4155;"HCOP"
160 REPEAT
170   OUTPUT @Hp4155;"*ESR?"
180   ENTER @Hp4155;Event_status
190   UNTIL BIT(Event_status,1)
200 !
210 PASS CONTROL @Hp4155
220 DISP "Printing"
230 REPEAT
240   STATUS 7,6;Hpib_status
250   UNTIL BIT(Hpib_status,6)
260   DISP "Done"
270 END

```

HP 4155A/4156A SCPI Programming  
**Programming: Print/Plot Operation**

<b>Line Number</b>	<b>Description</b>
10	Assigns I/O path to control HP 4155A/4156A from external computer.
20	Sets the HP-IB address of external computer. This will be necessary to return Active Controller capability from HP 4155A/4156A back to the external computer.
40	Resets HP 4155A/4156A
50	Specifies to pass Active Controller capability back to external computer after printing is completed.
70	Loads measurement setup data from diskette file <b>SWP.MES</b> .
80	Specifies to not print the page number.
90	Defines a print/plot comment.
100	Selects HP-IB interface. If serial interface, change the parameter to "SER".
110 to 130	Specifies to print/plot the setup data of the MEASURE: SWEEP SETUP page.
150 to 190	Sends print command and waits for Active Controller request from HP 4155A/4156A.
210	Passes Active Controller capability to HP 4155A/4156A, then HP 4155A/4156A starts printing.
230 to 250	Waits until printing is complete.

HP 4155A/4156A SCPI Programming  
**Programming: Print/Plot Operation**

**Example 2.**

From built-in IBASIC:

```

10  ASSIGN @Hp4155 TO 800
20  !
30  OUTPUT @Hp4155;"*RST"
40  !
50  OUTPUT @Hp4155;":MMEM:LOAD:STAT 0,'SWP.MES','DISK'"
60  OUTPUT @Hp4155;":HCOP:ITEM:PNUM:STAT OFF"
70  OUTPUT @Hp4155;":HCOP:ITEM:LAB:TEXT 'This is an example'"
80  OUTPUT @Hp4155;":HCOP:DEST RDEV"
90  OUTPUT @Hp4155;":HCOP:OPAG CURR"
100 !
110 OUTPUT @hp4155;":DISP:ALL INST"
110 OUTPUT @Hp4155;":PAGE:MEAS"
120 !
130 OUTPUT @Hp4155;":HCOP"
140 DISP "Printing"
150 OUTPUT @Hp4155;"*OPC?"
160 ENTER @Hp4155;Complete
170 DISP "Done"
180 !
190 END

```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A from built-in IBASIC.
30	Resets HP 4155A/4156A
50	Loads measurement setup data from diskette file SWP.MES.
60	Specifies to not print the page number.
70	Defines a print/plot comment.
80	Selects HP-IB interface. If serial interface, change the parameter to "SER".
90 to 110	Specifies to print/plot the setup data of the MEASURE: SWEEP SETUP page.
130	Starts printing.
150 and 160	Waits until printing is complete.

---

## To Output Graphics Result Data to Printer/Plotter

1. If you want to output print/plot comment, enter comment by using :HCOPY:ITEM:LABel:TEXT command.
2. Display GRAPH/LIST: GRAPHICS page by using :PAGE:GLISt[:GRAPHics] command.  
  
If you print/plot from built-in IBASIC, change display mode to All Instrument or IBASIC Status display mode by sending :DISPlay[:WINDow]:ALLocation command.
3. Execute print/plot by using :HCOPY command.  
  
If you print/plot from an external computer, pass Active Controller capability to HP 4155A/4156A after sending :HCOPY command because HP 4155A/4156A requires Active Controller capability to print.

Refer to the following example.

### Example

The following two examples load a sweep setup file, execute measurement, then print measurement results of GRAPH/LIST: GRAPHICS page:

#### Example 1.

From an external computer:

```

10  ASSIGN @Hp4155 TO 717
20  CONTROL 7,3;21
30  !
40  OUTPUT @Hp4155;"*RST"
50  OUTPUT @Hp4155;"*PCB 21"
60  !
70  OUTPUT @Hp4155;" :MMEM:LOAD:STAT 0,'SWP.MES'"
80  !
90  OUTPUT @Hp4155;" :PAGE:SCON:SING"
100 OUTPUT @Hp4155;"*OPC?"
110 ENTER @Hp4155;Complete
120 !
130 OUTPUT @Hp4155;" :HCOP:DEST RDEV"
140 !
150 OUTPUT @Hp4155;" :PAGE:GLIS"
160 !
170 OUTPUT @Hp4155;" :HCOP"
180 REPEAT
190   OUTPUT @Hp4155;"*ESR?"

```

## HP 4155A/4156A SCPI Programming

**Programming: Print/Plot Operation**

```

200     ENTER @Hp4155;Event_status
210     UNTIL BIT(Event_status,1)
220     !
230     PASS CONTROL @Hp4155
240     DISP "Printing"
250     REPEAT
260         STATUS 7,6;Hpib_status
270     UNTIL BIT(Hpib_status,6)
280     DISP "Done"
290     END

```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A from external computer.
20	Sets the HP-IB address of external computer. This will be necessary to return Active Controller capability from HP 4155A/4156A back to the external computer.
40	Resets HP 4155A/4156A
50	Specifies to pass Active Controller capability back to external computer after printing is completed.
70	Loads measurement setup data from diskette file <b>SWP.MES</b> .
90 to 110	Executes measurement and waits until completed.
130	Selects HP-IB interface. If serial interface, change the parameter to "SER".
150	Changes page to GRAPH/LIST: GRAPHICS page.
170 to 210	Sends print command and waits for Active Controller request from HP 4155A/4156A.
230	Passes Active Controller capability to HP 4155A/4156A, then HP 4155A/4156A starts printing.
250 to 270	Waits until printing is complete.

HP 4155A/4156A SCPI Programming  
**Programming: Print/Plot Operation**

**Example 2.**

From built-in IBASIC:

```

10  ASSIGN @Hp4155 TO 800
20  !
30  OUTPUT @Hp4155; "*RST"
40  !
50  OUTPUT @Hp4155; ":MMEM:LOAD:STAT 0, 'SWP.MES'"
60  !
70  OUTPUT @Hp4155; ":PAGE:SCON:SING"
80  OUTPUT @Hp4155; "*OPC?"
90  ENTER @Hp4155; Complete
100 !
110 OUTPUT @Hp4155; ":HCOP:DEST RDEV"
120 !
130 OUTPUT @Hp4155; ":DISP:ALL INST"
140 OUTPUT @Hp4155; ":PAGE:GLIS"
150 !
160 OUTPUT @Hp4155; ":HCOP"
170 DISP "Printing"
180 OUTPUT @Hp4155; "*OPC?"
190 ENTER @Hp4155; Complete
200 DISP "Done"
210 END

```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A from built-in IBASIC.
30	Resets HP 4155A/4156A
50	Loads measurement setup data from diskette file <b>SWP.MES</b> .
70 to 90	Executes measurement and waits until complete.
110	Selects HP-IB interface. If serial interface, change the parameter to "SER".
130 to 140	Changes page to GRAPH/LIST: GRAPHICS page.
160 to 190	Starts printing and waits until completion.

HP 4155A/4156A SCPI Programming  
**Programming: Print/Plot Operation**

---

## To Output List Results Data to Printer/Plotter

1. Specify the range of measurement results to output by using :HCOPY:LINDEX command.
2. If you want to output print/plot comment, enter comment by using :HCOPY:ITEM:LABEL:TEXT command.
3. Display GRAPH/LIST: GRAPHICS page by using :PAGE:GLIST:LIST command.

If you print/plot from built-in IBASIC, change display mode to All Instrument or IBASIC Status display mode by sending :DISPLAY[:WINDOW]:ALLOCATION command.

4. Execute print/plot by using :HCOPY command.

If you print/plot from an external computer, pass Active Controller capability to HP 4155A/4156A after sending :HCOPY command because HP 4155A/4156A requires Active Controller capability to print.

Refer to the following example.

Example

The following two examples load a sweep setup file, execute measurement, then print measurement results of GRAPH/LIST: LIST page:

**Example 1.**

From an external computer:

```

10  ASSIGN @Hp4155 TO 717
20  CONTROL 7,3;21
30  !
40  OUTPUT @Hp4155;"*RST"
50  OUTPUT @Hp4155;"*PCB 21"
60  !
70  OUTPUT @Hp4155;"MMEM:LOAD:STAT 0,'SWP.MES'"
80  !
90  OUTPUT @Hp4155;"PAGE:SCON:SING"
100 OUTPUT @Hp4155;"*OPC?"
110 ENTER @Hp4155;Complete
120 !
130 OUTPUT @Hp4155;"HCOP:LIND MAX"
140 !
150 OUTPUT @Hp4155;"PAGE:GLIS:LIST"
160 !

```

HP 4155A/4156A SCPI Programming  
**Programming: Print/Plot Operation**

```

170 OUTPUT @Hp4155;":HCOP"
180 REPEAT
190     OUTPUT @Hp4155;"*ESR?"
200     ENTER @Hp4155;Event_status
210 UNTIL BIT(Event_status,1)
220 !
230 PASS CONTROL @Hp4155
240 DISP "Printing"
250 REPEAT
260     STATUS 7,6;Hpib_status
270 UNTIL BIT(Hpib_status,6)
280 DISP "Done"
290 END

```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A from external computer.
20	Sets the HP-IB address of external computer. This will be necessary to return Active Controller capability from HP 4155A/4156A back to the external computer.
40	Resets HP 4155A/4156A
50	Specifies to pass Active Controller capability back to external computer after printing is completed.
70	Loads measurement setup data from diskette file SWP.MES.
90 to 110	Executes measurement and waits until completed.
130	Sets the range of list results to be output.
150	Changes page to GRAPH/LIST: LIST page.
170 to 210	Sends print command and waits for Active Controller request from HP 4155A/4156A.
230	Passes Active Controller capability to HP 4155A/4156A, then HP 4155A/4156A starts printing.
250 and 270	Waits until completion of printing.

HP 4155A/4156A SCPI Programming  
**Programming: Print/Plot Operation**

**Example 2.**

From built-in IBASIC:

```

10  ASSIGN @Hp4155 TO 800
20  !
30  OUTPUT @Hp4155; "*RST"
40  !
50  OUTPUT @Hp4155; ":MMEM:LOAD:STAT 0, 'SWP.MES'"
60  !
70  OUTPUT @Hp4155; ":PAGE:SCON:SING"
80  OUTPUT @Hp4155; "*OPC?"
90  ENTER @Hp4155; Complete
100 !
110 OUTPUT @Hp4155; ":HCOP:LIND MAX"
120 !
130 OUTPUT @Hp4155; ":DISP:ALL INST"
140 OUTPUT @Hp4155; ":PAGE:GLIS:LIST"
150 !
160 OUTPUT @Hp4155; ":HCOP"
170 DISP "Printing"
180 OUTPUT @Hp4155; "*OPC?"
190 ENTER @Hp4155; Complete
200 DISP "Done"
210 END

```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A from built-in IBASIC.
30	Resets HP 4155A/4156A
50	Loads measurement setup data from diskette file SWP.MES.
70 to 90	Executes measurement and waits until completion.
110	Sets the range of list results to be output.
130 to 140	Changes page to GRAPH/LIST: LIST page.
160 to 190	Starts printing and waits until completion.

---

## To Dump Screen Image to Printer/Plotter

1. Display the page to be dumped.
2. Execute print/plot by using :HCOPY:SDUMp command.

If you print/plot from an external computer, pass Active Controller capability to HP 4155A/4156A after sending :HCOPY:SDUMp command because HP 4155A/4156A requires Active Controller capability to print.

Refer to the following example.

### Example

The following two examples load a sweep setup file, execute measurement, display GRAPH/LIST: GRAPHICS page, then dump screen image of GRAPH/LIST: GRAPHICS page to printer/plotter:

#### Example 1.

From an external computer:

```

10  ASSIGN @Hp4155 TO 717
20  CONTROL 7,3;21
30  !
40  OUTPUT @Hp4155;"*RST"
50  OUTPUT @Hp4155;"*PCB 21"
60  !
70  OUTPUT @Hp4155;"MMEM:LOAD:STAT 0,'SWP.MES'"
80  !
90  OUTPUT @Hp4155;"PAGE:SCON:SING"
100 OUTPUT @Hp4155;"*OPC?"
110 ENTER @Hp4155;Complete
120 !
130 OUTPUT @Hp4155;"HCOP:DEST RDEV"
140 !
150 OUTPUT @Hp4155;"PAGE:GLIS"
160 !
170 OUTPUT @Hp4155;"HCOP:SDUM"
180 REPEAT
190   OUTPUT @Hp4155;"*ESR?"
200   ENTER @Hp4155;Event_status
210   UNTIL BIT(Event_status,1)
220   !
230 PASS CONTROL @Hp4155
240 DISP "Printing"
250 REPEAT
260   STATUS 7,6;Hpib_status

```

HP 4155A/4156A SCPI Programming  
**Programming: Print/Plot Operation**

```
270 UNTIL BIT(Hpib_status,6)
280 DISP "Done"
290 END
```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A from external computer.
20	Sets the HP-IB address of external computer. This will be necessary to return Active Controller capability from HP 4155A/4156A back to the computer.
40	Resets HP 4155A/4156A
50	Specifies to pass Active Controller capability back to external computer after printing is completed.
70	Loads measurement setup data from diskette file <b>SWP.MES</b> .
90 to 110	Executes measurement and waits until completed.
130	Selects HP-IB interface. If serial interface, change the parameter to "SER".
150	Changes page to GRAPH/LIST: GRAPHICS page.
170 to 210	Sends screen dump command and waits for Active Controller request from HP 4155A/4156A.
230	Passes Active Controller capability to HP 4155A/4156A, then HP 4155A/4156A starts printing.
250 and 270	Waits until printing is complete.

HP 4155A/4156A SCPI Programming  
**Programming: Print/Plot Operation**

**Example 2.**

From built-in IBASIC:

```

10  ASSIGN @Hp4155 TO 800
20  !
30  OUTPUT @Hp4155;"*RST"
40  !
50  OUTPUT @Hp4155;"MMEM:LOAD:STAT 0,'SWP.MES'"
60  !
70  OUTPUT @Hp4155;"PAGE:SCON:SING"
80  OUTPUT @Hp4155;"*OPC?"
90  ENTER @Hp4155;Complete
100 !
110 OUTPUT @Hp4155;"DISP:ALL INST"
120 OUTPUT @Hp4155;"PAGE:GLIS"
130 !
140 OUTPUT @Hp4155;"HCOP:SDUM"
150 OUTPUT @Hp4155;"*OPC?"
160 ENTER @Hp4155;Complete
170 END

```

Line Number	Description
10	Assigns I/O path to control HP 4155A/4156A from built-in IBASIC.
30	Resets HP 4155A/4156A.
50	Loads measurement setup data from diskette file <b>SWP.MES</b> .
70 to 90	Executes measurement and waits until completion.
110 to 120	Displays GRAPH/LIST: GRAPHICS page.
140 to 160	Starts printing and waits until completion.

HP 4155A/4156A SCPI Programming  
**Programming: Print/Plot Operation**

---

## To Save Hardcopy Image to Diskette

1. To set print/plot destination to diskette file, send :HCOPY:DESTINATION command with MMEMemory parameter.
2. Specify the file name by using :MMEMemory:NAME command.
3. Execute the print/plot operation. Refer to print/plot tasks described previously.

### Example

To load sweep setup file, execute measurement, and then saves a hardcopy image of the measurement results of GRAPH/LIST: GRAPHICS page to a diskette:

```
10  ASSIGN @Hp4155 TO 717
20  !
30  OUTPUT @Hp4155;"*RST"
40  !
50  OUTPUT @Hp4155;":MME:LOAD:STAT 0,'SWP.MES'"
60  !
70  OUTPUT @Hp4155;":PAGE:SCON:SING"
80  OUTPUT @Hp4155;"*OPC?"
90  ENTER @Hp4155;Complete
100 !
110 OUTPUT @Hp4155;":HCOP:DEST MME"
120 OUTPUT @Hp4155;":MME:NAME 'TEST1'"
130 !
140 OUTPUT @Hp4155;":PAGE:GLIS"
150 !
160 OUTPUT @Hp4155;":HCOP"
170 OUTPUT @Hp4155;"*OPC?"
180 ENTER @Hp4155;Complete
190 END
```

HP 4155A/4156A SCPI Programming  
**Programming: Print/Plot Operation**

<b>Line Number</b>	<b>Description</b>
10	Assigns I/O path to control HP 4155A/4156A.
30	Resets HP 4155A/4156A
50	Loads measurement setup data from diskette file <b>SWP.MES</b> .
70 to 90	Executes measurement and waits until completion.
110	Specifies the destination to be diskette.
120	Specifies the diskette file name.
140	Displays GRAPH/LIST: GRAPHICS page.
160 to 180	Starts printing and waits until completion.

---

## Other Programming Tips

This section provides the advanced programming techniques and useful tips:

- Speed Improvement
- Auto-loading of Files

---

### Disabling Instrument Screen Update to Improve Speed

Most of the commands that control and set the HP 4155A/56A will also update the instrument screen.

For example, `:PAGE:CHAN:MODE` command changes the measurement mode. This command also changes the instrument screen to the CHANNELS: CHANNEL DEFINITION page and updates the MEASUREMENT MODE field setting.

This instrument screen update is useful for confirming the settings that were changed by the commands, but it takes time.

You can enable or disable this time consuming instrument screen update as follows:

<code>:DISP OFF</code>	Instrument screen is not updated
<code>:DISP ON</code>	Instrument screen is updated

---

## Auto-loading of Files

The HP 4155A/56A can automatically load files when it is turned on.

### **INIT files for Initial Settings.**

If any setup files named `INIT.MES`, `INIT.STR`, `INIT.CST`, or `INIT.DAT` are on the diskette (in the built-in drive) when the HP 4155A/56A is turned on, the HP 4155A/56A automatically loads these setup files to be the initial settings.

This function saves you the trouble of getting application files every time you turn on the HP 4155A/56A.

#### **INIT.MES and INIT.DAT files**

`INIT.MES` and `INIT.DAT` both contain measurement setup data. If both these files exist on the diskette, the HP 4155A/56A gets `INIT.DAT`, not `INIT.MES`.

### **MEM $n$ o Files.**

If any files named `MEM $n$ o.DAT`, `MEM $n$ o.MES`, or `MEM $n$ o.STR` are on the diskette in the drive, the files are automatically loaded from diskette to internal memory when HP 4155A/56A is turned on. Where `MEM $n$ o` means `MEM1`, `MEM2`, `MEM3`, or `MEM4`, which correspond to the four internal memory areas.

If the same internal memory is specified by multiple files (for example, `MEM1.MES` and `MEM1.DAT`), the priority is as follows:

1. `DAT`
2. `MES`
3. `STR`

### **IBASIC Program File to Auto-execute.**

If an IBASIC program is stored in a file named "AUTOST" on the diskette in the built-in drive, the program is automatically loaded and started when you turn on the HP 4155A/56A.

---

## Programming Example for HP 4145 Users

This section shows a programming example with SCPI commands that performs the same operations as the desired HP 4145 ASP program.

Built-in IBASIC can execute ASP-like commands for controlling the HP 4155A/4156A. Refer to "Creating ASP-like IBASIC Programs" in Chapter 1 on programming this commands.

Following program is the simplest example of creating an HP BASIC program (with SCPI commands) that performs the same operations as the desired HP 4145 ASP program. The ASP program gets a setup file named "VTH" from the diskette, makes a single measurement, then saves measurement to a file named "VTH1".

```

1 GET P      VTH          1 ASSIGN @Hp415x TO 800
2 SINGLE                    10 OUTPUT @Hp415x;":MMEM:LOAD:STAT 0,'VTH.PRO'"
                               20 OUTPUT @Hp415x;":PAGE:SCON:SING"
                               30 OUTPUT @Hp415x;":*OPC?"
                               40 ENTER @Hp415x;Complete
3 SAVE D     VTH1         50 OUTPUT @Hp415x;":MMEM:STOR:TRAC DEF,'VTH1.DAT'"
                               60 END

```

The above HP BASIC program (with SCPI commands) does as follows:

- Line 1 assigns a path named @Hp415x to 800, which is the select code/HP-IB address to use if this is an IBASIC program running in the HP 4155A/56A. If this program will run on an external computer, use the select code of the HP-IB interface and the HP-IB address of the HP 4155A/4156A instead.
- Line 10 gets a measurement setup file named "VTH.MES". So, you need to save setup data to a file named "VTH.MES" on the diskette before executing this program. For an example setup, see "Example Application Setup for Vth Measurement" in Chapter 3.
- Line 20 performs a single measurement.
- Line 50 saves measurement setup and result data to a file named VTH1.DAT.

For built-in help function, which makes it easier to enter the desired SCPI command, see the "To Use the Help Function" in Chapter 1.

HP 4155A/4156A SCPI Programming  
Programming Example for HP 4145 Users

Following shows HP 4145A/B's ASP keywords and corresponding SCPI commands of HP 4155A/4156A:

**Table 4-2. Corresponding HP 4145 ASP and HP 4155A/56A SCPI Commands**

4145A/B	SCPI Commands	Function	Remark
GET P	:MMEM:LOAD:STAT	Gets setup .MES or .PRO file	
SINGLE	:PAGE:SCON:SING	Initiates single measurement	
SAVE D	:MMEM:STOR:TRAC	Saves data to .DAT file	
PLOT	:HCOP	Prints/plots present instrument page.	
CPLLOT	:HCOP:ITEM:TRAC	Prints/plots measurement graph.	
PRINT	:HCOP	Prints/plots present instrument page.	
PAUSE			Use BASIC keyword PAUSE
WAIT			Use BASIC keyword WAIT
PAGE			Set in the Print/Plot setup

HP 4155A/4156A SCPI Programming  
**Programming Example for HP 4145 Users**



---

Running HP 4145A/B  
Program Directly on HP  
4155A/4156A

---

## Running HP 4145A/B Program Directly on HP 4155A/4156A

This chapter describes how to directly run an HP 4145A/B HP-IB program (non-ASP program) on the HP 4155A/4156A with little or no modification. To run these programs directly, you need to use the *HP 4145 syntax command mode* of the HP 4155A/4156A.

### To Enter into HP 4145 Syntax Command Mode

When HP 4155A/4156A is turned on, HP 4155A/4156A is always in HP 4155A/4156A command mode.

To enter into HP 4145 syntax command mode:

- From front-panel

Set **COMMAND SET** field on the **SYSTEM: MISCELLANEOUS** page to **HP4145**.

- From remote control

Send **":SYSTEM:LANGUage COMPatibility"** command to HP 4155A/4156A.

Usually, you can run these programs with no modification. But sometimes small modifications are required due to the following, which are described in this chapter:

- Non-supported commands
- Consideration about Differences

---

## Non-supported Commands

The following HP 4145A/B commands are not supported in HP 4145B syntax command mode:

GL0	Disables HP-GL
GL1	Enables HP-GL overlay graphics
GL2	Enables HP-GL stand-alone graphics
MX	Matrix
SH	Schmoo
SV S	Save ASP file
GT S	Get ASP file
DM3	Display mode Matrix
DM4	Display mode Schmoo
AS1	Auto Sequence Program Start
AS2	Auto Sequence Program Continue
AS3	Auto Sequence Program Stop

If you have HP 4145A/B programs that include any of the above commands, they will not work with the HP 4155A/4156A. Please refer to Chapter 2 in *HP-IB Command Reference* of HP 4155A/4156A for details.

---

## Considerations about Differences

---

### Spot Measurement

HP 4145A/B can execute a spot measurement by setting both start and stop of the sweep to the same value, but the HP 4155A/4156A executes the measurement twice even if you set both start and stop of the sweep to the same value.

---

### Sweep Steps in Logarithmic Step Mode

Calculation algorithm for primary sweep steps in logarithmic step mode is slightly different between HP 4155A/4156A and HP 4145A/B, so step values and number of steps may be different between HP 4155A/4156A and HP 4145A/B.

Running HP 4145A/B Program Directly on HP 4155A/4156A

**Considerations about Differences**

---

## Terminator

If you run your program on an external controller, use <CR> + <LF> as the command terminator if you execute serial polling to read a status of HP 4155A/4156A in your program.

If you use only <CR> or <LF> as command terminator, HP 4155A/4156A may respond with incorrect status.

This is due to the differences of reading and parsing commands between HP 4145A/B and HP 4155A/4156A.

The following example and explanation gives a better understanding of this.

```
10 OUTPUT @Hp415x;"ME1"
20 REPEAT
30 Status=SPOLL(@Hp415x)
40 UNTIL BIT(Status,0)
```

line number	Description
10	triggers measurement and clears the data ready bit (bit1) of status register.
20 to 40	waits until the data ready bit of status register is set to 1.

- When the Terminator is only <CR>

- HP 4145A/B

At line 10:

1. HP 4145A/B starts reading data with RFD line set to false (data bus is halted) after each byte.

In this example:

M ⇒ bus halted ⇒ E ⇒ bus halted ⇒ 1 ⇒ bus halted

2. After receiving 1, HP 4145A/B recognizes valid command ME1, then executes ME1.

At this time, the program is paused because the controller is trying to send <CR>, which is a terminator, but HP 4145A/B has halted data bus and does not receive <CR>.

Running HP 4145A/B Program Directly on HP 4155A/4156A

### Considerations about Differences

3. After HP 4145A/B triggers measurement and clears status bit1, HP 4145A/B reads <CR>, then the program proceeds to next step (line 20).

The program reads the correct status at line 30.

#### □ HP 4155A/4156A

1. At line 10:
  - a. HP 4155A/4156A starts and continues reading data until reading a terminator.  
In this example, HP 4155A/4156A reads ME1<CR>, then halts data bus.
  - b. HP 4155A/4156A starts executing "ME1". At the same time, the external controller can proceed to the next line, because all data of this line has transferred, then program continues.

2. At line 30, controller can read status of HP 4155A/4156A even if RFD line is false. RFD holdoff is not effective for serial polling.

However, the clearing of the status register bit by line 10 may not have been completed yet, so line 30 may get the incorrect status.

- When the Terminator is <CR> + <LF>

The example program for HP 4155A/4156A performs as follows:

1. HP 4155A/4156A starts and continues reading data until reading a terminator.

In this example, HP 4155A/4156A reads ME1<CR>, then halts data bus.

2. HP 4155A/4156A executes "ME1".

At this time, the program is paused because the controller is trying to send <LF>, which is part of the terminator, but HP 4155A/4156A has halted data bus and does not receive <LF>.

3. After HP 4155A/4156A triggers measurement and clears the status bit1, HP 4155A/4156A reads <LF>, then the program proceeds to next step (line 20).

The program reads the correct status at line 30.

---

Sample Application  
Programs

---

## Sample Application Programs

This chapter describes some sample application programs and setup files, which will be helpful for creating your own applications.

All programs and setup files described in this chapter are stored on a DOS formatted 3.5-inch diskette that is provided with your HP 4155A/4156A. You should copy this diskette to a diskette that you will use as your working diskette. The 3.5-inch diskette includes eight programs. This chapter provides only the following three examples.

- Flash EEPROM Test
- TDDB
- Electromigration

See *Sample Application Programs' Guide Book* if you want to use the other programs on the 3.5-inch diskette. All programs are written in HP Instrument BASIC and ready to run in HP 4155A/4156A's HP Instrument BASIC environment.

---

**CAUTION**

These programs are only examples, so you may need to modify these programs and setup files for your own application before executing. If these example programs damage your devices, Hewlett-Packard is *NOT LIABLE* for the damage.

You can modify setup files by remote programming or interactively by front-panel keys.

---

## Flash EEPROM Test

This program forces write and erase pulses, then measures Vth shift.

	name
<b>Program</b>	NOR_TEST
<b>Setup files</b>	ROMVTH.MES, NORWRT.STR, NORERS.STR, NANWRT.STR, NANERS.MES

This program uses NORWRT.STR and NORERS.STR stress setup files for write and erase pulses. These setup files are for NOR type flash EEPROM.

To use this program for NAND type flash EEPROM, please modify as follows to use NANWRT.STR and NANERS.STR stress setup files:

- Modify the following two lines:

```
1990  Wrt_file$="NORWRT.STR"    ! Write Stress Setup File Name
2000  Ers_file$="NORERS.STR"    ! Erase Stress Setup File Name
```

as follows:

```
1990  Wrt_file$="NANWRT.STR"    ! Write Stress Setup File Name
2000  Ers_file$="NANERS.STR"    ! Erase Stress Setup File Name
```

Sample Application Programs  
Flash EEPROM Test

Program Overview

Device connections for NOR and NAND type flash EEPROM are different.

**Device Connection for NOR type flash EEPROM.**

As shown in Figure 6-1, one HP 16440A SMU/Pulse Generator Selector is used to switch units for forcing write pulse and erase pulse, and measuring  $V_{th}$ .

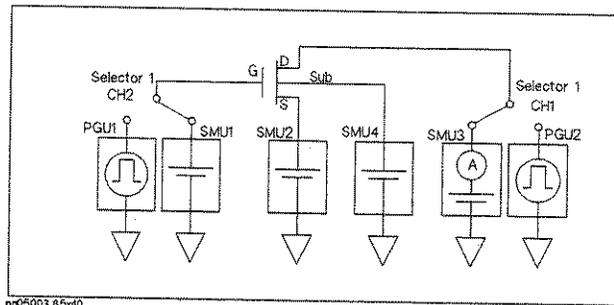


Figure 6-1. Device Connection (NOR Type)

The following table shows the selector's state for each phase:


Table 6-1. Selector's State in Each Phase

Selector Channel	Write	Erase	Vth Measure
CH1 (Drain)	PGU	PGU OPEN	SMU
CH2 (Gate)	PGU	PGU	SMU

Sample Application Programs  
Flash EEPROM Test

**Device Connection for NAND type flash EEPROM.**

As shown in Figure 6-2, two HP 16440A SMU/Pulse Generator Selectors are used to switch units for forcing write pulse and erase pulse, and measuring  $V_{th}$ .

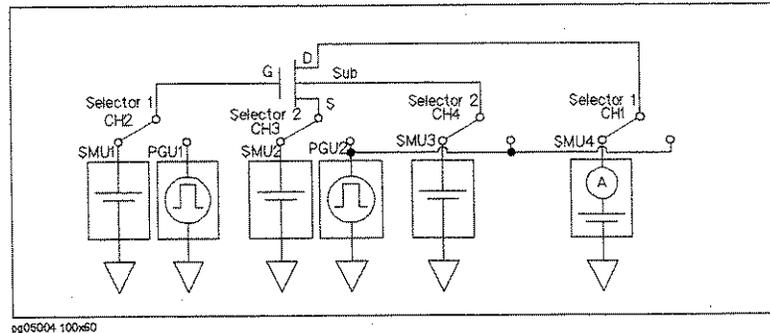

**Figure 6-2. Device Connection (NAND Type)**

Table 6-2 shows the selector's state for each phase:

**Table 6-2. Selector's State in Each Phase**

Selector Channel	Write	Erase	$V_{th}$ Measure
CH1 (Drain)	PGU	PGU	SMU
CH2 (Gate)	PGU	PGU	SMU
CH3 (Source)	PGU	PGU	SMU
CH4 (Substrate)	PGU	PGU	SMU



Sample Application Programs  
Flash EEPROM Test

Line	Description
1570	initializes HP 4155A/4156A.
	enables the Service Request "Enable" Register for Command, Execution, Device-dependent, and Query errors to generate service requests.
1580 and 1590	enables service request from HP 4155A/56A to interrupt program.
1610	defines names of measurement setup files for Vth measurement and stress setup files for write stress and erase stress, and other stress setup.
1620	loads measurement setup file for Vth measurement and stress setup files for write and erase into internal memories.
1650	<i>Meas_points</i> is specified in subprogram "Test_setting".
1660	forces write and erase pulses. Refer to "Stress_loop" for details.
1690 and 1700	loads measurement setup file for Vth measurement and stress setup file for write pulse from internal memories.
1710	forces last write pulse, then measures Vth. Refer to "Vth_meas".
1730	loads stress setup file for erase pulse from an internal memory.
1740	forces last erase pulse, then measures Vth. Refer to "Vth_meas".
1760	transfers measurement results (Vth shifts) to HP 4155A/4156A.
1770	displays measurement results.
1880	stores measurement results onto the diskette.

Sample Application Programs  
Flash EEPROM Test

Stress\_loop

Subprogram "Stress\_loop" to force write and erase stress is shown below:

```

2610 Stress_loop:SUB Stress_loop(INTEGER I)
2620   COM @Hp4155,@Form_off,Start_time,End_time
2630   COM /Meas_info/ INTEGER Meas_points,REAL Str,Str_num,Meas_str_num(*)
2640   INTEGER K
2650   REAL Str_end
2660   !
2670   OUTPUT @Hp4155;":STAT:MEAS:EVEN?"
2680   ENTER @Hp4155;K
2690   OUTPUT @Hp4155;":STAT:MEAS:ENAB 267"
2700   !
2710   OUTPUT @Hp4155;":PAGE:SCDN:STAN ON"
2720   Str_end=Meas_str_num()-1
2730   FOR Str=Str_num TO Str_end
2740     DISP VAL$(Str);"/";VAL$(Meas_str_num(I))
2750     OUTPUT @Hp4155;"MEM:LOAD:STAT 0,'MEM2','MEMORY';:PAGE:SCDN:STR;*WAI"
2760     OUTPUT @Hp4155;"MEM:LOAD:STAT 0,'MEM3','MEMORY';:PAGE:SCDN:STR"
2770     OUTPUT @Hp4155;"*GPC?"
2780     ENTER @Hp4155;A
2790   NEXT Str
2800   !
2810   Str_num=Str
2820   OUTPUT @Hp4155;":PAGE:SCDN:STAN OFF"
2830   OUTPUT @Hp4155;":STAT:MEAS:ENAB 0"
2840 SUBEND

```

Line	Description
2670 and 2680	clears the Measurement/Stress Status "Event" register.
2690	enables Bit 0 (A/D Overflow), 1 (Oscillation Status), 3 (Compliance Status), and 8 (PGU Status) of enable mask for the Measurement/Stress Status "Event" register.
2710	enables standby state so that state does <i>not</i> become idle between write and erase stress. If state becomes idle, the relay will switch after every write and erase stress, which will damage the relay.
2730 to 2790	repeats forcing write/erase pulses until one write/erase pulse before next Vth measurement.
2820	disables standby state.

Sample Application Programs  
Flash EEPROM Test

Vth\_meas

Subprogram "Vth\_meas" to force last write and erase pulses, then measure Vth:

```

2860 Vth_meas:SUB Vth_meas(Str_type$,INTEGER I)
2870   COM @Hp4155,@Form_off,Start_time,End_time
2880   COM /Meas_info/ INTEGER Meas_points,REAL Str,Str_num,Meas_str_num(*)
2890   COM /Meas_data/ Vth_w(*),Vth_e(*)
2900   INTEGER K
2910   !
2920   OUTPUT @Hp4155;":PAGE:SCDN:STR;*0PC?"
2930   ENTER @Hp4155;A
2940   DISP Str_type$;" Times = "&VAL$(Str_num)
2950   !
2960   OUTPUT @Hp4155;":PAGE:CHAN:COMM 'Flash ROM Vth Meas. @"&Str_type$&" Times = "&VAL$(Str_num)&"'"
2970   OUTPUT @Hp4155;":PAGE:GLIS"
2980   OUTPUT @Hp4155;":DISP ON"
2990   OUTPUT @Hp4155;":PAGE:SCDN:SING;*0PC?"
3000   ENTER @Hp4155;A
3010   OUTPUT @Hp4155;":DISP OFF"
3020   OUTPUT @Hp4155;":STAT:MEAS:EVEN?"
3030   ENTER @Hp4155;K
3040   OUTPUT @Hp4155;":TRAC? 'VTH'"
3050   SELECT Str_type$
3060   CASE "Write"
3070     ENTER @Hp4155;Vth_w(I)
3080     PRINT USING "#,4X,DESZ,10X,SD.DDD";Str_num,Vth_w(I)
3090   CASE "Erase"
3100     ENTER @Hp4155;Vth_e(I)
3110     PRINT USING "10X,SD.DDD,7X,SD.DDE";Vth_e(I),Vth_w(I)-Vth_e(I)
3120   END SELECT
3130 SUBEND

```

Line	Description
2990 and 3000	executes Vth measurement and waits until completion.
3040	gets measurement result.

Sample Application Programs  
Flash EEPROM Test

---

## Program Customization

This section describes how to customize program for your own application.

### Subprogram "Test\_setting".

In this subprogram, you may need to customize the following:

- Name of setup files.

If you want to use your own measurement or stress setup files, store the files on diskette, then modify the file names on the following lines:

- Measurement setup file name for Vth measurement.

```
1980 Vth_file$="ROMVTH.MES" ! Vth Measurement Setup File Name
```

- Stress setup file name for write pulse.

```
1990 Wrt_file$="NORWRT.STR" ! Write Stress Setup File Name
```

- Stress setup file name for erase pulse.

```
2000 Ers_file$="NORERS.STR" ! Erase Stress Setup File Name
```

- File name for saving measurement results.

Following two lines create following file name for saving measurement results: *time.DAT*. To change this file name, modify these lines:

```
2010 Save_file$=TIME$(TIMEDATE) ! File Name for saving measurement results
2020 Save_file$=Save_file$[1,2]&Save_file$[4,5]&Save_file$[7,7]&".DAT"
```

- Number of times to repeat measurement (FOR loop of Main Program)  
Following line specifies how many times to measure Vth during stress.

```
2030 Meas_points=16 ! Number of times to repeat Measurement
```

- Stress pulse count data.

For example, if **Meas\_points=4**, a total of ten write/erase pulses are forced, and Vth is measured after 1st, 2nd, 5th, and 10th pulse.

```
2060 Str_num: ! ! Stress Pulse Count data
2070 DATA 1, 2, 5
2080 DATA 10, 20, 50
2090 DATA 100, 200, 500
2100 DATA 1000, 2000, 5000
2110 DATA 10000, 20000, 50000
2120 DATA 100000, 200000, 500000
2130 DATA 1000000
```

Sample Application Programs  
Flash EEPROM Test

**Measurement setup file for Vth measurement (for NOR type).**

Measurement setup for Vth measurement is stored in "ROMVTH.MES" file on provided diskette. As described previously, if you use your own setup file with a different file name, change line 2000.

In the ROMVTH.MES file, the following is set up. You can modify these settings in the ROMVTH.MES file or your own file:

- Gate voltage sweep setup.

Start voltage	Stop voltage	Sweep step	Compliance
0 V	8 V	10 mV	1 nA

SMU1 is gate voltage source as shown in Figure 6-1 and Figure 6-2.

- Constant source setup.

Units	Output	Compliance
SMU2 (Source)	0 V	100 $\mu$ A
SMU3 (Drain)	100 mV	2 $\mu$ A
SMU4 (Substrate)	0 V	100 $\mu$ A

- Analysis function for Vth extraction.

In this example, Vth is extracted by moving marker to the point where Id is 1  $\mu$ A, then reading the voltage at that point. Refer to the following user function and auto-analysis setup:

User Function Definition		
Name	Unit	Definition
Vth	V	@MX

Analysis Setup	
Setup	Definition
Marker	Id = 1 $\mu$ A
Interpolate	ON

## Sample Application Programs

**Flash EEPROM Test****Stress setup file for write pulse of NOR type.**

Stress setup for write pulse of NOR type is stored in "NORWRT.STR" file on provided diskette. As described previously, if you use your own setup file with a different file name, change line 2010.

In the NORWRT.STR file, the following is set up. You can modify these settings in the NORWRT.STR file or your own file:

- PGUs

Unit	Period	Width	Delay Time	Peak Value	Base Value	Leading Time	Trailing Time	Impedance
<b>PGU1 (Gate)</b>	1.03 ms	1.02 ms	0.0 s	14 V	0 V	1 $\mu$ s	1 $\mu$ s	50 ohm
<b>PGU2 (Drain)</b>		1.00 ms	10 $\mu$ s	7 V	0 V	1 $\mu$ s	1 $\mu$ s	50 ohm

- Constant source setup

Unit	Source	Compliance
<b>SMU2 (Source)</b>	0 V	100 mA
<b>SMU4 (Substrate)</b>	0 V	100 mA

**Stress setup file for erase pulse of NOR type.**

Stress setup for erase pulse is stored on "NORERS.STR" file on provided diskette. As described previously, if you use your own setup file with a different file name, change line 2020.

In the NORERS.STR file, the following is set up. You can modify these settings in the NORERS.STR file or your own file:

- Constant source setup

Unit	Source	Compliance
<b>SMU2 (Source)<sup>1</sup></b>	11 V	100 mA
<b>SMU4 (Substrate)</b>	0 V	100 mA

<sup>1</sup> Erase pulse source

- Erase pulse width

Pulse width of erase pulse is specified as stress DURATION and set to 20ms.

## Sample Application Programs

## Flash EEPROM Test

**Stress setup file for write pulse of NAND type.**

Stress setup for write pulse of NAND type is stored in "NANWRT.STR" file on provided diskette. As described previously, you must change line 2010 to "NANWRT.STR" or your own custom file name.

In the NANWRT.STR file, the following is set up. You can modify these settings in the NANWRT.STR file or your own file:

- PGUs

Unit	Period	Width	Delay Time	Peak Value	Base Value	Leading Time	Trailing Time	Impedance
PGU1 (Gate)	413 $\mu$ s	400 $\mu$ s	0.0 s	20 V	0 V	10 $\mu$ s	10 $\mu$ s	50 ohm

Unit	Source	Impedance
PGU2 <sup>1</sup>	0 V	50 ohm

<sup>1</sup> Connected to drain, source, and substrate, and set to constant source.

**Stress setup file for erase pulse of NAND type.**

Stress setup for erase pulse of NAND type is stored in "NANERS.STR" file on provided diskette. As described previously, you must change line 2020 to "NANERS.STR" or your own custom file name.

In the NANERS.STR file, the following is set up. You can modify these settings in the NANERS.STR file or your own file:

- PGUs

Unit	Period	Width	Delay Time	Peak Value	Base Value	Leading Time	Trailing Time	Impedance
PGU2 <sup>1</sup>	5.02 ms	5.00 ms	0.0 s	20 V	0 V	10 $\mu$ s	10 $\mu$ s	50 ohm

<sup>1</sup> connected to drain, source, and substrate.

Unit	Source	Impedance
PGU1 <sup>1</sup>	0 V	50 ohm

<sup>1</sup> Connected to gate, and set to constant source

Sample Application Programs  
Flash EEPROM Test

---

## Program Listing

```

1000 !*****
1010 !*
1020 !* FILE:          NOR_TEST
1030 !* DESCRIPTION:  Program for NOR-FLASH RDM Stress Test.
1040 !*
1050 !* AUTHOR:       Yukoh Iwasaki , YHP
1060 !* CREATED:     12/21/1993
1070 !* MODIFIED:    01/25/1994
1080 !* PRODUCT:     HP4156A,HP4156A
1090 !* REVISION:    Rev.A.01.02
1100 !*
1110 !* (c) Copyright 1994, Hewlett-Packard Co,
1120 !*               All rights reserved.
1130 !*
1140 !*
1150 !* Customer shall have the personal, non-
1160 !* transferable rights to use, copy or modify
1170 !* this SAMPLE PROGRAM for Customer's internal
1180 !* operations. Customer shall use the SAMPLE
1190 !* PROGRAM solely and exclusively for its own
1200 !* purpose and shall not license, lease, market
1210 !* or distribute the SAMPLE PROGRAM or modification
1220 !* or any part thereof.
1230 !*
1240 !* HP shall not be liable for the quality,
1250 !* performance or behavior of the SAMPLE PROGRAM.
1260 !* HP especially disclaims that the operation of
1270 !* the SAMPLE PROGRAM shall be uninterrupted or
1280 !* error free. This SAMPLE PROGRAM is provided
1290 !* AS IS.
1300 !*
1310 !* HP DISCLAIMS THE IMPLIED WARRANTIES OF
1320 !* MERCHANTABILITY AND FITNESS FOR A PARTICULAR
1330 !* PURPOSE.
1340 !*
1350 !* HP shall not be liable for any infringement
1360 !* of any patent, trademark, copyright or other
1370 !* proprietary rights by the SAMPLE PROGRAM or
1380 !* its use. HP does not warrant that the SAMPLE
1390 !* PROGRAM is free from infringements or such
1400 !* rights of third parties. However, HP will not
1410 !* knowingly infringe or deliver a software that
1420 !* infringes the patent, trademark, copyright or
1430 !* other proprietary right of a third party.
1440 !*
1450 !*****
1460 Start_time=TIMEDATE
1470 ASSIGN @Hp4156 TO 800
1480 ASSIGN @Form_off TO 800;FORMAT OFF
1490 COM @Hp4155,@Form_off,Start_time,End_time
1500 COM /File_name/ Vth_file$[12],Wrt_file$[12],Ers_file$[12],Save_file$[12]
1510 COM /Meas_info/ INTEGER Meas_points,REAL Str,Str_num,Meas_str_num(1:55)
1520 COM /Meas_data/ Vth_w(1:55),Vth_e(1:55)
1530 COM /Err/ Err_num(1:6),Err_message$(1:6)[50]

```

Sample Application Programs  
Flash EEPROM Test

```

1540 INTEGER I
1550 !
1560 !!!!!!!!!!!!!!! Main !!!!!!!!!!!!!!!
1570 CALL Init_hp4155
1580 ON INTR 8 CALL Err_check
1590 ENABLE INTR 8;2
1600 !
1610 CALL Test_setting
1620 CALL Get_file
1630 !
1640 Str_num=1
1650 FOR I=1 TO Meas_points
1660   CALL Stress_loop(I)
1670   IF Meas_str_num(I)>4500 THEN CALL Calibration
1680   !
1690   OUTPUT @Hp4155;"MMEM:LOAD:STAT 0,'MEM2.STR','MEMORY'"
1700   OUTPUT @Hp4155;"MMEM:LOAD:STAT 0,'MEM1.MES','MEMORY'"
1710   CALL Vth_meas("Write",I)
1720   !
1730   OUTPUT @Hp4155;"MMEM:LOAD:STAT 0,'MEM3.STR','MEMORY'"
1740   CALL Vth_meas("Erase",I)
1750   !
1760   CALL Trans_data(I)
1770   CALL Stress_graph(I)
1780   !
1790   IF Vth_w(I)<.1 OR Vth_e(I)<.1 THEN
1800     PRINT "   ### The Device is broken. Test Aborted ###"
1810     PRINT "           Final Stress Times : ";Str_num
1820     CALL Final_session
1830     STOP
1840   END IF
1850   Str_num=Str_num+1
1860 NEXT I
1870 !
1880 CALL Final_session
1890 !
1900 END
1910 !
1920 !!!!!!!!!!!!!!! Sub !!!!!!!!!!!!!!!
1930 Test_setting:SUB Test_setting
1940   CD# /File_name/ Vth_file$,Wrt_file$,Ers_file$,Save_file$
1950   CD# /Meas_info/ INTEGER Meas_points,REAL Str,Str_num,Meas_str_num(*)
1960   CD# /Meas_data/ Vth_w(*),Vth_e(*)
1970   !
1980   Vth_file$="RDNVTH.MES"   ! Vth Measurement Setup File Name
1990   Wrt_file$="NDRWRT.STR"   ! Write Stress Setup File Name
2000   Ers_file$="NDRERS.STR"   ! Erase Stress Setup File Name
2010   Save_file$=TIME$(TIMEDATE) ! File Name for saving measurement results
2020   Save_file$=Save_file$[1,2]&Save_file$[4,5]&Save_file$[7,7]&".DAT"
2030   Meas_points=16           ! Number of times to repeat Measurement
2040   REDIM Meas_str_num(1:Meas_points)
2050   REDIM Vth_w(1:Meas_points),Vth_e(1:Meas_points)
2060   Str_num: !               ! Stress Pulse Count data
2070   DATA      1,      2,      5
2080   DATA     10,     20,     50
2090   DATA    100,    200,    500
2100   DATA   1000,   2000,   5000
2110   DATA  10000, 20000, 50000
2120   DATA 100000,200000,500000
2130   DATA 1000000
2140   RESTORE Str_num

```

## Sample Application Programs

## Flash EEPROM Test

```

2150 READ Meas_str_num(*)
2160 SUBEND
2170 !
2180 Init_hp4155:SUB Init_hp4155
2190 COM @Hp4155,@Form_off,Start_time,End_time
2200 !
2210 CLEAR SCREEN
2220 CLEAR @Hp4155
2230 OUTPUT @Hp4155;"*RST"
2240 OUTPUT @Hp4155;"*CLS"
2250 OUTPUT @Hp4155;"*STAT:PRES"
2260 OUTPUT @Hp4155;"*ESE 60;*SRE 34;*DPC?"
2270 ENTER @Hp4155;A
2280 OUTPUT @Hp4155;"*DISP:WIND:ALL BST"
2290 OUTPUT @Hp4155;"*DISP OFF"
2300 PRINT "          <<< Flash ROM Stress Test >>>"
2310 PRINT "Stress Times  Vth Write [V]  Vth Erase [V]  Diff [V]"
2320 SUBEND
2330 !
2340 Get_file:SUB Get_file
2350 COM @Hp4155,@Form_off,Start_time,End_time
2360 COM /File_name/ Vth_file$,Wrt_file$,Ers_file$,Save_file$
2370 !
2380 OUTPUT @Hp4155;"*MEM:COPY "&Vth_file$&"', 'DISK', 'MEM1.MES', 'MEMORY'"
2390 OUTPUT @Hp4155;"*MEM:COPY "&Wrt_file$&"', 'DISK', 'MEM2.STR', 'MEMORY'"
2400 OUTPUT @Hp4155;"*MEM:COPY "&Ers_file$&"', 'DISK', 'MEM3.STR', 'MEMORY'"
2410 SUBEND
2420 !
2430 Calibration:SUB Calibration
2440 COM @Hp4155,@Form_off,Start_time,End_time
2450 !
2460 OUTPUT @Hp4155;"*PAGE:SYST:CDI"
2470 OUTPUT @Hp4155;"*DISP ON"
2480 OUTPUT @Hp4155;"*CAL:ALL?"
2490 ENTER @Hp4155;A
2500 SELECT A
2510 CASE 0
2520 OUTPUT @Hp4155;"*PAGE:GLIS"
2530 OUTPUT @Hp4155;"*DISP OFF"
2540 CASE ELSE
2550 PRINT "   *** Calibration FAIL ,Test Aborted ***"
2560 CALL Final_session
2570 STOP
2580 END SELECT
2590 SUBEND
2600 !
2610 Stress_loop:SUB Stress_loop(INTEGER I)
2620 COM @Hp4155,@Form_off,Start_time,End_time
2630 COM /Meas_info/ INTEGER Meas_points,REAL Str,Str_num,Meas_str_num(*)
2640 INTEGER K
2650 REAL Str_end
2660 !
2670 OUTPUT @Hp4155;"*STAT:MEAS:EVEN?"
2680 ENTER @Hp4155;K
2690 OUTPUT @Hp4155;"*STAT:MEAS:ENAB 267"
2700 !
2710 OUTPUT @Hp4155;"*PAGE:SCON:STAN ON"
2720 Str_end=Meas_str_num(I)-1
2730 FOR Str=Str_num TO Str_end
2740 DISP VAL$(Str);"/";VAL$(Meas_str_num(I))
2750 OUTPUT @Hp4155;"*MEM:LOAD:STAT 0,'MEM2','MEMORY';:PAGE:SCON:STR;*WA!"

```

Sample Application Programs  
Flash EEPROM Test

```

2760 OUTPUT @Hp4155;"MMEN:LOAD:STAT 0,'MEM3','MEMDRY';:PAGE:SCON:STR"
2770 OUTPUT @Hp4155;"*DPC?"
2780 ENTER @Hp4155;A
2790 NEXT Str
2800 !
2810 Str_num=Str
2820 OUTPUT @Hp4155;"PAGE:SCON:STAN OFF"
2830 OUTPUT @Hp4155;"STAT:MEAS:ENAB 0"
2840 SUBEND
2850 !
2860 Vth_meas:SUB Vth_meas(Str_type$,INTEGER I)
2870 COM @Hp4155,@Form_off,Start_time,End_time
2880 COM /Meas_info/ INTEGER Meas_points,REAL Str,Str_num,Meas_str_num(*)
2890 COM /Meas_data/ Vth_w(*),Vth_e(*)
2900 INTEGER K
2910 !
2920 OUTPUT @Hp4155;"PAGE:SCON:STR;*DPC?"
2930 ENTER @Hp4155;A
2940 DISP Str_type$;" Times = "&VAL$(Str_num)
2950 !
2960 OUTPUT @Hp4155;"PAGE:CHAN:COM 'Flash ROM Vth Meas. @"&Str_type$&" Times = "&VAL$(Str_num)&""
2970 OUTPUT @Hp4155;"PAGE:GLIS"
2980 OUTPUT @Hp4155;"DISP DN"
2990 OUTPUT @Hp4155;"PAGE:SCON:SING;*DPC?"
3000 ENTER @Hp4155;A
3010 OUTPUT @Hp4155;"DISP OFF"
3020 OUTPUT @Hp4155;"STAT:MEAS:EVEN?"
3030 ENTER @Hp4155;K
3040 OUTPUT @Hp4155;"TRAC? 'VTH'"
3050 SELECT Str_type$
3060 CASE "Write"
3070 ENTER @Hp4155;Vth_w(I)
3080 PRINT USING "#,4X,DESZ,10X,SD.DDD";Str_num,Vth_w(I)
3090 CASE "Erase"
3100 ENTER @Hp4155;Vth_e(I)
3110 PRINT USING "10X,SD.DDD,7X,SD.DDE";Vth_e(I),Vth_w(I)-Vth_e(I)
3120 END SELECT
3130 SUBEND
3140 !
3150 Trans_data:SUB Trans_data(INTEGER I)
3160 COM @Hp4155,@Form_off,Start_time,End_time
3170 COM /Meas_info/ INTEGER Meas_points,REAL Str,Str_num,Meas_str_num(*)
3180 COM /Meas_data/ Vth_w(*),Vth_e(*)
3190 !
3200 REDIN Meas_str_num(1:1),Vth_w(1:1),Vth_e(1:1)
3210 OUTPUT @Hp4155;"TRAC:DEL:ALL"
3220 OUTPUT @Hp4155;"TRAC:DEF 'Stress',"&VAL$(I)
3230 OUTPUT @Hp4155;"TRAC:DEF 'VthWRT',"&VAL$(I)
3240 OUTPUT @Hp4155;"TRAC:DEF 'VthERS',"&VAL$(I)
3250 OUTPUT @Hp4155;"TRAC:UNIT 'Stress','Times'"
3260 OUTPUT @Hp4155;"TRAC:UNIT 'VthWRT','V'"
3270 OUTPUT @Hp4155;"TRAC:UNIT 'VthERS','V'"
3280 !
3290 OUTPUT @Hp4155;"FORM:DATA REAL,64"
3300 OUTPUT @Hp4155;"FORM:BORD NORM"
3310 OUTPUT @Hp4155;"TRAC 'Stress',#0";
3320 OUTPUT @Form_off;Meas_str_num(*),END
3330 OUTPUT @Hp4155;"TRAC 'VthWRT',#0";
3340 OUTPUT @Form_off;Vth_w(*),END
3350 OUTPUT @Hp4155;"TRAC 'VthERS',#0";
3360 OUTPUT @Form_off;Vth_e(*),END

```

## Sample Application Programs

## Flash EEPROM Test

```

3370 OUTPUT @Hp4155;":FORM:DATA ASCII"
3380 REDIM Meas_str_num(1:Meas_points),Vth_w(1:Meas_points),Vth_e(1:Meas_points)
3390 SUBEND
3400 !
3410 Stress_graph:SUB Stress_graph(INTEGER I)
3420 CDM @Hp4155,@Form_off,Start_time,End_time
3430 CDM /Meas_info/ INTEGER Meas_points,REAL Str,Str_num,Meas_str_num(*)
3440 !
3450 OUTPUT @Hp4155;":PAGE:CHAN:CDM 'Flash ROM Vth Shift(Stress=&VAL$(Meas_str_num(I))&)"'"
3460 OUTPUT @Hp4155;":PAGE:CHAN:UFUN:DEF 'Diff','V','VthWRT-VthERS'"
3470 !
3480 OUTPUT @Hp4155;":PAGE:DISP:GRAP:X:NAME 'Stress'"
3490 OUTPUT @Hp4155;":PAGE:DISP:GRAP:Y1:NAME 'VthWRT'"
3500 OUTPUT @Hp4155;":PAGE:DISP:GRAP:Y2:NAME 'VthERS'"
3510 OUTPUT @Hp4155;":PAGE:DISP:GRAP:X:SCAL LOG"
3520 OUTPUT @Hp4155;":PAGE:DISP:GRAP:X:MIN 1"
3530 OUTPUT @Hp4155;":PAGE:DISP:GRAP:X:MAX "&VAL$(MAX(Meas_str_num(Meas_points),2))"
3540 OUTPUT @Hp4155;":PAGE:DISP:GRAP:Y1:SCAL LIN"
3550 OUTPUT @Hp4155;":PAGE:DISP:GRAP:Y1:MIN 0"
3560 OUTPUT @Hp4155;":PAGE:DISP:GRAP:Y1:MAX 7"
3570 OUTPUT @Hp4155;":PAGE:DISP:GRAP:Y2:SCAL LIN"
3580 OUTPUT @Hp4155;":PAGE:DISP:GRAP:Y2:MIN 0"
3590 OUTPUT @Hp4155;":PAGE:DISP:GRAP:Y2:MAX 7"
3600 !
3610 OUTPUT @Hp4155;":PAGE:DISP:DVAR:DEL 'VTH'"
3620 OUTPUT @Hp4155;":PAGE:DISP:DVAR 'Diff'"
3630 !
3640 OUTPUT @Hp4155;":PAGE:DISP:ANAL:LINE1:NO DE DIS"
3650 OUTPUT @Hp4155;":PAGE:DISP:ANAL:LINE2:NO DE DIS"
3660 OUTPUT @Hp4155;":PAGE:DISP:ANAL:MARK:DIS"
3670 !
3680 OUTPUT @Hp4155;":PAGE:GLIS:INT OFF"
3690 OUTPUT @Hp4155;":PAGE:GLIS:LINE OFF"
3700 OUTPUT @Hp4155;":PAGE:GLIS:MARK ON"
3710 OUTPUT @Hp4155;":PAGE:GLIS:MARK:DIR:X MAX"
3720 !
3730 OUTPUT @Hp4155;":DISP ON;:DISP OFF"
3740 SUBEND
3750 !
3760 Final_session:SUB Final_session
3770 CDM @Hp4155,@Form_off,Start_time,End_time
3780 CDM /File_name/ Vth_file$,Wrt_file$,Ers_file$,Save_file$
3790 CDM /Meas_info/ INTEGER Meas_points,REAL Str,Str_num,Meas_str_num(*)
3800 CDM /Err/ Err_num(*),Err_message$(*)
3810 !
3820 IF Str_num-1=Meas_str_num(Meas_points) THEN
3830 Save_file$="D"&Save_file$
3840 PRINT "===== Measurement Completed !!! ====="
3850 PRINT "Final Stress Times : ";Str_num-1
3860 ELSE
3870 Save_file$="F"&Save_file$
3880 END IF
3890 !
3900 PRINT "Save Data File Name : ";Save_file$
3910 PRINT "Test Duration : ";
3920 End_time=TIMEDATE
3930 PRINT DATES$(Start_time);",",TIMES$(Start_time);" ~ ";DATES$(End_time);",",TIMES$(End_time)
3940 !
3950 DISABLE INTR 8
3960 OUTPUT @Hp4155;":MMEM:STOR:TRAC DEF,'"&Save_file$&',"DISK'"
3970 OUTPUT @Hp4155;":*OPC?"

```

Sample Application Programs  
Flash EEPROM Test

```

3980 ENTER @Hp4155;A
3990 OUTPUT @Hp4155;":SYST:ERR?"
4000 ENTER @Hp4155;Err_num(1),Err_message$(1)
4010 IF Err_num(1)<>0 THEN PRINT "### ";Err_num(1);Err_message$(1);" ###"
4020 !
4030 OUTPUT @Hp4155;":DISP:ALL INST"
4040 OUTPUT @Hp4155;":PAGE:GLIS"
4050 OUTPUT @Hp4155;":DISP ON"
4060 SUBEND
4070 !
4080 Err_check:SUB Err_check
4090 COM @Hp4155,@Form_off,Start_time,End_time
4100 COM /Err/ Err_num(*),Err_message$(*)
4110 INTEGER I,J
4120 !
4130 I=0
4140 REPEAT
4150 I=I+1
4160 OUTPUT @Hp4155;":SYST:ERR?"
4170 ENTER @Hp4155;Err_num(I),Err_message$(I)
4180 UNTIL Err_num(I)=0
4190 !
4200 IF I=1 THEN
4210 CALL Meas_stat_check
4220 ELSE
4230 FOR J=1 TO I-1
4240 PRINT "### ERROR Occurred ###";Err_num(J);Err_message$(J)
4250 DISP "### ERROR Occurred ###";Err_num(J);Err_message$(J)
4260 NEXT J
4270 CALL Meas_stat_check
4280 PRINT " === Test Aborted ==="
4290 CALL Final_session
4300 STOP
4310 END IF
4320 SUBEND
4330 !
4340 Meas_stat_check:SUB Meas_stat_check
4350 COM @Hp4155,@Form_off,Start_time,End_time
4360 COM /Meas_info/ INTEGER Meas_points,REAL Str,Str_num,Meas_str_num(*)
4370 INTEGER K
4380 !
4390 OUTPUT @Hp4155;":STAT:MEAS:EVEN?"
4400 ENTER @Hp4155;K
4410 !
4420 IF K<>0 THEN
4430 PRINT "### Abnormal Stress Status Event Occurred ###";K
4440 PRINT " at Stress Number = ";Str;"[Times]"
4450 PRINT " === Test Aborted ==="
4460 CALL Final_session
4470 STOP
4480 END IF
4490 SUBEND

```

---


## Time Dependent Dielectric Breakdown (TDDB)

This setup forces a constant voltage to the gate until the gate oxide breakdowns or a maximum time limit is reached, then calculates the total forced electric charge.

	name
<b>Program</b>	none
<b>Setup file</b>	TDDB.MES

---

## Application Overview

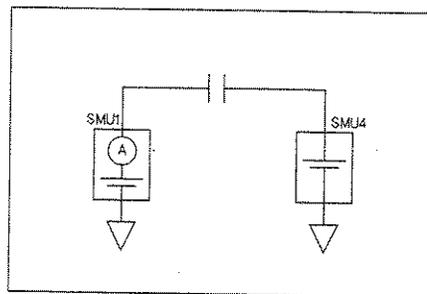

pg05002 60x40

**Figure 6-3. Device Connection**

The measurement flow is as follows:

1. Forces a constant voltage to the gate.
2. Measures gate current by sampling measurement.
3. If gate current exceeds specified threshold, measurement is stopped.
4. Calculates total electric charge that was forced by using a user function with definition `INTEG(Ig, @TIME)`.

Sample Application Programs  
**Time Dependent Dielectric Breakdown (TDDB)**

## Customization

Measurement setup file is stored in "TDDB.MES" file on provided diskette. In the TDDB.MES file, the following is set up. You can modify these settings in the TDDB.MES file or your own file, then use the setup for your own application.

- Constant source setup

Units	Output	Compliance
<b>SMU1 (Gate)</b>	20 V	1.001 $\mu$ A
<b>SMU4 (Substrate)</b>	0 V	100 $\mu$ A

- Sampling Parameters

Mode	Initial interval	No. of samples	Total samp. time
Thinned-out	100 ms	1001	999.9 s

- Stop Condition

This setup is used to judge the oxide breakdown. If gate current exceeds the specified threshold, measurement is stopped.

Enable Delay	Threshold
200 ms	1 $\mu$ A

---


## Electromigration

This setup forces a constant current to the DUT (metal), measures time-to-failure of DUT, then calculates the total forced electric charge.

	name
Program	none
Setup file	EM.MES

---

## Application Overview

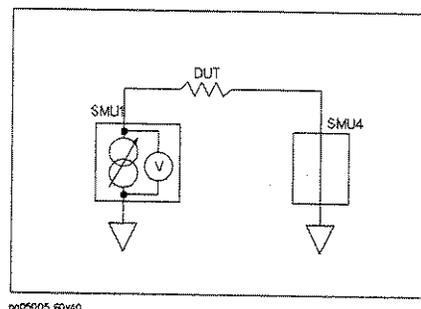

**Figure 6-4. Device Connection**

The measurement flow is as follows:

1. Forces constant current.
2. Monitors DUT voltage by sampling measurement.
3. If the DUT voltage reaches specified threshold, the forcing stops.
4. Calculates total electric charge that was forced by using a user function with definition `INTEG(Idut1, @TIME)`.

---

## Customization

Measurement setup file is stored in "EM.MES" file on provided diskette. In the EM.MES file, the following is set up. You can modify these settings in the EM.MES file or your own file, then use the setup for your own application.

- Constant source setup

Units	Output	Compliance
SMU1	50 mA	20.002 V

- Sampling Parameters

Mode	Initial interval	No. of samples	Total samp. time
Linear	1 s	10001	AUTO <sup>1</sup>

<sup>1</sup> Initial interval \* No. of samples

- Stop Condition

If the DUT voltage exceeds the specified threshold, measurement is stopped.

Enable Delay	Threshold
20 ms	20 V

Sample Application Programs  
**Electromigration**



---

**Manual Changes  
Depending on ROM Version**

---

## Manual Changes Depending on ROM Version

HP 4155A/4156A may vary slightly, depending on the version of the ROM based firmware. The information in this manual applies to an HP 4155A/4156A with the following ROM version.

### Manual Applies to this ROM Version

ROM	ROM Version
HOSTC	01.02

### ROM version

To confirm your ROM version, check the SOFTWARE REVISION field on the SYSTEM: CONFIGURATION page.

This chapter contains information for customizing this manual so that it is correct for the HP 4155A/4156A that you are using.

To customize this manual for your HP 4155A/4156A, refer to the following table, and make the manual changes depending on the ROM version of your HP 4155A/56A.

### Manual Changes by ROM version

ROM version (HOSTC)	Make Manual Changes
01.00	1
01.01	1

---

## Change 1


Add the following section to Chapter 5.

---

### Timing Considerations

You may need timing considerations for synchronizing measurements with external instruments.

Following example program controls a DMM with the HP 4155A/4156A. Measurement circuit is shown below:

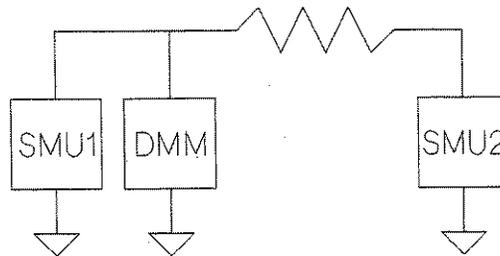

The HP 4155A/4156A has an HP-IB I/O buffer and can receive commands before executing previous command. So the execution order of HP 4155A/4156A and DMM is different from the order in the program.

In the following example, the HP 3458A receives a measurement trigger command right after the HP 4155A/4156A receives a force voltage trigger.

## Manual Changes Depending on ROM Version

## Change 1

But due to the HP-IB I/O buffer, the voltage measurement is made by HP 3458A before HP 4155A/4156A forces voltage.

```

10  ASSIGN @Hp415x TO 717
20  ASSIGN @Hp3458 TO 722
30  !
40  DIM Moe_data$[17]
50  DIM Dmm_data$[100]
60  !
70  OUTPUT @Hp3458;"RESET"           ! Reset DMM
80  OUTPUT @Hp3458;"TARM HOLD"      ! Suspend reading
90  OUTPUT @Hp3458;"DCV 10"        ! DC voltage 10 V range
100 OUTPUT @Hp3458;"NPLC 1"        ! Integ NPLC=1
110 OUTPUT @Hp3458;"AZERO OFF"     ! Auto zero off
120 !
130 OUTPUT @Hp415x;"US"            ! User mode
140 OUTPUT @Hp415x;"IT1 CA0 BC"    ! Integ Short, Cal off, buffer clear
150 Force_v=1.5
160 OUTPUT @Hp415x;"DV1, 1, ";Force_v;" , 20E-3" ! SMU1 forces 1.5 V
170 OUTPUT @Hp415x;"DV2, 1, 0, 20E-3" ! SMU2 forces 0 V
180 !
190 OUTPUT @Hp3458;"TARM SGL"      ! V meas trigger to DMM
200 ENTER @Hp3458;Dmm_data$
210 !
220 OUTPUT @Hp415x;"T11"          ! I meas trigger to 4155/56
230 ENTER @Hp415x;Moe_data$
240 !
250 PRINT Dmm_data$
260 PRINT Moe_data$
270 !
280 OUTPUT @Hp415x;"DV1; DV2"     ! Reset SMU1 & SMU2
290 END

```

Following is an example of test result:

```

-3.870540468E-04
NAI-1.256700E-010

```

DMM should measure about 1.5 V, but does not because DMM measures before SMU1 forces voltage.

You can insert a WAIT command before sending trigger command to the DMM (HP 3458A). In this example, 0.1 sec should be sufficient. So, you can insert the following in the above program:

```

181  WAIT .1                       ! <<< Modified

```

Or maybe the following is a better way to modify the program. The measurement order is changed. First, SMU measures current, and controller enters data from HP 4155A/4156A. Then, the measurement trigger is sent to the DMM.

Manual Changes Depending on ROM Version  
Change 1

```
10 ASSIGN @Hp415x TO 717
20 ASSIGN @Hp3458 TO 722
30 !
40 DIM Moe_data$(17)
50 DIM Dmm_data$(100)
60 !
70 OUTPUT @Hp3458;"RESET"
80 OUTPUT @Hp3458;"TARM HOLD"
90 OUTPUT @Hp3458;"DCV 10"
100 OUTPUT @Hp3458;"NPLC 1"
110 OUTPUT @Hp3458;"AZERO OFF"
120 !
130 OUTPUT @Hp415x;"US"
140 OUTPUT @Hp415x;"IT1 CA0 BC"
150 Force_v=1.5
160 OUTPUT @Hp415x;"DV1, 1, ";Force_v;", 20E-3"
170 OUTPUT @Hp415x;"DV2, 1, 0, 20E-3"
180 !
190 OUTPUT @Hp415x;"T11"
200 ENTER @Hp415x;Moe_data$
210 !
220 OUTPUT @Hp3458;"TARM SGL" ! <<< Changed order of measurement
230 ENTER @Hp3458;Dmm_data$
240 !
250 PRINT Dmm_data$
260 PRINT Moe_data$
270 !
280 OUTPUT @Hp415x;"DV1; DV2"
290 END
```

The test result should be similar to following example:

```
1.499301638E+00
NAI+7.150000E-011
```

Manual Changes Depending on ROM Version

**Change 1**

## Data Length Considerations

When one of the following commands is sent from a controller to the HP 4155A/4156A in the *HP 4145 syntax command mode*, the HP 4155A/4156A outputs data to the controller.

- DO Data output request in the system mode
- TI Current measurement trigger and data output request in the user mode
- TV Voltage measurement trigger and data output request in the user mode
- ID Identification output

### Different Data Length in System Mode.

The following program is equivalent to sample program 1 listed in Section 3 of HP 4145B manual. This program is an example of data output in the system mode. This program controls instrument to measure the IC-VC characteristics of a bipolar transistor, then returns IC data to the controller.

```

10  ASSIGN @Hp415x TO 717
20  DIM A$(1100)
30  OUTPUT @Hp415x;"IT1 CA1 DRO BC"
40  OUTPUT @Hp415x;"DE CH1, 'VE', 'IE', 3, 3; CH2, 'VB', 'IB', 2, 2; CH3, 'VC', 'IC', 1, 1; CH4"
50  OUTPUT @Hp415x;"VS1; VS2;VM1; VM2"
60  OUTPUT @Hp415x;"SS VR1, 0, 1, .05, 50E-3; IP 10E-6, 10E-6, 4, 3"
70  OUTPUT @Hp415x;"SM DM1; XM 'VC', 1, 0, 1; YA 'IC', 1, 0, 10E-3"
80  OUTPUT @Hp415x;"MD ME1"
90  A=SPOLL(@Hp415x)
100 IF BIT(A,0)=0 THEN 90
110 OUTPUT @Hp415x;"DO 'IC'"
120 ENTER @Hp415x;A$
130 PRINT A$
140  END

```

You must execute this program in the *HP 4145 syntax command mode* of the HP 4155A/4156A. The following will be displayed on the controller's screen. (Or you can display on HP 4155A/4156A's screen by changing the select code/HP-IB address assigned in line 10 to 800, which will execute the program using built-in IBASIC of the HP 4155A/4156A.) As you can see, the length of data string A\$ is too short, so not all the data is displayed.

```

N-9.985900E-006,N-5.923600E-007,N+6.087900E-005,N+3.772100E-004,
N+1.106890E-003,N+1.642500E-003,N+1.824900E-003,N+1.870700E-003,
N+1.880600E-003,N+1.883000E-003,N+1.884600E-003,N+1.885700E-003,
N+1.886900E-003,N+1.887900E-003,N+1.888900E-003,N+1.889800E-003,
N+1.890800E-003,N+1.891700E-003,N+1.892600E-003,N+1.893000E-003,
N+1.893800E-003,N-1.996500E-005,N+1.685000E-006,N+1.426100E-004,

```

Manual Changes Depending on ROM Version  
Change 1

```
N+8.321900E-004,N+2.290100E-003,N+3.298500E-003,N+3.635200E-003,
N+3.723200E-003,N+3.744200E-003,N+3.750600E-003,N+3.753600E-003,
N+3.756300E-003,N+3.758900E-003,N+3.761200E-003,N+3.763700E-003,
N+3.765400E-003,N+3.767700E-003,N+3.769600E-003,N+3.771600E-003,
N+3.773400E-003,N+3.775300E-003,N-2.994400E-005,N+5.370400E-006,
N+2.329300E-004,N+1.301200E-003,N+3.434400E-003,N+4.893700E-003,
N+5.395400E-003,N+5.534300E-003,N+5.571000E-003,N+5.582700E-003,
N+5.588900E-003,N+5.593600E-003,N+5.597700E-003,N+5.601500E-003,
N+5.605600E-003,N+5.608800E-003,N+5.612400E-003,N+5.615200E-003,
N+5.618500E-003,N+5.621600E-003,N+5.624300E-003,N-3.992100E-005,
N+1.014500E-005,N+3.293800E-004,N+1.772600E-003,N+4.517500E-003,
N+6.396500E-
```

This is because the length of data output from the HP 4155A/4156A and HP 4145B is different as follows:

*HP 4145B data output format in system mode:*

```
X+NN.NNNE+NN,X+NN.NNNE+NN, ... X+NN.NNNE+NN[cr][!r]
```

Each data consists of 13 characters (including a comma) except for the last data, which consists of 12 characters.

*HP 4155A/4156A data output format in system mode of 4145 syntax command mode:*

```
X+N.NNNNNE+NNN,X+N.NNNNNE+NNN,X+N.NNNNNE+NNN, ... X+N.NNNNNE+NNN
```

Each data consists of 16 characters (including a comma), except for the last data, which consists of 15 characters.

X                   Data status  
+                   + or -  
N                   Numeric character

In this example, number of data points is  $21 \times 4 = 84$  (21 Var1 steps and 4 Var2 steps). So, length of data string A\$ should be at least 1343 (16 char  $\times$  84 points - 1). Please modify line 20 as follows:

```
20. DIM A$(1343)                   ! <<< Modified 16 x 84 - 1 = 1343
```

The result display is as follows (all data is displayed):

```
N-9.984700E-006,N-E.928300E-007,N+6.088100E-005,N+3.772600E-004,
N+1.107160E-003,N+1.642400E-003,N+1.825100E-003,N+1.870300E-003,
N+1.879800E-003,N+1.882700E-003,N+1.884200E-003,N+1.885200E-003,
N+1.886500E-003,N+1.887500E-003,N+1.888700E-003,N+1.889700E-003,
N+1.890600E-003,N+1.891200E-003,N+1.892300E-003,N+1.893100E-003,
N+1.893700E-003,N-1.996500E-005,N+1.678600E-006,N+1.426100E-004,
N+8.323300E-004,N+2.290400E-003,N+3.298600E-003,N+3.634900E-003,
N+3.722600E-003,N+3.743600E-003,N+3.749900E-003,N+3.753400E-003,
N+3.756100E-003,N+3.758400E-003,N+3.761100E-003,N+3.763100E-003,
N+3.765100E-003,N+3.767500E-003,N+3.769500E-003,N+3.771400E-003,
N+3.773200E-003,N+3.775000E-003,N-2.994400E-005,N+5.361800E-006,
```

Manual Changes Depending on ROM Version

**Change 1**

N+2.329700E-004, N+1.301800E-003, N+3.434800E-003, N+4.893700E-003,  
N+5.394900E-003, N+5.533900E-003, N+5.570600E-003, N+5.582100E-003,  
N+5.588300E-003, N+5.593000E-003, N+5.597400E-003, N+5.601100E-003,  
N+5.605200E-003, N+5.608200E-003, N+5.611900E-003, N+5.614500E-003,  
N+5.617800E-003, N+5.620900E-003, N+5.624000E-003, N-3.991500E-005,  
N+1.014500E-005, N+3.295400E-004, N+1.773000E-003, N+4.518400E-003,  
N+6.396700E-003, N+7.076300E-003, N+7.288700E-003, N+7.354300E-003,  
N+7.376500E-003, N+7.387800E-003, N+7.395800E-003, N+7.402100E-003,  
N+7.408100E-003, N+7.413600E-003, N+7.418800E-003, N+7.423500E-003,  
N+7.428000E-003, N+7.432600E-003, N+7.437100E-003, N+7.440800E-003

**Different Data Length in User Mode.**

The following program is equivalent to sample program 2 listed in Section 3 of the HP 4145B manual. This program is an example of data output in the user mode.

```

10  ASSIGN @Hp415x TO 717
20  DIM A$[14]
30  OUTPUT @Hp415x;"US"
40  OUTPUT @Hp415x;"IT1 CA0 BC"
50  Force_v=1.5
60  OUTPUT @Hp415x;"DV1, 1, ";Force_v;", 20E-3"
70  OUTPUT @Hp415x;"DV2, 1, 0, 20E-3"
80  OUTPUT @Hp415x;"TI1"
90  ENTER @Hp415x;A$
100 PRINT A$
110 OUTPUT @Hp415x;"DV1; DV2"
120 END

```

This program displays the following for example. As you can see, the length of data string A\$ is too short, so not all the data is displayed.

```
NAI+4.300000E-
```

This is because the length of data output from the HP 4155A/4156A and HP 4145B is different as follows:

*HP 4145B data output format in user mode (14 characters):*

```
XXX+NN.NNNE+NN[cr][lf]
```

*HP 4155A/4156A data output format in user mode of 4145 syntax command mode (17 characters):*

```
XXX+N.NNNNNNE+NNN[cr][lf]
```

X	Data status
+	+ or -
N	Numeric character

So, you need to change line 20 as follows:

```
20  DIM A$[17]          ! <<< Modified
```

The test result will be as follows:

```
NAI+4.300000E-013
```

Manual Changes Depending on ROM Version

**Change 1**

**TV and ID Commands**

For "TV" command, the data length is 14 characters for HP 4145, and 17 characters for HP 4155A/4156A. For "ID" command, the data length is 16 characters for HP 4145 and 41 characters for HP 4155A/4156A. So, if these commands are used, you need to change the data string length accordingly.



Index

---

## Index

- A
- ALL IBASIC**
  - screen. *See* screen modes
- All Instrument**
  - screen. *See* screen modes
- ANALYSIS SETUP**
  - Vth measurement example, 3-26
- append**
  - SCPI command for append measurement, 4-13
- application**
  - sample programs. *See* sample programs
- array data**
  - transferring to file. *See* file
- ASCII**
  - data transfer, 3-19, 4-27, 4-28
  - file type. *See* LIF
- ASP programs**
  - converting HP 4145 ASP program to IBASIC, iv, 1-41-44
  - converting HP 4145 ASP program to SCPI, iv, 4-50
  - corresponding IBASIC directives, 1-48, 2-31-37
  - corresponding SCPI commands, 4-51
- ASSIGN**
  - IBASIC keyword, 3-19, 4-6
- auto**
  - execute file at power on. *See* AUTOST
  - loading of files at power on, 4-49
  - scaling for image dumps, 1-47
  - sequence programs. *See* ASP programs
- AUTOSCALE directive**, 1-47, 1-48, 2-34
- AUTOST**
  - auto execute file at power on, 4-49
- B
- BASIC**
  - HP BASIC. *See* HP BASIC
  - IBASIC. *See* IBASIC
- BDAF**
  - file type. *See* binary
- binary**
  - file type, 3-19
- Blue key**
  - shift status. *See* shift status
- branching**
  - IBASIC. *See* IBASIC

- breakdown
  - TDDB sample test program. *See* TDDB
- built-in IBASIC controller, iv, 1-2, 3-5, 4-2, 4-4
  - HP-IB. *See* HP-IB
  - select code. *See* HP-IB
- byte
  - length for transfer. *See* REAL
  - order transfer format. *See* REAL
- C** carriage return (CR)
  - terminator. *See* terminator
- carrier
  - hot injection sample test program. *See* hot carrier injection
- case sensitive
  - variable names, 3-17
- CAT
  - IBASIC listing command, 1-17
  - IBASIC softkey, 1-26
- changing
  - manual depending on ROM version, 7-2
  - setup data values. *See* measurement program
- CHANNEL DEFINITION
  - example setup for  $V_{th}$ , 3-23
- clearing
  - IBASIC program. *See* IBASIC editor
- closing
  - I/O path for data transfer. *See* I/O
- codes
  - select. *See* HP-IB
- COM blocks
  - IBASIC. *See* IBASIC
- commands
  - help function. *See* help function
  - HP 4145 ASP. *See* ASP programs
  - HP 4145 commands not supported, 5-3
  - HP 4145 syntax command mode, iv, 4-4, 5-2, 7-6
  - HP 4155/56 command mode, iv, 4-4, 5-2
  - IBASIC keywords. *See* IBASIC
  - SCPI. *See* SCPI
  - terminator. *See* terminator
- computer
  - external. *See* external controller
- controller
  - external. *See* external controller
- converting
  - HP 4145 programs to HP 4155/56. *See* HP 4145
- CPLOT
  - ASP keyword, 1-48, 4-51

- CR
  - terminator. *See* terminator
- CREATE
  - IBASIC keyword, 3-18
- creating
  - HP 4145 ASP-like program. *See* ASP programs
  - measurement program. *See* measurement program
- CRT display
  - HP 4155/56, 2-28
  - select code, 2-27
- cursor
  - IBASIC editor. *See* IBASIC editor
- CURVEPLOT directive, 1-44, 1-48, 2-37

**D** data

- array. *See* array data
- ASCII. *See* ASCII
- extraction. *See* transferring
- internal HP 4155/56, 3-19
- length considerations for previous ROM versions, 7-6
- numeric. *See* numeric data
- string. *See* string data
- transfer. *See* transferring
- DATA? query command, 3-17, 4-26
- data variables
  - names are case sensitive, 3-17
  - transferring from HP 4155/56 to IBASIC variables, 1-46, 3-17, 4-26
- DAT suffix. *See* file types
- DEFUSERVAR directive, 1-48, 2-36
- Delete line
  - editor softkey, 1-12, 1-33
- deleting
  - characters. *See* IBASIC editor
  - lines. *See* IBASIC editor
- dielectric
  - TDDB sample test program. *See* TDDB
- differences
  - between ROM versions, 7-2
  - HP 4145 and HP 4155/56 programs, 5-2
- direct
  - execution of HP 4145 program. *See* HP 4145
- directives
  - IBASIC. *See* IBASIC
- disk drive
  - built-in, 2-27, 2-30
  - external controller drive, 1-36, 1-38
  - external HP 4155/56 drive, 1-27
- diskette, 2-30

- listing contents. *See* listing
- loading results from. *See* measurement program
- loading setup data from. *See* measurement program
- saving hardcopy image to diskette. *See* printing
- saving program to. *See* IBASIC
- saving results to. *See* measurement program
- saving setup data to. *See* measurement program
- DISP command, 4-48
- display
  - changing setup parameters from program, 3-10
  - CRT. *See* CRT
  - disabling update to improve speed. *See* speed
  - Display** key
    - IBASIC key group, 1-4, 2-3
- DISPLAY SETUP
  - Vth measurement example, 3-26
- DOS
  - diskette format, 2-30
  - file, 3-18
- downloading
  - program to HP 4155A/4156A. *See* external controller
- drive
  - disk. *See* disk drive
- dumping
  - screen. *See* printing

## E **Edit.** *See* execution status

### **EDIT**

- IBASIC softkey, 1-7, 1-30

### editor

- IBASIC. *See* IBASIC editor

### EEPROM

- flash sample test program. *See* flash EEPROM test

### electromigration

- sample program, 6-22

### ELSE

- IBASIC keyword, 1-21

### END

- IBASIC keyword. *See* IBASIC

### **End edit**

- editor softkey, 1-8, 1-11, 1-30

### END IF

- IBASIC keyword, 1-21

### END WHILE

- IBASIC keyword, 1-21

### ENTER

- IBASIC keyword, 3-19, 4-6, 4-26

### error messages

- IBASIC. *See* IBASIC
- example
  - application programs. *See* sample programs
- EXECUTE keyword, 1-48, 2-15, 2-25, 2-31
  - converting ASP to IBASIC program, 1-41
- executing
  - HP 4145 program directly. *See* HP 4145
  - IBASIC command. *See* IBASIC
  - IBASIC program. *See* IBASIC
  - measurement from program. *See* measurement program
- execution status (IBASIC), 2-5
  - Edit, 2-5, 2-14, 2-15
  - Idle, 2-5, 2-11, 2-12
  - Input?, 2-5, 2-11, 2-13
  - Pause, 2-5, 2-11, 2-12
  - Run, 2-5, 2-11, 2-13
- exiting
  - IBASIC editor. *See* IBASIC editor
- external
  - controller. *See* external controller
  - disk drive. *See* disk drive
  - instruments. *See* external instruments
  - keyboard. *See* keyboard
- external controller, iv, 1-35
  - controlling HP 4155/56 from external program, 3-7, 4-4
  - controlling state of IBASIC program in HP 4155A/4156A, 1-40
  - downloading IBASIC program to HP 4155A/4156A, 1-36
  - HP-IB. *See* HP-IB
  - select codes. *See* HP-IB
  - terminator caution for running HP 4145 program directly, 5-5
  - uploading IBASIC program from HP 4155A/4156A, 1-38
- external instruments
  - timing considerations for previous ROM version, 7-3
- extraction
  - data from HP 4155/56 to IBASIC variable. *See* transferring

## F file

- binary type. *See* binary
- creating from program, 3-18
- DOS type. *See* DOS
- LIF type. *See* LIF
- saving hardcopy image to. *See* printing
- saving HP 4155/56 data to diskette. *See* measurement program
- transferring array data to, 3-20
- transferring numeric data to, 3-20
- transferring string data to, 3-20
- types. *See* file types

Filer, 1-17

- file types
  - ASCII. *See* ASCII
  - BDAT. *See* binary
  - binary. *See* binary
  - DAT, 1-42, 4-49, 4-51
  - DOS. *See* DOS
  - LIF. *See* LIF
  - MES, 1-42, 4-49, 4-51
  - PRD, 1-42, 4-51
  - STR, 4-49
- flash EEPROM test
  - sample program, 6-3
- FOR
  - IBASIC keyword, 1-21
- forcing
  - stress. *See* measurement program
- FORMAT
  - data transfer format for user variable, 4-27
  - IBASIC keyword, 3-19
- front-panel
  - editor keys. *See* IBASIC editor
  - IBASIC keys. *See* IBASIC
  - select code, 2-27
- functions
  - user. *See* user function data

**G****GET**

- IBASIC softkey, 1-27
- GET P
  - ASP keyword, 1-48, 4-51
- GETSETUP directive, 1-41, 1-48, 2-32
- getting
  - HP 4155/56 data to IBASIC variable. *See* transferring
  - IBASIC program. *See* IBASIC
  - setup file. *See* setup data
- graphics
  - printing result data. *See* printing
- Green key
  - shift status. *See* shift status

- H** hardcopy. *See* printing
  - HCOP system commands, 4-32
  - help function
    - IBASIC commands, 1-5
    - SCPI commands, 1-5
    - using to create program, 3-5
  - Help** key, 1-5, 3-5
  - HP 4145
    - commands not supported on HP 4155/56, 5-2
    - converting ASP programs to IBASIC. *See* ASP programs
    - converting HP-IB programs to SCPI, iv
    - differences from HP 4155/56 programs, 5-2
    - previous ROM version considerations, 7-6
    - running programs directly on HP 4155/56, iv, 5-2
    - syntax command mode. *See* commands
  - HP 4155/56
    - command mode. *See* commands
    - differences from HP 4145 programs, 5-2
    - previous ROM version considerations, 7-2
  - HP BASIC, 1-2, 3-5
  - HP-IB
    - address, 3-5, 4-6
    - internal pseudo interface, 2-27, 2-28, 4-4
    - printer address, 4-31
    - select code, 2-27, 2-28, 3-5, 4-4, 4-6
  - HP Instrument BASIC. *See* IBASIC
- 
- I** IBASIC, iv. *See also* measurement program
    - branching, 1-21
    - built-in controller. *See* built-in IBASIC controller
    - COM blocks, 1-22, 3-5
    - controlling from external computer. *See* external controller
    - corresponding ASP keywords. *See* ASP programs
    - creating a file. *See* file
    - creating measurement program. *See* measurement program
    - directives, 2-31-37
    - editor. *See* IBASIC editor
    - END statement, 1-8
    - error messages, 2-4
    - executing commands, 1-25
    - executing programs, 1-9, 1-25
    - front-panel keys, 2-8
    - getting a program, 1-18
    - help function. *See* help function
    - HP-IB. *See* HP-IB
    - I/O resources. *See* I/O
    - keyboard keys, 2-19-24
    - keywords, 1-21, 2-25

- keywords (non-standard in HP 4155/56), 2-25
- keywords (not allowed in HP 4155/56), 2-26
- printing results. *See* printing
- relation to HP BASIC, 1-2
- repeating, 1-21
- saving program to diskette, 1-17, 1-28
- SCPI commands. *See* SCPI commands
- screen modes. *See* screen modes
- select codes. *See* HP-IB
- softkeys, 2-6, 2-11-18
- status. *See* execution status
- subprograms, 1-22

IBASIC editor, 1-10-20, 1-29-34

- clearing a program, 1-18
- creating HP 4145 ASP-like programs. *See* ASP programs
- creating measurement program. *See* measurement program
- deleting characters, 1-32
- deleting lines, 1-12, 1-33
- exiting, 1-9, 1-30
- front-panel keys, 1-19, 1-31
- getting a program. *See* IBASIC
- help function. *See* help function
- indenting lines, 1-15
- inserting characters, 1-14, 1-31
- inserting lines, 1-11, 1-32
- insert mode, 1-8
- keyboard keys, 1-19, 2-19-24
- moving cursor, 1-31
- overwrite mode, 1-8
- recalling deleted line, 1-15, 1-34
- relation to screen mode, 1-3, 2-3
- renumbering lines, 1-13
- saving a program. *See* IBASIC
- scrolling pages, 1-33
- softkeys, 1-19, 2-14-18
- specifying start label, 1-7
- specifying start linenumber, 1-7
- starting, 1-7, 1-30
- status. *See* execution status
- typing aid (ASP-like) softkeys, 1-41

IBASIC Status

- screen. *See* screen modes

Idle. *See* execution status

IEEE

- 488.1, 4-2
- 488.2, 4-2

IF

- IBASIC keyword, 1-21

improving

- speed by disabling screen update, 4-48
  - Indent**
    - editor softkey, 1-15
  - indenting
    - line. *See* IBASIC editor
  - INIT
    - auto loading files for initial setup, 4-49
  - initial
    - auto setup file at power on. *See* INIT
  - injection
    - hot carrier test. *See* hot carrier injection
  - INPUT
    - IBASIC keyword, 3-19
  - Input?**. *See* execution status
  - insert
    - characters. *See* IBASIC editor
    - IBASIC editor mode. *See* IBASIC editor
    - lines. *See* IBASIC editor
  - Insert line**
    - editor softkey, 1-11, 1-32
  - instrument
    - All Instrument screen. *See* screen modes
    - BASIC. *See* IBASIC
  - interface
    - HP-IB. *See* HP-IB
    - internal pseudo. *See* HP-IB
    - I/O resources. *See* I/O
    - serial. *See* serial
  - internal
    - controller. *See* built-in IBASIC controller
    - data representation. *See* data
    - memory. *See* memory
    - pseudo interface. *See* HP-IB
  - I/O
    - assigning path for controlling HP 4155/56, 3-5
    - closing path for data transfer to file, 3-20
    - IBASIC resources, 2-27-30
    - opening path for data transfer to file, 3-19
- K** keyboard
- editor keys. *See* IBASIC editor
  - IBASIC keys. *See* IBASIC
  - select code, 2-27
- keys
- front-panel. *See* front-panel
- keywords
- corresponding IBASIC and ASP keywords. *See* ASP programs
  - non-standard in HP 4155/56. *See* IBASIC

not allowed in HP 4155/56. *See* IBASIC  
knob sweep  
starting. *See* measurement program

**L** label  
starting IBASIC editor. *See* IBASIC editor  
length  
byte. *See* REAL  
data length considerations for previous ROM versions, 7-6  
LF  
terminator. *See* terminator  
LIF  
diskette format, 2-30  
file, 3-18  
line feed (LF)  
terminator. *See* terminator  
linenumber  
starting IBASIC editor. *See* IBASIC editor  
list  
contents of diskette, 1-17, 1-26  
printing list result data. *See* printing  
loading  
results from diskette. *See* measurement program  
results from internal memory. *See* measurement program  
setup data from diskette. *See* measurement program  
setup data from internal memory. *See* measurement program  
logarithmic  
sweep caution when running HP 4145 program directly, 5-4

**M** manual  
changes depending on ROM version, 7-2  
measurement program. *See* IBASIC  
before creating, 3-4  
changing setup data values, 3-8, 3-10, 4-8, 4-9  
controlling standby units, 4-18  
corresponding ASP keywords. *See* ASP programs  
creating, 1-7, 3-4  
creating a file, 3-18  
displaying plot of transferred data, 4-30  
executing measurement, 3-6, 4-13  
forcing stress, 4-15  
HP-IB. *See* HP-IB  
I/O. *See* I/O  
loading results from diskette, 4-24  
loading results from internal memory, 4-24  
loading setup data from diskette, 3-4, 4-23  
loading setup data from internal memory, 4-23  
making measurement, 3-4

- printing results. *See* printing
- reading measurement data from HP 4155/56, 1-46, 3-17, 4-26
- reading setup data from HP 4155/56, 3-16, 4-8, 4-11
- saving results (all) to diskette, 3-12, 4-22
- saving results (specific) to diskette, 3-18
- saving results to internal memory, 4-22
- saving setup data to diskette, 4-21
- saving setup data to internal memory, 4-21
- SCPI commands. *See* SCPI commands
- select codes. *See* HP-IB
- setting setup data values, 4-9
- starting knob sweep, 4-17
- transferring user variable data to HP 4155/56, 4-27
- using help function to create. *See* help function
- Vth measurement example. *See* Vth
- waiting for measurement completion. *See* waiting
- measurement results
  - loading from diskette, 4-24
  - loading from internal memory, 4-24
  - reading from HP 4155/56 to IBASIC variable, 1-46, 3-17, 4-26
  - saving (all) to diskette, 3-12, 4-22
  - saving (specific) to diskette, 3-18
  - saving to internal memory, 4-22
- MEM
  - initial auto setup file for internal memory, 4-49
- memory
  - auto loading of setup file at power on. *See* MEM
  - loading results from. *See* measurement program
  - loading setup data from. *See* measurement program
  - saving results to. *See* measurement program
  - saving setup data to. *See* measurement program
- MES suffix. *See* file types
- migrating
  - electromigration sample test program. *See* electromigration
  - HP 4145 programs to HP 4155/56. *See* HP 4145
- modes
  - command. *See* commands
  - screen. *See* screen modes
- moving
  - IBASIC cursor. *See* IBASIC editor

- N** NAND  
flash EEPROM sample test program. *See* flash EEPROM test
- NEXT**  
IBASIC keyword, 1-21
- NOR**  
flash EEPROM sample test program. *See* flash EEPROM test
- numeric data  
transferring to file. *See* file
- O** **ON KEY**  
IBASIC keyword, 2-13, 2-25
- opening  
I/O path for data transfer. *See* I/O
- order  
byte. *See* REAL
- OUTPUT**  
IBASIC keyword, 3-19, 4-6, 4-26
- overwrite  
existing file, 1-28  
IBASIC editor mode. *See* IBASIC editor
- P** **PAGE**  
ASP keyword, 1-48, 4-51  
setup. *See* setup pages  
subsystem commands relation to SCPI commands. *See* SCPI commands
- parameters  
changing HP 4155/56 setup data. *See* measurement program  
reading HP 4155/56 setup data to IBASIC variable. *See* measurement program  
setting HP 4155/56 setup data. *See* measurement program
- path  
I/O. *See* I/O
- Pause.** *See* execution status
- PAUSE**  
ASP keyword, 1-48, 4-51  
BASIC keyword, 1-48
- PEN**  
IBASIC keyword, 2-25
- PLOT**  
ASP keyword, 1-48, 4-51
- plotting. *See* printing
- polling  
serial. *See* serial polling
- power on  
auto loading setup data. *See* INIT  
auto loading setup file into memory. *See* MEM  
starting auto execute file. *See* AUTOST
- previous  
ROM version considerations, 7-2

**PRINT**

- ASP keyword, 1-48, 4-51
- printing
  - from built-in IBASIC, 4-4, 4-32
  - graphics result data, 4-37
  - HP-IB address. *See* HP-IB
  - list result data, 4-40
  - measurement results, 3-14
  - saving image to diskette file, 4-46
  - SCPI commands. *See* SCPI commands
  - screen dump, 4-43
  - setting items by SCPI commands, 4-32
  - setup data, 4-33
- PRINTPLOT directive, 1-44, 1-47, 1-48, 2-37
- program
  - measurement. *See* measurement program
  - sample applications. *See* sample programs
- programming commands
  - help function. *See* help function
- PRO suffix. *See* file types

**Q** query

- DATA?. *See* DATA? query command
- using commands in program, 3-16
- quitting
  - IBASIC editor. *See* IBASIC editor

**R** ramp

- voltage sample test program. *See* voltage ramp
- READDATAVAR directive, 1-46, 1-48, 2-35
- reading
  - HP 4155/56 measurement data to IBASIC. *See* measurement program
  - HP 4155/56 setup data to IBASIC. *See* measurement program
- read out function data
  - transferring from HP 4155/56 to IBASIC variables, 1-46, 3-17, 4-26
  - using for Vth measurement, 3-25
- REAL
  - byte length, 4-27
  - byte order, 4-27
  - data transfer, 4-27, 4-29
- recalling
  - deleted line. *See* IBASIC editor
- Recall** key, 1-15, 1-34
- REN
  - IBASIC renumbering command, 1-13, 2-13
- Re-number**
  - editor softkey, 1-13

- renumbering
    - lines. *See* IBASIC editor
    - REN command. *See* REN
  - REPEAT
    - IBASIC keyword, 1-21
  - repeating
    - IBASIC. *See* IBASIC
    - SCPI command for repeat measurement, 4-13
  - RE-SAVE**
    - IBASIC softkey, 1-28
  - resources
    - HP-IB. *See* HP-IB
    - I/O. *See* I/O
  - results
    - measurement. *See* measurement results
  - retrieving
    - HP 4155/56 data to IBASIC variable. *See* transferring
    - IBASIC program. *See* IBASIC
  - revisions
    - differences between ROM versions, 7-2
  - RFD
    - holdoff not effective for HP 4145 program, 5-6
  - ROM
    - changing manual for previous ROM versions, 7-2
    - difference between ROM versions, 7-2
    - version of this manual, 7-2
  - RS-232-C. *See* serial interface
  - Run. *See* execution status
  - Run** key
    - IBASIC key group, 1-9, 1-25
  - running. *See* executing
- S**
- sample programs
    - electromigration. *See* electromigration
    - flash EEPROM test. *See* flash EEPROM test
    - hot carrier injection. *See* hot carrier injection
    - TDDB. *See* TDDB
    - voltage ramp. *See* voltage ramp
    - Vth. *See* Vth
  - sampling
    - executing by SCPI command, 4-13
  - SAVE**
    - IBASIC softkey, 1-28
  - SAVE D
    - ASP keyword, 1-48, 4-51
  - SAVEDATA directive, 1-41, 1-48, 2-34
  - saving
    - IBASIC program. *See* IBASIC

measurement results (all) to diskette. *See* measurement program  
measurement results (specific) to diskette. *See* measurement program  
measurement results to internal memory. *See* measurement program  
setup data to diskette. *See* measurement program  
setup data to internal memory. *See* measurement program

#### scaling

auto. *See* auto scaling

SCPI commands, iv, 4-2-51

append measurement, 4-13

before using, 4-4

changing setup data values, 3-8, 3-10, 4-9

command hierarchy, 4-4

controlling standby units, 4-18

corresponding HP 4145 ASP commands, 4-51

disabling screen update to improve speed, 4-48

executing measurement, 3-6, 4-13

forcing stress, 4-15

help function. *See* help function

loading measurement data from diskette, 4-24

loading measurement data from internal memory, 4-24

loading setup data from diskette, 3-4, 4-23

loading setup data from internal memory, 4-23

printing graphics result data, 4-37

printing list result data, 4-40

printing screen dump, 3-14, 4-43

printing setup data, 4-33

print/plot operation, 4-31-47

reading measurement data from HP 4155/56, 3-17, 4-26

reading setup data values, 3-16, 4-11

relation to HP 4155/56 setup pages, 4-9

repeat measurement, 4-13

saving hardcopy image to diskette, 4-46

saving measurement data (all) to diskette, 3-12, 4-22

saving measurement data (specific) to diskette, 3-18

saving measurement data to internal memory, 4-22

saving setup data to diskette, 4-21

saving setup data to internal memory, 4-21

single measurement, 4-13

starting knob sweep function, 4-17

transferring user variable data to HP 4155/56, 4-27

two commands on same line, 4-4

using semicolon to reduce typing, 4-4

#### **Scratch**

editor softkey, 1-18

#### screen

disabling update to improve speed, 4-48

dump. *See* printing

screen modes, 2-3-6

All IBASIC, 1-3, 2-3, 2-4

- auto load setup file at power on. *See* auto
    - IBASIC editor. *See* IBASIC editor
  - statements
    - IBASIC keywords. *See* IBASIC
  - status
    - IBASIC execution. *See* execution status
    - IBASIC Status screen. *See* screen modes
    - incorrect when running HP 4145 program directly, 5-5
    - key shift. *See* shift status
  - step
    - sweep caution when running HP 4145 program directly, 5-4
  - storing. *See* saving
  - STRESS
    - directive, 1-48, 2-33
    - forcing. *See* measurement program
  - string data
    - transferring to file. *See* file
  - subprograms
    - COM blocks. *See* IBASIC
    - IBASIC. *See* IBASIC
  - swapped
    - byte order. *See* REAL
  - sweep
    - caution when running HP 4145 program directly, 5-4
    - executing by SCPI command, 4-13
    - knob. *See* knob sweep
  - SWEEP SETUP
    - Vth measurement example, 3-24
  - syntax
    - HP 4145 syntax command mode. *See* commands
  - SYSTEM:FILER page, 1-17
- T** TDDB
- sample program, 6-20
  - terminator
    - caution for running HP 4145 program directly, 5-5
  - THEN
    - IBASIC keyword, 1-21
  - throughput
    - improving. *See* speed
  - time dependent dielectric breakdown. *See* TDDB
  - timing
    - considerations for previous ROM versions, 7-3
  - transferring. *See* measurement program
    - HP 4155/56 data to a file, 3-12, 3-18, 4-22
    - HP 4155/56 data to IBASIC variables, 1-46, 3-17, 4-26
    - user variable data to HP 4155/56. *See* measurement program
  - typing-aid (ASP-like) softkeys. *See* IBASIC editor

- All Instrument, 1-3, 2-3
- for executing IBASIC commands, 1-25
- IBASIC Status, 1-3, 2-3, 2-6
- switching, 1-4, 2-3
- scrolling
  - pages. *See* IBASIC editor
- select codes
  - HP-IB. *See* HP-IB
- semicolon
  - using to execute two SCPI commands, 4-4
- serial interface, 2-29
  - printer settings, 4-31
  - select code, 2-27, 2-29
- serial polling
  - caution for running HP 4145 program directly, 5-5
- set
  - command set. *See* commands
- setup data
  - auto loading at power on. *See* INIT
  - loading from diskette. *See* measurement program
  - loading from internal memory. *See* measurement program
  - printing. *See* printing
  - saving to diskette. *See* measurement program
  - saving to internal memory. *See* measurement program
  - Vth measurement example, 3-23
- setup pages
  - changing settings from program. *See* measurement program
  - printing. *See* printing
  - relation to SCPI commands. *See* SCPI commands
- shift status
  - Blue key, 2-5
  - Green key, 2-5
- SINGLE
  - ASP keyword, 1-48, 4-51
  - directive, 1-41, 1-48, 2-32
  - SCPI command for single measurement, 4-13
- softkeys
  - editor. *See* IBASIC editor
  - IBASIC. *See* IBASIC
  - IBASIC (ASP-like) typing aids. *See* IBASIC editor
- speed
  - improving by disabling screen update. *See* screen
- spot measurement
  - HP 4145 and HP 4155/56 difference, 5-4
- STANDBY
  - controlling standby units. *See* measurement program
  - directive, 1-48, 2-33
- starting
  - auto execute file at power on. *See* AUTOST

- U** UNTIL  
  IBASIC keyword, 1-21  
  update  
    disabling to improve speed. *See* screen  
  user function data  
    names are case sensitive, 3-17  
    transferring from HP 4155/56 to IBASIC variables, 1-46, 3-17, 4-26  
    Vth measurement example, 3-25  
  user variables  
    names are case sensitive, 3-17  
    transferring to HP 4155/56. *See* measurement program
- V** variables  
  case sensitive, 3-17  
  data. *See* data variables  
  user. *See* user variables  
  user functions. *See* user function data  
versions  
  differences between ROM versions, 7-2  
voltage  
  threshold sample test program. *See* Vth  
Vth  
  example measurement program, 3-21  
  example setup, 3-23
- W** WAIT  
  ASP keyword, 1-48, 4-51  
  BASIC keyword, 1-48  
  waiting  
    for measurement completion in program, 3-12, 3-17  
    for printing to complete, 3-14  
WHILE  
  IBASIC keyword, 1-21

---