

Read This  
FIRST

## Quick Start Guide

Agilent Technologies Models  
6811B - 6814B, 6834B, and 6843A  
AC Power Solutions



<b>Documentation Map</b>	
<p><i>Quick Start Guide</i> (this document)</p> <p>Condensed overview of ac source operation. Read this to quickly get started.</p>	<p><i>Quick Reference Card</i></p> <p>Memory jogger for front panel and remote programming commands. Use this if you are already familiar with programming the ac source.</p>
<p><i>User's Guide</i></p> <p>Includes the following information: Description and installation, Checkout and operation Specifications and calibration</p>	<p><i>Programmer's Guide</i></p> <p>Includes the following information: Introduction to SCPI, SCPI command reference dictionary Application examples</p>



**Agilent Technologies**

Agilent Part No. 5962-0883  
Microfiche p/n 5962-0884  
Printed in USA: April, 2000

---

## Contents

The front panel, at a glance	3
The rear panel, at glance	4
What the ac source can do	5
How to use the front panel	7
Some basic operations	9
Measuring the output	11
Programming output transients	13
Programming trigger synchronization and delays	15
The front panel menus, at a glance	17
Agilent sales and Support Offices	20

### Safety Notice

*The beginning of the User's Guide has a Safety Summary page for this instrument. Familiarize yourself with the contents of that page. The following safety precautions must be observed.*

#### **WARNING: LETHAL VOLTAGES**

**Ac sources can supply 425 V peak at their output. DEATH on contact may result if the output terminals or circuits connected to the output are touched when power is applied.**

#### **BEFORE APPLYING POWER**

Verify that the product is set to match the available line voltage, the correct fuse is installed, and all safety precautions are taken. Note the instrument's external markings described under "Safety Symbols".

#### **GROUND THE INSTRUMENT**

To minimize shock hazard, the instrument chassis and cover must be connected to an electrical ground. The instrument must be connected to the ac power mains through a grounded power cable, with the ground wire firmly connected to an electrical ground (safety ground) at the power outlet. Any interruption of the protective (grounding) conductor or disconnection of the protective earth terminal will cause a potential shock hazard that could result in personal injury.

#### **FUSES**

Only fuses with the required rated current, voltage, and specified type (normal blow, time delay, etc.) should be used. Do not use repaired fuses or short-circuited fuseholders. To do so could cause a shock or fire hazard.

#### **DO NOT REMOVE THE INSTRUMENT COVER**

Operating personnel must not remove instrument covers. Component replacement and internal adjustments must be made only by qualified service personnel.

#### **DO NOT EXCEED INPUT RATINGS**

This instrument may be equipped with a line filter to reduce electromagnetic interference and must be connected to a properly grounded receptacle to minimize electric shock hazard. Operation at line voltages or frequencies in excess of those stated on the line rating label may cause leakage current in excess of 5.0 mA

© Copyright 1995, 1996, 1998, 2000 Agilent Technologies, Inc.

This document contains proprietary information protected by copyright. All rights are reserved. No part of this document may be photocopied, reproduced, or translated into another language without the prior consent of Agilent Technologies. The information contained in this document is subject to change without notice.

## The front panel - at a glance

14-character display shows menu commands and measured values.

- ◆ Annunciators indicate operating modes and status conditions.


Rotary controls set voltage and frequency when ac source is in local mode.

- ◆ Turn rapidly for coarse control
- ◆ Turn slowly for fine control.

▼ and ▲ scroll through menu commands.

▼ index and ▲ index scroll through lists and harmonic arrays.

↓ and ↑ scroll through command parameters.

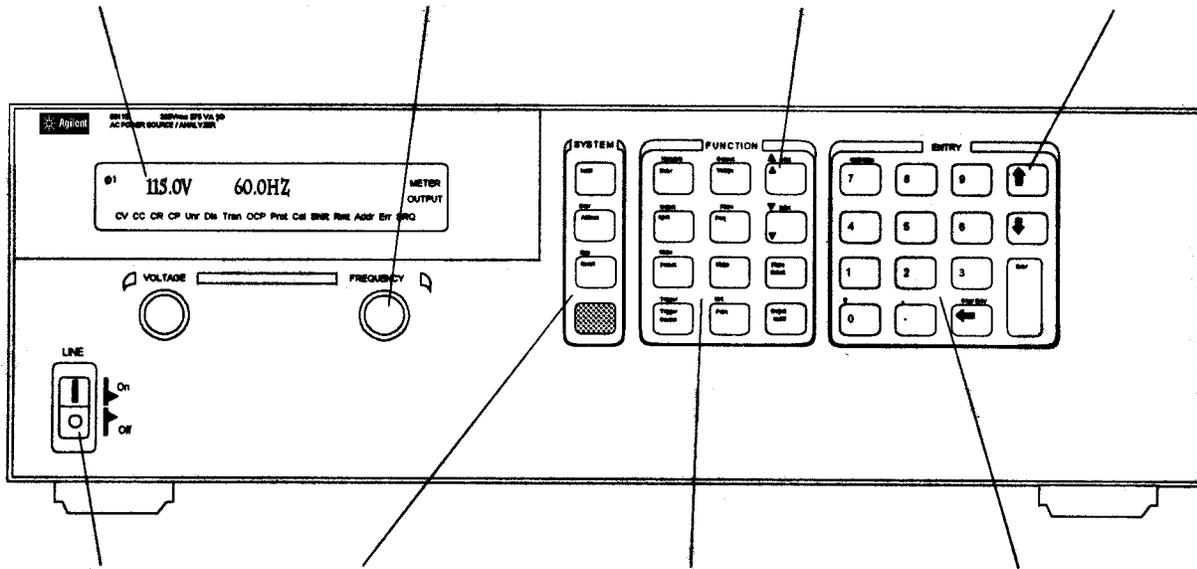

Turns the ac source on or off

System keys:

- ◆ Return to Local mode
- ◆ Set the GPIB address and other system parameters
- ◆ Set the RS-232 interface
- ◆ Display SCPI error codes
- ◆ Save and recall instrument states

Function keys:


- ◆ Enable/disable the output
- ◆ Select output phases
- ◆ Select front panel metering and harmonic analysis functions
- ◆ Program voltage frequency, phase, current limit, pulse parameters, and waveform shapes
- ◆ Set and clear protection functions
- ◆ Select output and input coupling
- ◆ Monitor status
- ◆ Scroll through front panel menu commands.

Entry keys:


- ◆ Enter values
- ◆ Increment or decrement values
- ◆ Scroll through command parameters.
- ◆ Calibrate the ac source.

## The rear panel - at a glance

Agilent Models 6814B 6834B 6843A

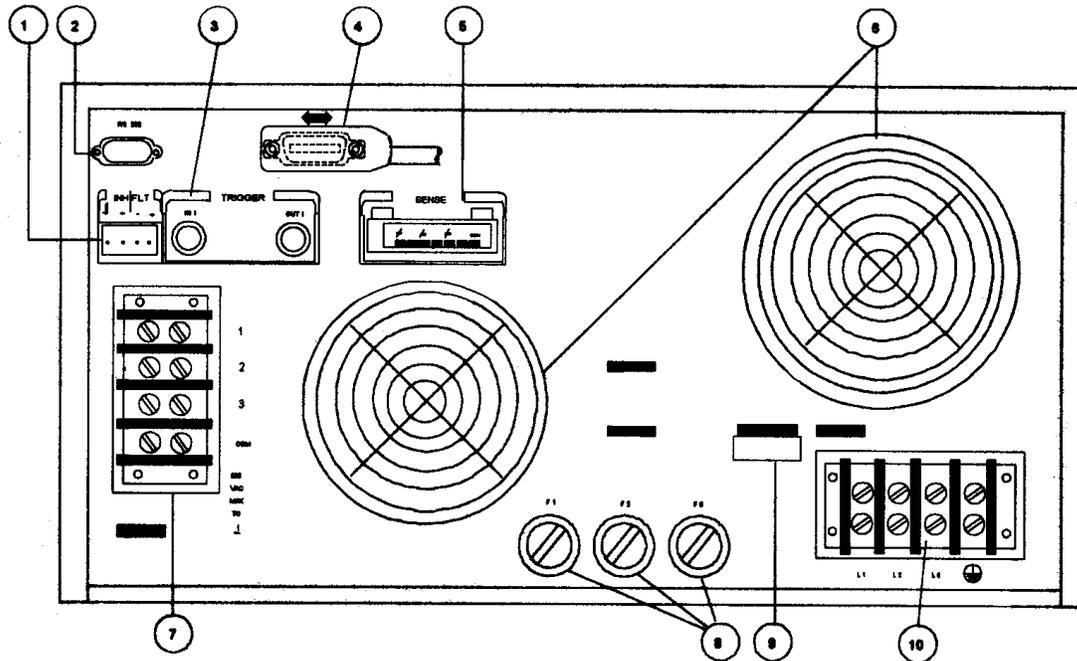

Agilent Models 6811B 6812B 6813B

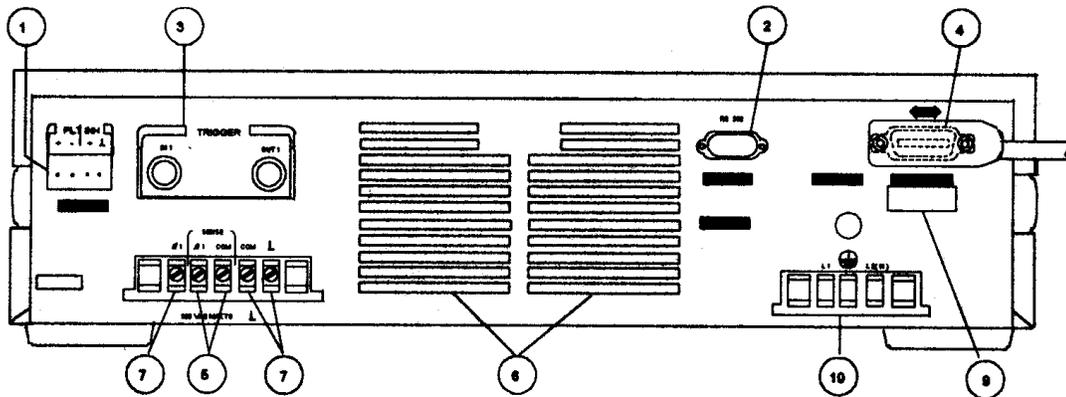


### Rear Panel Connections (see Chapter 3 in the User's Guide for details)

- 1 INH (Remote Inhibit) TTL input signal for externally disabling the power source.  
FLT (Discrete Fault Indicator) TTL output signal when there is a device fault.
- 2 RS-232 connector for remote controller.
- 3 TRIGGER BNC connectors for external trigger inputs and &source; trigger outputs.
- 4 GPIB connector and GPIB cable for remote controller.
- 5 SENSE connections for remote voltage sensing at the load.
- 6 Airflow Vents (do not block).
- 7 OUTPUT power connections to the load. ( $\phi 2$ ,  $\phi 3$  connections available on Agilent 6834B only.)
- 8 AC Input Line Fuses (Agilent 6814B/6834B/6843A only. Other models have internal fuses).
- 9 LINE RATING label specifies power source required by the power source.
- 10 AC Line Input connections from the power source.

## What the ac source can do

### Generate waveform shapes

- ◆ Sinewave
- ◆ Squarewave
- ◆ Clipped sinewave
- ◆ User-definable waveforms

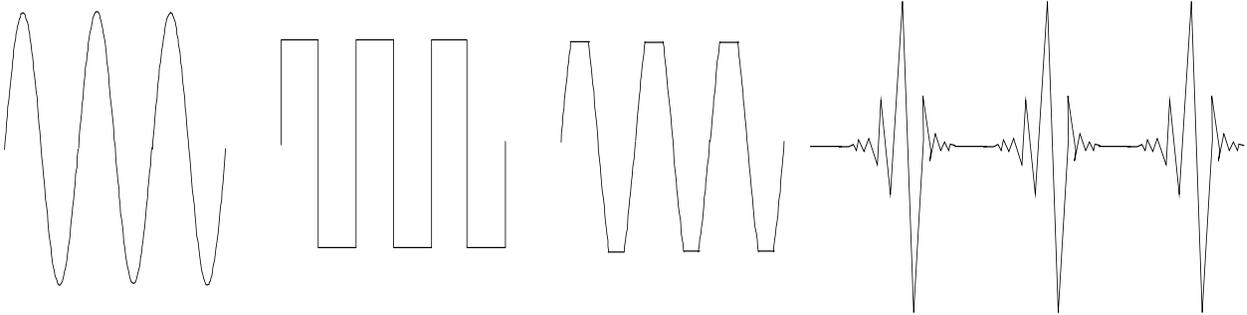

### Program the output


- ◆ Phase
  - ◆ Ac rms voltage
  - ◆ Distortion
  - ◆ Frequency
  - ◆ Voltage and frequency slew rates
  - ◆ Rms current limit
- Agilent Models 6811B, 6812B, 6813B program the following additional output functions:
- ◆ Dc voltage
  - ◆ Peak Current limit
  - ◆ AC coupling
  - ◆ Impedance

### Make the following measurements


- ◆ Ac rms, ac + dc rms voltage
  - ◆ Ac rms, ac + dc rms current; plus repetitive and non-repetitive peak current
  - ◆ Real, reactive, and apparent power
  - ◆ Harmonic analysis of voltage and current waveforms giving amplitude, phase, and total harmonic distortion results of up to the 50th harmonic.
  - ◆ Triggered acquisition of digitized voltage and current with extensive post-acquisition calculations
- Agilent Models 6811B, 6812B, 6813B make the following additional measurements:
- ◆ Dc voltage
  - ◆ Dc current
- Agilent Model 6834B makes the following additional measurement:
- ◆ Total power and neutral current

## Synchronize transient events or measurements with external signals

- ◆ Triggers applied to the unit

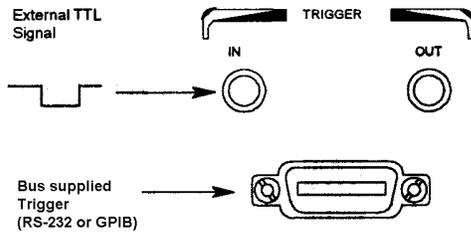


- ◆ Triggers generated by the unit




## Operate in four transient modes



- ◆ Fixed





- ◆ Step



- ◆ Pulse



- ◆ List



## Operate under local or remote control

- ◆ From the front panel keys
- ◆ Through the built-in GPIB or RS-232 interfaces

## Implement protection features

- ◆ Over-voltage
- ◆ Over-current
- ◆ Over-power
- ◆ Over-temperature
- ◆ User-defined external events (via a FLT shutdown signal)

## How to use the front panel

Make sure the unit is turned on.

### From the System key group

**Local**


Press **Local** to activate the front panel keypad if the unit is not already in local mode. (If the Local Lockout command is in effect, cycle power to return the unit to local mode.)

### From the Function key group

**Voltage**

Press **Voltage** to select the voltage function. To select a different function, simply press the appropriate key.


To select a function appearing above a key (such as **Current**), first press the blue shift key, then press the key below the function.

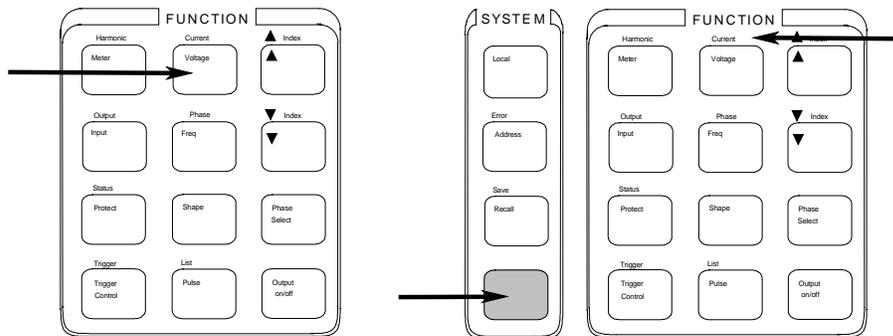

**NOTE:** Pressing **Output on/off**, **Phase Select**, or **(Shift) + Trigger** immediately implements the function. Display annunciators indicate that an immediate action has occurred. All other function keys have command menus underneath them that are accessed via the ▲ and ▼ keys after the function key is pressed. Refer to “The front panel menus- at a glance”.



Use these keys to move through the command menus of the selected function.

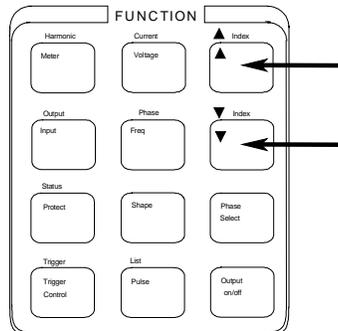


The following chart shows the commands in the Voltage function menu. Some commands may not appear on all models. Menus are circular, you can return to the starting position by continuously pressing ▲ or ▼.

Key	Display	Command Function
Voltage	VOLT <value>	Set immediate rms output voltage
▼	VOLT:T <value>	Set triggered rms output voltage
▼	VOLT:M FIXED	Select the voltage mode
▼	OFFSET <value>	Set immediate dc offset voltage
▼	OFFSET:T <value>	Set triggered dc offset voltage
▼	OFFSET:M FIXED	Select the dc offset voltage mode
▼	RANGE 150	Selects the voltage range
▼	SLEW <value>	Set immediate voltage slew rate in volts/second
▼	SLEW:T <value>	Set triggered voltage slew rate in volts/second
▼	SLEW:M FIXED	Select the voltage slew mode
▼	ALC INT	Select the voltage sense source
▼	ALC:DET RMS	Select the voltage sense detector


### From the Entry key group



Use these keys to increment/decrement or select the command parameters to be executed. If the parameter is a number, use these keys to make minor changes to the value. **Enter** enters the selection and returns to the Meter function.

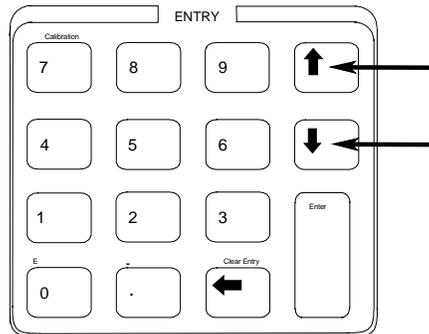

Key	Display	Description
Voltage, ▼	VOLT:M FIXED	Sets fixed mode
▼	VOLT:M STEP	Sets step mode
▼	VOLT:M PULSE	Sets pulse mode
▼	VOLT:M LIST	Sets list mode



Use the numeric Entry keys to directly enter a value for the command parameter. For example, to enter a value for the voltage parameter:

Key	Display	Description
Voltage	VOLT 0	0 volts
6, 0	VOLT 60	60 volts
Enter	60 V 60 Hz	enters the value and returns to the Meter function

## Some basic operations

Make sure the unit is turned on. Use either the front panel keys or the corresponding SCPI commands.

The column on the left indicates the front panel keys that program the indicated action. If the SCPI programming syntax is substantially different from the front panel menu command, it is shown inside parentheses ( ).

The text to the right describes the result. If appropriate, the resultant output waveshape is shown underneath the description.

### Enable the output

Output On/Off

When the output is enabled, the programmed voltage appears at the output and the Dis annunciator turns off.

### Select the output phase (Agilent 6834B only)

Phase Select

(INST:NSEL)

You can specify phases individually, or you can couple the phases. When phases are coupled, all three phase annunciators ( $\phi 1$ ,  $\phi 2$ ,  $\phi 3$ ) on the front panel are on, indicating that commands will be sent to all three phases. Note that front panel metering is only done one phase at a time (except for the total power and neutral current measurements).

### Set the voltage

Voltage

1


2

0

VOLT 120

Enter

When this command is sent, the output voltage is set to 120 V rms.

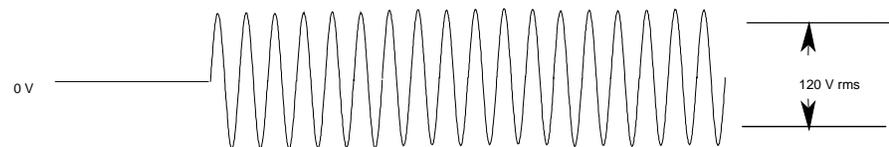

### Set the frequency

Freq


5

0

FREQ 50

Enter


When this command is sent, the output frequency is set to 50 Hz.

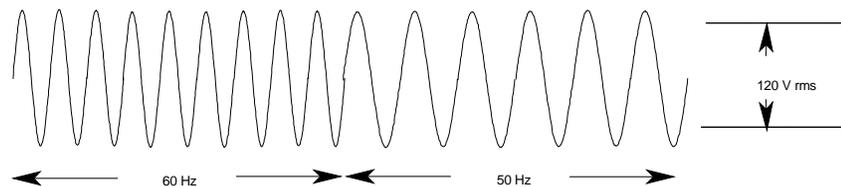

## Set the rms current limit (and peak current on Agilent 6811B/6812B/6813B units)

Shift  
 Current  
 1  
 0  
 CURR:LEV 10  
 Enter

When this command is sent, the rms current limit is set to 10 A. If more current than the programmed limit is drawn, the output voltage amplitude is reduced to keep the rms current within the specified limit. Press **Shift Current** and ▼ to access CURR:PEAK, which lets you set the peak current limit on Agilent 6811B/6812B/6813B units. Note that the peak current limit circuit on these units acts instantly and clips the output voltage to maintain the programmed peak limit.

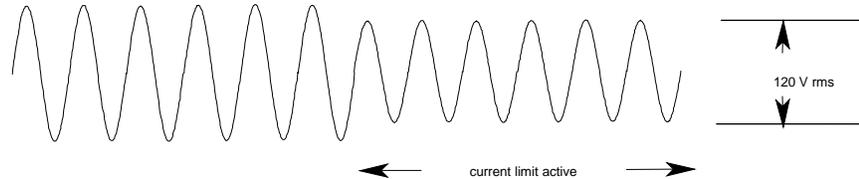


**NOTE:** The rms current limit circuit is slower than the peak current limit circuit and, depending on the setting of the peak current limit and the load on the output, your unit may generate momentary peak currents that can well exceed the rms current limit.

## Select a waveshape

Shape  
 ↓  
 SHAPE SQUARE  
 Enter


When this command is sent, the output generates a squarewave. Note that the peak-to-peak amplitude of the squarewave is less than that of a sinewave when it is programmed to the same rms voltage amplitude.

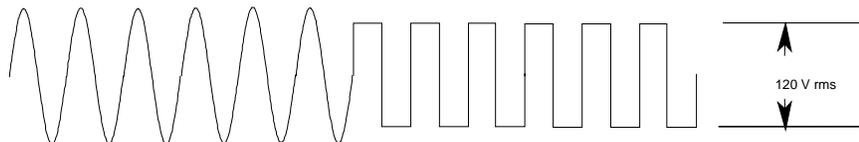

## Program a protection function

Protect  
 CURR:LEV 10  
 Enter  
 Protect  
 ▼  
 ↓  
 CURR:PROT ON  
 Enter

These commands clear all previously set protection functions and then set the current protection, which disables the output when an overcurrent condition is detected. The OCP annunciator will light when this command is programmed.

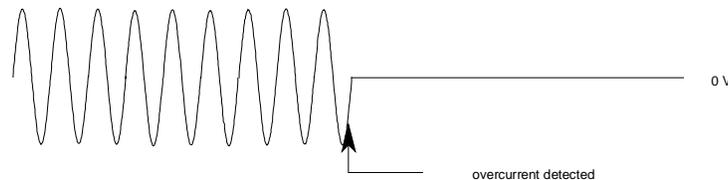

## Measuring the output

All measurements are based on acquiring and subsequently processing output waveform information. When the ac source is on, it takes measurements and updates the front panel meter continuously. The **Meter** key accesses the measurement functions from the front panel.

The SCPI MEASure command acquires **new** waveform information each time it is executed. The SCPI FETCh command does not acquire new waveform information but extracts the desired information from previously acquired waveform data. SCPI commands let you measure phases individually or simultaneously measure all phases using the FETCh command.

### Measurement functions

The following example illustrates the measurements that can be returned by the front panel of the ac source when sourcing power to a typical non-resistive load such as a power supply. The ac source output voltage and current waveforms are shown on the next page.

**NOTE:** On Agilent 6811B, 6812B, and 6813B units, the **Input** key selects the meter coupling and hence, what the meter will measure. The choices are: AC only, DC only, or AC + DC.

Meter (FETC/MEAS)	120V 60HZ	rms voltage and frequency
▼	120V 1.925A	rms voltage and current
▼	1.93A 60HZ	rms current and frequency
▼	120V 150.5W	rms voltage and power
▼	2.82 CREST F	current crest factor
▼	5.379A PK REP	peak current, repetitive
▼	36.83A PK NR	peak current, non repetitive
▼	230.6VA	apparent power
▼	175.2 VAR	reactive power
▼	0.65 PFACTOR	power factor


Note that in addition to the measurement functions listed above, the Agilent 6834B unit can also measure total power of all phases and neutral rms current.

## Harmonic measurements

Use the harmonic menu to make harmonic measurements of the output current. The following example illustrates the current magnitude measurements returned at harmonics 0 to 5. Note that harmonic 1 is the fundamental. Harmonic 0 is the dc component.

Shift	Harmonic	0.01A I:MAG:0	current amplitude at harmonic 0
(FETC/MEAS)			
Shift	▲Index	1.43A I:MAG:1	current amplitude at harmonic 1
Shift	▲Index	0.01A I:MAG:2	current amplitude at harmonic 2
Shift	▲Index	0.91A I:MAG:3	current amplitude at harmonic 3
Shift	▲Index	0.01A I:MAG:4	current amplitude at harmonic 4
Shift	▲Index	0.74A I:MAG:5	current amplitude at harmonic 5

## Output voltage and current waveforms

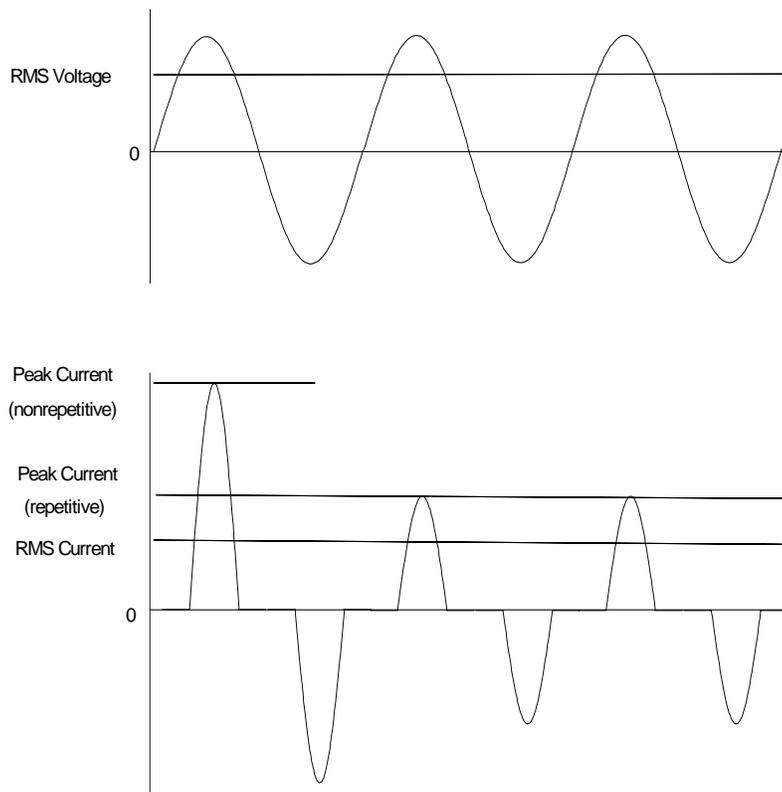

## Programming output transients


Up to now the ac source has been programmed with the transient system in Fixed mode. The following examples briefly describe the transient system's Step, Pulse, and List modes, which require the application of a trigger to implement the transient mode.

**NOTE:** For the examples that follow, press **Shift Output**, scroll to \*RST and press **Enter** to reset the unit prior to each example. Also press **Enter** to enter or activate each selection.

### Program an output step

Voltage  
 VOLT:M STEP  
 VOLT 120  
 VOLT:T 150  
 Trigger Control  
 INIT IMMED  
 Shift Trigger


Step transients transition to a new output level upon receipt of a trigger. When these commands are sent, the voltage amplitude is stepped from its previous setting to 150 V rms upon receipt of a trigger.

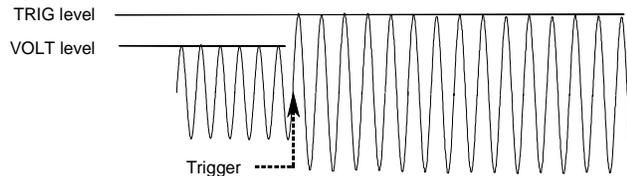

### Program an output pulse

Voltage  
 VOLT:M PULSE  
 VOLT 120  
 VOLT:T 90  
 Pulse  
 WIDTH .01  
 PER .03  
 COUNT 2  
 Trigger Control  
 INIT IMMED  
 Shift Trigger


Pulse transients transition to a new output level upon receipt of a trigger and return to the original level after a specified time, repeating this action by the number of times specified by the count. When these commands are sent, two output pulses step the voltage amplitude from its previous setting to 90 V rms upon receipt of a trigger. At the end of the specified period (multiplied by the count), the voltage returns to its original level.

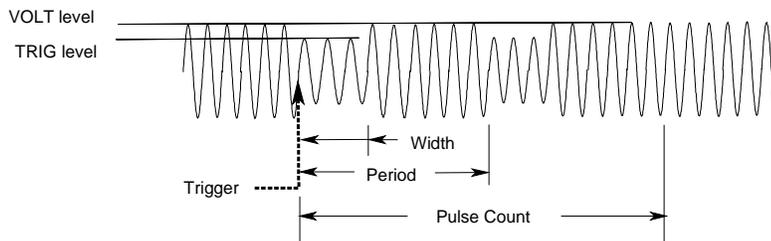

### Program an output list

Voltage  
 VOLT: M LIST  
 VOLT 120  
 Shift List  
 DWELL [0] .5  
 DWELL [1] .5  
 DWELL [2] .5  
 VOLT [0] 130  
 VOLT [1] 140  
 VOLT [2] 150  
 STEP AUTO  
 Trigger Control  
 INIT IMMED  
 Shift Trigger

List transients generate complex output sequences. When these commands are sent, the voltage amplitude is sequentially stepped to three levels upon receipt of a trigger, and then returns to the original voltage level. The output remains at each list step for .5 seconds. The values inside the brackets ([ ]) are the list index references. Use **Clear Entry** to clear a list.

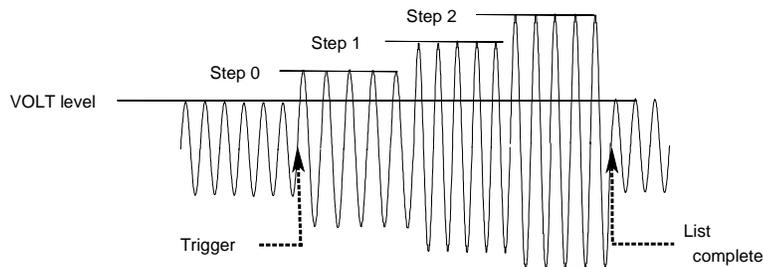


### More transient examples

The previous examples showed how the transient system can be used to control the output voltage amplitude. The transient system can also control output frequency, phase, waveform shape, voltage and frequency slew rates, offset voltage, and peak current limit. The following examples illustrate how the transient system's Pulse mode can generate frequency, shape, phase, and voltage slew pulses.


```

Freq
FREQ:M PULSE
FREQ 60
FREQ:T 50
Pulse
WIDTH .1
Trigger Control
INIT IMMED
Shift Trigger
    
```

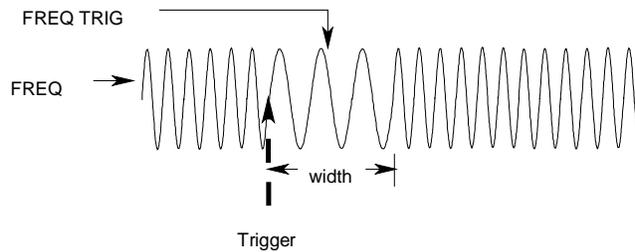


```

Shape
SHAPE:M PULSE
SHAPE SINE
SHAPE:T SQUARE
Pulse
WIDTH .05
Trigger Control
INIT IMMED
Shift Trigger
    
```

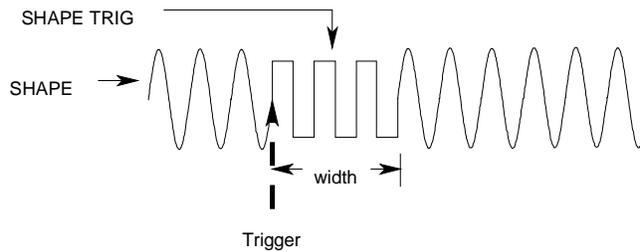


```

Shift Phase
PHASE:M PULSE
PHASE 0
PHASE:T 180
Pulse
WIDTH .05
Trigger Control
INIT IMMED
Shift Trigger
    
```

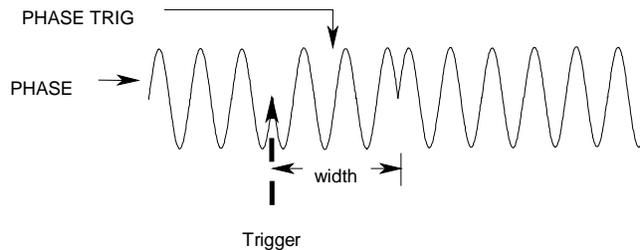

```

Voltage
VOLT:M PULSE
VOLT 120
VOLT:T 150
SLEW:M PULSE
SLEW 10000
SLEW:T 1000
Pulse
WIDTH .1
Trigger Control
INIT IMMED
Shift Trigger
    
```

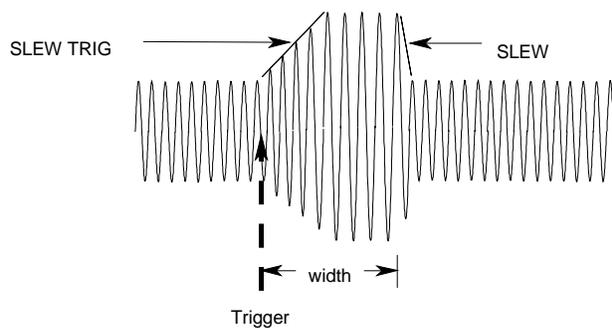


## Programming trigger synchronization and delays

The previous transient examples were programmed to respond to immediate triggers. However, delayed and phase synchronized triggers can also be programmed as shown in the following examples.

### No delay; no phase synchronization

Voltage  
 VOLT:M STEP  
 VOLT 120  
 VOLT:T 150  
 Trigger Control  
 DELAY 0  
 SYNC:SOUR IMM  
 INIT:IMMED  
 Shift Trigger


When these commands are sent, the voltage amplitude changes immediately upon the receipt of a trigger.

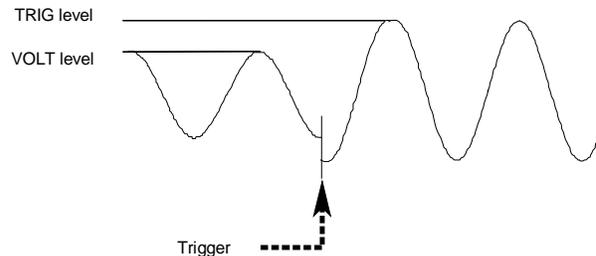

### No delay; 90 degrees phase synchronization

Voltage  
 VOLT:M STEP  
 VOLT 120  
 VOLT:T 150  
 Trigger Control  
 DELAY 0  
 SYNC:SOUR PHAS  
 SYNC:PHAS 90  
 INIT:IMMED  
 Shift Trigger


When these commands are sent, the voltage amplitude changes at the next 90 degree phase angle that occurs following the receipt of a trigger.

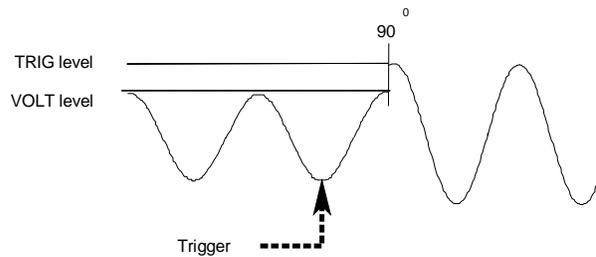

### Trigger delay; no phase synchronization

Voltage  
 VOLT:M STEP  
 VOLT 120  
 VOLT:T 150  
 Trigger Control  
 DELAY .0167  
 SYNC:SOUR IMM  
 INIT:IMMED  
 Shift Trigger

When these commands are sent, the voltage amplitude changes .0167 seconds after the receipt of a trigger.

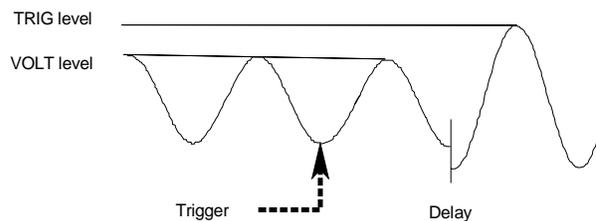


### Trigger delay; 90 degree phase synchronization

```

Voltage
VOLT:M STEP
VOLT 120
VOLT:T 150
Trigger Control
DELAY .0167
SYNC:SOUR PHAS
SYNC:PHAS 90
INIT:IMMED
Shift Trigger
    
```


When these commands are sent, the voltage amplitude changes at the next 90 degree phase angle that occurs after the .0167 second delay has expired, following the receipt of a trigger.

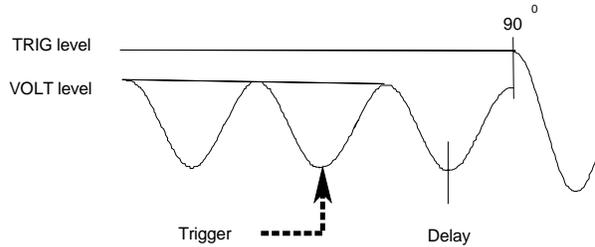

### More about the trigger system

In the previous examples, a front panel trigger is used to generate the output transients. The trigger is shown occurring at 270 degrees but actual triggers may occur at any phase. Delay and phase synchronization however, will occur as programmed.

Note that trigger system used in the ac source provides great flexibility in generating triggers. The following figure is a simplified model of the trigger system. A complete discussion of the capabilities of the trigger system is found in the ac source Programming Guide.

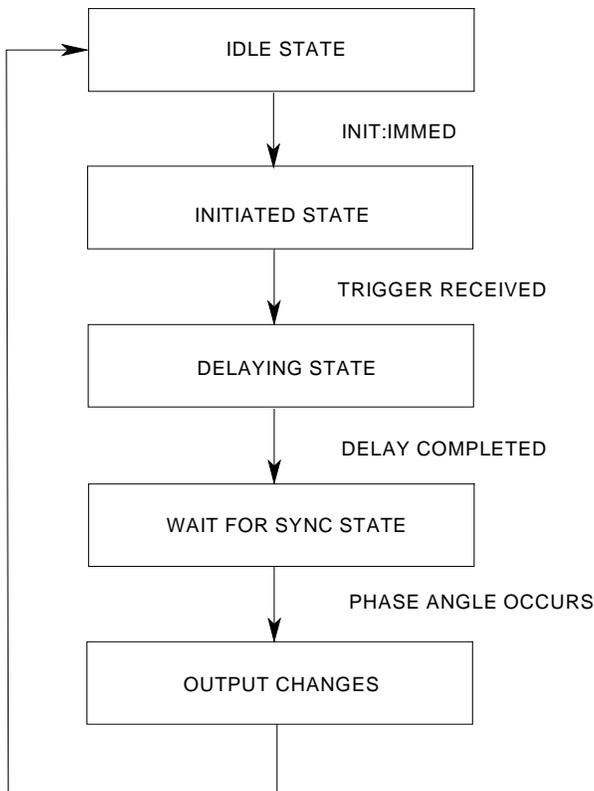

## The front panel menus - at a glance

### SYSTEM Keys

**Local** Press to change the ac source's selected interface from remote operation to local (front panel) operation. Pressing the key will have no effect if the interface state is already Local, Local-with-Lockout, or Remote-with-Lockout.

**Error Address**

<b>Error Functions</b>	
ERROR <value>	Displays system error codes stored in the SCPI error queue. If no errors exist, a 0 is displayed. The Err annunciator is lit when there are errors.
<b>Address Functions</b>	
ADDRESS <value>	sets the GPIB address
INTF GPIB   RS232	selects an interface
BAUDRATE 300   600   1200 2400   4800   9600	selects the baud rate
PARITY NONE   EVEN   ODD	selects message parity
LANG SCPI   E9012	selects the language
NOOUTPUTS 1   3	selects the number of outputs <sup>1</sup>

**Save Recall**

<b>Save Functions</b>	
Press to save an existing ac source state in nonvolatile memory. Up to 16 states can be saved (0-15).	
<b>Recall Functions</b>	
Press to place the ac source into a previously saved state. Up to 16 states can be recalled (0-15).	

 First press and release this blue shift key to select a shifted function. The Shift annunciator lights when this key is pressed.

### FUNCTION Keys

**Harmonic Meter**

<b>Harmonic Functions</b>	
<reading>A I:MAG: <index>	current harmonic magnitude
<reading>° I:PHASE: <index>	current harmonic phase
<reading>V V:MAG: <index>	voltage harmonic magnitude
<reading>° V:PHASE: <index>	voltage harmonic phase
<reading>N N:MAG: <index>	neutral current harmonic magnitude
<reading>° N:PHASE: <index>	neutral current harmonic phase
<reading> CURR:THD	current total % harmonic distortion
<reading> VOLT:THD	voltage total % harmonic distortion

Meter functions continued on next column

### FUNCTION Keys

<b>Meter Functions</b>	
<reading>V <reading>Hz	rms voltage and frequency
<reading>V <reading>A	rms voltage and rms current
<reading>A <reading>Hz	rms current and frequency
<reading>V <reading>W	rms voltage and power
<reading> CREST F	current crest factor
<reading>A PK REP	peak current, repetitive
<reading>A PK NR	peak current, nonrepetitive
<reading>VA	apparent power
<reading> VAR	reactive power
<reading>W TOTAL	total power all phases <sup>1</sup>
<reading> PFACTOR	power factor
<reading>A NEUTRAL	neutral rms current <sup>1</sup>

**Output Input**

<b>Output Functions</b>	
OUTP:COUP AC   DC	select output coupling <sup>3</sup>
*RST	executes the *RST command
TTLT:SOUR BOT   EOT   LIST	select Trigger Out source coupling
TTLT:STATE ON   OFF	set Trigger Out state
IMP:STATE ON   OFF	set output impedance programming <sup>3</sup>
IMP:REAL <value>	set real part of output impedance <sup>3</sup>
IMP:REAC <value>	set reactive part of output impedance <sup>3</sup>
PON:STATE RST   RCL0	select power-on state command
RI LATCHING   LIVE   OFF	sets remote inhibit mode
DFI ON   OFF	sets discrete fault indicator state
DFI:SOUR QUES   OPER ESB   RQS   OFF	select the DFI source
<b>Input Functions</b>	
INP:COUP AC   DC   ACDC	choose meter coupling
CURR:RANGE HIGH   LOW	current measurement range <sup>3</sup>
WINDOW KBESSEL   RECT	select harmonic measurement window meter

**Status Prot**

<b>Status Functions</b>	
*CLS	executes the *CLS command
STATUS:PRESET	executes STATUS:PRESet command
*ESR? <value>	return Event Status register value
*STB <value>	return Status Byte register value
OPER:EVENT? <value>	return STAT:OPER:EVENT? value
OPER:COND <value>	return STAT:OPER:COND? value
QUES:EVENT? <value>	return STAT:QUES:EVENT? value
QUES:COND <value>	return STAT:QUES:COND? value
<b>Protect Functions</b>	
PROT:CLEAR	clears latched protection signal
CURR:PROT ON   OFF	set overcurrent protection function
VOLT:PROT ON   OFF	set overvoltage protection function <sup>3</sup>
VOLT:PROT <value>	set overvoltage protection level
DELAY <value>	set a time delay for activating a protection fault

**Trigger**

**Trigger Control**

Trigger Function	
Pressing the Shift <b>Trigger</b> key generates an immediate trigger	
Trigger Control Functions	
INIT:IMMED	Initiate trigger immediately
INIT:CONT ON   OFF	Initiate trigger continuously
TRIG:SOUR BUS   EXT	Select transient trigger source
TTLT   IMM	
DELAY <value>	Set trigger delay in seconds
ABORT	Abort all trigger sequences
SYNC:SOUR PHASE   IMM	Select synchronous trigger source
SYNC:PHASE <value>	Set synchronous phase reference

**Current**

**Voltage**

Current Functions	
CURR:LEV <value>	set immediate rms current limit <sup>4</sup>
CURR:PEAK <value>	set immediate peak current limit <sup>3</sup>
CURR:PEAK:T <value>	set triggered peak current limit <sup>3</sup>
CURR:PEAK:M FIXED   STEP	select the peak current limit mode <sup>3</sup>
PULSE   LIST	
Voltage Functions	
VOLT <value>	set immediate ac output voltage <sup>4</sup>
VOLT:T <value>	set triggered output voltage <sup>4</sup>
VOLT:M FIXED   STEP	select the voltage mode <sup>4</sup>
PULSE   LIST	
RANGE 150   300	set the voltage range <sup>2, 4</sup>
OFFSET <value>	set immediate dc offset voltage <sup>3</sup>
OFFSET:T <value>	set triggered dc offset voltage <sup>3</sup>
OFFSET:M FIXED   STEP	select the dc offset voltage mode <sup>3</sup>
PULSE   LIST	
SLEW <value>	set voltage slew in V/sec <sup>4</sup>
SLEW:T <value>	set triggered voltage slew in V/sec <sup>4</sup>
SLEW:M FIXED   STEP	select the voltage slew mode <sup>4</sup>
PULSE   LIST	
OFF:SLW <value>	set dc offset slew in V/sec <sup>3</sup>
OFF:SLW:T <value>	set triggered dc offset slew in V/sec <sup>3</sup>
OFF:SLW:M FIXED   STEP	select the dc offset voltage slew mode <sup>3</sup>
PULSE   LIST	
ALC INT   EXT	select the voltage sense source
ALC:DET RTIME   RMS	select the voltage sense detector <sup>3</sup>

**Phase**

**Freq**

Phase Functions	
PHASE <value>	set immediate output phase <sup>4</sup>
PHASE:T <value>	set triggered output phase <sup>4</sup>
PHASE:M FIXED   STEP	select the phase mode <sup>4</sup>
PULSE   LIST	
Freq Functions	
FREQ <value>	set immediate output frequency
FREQ:T <value>	set triggered output frequency
FREQ:M FIXED   STEP	select the frequency mode
PULSE   LIST	
SLEW <value>	set frequency slew in Hz/sec
SLEW:T <value>	set triggered frequency slew Hz/sec
SLEW:M FIXED   STEP	select the frequency slew mode
PULSE   LIST	

**Shape**

Shape Functions		
SHAPE	SINE   SQUARE	set immediate shape
	CSIN   <user>	
SHAPE:T	SINE   SQUARE	set triggered shape
	CSIN   <user>	
SHAPE:M	FIXED   STEP	set shape mode
	PULSE   LIST	
CLIP <value>		set clipping level

**List**

**Pulse**

List Functions	
COUNT <value>	number of times a list repeats
DWEL:<index> <value>	list of output dwell times
FREQ:<index> <value>	list of output frequencies
FSLW:<index> <value>	list of output frequency slew rates
IPK:<index> <value>	list of output peak current limits <sup>3</sup>
OFFS:<index> <value>	list of dc output voltages <sup>3</sup>
OSLW:<index> <value>	dc offset voltage slew rate list <sup>3</sup>
PHASE:<index> <value>	list of output voltage phase angles <sup>4</sup>
SHAP:<index> SINE   SQUARE	list of output waveform shapes
CSIN   <user>	
STEP ONCE   AUTO	set response of list to triggers
TTLT:<index> ON   OFF	set trigger out pulse list
VOLT:<index> <value>	list of ac output voltages <sup>4</sup>
VSLW:<index> <value>	list of output voltage slew rates <sup>4</sup>
Pulse Functions	
WIDTH <value>	set the pulse width
COUNT <value>	set the number of output pulses
DCYCLE <value>	set the pulse duty cycle
PER <value>	set the pulse period count
HOLD WIDTH   DCYCLE	set parameter that is held constant

▼ **Index**



▲ **Index**



▼ ▲ **Index Functions**

These are Shift Index keys which are used to scroll through indexed functions. Press these keys to step through integers 0 through 50 for a harmonic list, or 0 through 99 for list points. Hold down these keys to rapidly access any harmonic or list point.

▼ ▲ **Functions**

These keys let you move through the choices in a command list. Command lists are circular; you can return to the starting position by continuously pressing either key.

**Phase Select**

This key applies to 3-phase ac sources only. Pressing this key successively selects phase 1 first, followed by phase 2, phase 3, and then all three phases.

**Output On/Off**

This key toggles the output on and off. When off, the ac source output is disabled and the **Dis** annunciator is on.

## ENTRY Keys



These keys let you scroll through choices in a **parameter** list that apply to a specific command. Parameter lists are circular; you can return to the starting position by continuously pressing either key. If the command has a numeric range, these keys increment or decrement the existing value.



–



The numeric keys 0 through 9 are used for entering numeric values.



Press shift and this key to enter a minus.  
Press this key alone to enter a decimal point.

Enter

Until you press the Enter key, the values or parameters you enter with the other Entry keys are displayed but not entered into the ac source.

E



Press Shift and this key to enter an exponent.

**Clear Entry**



Press Shift and this key to abort a keypad entry and clear the value. **When editing a list**, pressing Clear Entry truncates or clears the list at the presently displayed list point. Press this key alone to backspace and delete the last digit entered

**Calibration**



Press Shift and this key to access the calibration menu. Refer to appendix B in the user's for more information.

### Notes:

- 1 Valid for Model Agilent 6834B only
- 2 Valid for Models Agilent 6814B, 6834B, and 6843A only
- 3 Valid for Models Agilent 6811B, 6812B, and 6813B only
- 4 Phase selectable on Agilent 6834B

## Agilent Sales and Support Offices

For more information about Agilent Technologies test and measurement products, applications, services, and for a current sales office listing, visit our web site: <http://www.agilent.com/find/tmdir>

You can also contact one of the following centers and ask for a test and measurement sales representative.

### United States:

Agilent Technologies  
Test and Measurement Call Center  
P.O. Box 4026  
Englewood, CO 80155-4026  
(tel) 1 800 452 4844

### Latin America:

Agilent Technologies  
Latin American Region Headquarters  
5200 Blue Lagoon Drive, Suite #950  
Miami, Florida 33126  
U.S.A.  
(tel) (305) 267 4245  
(fax) (305) 267 4286

### Canada:

Agilent Technologies Canada Inc.  
5150 Spectrum Way  
Mississauga, Ontario  
L4W 5G1  
(tel) 1 877 894 4414

### Australia/New Zealand:

Agilent Technologies Australia Pty Ltd  
347 Burwood Highway  
Forest Hill, Victoria 3131  
(tel) 1-800 629 485 (Australia)  
(fax) (61 3) 9272 0749  
(tel) 0 800 738 378 (New Zealand)  
(fax) (64 4) 802 6881

### Europe:

Agilent Technologies  
Test & Measurement European Marketing Organisation  
P.O. Box 999  
1180 AZ Amstelveen  
The Netherlands  
(tel) (31 20) 547 9999

### Asia Pacific:

Agilent Technologies  
24/F, Cityplaza One, 1111 King's Road,  
Taikoo Shing, Hong Kong  
tel: (852)-3197-7777  
fax: (852)-2506-9284

### Japan:

Agilent Technologies Japan Ltd.  
Measurement Assistance Center  
9-1, Takakura-Cho, Hachioji-Shi,  
Tokyo 192-8510, Japan  
(tel) (81) 426 56 7832  
(fax) (81) 426 56 7840

Technical data is subject to change.

5962-0883



Agilent Technologies