

**8410S
NETWORK
ANALYZER
SYSTEMS**

OPERATING AND SERVICE MANUAL

All Hewlett-Packard products are warranted against defects in materials and workmanship. This warranty applies for one year from the date of delivery, or, in the case of certain major components listed in the operating manual, for the specified period. We will repair or replace products which prove to be defective during the warranty period provided they are returned to Hewlett-Packard. No other warranty is expressed or implied. We are not liable for consequential damages.

Service contracts or customer assistance agreements are available for Hewlett-Packard products that require maintenance and repair on-site.

For any assistance, contact your nearest Hewlett-Packard Sales and Service Office. Addresses are provided at the back of this manual.

WARRANTY AND ASSISTANCE

The Hewlett-Packard Company certifies that this instrument was thoroughly tested and inspected and found to meet its published specifications when it was shipped from the factory. The Hewlett-Packard Company further certifies that its calibration measurements are traceable to the U.S. National Bureau of Standards to the extent allowed by the Bureau's calibration facility.

CERTIFICATION



08410-91008 Printed: SEPT 1969
 Copyright HEWLETT-PACKARD COMPANY 1969
 1501 PAGE MILL ROAD, PALO ALTO, CALIFORNIA, U.S.A.

INSTRUMENT	SERIAL NO. PREFIX
8410A	932- and above
8411A	930- and above
8413A	903- and above
8414A	936- and above
8743A	917- and above
8745A	906- and above

This manual applies directly to component instruments with the serial numbers listed below.

SERIALS PREFIXED

8410S
Option 100
Option 200
Option 300
NETWORK ANALYZER SYSTEMS

TABLE OF CONTENTS


Section	Page	Section	Page
I	1-1	III	3-1
GENERAL INFORMATION	1-1	OPERATION	3-1
Description	1-1	Introduction	3-1
Accessories Furnished	1-1	Operating Precautions	3-1
Accessory Kit	1-1	Measurement Procedures	3-1
Other Accessories	1-2	Measurements with 8410S-100	3-1
Accessories Available	1-2	System (0.11 to 2 GHz)	3-1
Adapters	1-2	Measurements with 8410S-200	3-1
Fixed Coaxial Attenuators	1-2	System (2 to 12.4 GHz)	3-1
Accessories for Transistor	1-2	Measurements with 8410S-300	3-1
Measurement with 8410S-100	1-2	System (0.11 to 12.4 GHz)	3-1
System	1-2	Increased Accuracy for Reflection Measurements	3-1
Installation	2-1	Increased Accuracy for Transmission Measurements	3-1
Incoming Inspection	2-1	8410S-200 System	3-12
Preparation for Use	2-1	MAINTENANCE	4-1
Power Requirements	2-1	Introduction	4-1
115/230 Volt Operation	2-1	Performance Test	4-1
Power Cable	2-1	Performance Test	4-1
Bench Use	2-1	Performance Test	4-1
Rack Mounting	2-1	Performance Test	4-1
Repackaging for Shipment	2-1	Performance Test	4-1
2-16.	2-1	Performance Test	4-1
2-14.	2-1	Performance Test	4-1
2-12.	2-1	Performance Test	4-1
2-9.	2-1	Performance Test	4-1
2-6.	2-1	Performance Test	4-1
2-4.	2-1	Performance Test	4-1
2-3.	2-1	Performance Test	4-1
2-1.	2-1	Performance Test	4-1

Section	Page	Section	Page
I	1-1	III	3-1
Model 8410S Network Analyzer	1-1	LIST OF ILLUSTRATIONS	3-7
System	1-0	Typical Polar Plot Showing Locus of Measured Reflection when Sliding Load is Moved	3-12
Preparation for Rack Mounting	2-0	Center of Polar Display, Showing Locus of Sliding Load Vector with Directivity Cancelled	3-12
Transmission and Reflection Measurement with 8410S-100 System	3-2	Performance Test Procedures Common to all Systems	4-3
Reflection Measurement with 8410S-200 System Using 8414A Polar Display	3-4	Performance Test for 8410S-100 System	4-23
Transmission Measurement with 8410S-200 System Using 8414A Polar Display	3-6	Performance Test for 8410S-200 System	4-30
Reflection Measurements with 8410S-200 System Using 8413A Display Unit	3-8	Typical Pattern of a Swept VSWR Measurement	4-36
8410S-200 System Using 8413A Display Unit	3-10	Test Setup for Model 8410S-100 and 8410S-300 Troubleshooting Tree	4-37
Typical Polar Plot Showing Measured Reflection as the Sum of Directivity and Load Vectors	4-8	Test Setup for Model 8410S-200 and 8410S-300 Troubleshooting Tree	4-39
3-6.	3-1	System Troubleshooting Tree	4-39
3-5.	3-10	System Troubleshooting Tree	4-39
3-4.	3-8	System Troubleshooting Tree	4-39
3-3.	3-6	System Troubleshooting Tree	4-39
3-2.	3-4	System Troubleshooting Tree	4-39
3-1.	3-2	System Troubleshooting Tree	4-39

LIST OF TABLES

Number	Title	Page
1-1.	Specifications	1-3
1-2.	Instruments Included in 8410S System	1-1
1-3.	Parts Included in Accessory Kit No. 11650A	1-1
1-4.	Adapters for Non-APC-T Connectors	1-2
1-5.	HP 8492A Series Attenuators	1-2
4-1.	Recommended Test Equipment	4-1

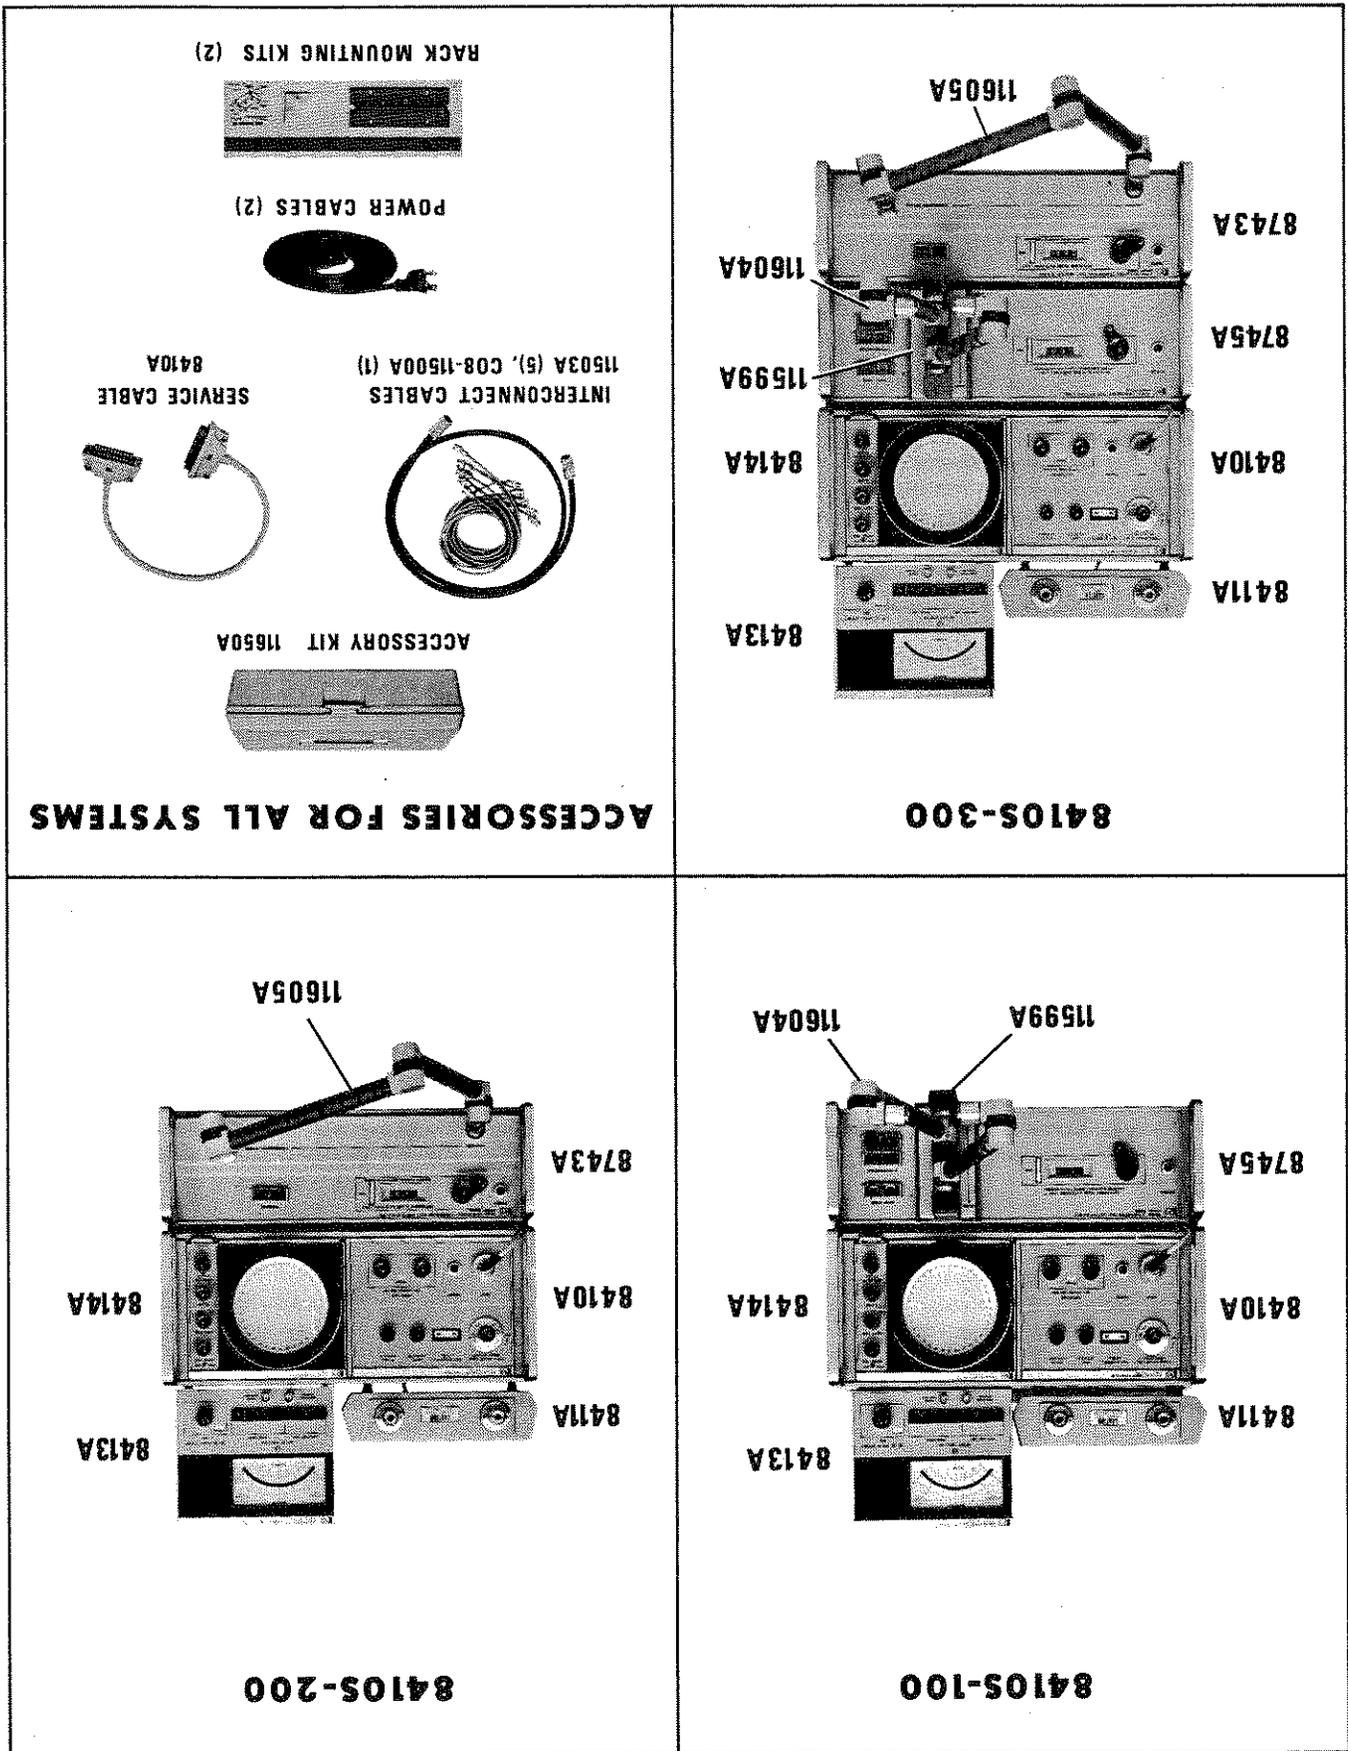Figure 1-1. Model 8410S Network Analyzer Systems



Qty.	Model	Description
2	11524A	APC-7 to N Female Adapter
2	11525A	APC-7 to N Male Adapter
1	8492A	3-dB Attenuator with APC-7 Connectors
Option 03		
1	8492A	10-dB Attenuator with APC-7 Connectors
Option 10		
1	8492A	20-dB Attenuator with APC-7 Connectors
Option 20		
1	5060-0236	APC-7 Contact Extractor
1	5060-0237	Spanner Wrench
1	8710-0877	1/2 Inch and 9/16 Inch Open End Wrench
1	1250-0907	Replacement APC-7 Inner Conductor Contacts
5	11511A	Type N Female Short
1	11512A	Type N Male Short
1	11565A	APC-7 Short
For maintenance of precision 7-mm APC-7 Connectors.		

Table 1-3. Parts Included in Accessory Kit No. 11650A

Instrument or Accessory	Included in System		
	-100	-200	-300
8410A Network Analyzer	X	X	X
8411A Harmonic Freq. Converter	X	X	X
8413A Phase-Gain Indicator Plug-In	X	X	X
8414A Polar Display Plug-In	X	X	X
8745A S-Parameter Test Set	X		
11599A Quick-Connect Adapter	X		
11604A Universal Extension	X		
8743A Reflection-Transmission Test Unit	X	X	X
11605A Flexible Arm	X	X	X
11650A Accessory Kit	X	X	X
11503A Interconnect Cable (5)	X	X	X
C08-11500A Interconnect Cable (1)	X	X	X

Table 1-2. Instruments Included in 8410S Systems

This eliminates the need for changing connections when making both transmission and reflection tests. Both transducers have flexible arm accessories which allow connection to a unit under test of almost any configuration.

1-5. The instruments which form the three systems are listed in Table 1-2. Basically, there is a low frequency system (8410S-100) and a high frequency system (8410S-200). The 8410S-300 system includes two transducer instruments (8743A and 8745A) and their accessories to cover the full frequency range covered by both the 8410S-100 and 8410S-200 systems and provides all the measurement capabilities of the other two systems.

1-6. The 8410S Network Analyzer Systems were designed to work with Hewlett-Packard sweep oscillators such as the HP 690 and 8690 Series. If any other sweep oscillator is used, the sweep signal specifications should be checked against the signal requirements listed in the 8410A Operating and Service Manual.

1-7. ACCESSORIES FURNISHED.

1-8. ACCESSORY KIT.

1-9. An accessory kit, HP Model 11650A, is included with each system. It contains the accessories most used for making various types of measurements, as well as tools for repairing the APC-7 type connectors. A list of the parts included in the accessory kit is presented in Table 1-3.

GENERAL INFORMATION

SECTION I

1-1. DESCRIPTION.

1-2. The Model 8410S Network Analyzer System is composed of a number of instruments grouped together to form a measurement system. The system measures reflection and transmission characteristics of micro-components, both active and passive. Three different systems are available, the Model 8410S-100 system covers the frequency range between 0.11 and 2.0 GHz, the Model 8410S-200 system covers the frequency range between 2.0 and 12.4 GHz, and the 8410S-300 system combines instruments of the -100 and -200 systems to cover the entire range of 0.11 to 12.4 GHz. The specifications for the three systems are listed in Table 1-1.

1-3. All three systems contain two readout plug-ins. The Model 8413A Phase-Gain Indicator produces a meter readout of both amplitude and phase information of the unit under test. Front-panel output connectors allow swept measurements to be displayed on an oscilloscope. The Model 8414A Polar Display has a built-in cathode ray tube (CRT) which displays both amplitude and phase of CW or swept-frequency signals in polar coordinates. Readouts at the 8413A or 8414A may represent either transmission or reflection quantities.

1-4. The Model 8743A and 8745A transducers included in the system may be changed from transmission to reflection mode by front-panel pushbuttons.

Adapter	Mfr. Number	Number
APC-7 to N female	11524A	1
APC-7 to N male	11525A	1
APC-7 to OSM male	11533A	1
APC-7 to BNC		2
APC-7 to TNC		2
APC-7 to GR900		2
APC-7 to GR874		2
APC-7 to NPM		3

Table 1-4. Adapters for Non-APC-7 Connectors

1-11. A number of miscellaneous accessories are included with the system. Interconnecting cables are included to connect the individual instruments together. These include five cables with BNC connectors and one RF cable with type N connectors. A servicing cable is included with the 8410A to allow servicing the plug-in units outside of the mainframe. One end of the cable plugs into the rear of the plug-in and the other end of the cable plugs inside the 8410A mainframe at the rear of the plug-in compartment. Rack-mounting kits are included with each instrument to allow rack-mounting of the system. The 8410A has a helix filter kit included so that if an HP Model 690 or 8690A series sweep oscillator is used for the signal source, the sweeper may be modified by adding the kit to make it compatible with the 8410A phase lock system. Model 8690A sweep oscillators with serial number 803-2061 and above have the filter already installed.

1-12. ACCESSORIES AVAILABLE.

1-13. ADAPTERS.

1-14. Table 1-4 lists adapters available to accommodate some of the most common connector types.

1-15. FIXED COAXIAL ATTENUATORS.

1-16. Besides the three attenuators contained in the accessory kit, other values of attenuation may be used to reduce power or to improve the signal-to-noise ratio for wide range attenuation and amplification measurements. Table 1-5 lists the attenuation values available in the HP 8492A series units with APC-7 connectors.

Number	Attenuation	MAX. SWR (up to 12.4 GHz)
03	3 dB	1.3:1
06	6 dB	1.3:1
10	10 dB	1.25:1
20	20 dB	1.25:1
30	30 dB	1.25:1
40	40 dB	1.25:1
50	50 dB	1.25:1
60	60 dB	1.25:1

Table 1-5. HP 8492A Series Attenuators

1-17. ACCESSORIES FOR TRANSISTOR MEASUREMENT WITH 8410S-100 SYSTEM.

1-18. The Hewlett-Packard Models 11600A and 11602A Transistor Fixtures prove a convenient and accurate way to hold transistors and many other devices when making s-parameter measurements from 0.1 to 2.0 GHz. The 11600A accepts transistors with T0-18 and T0-72 base patterns, and has four snap-on dials, two for bi-polar transistors and two for FET's. The 11602A accepts transistors with T0-5 and T0-12 base patterns. It has two snap-on dials for different types of bipolar transistors and provides for FET's without a dial.

1-19. The 11601A and 11603A Calibration Sets are used with transistor fixtures to obtain greater accuracy. The kit consists of a short circuit termination, a 50-ohm through section, and a 50-ohm termination. The Model 11601A is used with the Model 11600A Transistor Fixture and the Model 11603A is used with the Model 11602A Transistor Fixture.

1-20. The Hewlett-Packard 8717A Transistor Power Supply is designed especially for use with the 8745A S-Parameter Test Set and the 11600A and 11602A Transistor Fixtures. This programmable supply provides bias levels for the semiconductor devices tested in the fixtures. Feedback circuits within the supply provide very stable bias conditions. Overload protection for the device under test is selectable. Maximum current is 500 mA and maximum voltage is 30 Vdc.

SPECIFICATIONS COMMON TO 8410S, 100, 200, and 300 SYSTEMS

AMPLITUDE VERNIER: 2-dB range. Meter: $\pm 3\%$ of full scale, ± 0.05 dB for readings between 0 and 0.5 dB only.

PHASE ACCURACY:

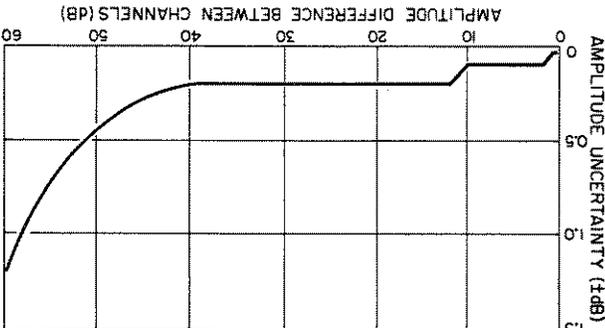
Accuracy curves show overall system uncertainty when measuring amplitude and phase. Sources of error included are IF gain control, meter accuracy, phase offset, system noise, and crosstalk. System frequency response is specified separately and is not included in accuracy curves.

OFFSET RANGE: $\pm 180^\circ$ in 10° steps. **OFFSET ACCURACY:** $\pm 0.3^\circ/10^\circ$ step, $\pm 1.5^\circ$ maximum cumulative for equal signal levels in reference and test channels. Add $\pm 2^\circ$ maximum to above for 60-dB difference between reference and test channels.


METER: $\pm 2\%$ of full scale.

PHASE VERNIER: 90° range.

REFERENCE PLANE EXTENSION: 0 to 15 cm for reflection; 0 to 30 cm for transmission; calibrated by digital dial indicator. Indicator is adjustable for initial calibration.



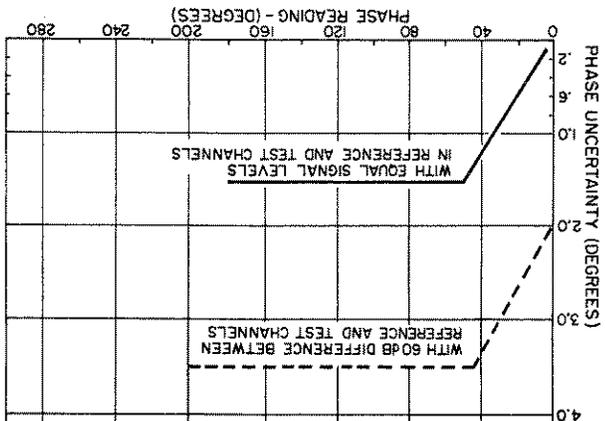Amplitude uncertainty for transmission measurements as a function of amplitude measured.



Phase uncertainty for transmission measurements as a function of phase shift measured.

DESCRIPTION

FUNCTION: All systems measure transmission and reflection parameters on a swept-frequency or CW basis in the form of attenuation, gain, phase shift, reflection coefficient, return loss, and impedance, depending on readout display.

DISPLAY UNITS

8413A PHASE GAIN INDICATOR:

Meter readout of amplitude in dB and phase in degrees.
AMPLITUDE RANGES: $\pm 3, \pm 10, \pm 30$ dB full scale.
PHASE RANGES: $\pm 6, \pm 18, \pm 60, \pm 180$ degrees full scale.

RESOLUTION: 0.1 dB, 0.1 degree.

Swept-frequency readout with oscilloscope or X-Y recorder.

AMPLITUDE: Front-panel analog output at 50mV/dB, 10-kHz bandwidth. Also, rear output 0-1 volt linear, proportional to ratio of test and reference signals.

PHASE: Front-panel analog output at 10 mV/degree, 10-kHz bandwidth.

8414A POLAR DISPLAY:

Polar coordinate CRT with magnitude calibration divisions at 20, 40, 60, 80, and 100% of full scale. Outer range settable by IF Gain Control and amplitude vernier.

Accepts marker signals from HP sweep oscillators, -5V peak, which appear as intensified dot on CRT face. Accepts blanking pulse, -4V, from HP sweep oscillators to blank retrace during sweep operation.

CONNECTORS: RF Input, Type N female, stainless steel; Measurement Ports APC-7 precision 7-mm connectors.

PERFORMANCE

TRANSMISSION MEASUREMENT ACCURACY

AMPLITUDE ACCURACY: (using 8413A)

RANGE: Full 60-dB dynamic range.

IF GAIN CONTROL: 69 dB in 10-dB and 1-dB steps.

± 0.1 dB/10 dB

± 0.2 dB maximum cumulative

Table 1-1. Specifications

Table 1-1. Specifications (Contd)

8410S-100 SPECIFICATIONS

FREQUENCY RANGE: 0.11 to 2.0 GHz.

TRANSMISSION-REFLECTION SELECTION: Manual by front panel, lighted pushbuttons; remote by contact closure or saturated transistors through 36-pin connector contacts. Short circuit current, 12 mA; open circuit voltage, 12 Vdc.

RF INPUT: 20-dB range between -21 dbm and +7 dbm. 20-dB variation causes less than 1.5 dB and 4° change in amplitude and phase readings.

SOURCE REFLECTION COEFFICIENT:¹
 ≤ 0.09 (<1.2 SWR), 0.11 - 2.0 GHz

TERMINATION REFLECTION COEFFICIENT:²
 ≤ 0.11 (<1.25 SWR), 100-200 MHz
 ≤ 0.09 (<1.20 SWR), 200-2000 MHz

DIRECTIVITY:
 >36 dB (typically >39 dB) 0.11 - 1.0 GHz
 >32 dB (typically >36 dB) 1.0 - 2.0 GHz

INSERTION LOSS, RF INPUT TO TEST PORT:
 4 dB nominal.

FREQUENCY RESPONSE:
TRANSMISSION: Typically ± 0.35 dB Amplitude and $\pm 3^\circ$ phase.

REFLECTION: Typically ± 0.06 Magnitude and $\pm 5^\circ$ phase as read on the 8414A polar display with a short on the test port.

TRANSMISSION MEASUREMENT ACCURACY
 (See common performance specifications)

REFLECTION MEASUREMENT ACCURACY:

Accuracy curves below show overall system uncertainty when measuring reflection coefficient. Sources of error included are directivity, source match, and polar display accuracy. System frequency response is specified separately and is not included in the accuracy curves.

1 Source Reflection Coefficient: Reflection coefficient of the port used to supply incident signal to the device under test.

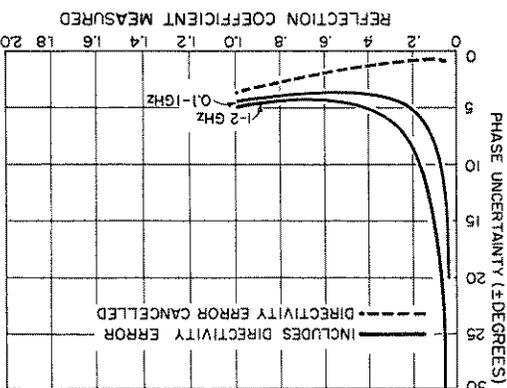
MAGNITUDE ACCURACY:

$$p_u = \pm(0.015 + 0.06p_L^2) \quad 0.11 - 1.0 \text{ GHz}$$

$$p_u = \pm(0.025 + 0.06p_L^2) \quad 1.0 - 2.0 \text{ GHz}$$

p_u = magnitude uncertainty

p_L = measured reflection coefficient magnitude




Reflection coefficient magnitude uncertainty including coupler directivity and when directivity is cancelled using a low VSWR load.

PHASE ACCURACY:

$$\phi_u = \sin^{-1} \frac{p_L}{p_u} \quad \text{for } \phi < 90^\circ$$

ϕ_u = phase uncertainty

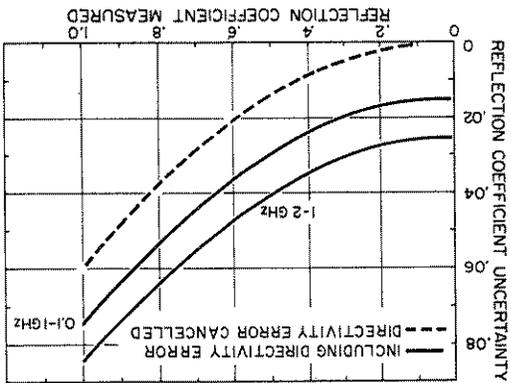(See Magnitude above for p_u , p_L terms)



Reflection coefficient phase uncertainty including coupler directivity and when directivity is cancelled using a low VSWR load.

2 Termination Reflection Coefficient: Reflection coefficient of port connected to output of test device when transmission or reflection measurement is being made.

8410S-200 SPECIFICATIONS

FREQUENCY RANGE: 2.0 to 12.4 GHz.

TRANSMISSION-REFLECTION SELECTION: Manual, by front panel, lighted pushbuttons; remote, by contact closure or saturated transistors through 36-pin connector contacts. Short circuit current, 12 mA; open circuit voltage, 12 Vdc.

RF INPUT: 20-dB range between -14 dBm and +14 dBm. 20-dB variation causes less than 1.5 dB and 4° change in amplitude and phase readings.

SOURCE REFLECTION COEFFICIENT: 1.

≤ 0.09 (1.2 SWR), 2-8 GHz

≤ 0.13 (1.3 SWR), 8-12.4 GHz

TERMINATION REFLECTION COEFFICIENT: 2

≤ 0.09 (1.2 SWR), 2-8 GHz

≤ 0.13 (1.3 SWR), 8-12.4 GHz

DIRECTIVITY: ≥ 30 dB, 2-12.4 GHz.

INSERTION LOSS, RF INPUT TO TEST PORT: 20 dB nominal.

FREQUENCY RESPONSE:

TRANSMISSION: Typically ± 0.5 dB Amplitude $\pm 5^\circ$ phase.

REFLECTION: Typically ± 0.06 Magnitude and $\pm 7^\circ$ phase, as read on the 8414A with a short on the unknown port.

TRANSMISSION MEASUREMENT ACCURACY

(See common performance specifications)

REFLECTION MEASUREMENT ACCURACY:

Accuracy curves show overall system uncertainty when measuring reflection coefficient. Sources of error included are directivity, source match, and polar display accuracy. System frequency responses is specified separately and is not included in the accuracy curves.

1 Source Reflection Coefficient: Reflection coefficient of the port used to supply incident signal to the device under test.

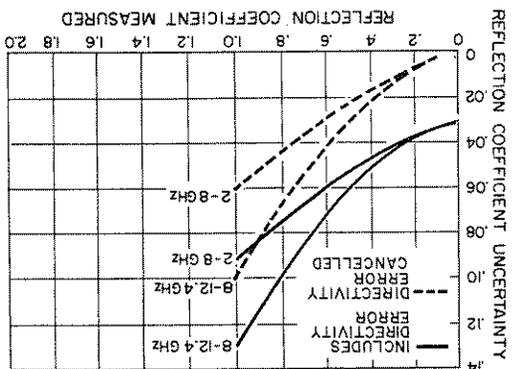
MAGNITUDE ACCURACY:

$p_u = \pm(0.032 + 0.03p_L + 0.03p_L^2)$, 2-8 GHz

$p_u = \pm(0.032 + 0.04p_L + 0.04p_L^2)$, 8-12.4 GHz

p_u = magnitude uncertainty

p_L = measured reflection coefficient magnitude




Reflection coefficient magnitude uncertainty including coupler directivity and when directivity is cancelled using a sliding load.

PHASE ACCURACY:

$$\phi_u = \sin^{-1} \frac{p_L}{p_u} \text{ for } \phi_u < \pm 90^\circ$$

p_u = phase uncertainty

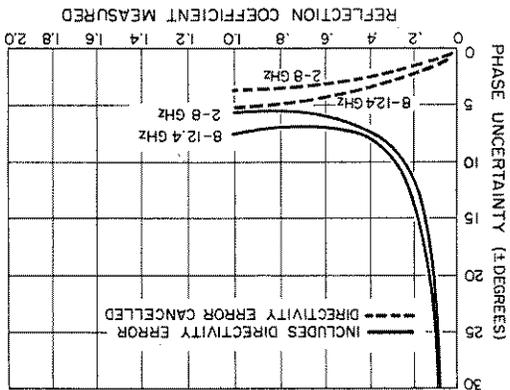(See Magnitude above for p_u , p_L terms)



Reflection coefficient phase uncertainty including coupler directivity and when directivity is cancelled using a sliding load.

2 Termination Reflection Coefficient: Reflection coefficient of port connected to output of test device when transmission or reflection measurement is being made.

Table 1-1. Specifications (Contd)

Table 1-1. Specifications (Contd)

8410S-300 SPECIFICATIONS

FREQUENCY RANGE: 0.11 to 12.4 GHz,
 Specifications for Model 8410S-300 are a combination of
 Models 8410S-100 and 8410S-200. All specifications for
 those models pertain directly to the 8410S-300 at the fre-
 quencies of interest.

INDIVIDUAL INSTRUMENT SPECIFICATIONS

**8410A NETWORK ANALYZER
 AND
 8411A HARMONIC FREQUENCY CONVERTER**

FUNCTION: 8411A Harmonic Frequency Converter
 converts RF signals to IF signals for processing in
 8410A mainframe. 8410A is the mainframe for dis-
 play plug-in units. The mainframe includes tuning
 circuits, IF amplifiers and precision IF attenuator.
FREQUENCY RANGE: 0.11 to 12.4 GHz.
8411A INPUT IMPEDANCE: 50 ohms nominal. SWR
 <1.5, 0.11 to 8 GHz; <2.0, 8 to 12.4 GHz; con-
 nectors precision 7 mm coax (APC-7).
CHANNEL ISOLATION: >65 dB, 0.1 to 6 GHz;
 >60 dB, 6 to 12.4 GHz.

AMPLITUDE

AMPLITUDE RANGE:

REFERENCE CHANNEL: 20-dB range between
 -16 and -44 dBm; meter indicates proper range.
 20 dB variation causes less than 1.5 dB and 4°
 change in amplitude and phase readings.

TEST CHANNEL: -10 to -78 dBm.

MAXIMUM RF INPUT TO EITHER CHANNEL:
 50 mW (+17 dBm) (damage level).

MAXIMUM DC ON RF LINE: +3V.

IF GAIN CONTROL: Adjusts gain of test channel
 relative to reference channel.

RANGE: 69 dB total in 10-dB and 1-dB steps;
 vernier provides continuous adjustment over
 at least 2 dB

ACCURACY: ±0.1 dB per 10-dB steps, ±0.05 dB
 per 1-dB step. Maximum cumulative, ±0.2 dB.

GENERAL

OUTPUTS: Two rear panel auxiliary outputs pro-
 vide 278 kHz IF signals; outputs may be used for
 signal analysis, special applications, and con-
 venient test points; modulation bandwidth nomi-
 nally 10 kHz.
REFERENCE CHANNEL IF: 2 volts peak-to-peak.
TEST CHANNEL IF: 10 volts peak-to-peak or less,
 depending on signal level and test channel gain
 setting.

POWER: 115 or 230 volts ±10%, 50 to 60 Hz, 70 watts
 (includes 8411A).

WEIGHT:

8410A: Net, 34 lb (15, 2 kg).

8411A: Net, 6-1/4 lb (2, 8 kg).

DIMENSIONS:

8410A: 7 in. high, 8-3/8 in. deep, 16-3/4 in. wide
 (17, 8 x 21, 3 x 42, 5 cm).

8411A: 2-5/8 in. high, 5-5/8 in. deep, 9 in. wide
 (6, 8 x 14, 3 x 22, 9 cm), exclusive of connectors.
 5-ft cable permanently attached for connection to
 8410A.

INDIVIDUAL INSTRUMENT SPECIFICATIONS	
<p>8743A REFLECTION/TRANSMISSION TEST UNIT</p> <p>INSERTION LOSS: FROM R.F. INPUT TO TEST DEVICE: 20 dB nominal. FROM R.F. INPUT TO REFERENCE CHANNEL</p> <p>REFERENCE PLANE EXTENSION: 0 to 15 cm for reflection; 0 to 30 cm for transmission; calibrated by digital dial indicator. Indicator is adjustable for initial calibration.</p> <p>CONNECTORS: Input, Type N female, stainless steel; all other connectors APC-7.</p> <p>REMOTE PROGRAMMING: Remote reflection or transmission selection by closing 2 contacts of 36-pin rear panel connector to ground pin. Contact is at 12 volts and short to ground will draw 12 mA.</p> <p>POWER: 115 Vac $\pm 10\%$, 50-400 Hz, 15 W.</p> <p>WEIGHT: Net, 27 lb (12, 4 kg).</p> <p>DIMENSIONS: 5-1/2 in. high, 16-3/4 in. wide 18-3/8 in. deep (140 x 426 x 467 mm).</p> <p style="text-align: center;">11605A FLEXIBLE ARM</p> <p>INSERTION LOSS: Approximately 1.5 dB.</p> <p>WEIGHT: Net, 4 lb (1, 8 kg).</p> <p>LENGTH: 10.1 in. (256, 5 mm) closed, 25.5 in. (647, 7 mm) extended.</p> <p>Reflection coefficient of port that connects to the 11605A flexible arm.</p>	<p>FUNCTION: Wideband RF power splitter and reflectometer with calibrated line stretcher. Pushbutton operated for either transmission or reflection measurements with network analyzer.</p> <p>FREQUENCY RANGE: 2-12.4 GHz.</p> <p>IMPEDANCE: 50 ohms nominal.</p> <p>REFLECTION COEFFICIENT:</p> <p>UNKNOWN PORT: 1 2-8 GHz, < 0.09 (SWR 1.2); 8-12.4 GHz, < 0.13 (SWR 1.30).</p> <p>TRANSMISSION RETURN PORT: 2 2-12.4 GHz, < 0.167 (SWR < 1.4).</p> <p>DIRECTIVITY: 2-12.4 GHz, > 30 dB.</p> <p>FREQUENCY RESPONSE: (Including 8411A Frequency Converter.)</p> <p>TRANSMISSION: Typically $> +0.5$ dB Amplitude, $< \pm 5^\circ$ phase.</p> <p>REFLECTION: Typically $< +0.1$ Magnitude, $\pm 5^\circ$ phase as read on 8414A Polar Display with a short on the unknown port.</p> <p>FUNCTION: Mounts on front of 8743A; connects to device under test. Rotary air lines and rotary joints connect any two-port geometry.</p> <p>IMPEDANCE: 50 ohms nominal. Reflection coefficient of ports: ≤ 0.11 (1.25 SWR), dc-12.4 GHz.</p> <p>CONNECTORS: APC-7</p> <p>Equivalent source reflection coefficient when used with Network Analyzer.</p>

Table 1-1. Specifications (Contd)

INDIVIDUAL INSTRUMENT SPECIFICATIONS

8745A S-PARAMETER TEST UNIT

FUNCTION: Wideband RF Power Splitter and reflectometer with calibrated line stretcher. Push-button operated for either transmission or reflection measurements with Network Analyzer.
FREQUENCY RANGE: 100 MHz to 2 GHz. Can be used below 100 MHz since coupler directivity remains above 36 dB and insertion loss to Reference and Test channel outputs increase \approx 6 dB/octave.
IMPEDANCE: 50 ohms nominal.
SOURCE REFLECTION COEFFICIENT: $1 \leq 0.057$ (< 1.12 SWR), 0.11-2.0 GHz.
TERMINATION REFLECTION COEFFICIENT: 2
TRANSMISSION: < 0.10 (< 1.22 SWR), 100-200 MHz
 < 0.063 (< 1.13 SWR), 200-2000 MHz.
REFLECTION: < 0.10 (< 1.22 SWR), 100-200 MHz
 < 0.063 (< 1.13 SWR), 200-2000 MHz.
DIRECTIVITY: 0.1 to 1 GHz, > 36 dB; 1-2 GHz, > 32 dB.
FREQUENCY RESPONSE: (Including 8411A frequency converter.)
TRANSMISSION: Typically ± 0.35 dB Amplitude $< \pm 5^\circ$ phase.
REFLECTION: Typically ± 0.06 Magnitude $< \pm 5^\circ$ phase as read on the 8414A with a short on the test port.

CONNECTORS:
RF INPUT: Type N female
TEST PORTS: APC-7 precision connectors.
OUTPUTS TO 8411A: Mates with APC-7 precision connectors.
REMOTE PROGRAMMING: Remote S-parameter selection by closing 2 contacts of 36-pin rear panel connector to ground pin. Contact is at 12 volts and short to ground will draw 12 mA.
TRANSISTOR BIASING: Bias and bias sensing connections are made to the biasing networks built into the 8745A via the 36-pin rear panel connector.
MAXIMUM BIAS: 100 Vdc; 1.0 amp.
POWER: 115 or 230 $\pm 10\%$, 50 to 400 Hz, 40 watts
WEIGHT: Net, 34-1/4 lb (15.9 kg).
DIMENSIONS: 5-1/2 x 16-3/4 x 25-3/4 in. (139 x 423 x 650 mm).

FUNCTION: Mounts on front of 8745A; connects to device under test. Rotary air lines and rotary joints connect to any two-port geometry.
FREQUENCY RANGE: dc to 2 GHz
Equivalent source reflection coefficient when used with Network Analyzer.

11604A UNIVERSAL EXTENSION

IMPEDANCE: 50 ohms nominal, reflection coefficient 0.035 (1.07 SWR).
WEIGHT: Net, 4 lb (1.8 kg).
DIMENSIONS: 10-1/2 x 5 x 1-1/4 in. (267 x 127 x 31, 6 mm).
Reflection coefficient of port that connects to the 11605A flexible arm.

Table 1-1. Specifications (Contd)

SECTION II INSTALLATION

2-12. BENCH USE.

2-13. The instruments in the system have plastic feet and foldaway tilt stands for convenience in bench operation. The tilt stands permit inclining the instruments for more convenient viewing of the control panels, and the plastic feet are shaped to make full width modular instruments self-aligning when stacked.

2-14. RACK MOUNTING.

2-15. Preparation for rack mounting is illustrated in Figure 2-1. All necessary hardware is contained in the rack mounting kits supplied with the individual instruments.

NOTE

If the rack-mounted instruments will be subjected to shock or vibration, provide additional bracing at the rear of the cabinets.

2-16. REPACKAGING FOR SHIPMENT.

2-17. If one of the instruments in the system is to be packaged for shipment, use the original shipping container and packing materials. If these have been discarded or are not in condition for reuse, contact your local Hewlett-Packard Sales and Service office (see rear of this manual for locations), or follow these general instructions.

a. If the instrument is a Model 8743A or 8745A, remove the rear-panel coaxial link, wrap it separately and include it in the instrument shipping container.

b. Wrap the instrument in heavy paper or plastic (if the instrument is being shipped to a Hewlett-Packard service facility, attach a tag indicating type of servicing required, return address, model number, and full serial number.)

c. Use a strong shipping container. A carton made of 600 pound test material will usually provide adequate protection.

d. Use enough shock-absorbing material (3 to 4 inch layer) around all sides of the instrument to provide firm cushion and prevent movement inside the container. Protect the control panel with cardboard. With Hewlett-Packard "float pack" packaging, the foam blocks provide sufficient shock protection, and additional material is unnecessary.

e. Seal the shipping container securely.

f. Mark the shipping container "FRAGILE" to assure careful handling.

g. In any correspondence, refer to the instrument by model number and full serial number.

2-1. INCOMING INSPECTION.

2-2. Instruments in the 8410S System were carefully inspected, both mechanically and electrically, prior to shipment. Inspect them for mechanical damage received in transit, check for supplied accessories, and test electrical performance using the performance test in Section IV. If there is any damage or deficiency, or if electrical performance is not within specifications, notify the carrier and your nearest Hewlett-Packard Sales and Service Office. The field office will arrange for repair or replacement of the instrument without waiting for a possible claim against the carrier to be settled.

2-3. PREPARATION FOR USE.

2-4. POWER REQUIREMENTS.

2-5. The Network Analyzer System requires a power source of 115 or 230 volts AC $\pm 10\%$, 50 to 60 Hz, single phase, which can supply approximately 200 watts.

2-6. 115/230 VOLT OPERATION.

2-7. Two-position slide switches on the rear panels permit operation from either a 115- or 230-volt power source. The number visible on the switch slider indicates the line voltage for which the instrument is connected. Adjacent to the switch is the correct fuse rating for each line voltage.

2-8. To prepare the instruments in the system for operation, position the 115-230 volt switches so that the numbers visible on the switch slider indicate the available line voltage, and install fuses of correct rating.

CAUTION


To avoid damage to the instruments, set the 115-230 volt switches for the line voltage to be used BEFORE connecting the power cables.

2-9. POWER CABLE.

2-10. To protect operating personnel, the National Electrical Manufacturers' Association (NEMA) recommends that the instrument panels and cabinets be grounded. Accordingly, all instruments in the 8410S system are equipped with three-conductor power cables which, when plugged into an appropriate receptacle, ground the panels and cabinets. The offset pin of the three-prong connector is the ground pin.

2-11. To preserve the protection feature when operating the system from a two-contact outlet, use a three-prong to two-prong adapter (HP Stock No. 1251-0048) and connect the green wire on the adapter to ground.

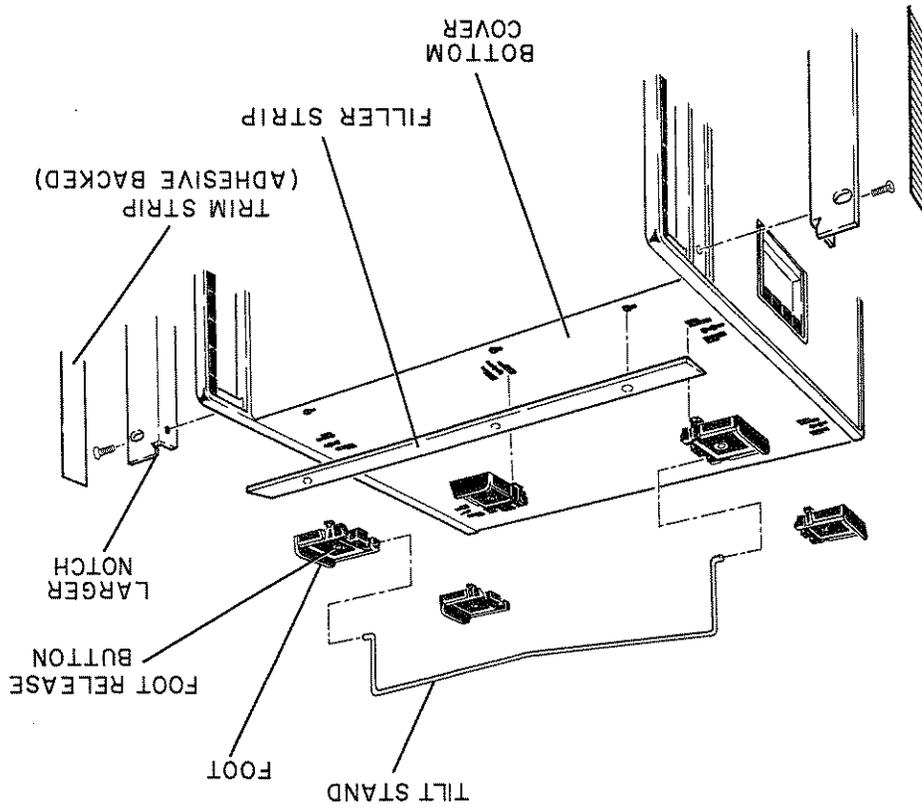Figure 2-1. Preparation for Rack Mounting



**SECTION III
OPERATION**

3-1. INTRODUCTION.

3-2. The 8410S System may be used to measure the magnitude and phase parameters of 50-ohm coaxial devices. These measurements can be made at single frequencies or at swept frequencies from 0.11 to 12.4 GHz. The 8410S-100 System covers the frequency range from 0.11 to 2.0 GHz, the 8410S-200 System covers the range from 2.0 to 12.4 GHz, and the 8410S-300 System covers the entire range from 0.11 to 12.4 GHz. The systems include two plug-in readout units for the network analyzer, the network analyzer mainframe and harmonic frequency converter, and the RF transducer unit(s) necessary to cover the selected frequency range. Flexible arm extensions are included with the transducers to connect almost any configuration of unit under test. The system was designed to be compatible with Hewlett-Packard 690 and 8690 series sweep oscillators. If any other type of sweeper or signal source is used, refer to the Model 8410A Network Analyzer Operating and Service Manual for the signal characteristics necessary for proper operation of the network analyzer.

3-3. OPERATING PRECAUTIONS.

3-4. The following operating precautions must be observed, or damage to an instrument may result:

- a. Maximum RF power to the RF input of the 8743A and 8745A is 2 watts.
- b. Maximum RF power to the inputs of the 8411A Harmonic Frequency Converter is 50 milliwatts.
- c. Maximum dc across the RF input connectors of the 8411A Harmonic Frequency Converter is +3 Vdc.
- d. Static electrical discharge into the center conductor of the 8411A Harmonic Frequency Converter may damage the unit. Discharge the center conductor of any line that might carry a static charge before connecting it directly to the 8411A input connector. If connection is made through the 8743A or 8745A transducer, there is no risk of static discharge because of the built-in discharge circuit paths.

3-5. MEASUREMENT PROCEDURES.

3-6. MEASUREMENTS WITH 8410S-100 SYSTEM (0.11 TO 2 GHz)
 3-7. Instructions for making reflection and transmission measurements with the 8410S-100 system in the 0.11 to 2 GHz range are given in Figure 3-1. Refer to paragraph 3-12 for methods of obtaining the highest measurement accuracy.

3-8. MEASUREMENTS WITH 8410S-200 SYSTEM (2 TO 12.4 GHz)
 3-9. Instructions for making reflection measurements with the 8410S-200 system in the 2 to 12.4 GHz range are given in Figures 3-2 and 3-4. Figures 3-3 and 3-5 give instructions for making transmission tests with this system. Refer to paragraphs 3-12 and 3-17

for methods of obtaining the highest measurement accuracy.

3-10. MEASUREMENTS WITH 8410S-300 SYSTEM (0.11 TO 12.4 GHz)

3-11. The 8410S-300 System is similar to either the 8410S-100 or 8410S-200 systems except it covers the entire range of the other two systems. This is accomplished by including both transducers (8743A and 8745A) in the system. To perform reflection or transmission measurements, use the appropriate procedure for the 100 or 200 system given in Figures 3-1 through 3-5. Refer to paragraphs 3-12 and 3-17 for methods of obtaining the highest measurement accuracy.

3-12. INCREASED ACCURACY FOR REFLECTION MEASUREMENTS.

3-13. Greatest accuracy for single-frequency, high resolution reflection measurements can be obtained by connecting the device under test directly to the front-panel ports of the 8743A or 8745A. If it is necessary to make connections through an I1604A or I1605A, an air line, or a coaxial cable, any movement of the swivel joints or flexing of coaxial cable will alter the phase relations of the reflections in the test setup; therefore, any component inserted between the 8743A or 8745A and the device under test should remain in the same position for both calibration and measurement.

3-14. Directivity errors are not significant unless small reflection coefficients are being measured. This error can be cancelled at single frequencies when necessary. The measured reflection is the vector sum of the directivity vector plus the reflection coefficient of the device under test (Figure 3-6). The error can be calibrated out at single frequencies by using a sliding

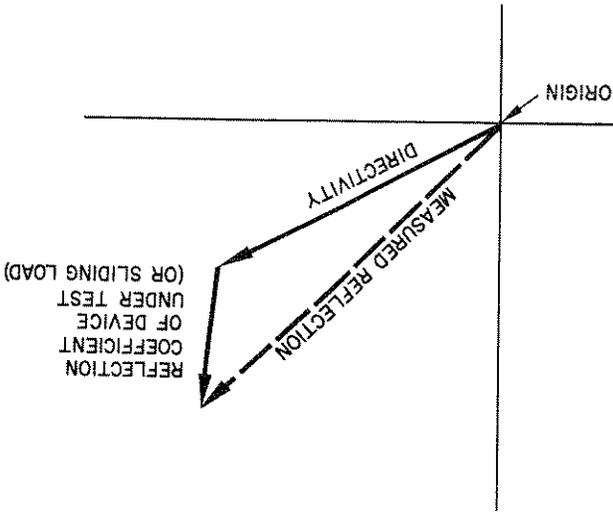


Figure 3-6. Typical Polar Plot Showing Measured Reflection as the Sum of Directivity and Load Vectors.

Figure 3-1. Transmission and Reflection Measurement with 8410S-100 System (Sheet 1 of 2)

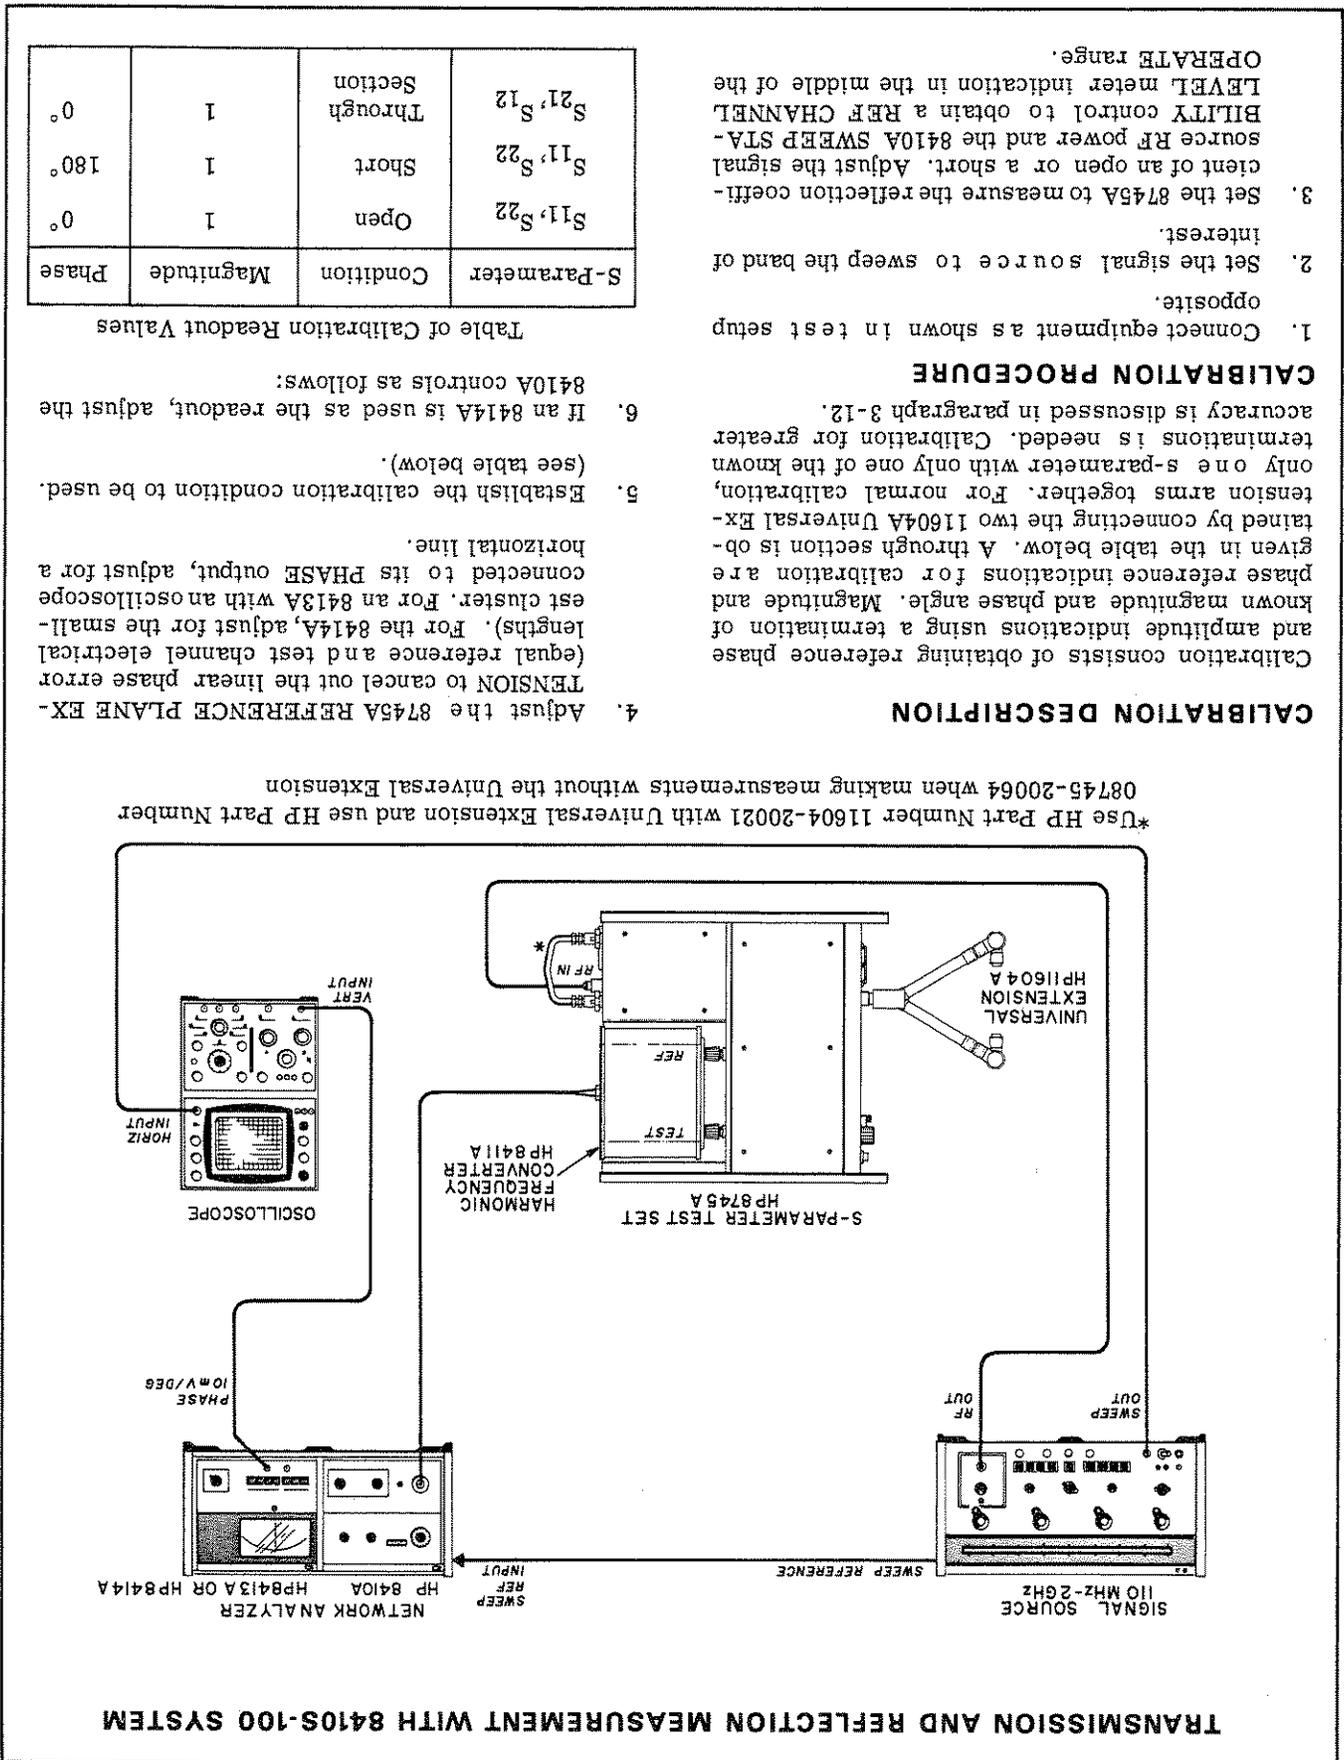


Figure 3-1. Transmission and Reflection Measurement with 8410S-100 System (Sheet 2 of 2)

MEASUREMENT

1. Insert the device to be tested between the arms of the Universal Extension and select INPUT PORT A or B as desired.
2. Select the S PARAMETER to be measured.
3. If an 8414A plug-in is used in the 8410A Network Analyzer, read the magnitude and phase from the CRT. Note from the table below that the 8414A magnitude scale may be changed by changing the 8410A TEST CHANNEL GAIN control settings. To use other TEST CHANNEL

- a. Adjust the PHASE VERNIER control for the appropriate reference phase indication (e.g., for a through section, press S21 or S12 and adjust for 0°).
 - b. Adjust the TEST CHANNEL GAIN and AMPL VERNIER controls for a zero dB indication. For S11 and S22 the 8413A indicates return loss (0 dB return loss equals a reflection coefficient of 1). For S21 and S12 the 8413A indicates gain or loss in dB.
7. If an 8413A is used as the readout, set the signal source for single frequency (CW) operation and adjust the 8410A controls as follows:
 - a. Adjust the PHASE VERNIER control for the appropriate reference phase indication (e.g., for a through section, press S21 or S12 and adjust for 0°).
 - b. Adjust the 8410A TEST CHANNEL GAIN and AMPL VERNIER controls for an 8414A magnitude indication of 1.0. This places the dot or cluster trace on the outside graphic circle of the CRT.

TRANSMISSION AND REFLECTION MEASUREMENT WITH 8410S-100 SYSTEM

4. If an 8413A is used in the 8410A, the amplitude display is relative magnitude in dB of the incident and reflected (S11, S22) or incident and transmitted (S21, S12) signals. These can be converted to reflection or transmission coefficients with the following equations:

or

$$p = \log^{-1}(0.05 \times \text{return loss in dB})$$

$$r = \log^{-1}(0.05 \times \text{return loss in dB})$$

NOTE

p = Reflection Coefficient Magnitude
 r = Transmission coefficient magnitude

Table of Magnitude Scale

8410A TEST CHANNEL GAIN Change from Cal. Setting (dB)		8414A Graticule Calibration	
		Full Scale	Each Ring
+32	0.025	0.025	0.005
+26	0.05	0.05	0.01
+20	0.1	0.1	0.02
+14	0.2	0.2	0.04
+12	0.25	0.25	0.05
+6	0.5	0.5	0.1
-6	1.0	1.0	0.2
-12	2.0	2.0	0.4
-14	4.0	4.0	0.8
-20	10.0	10.0	2.0
-26	20.0	20.0	4.0
-32	40.0	40.0	8.0

Figure 3-2. Reflection Measurement with 8410S-200 System Using 8414A Polar Display (Sheet 1 of 2)

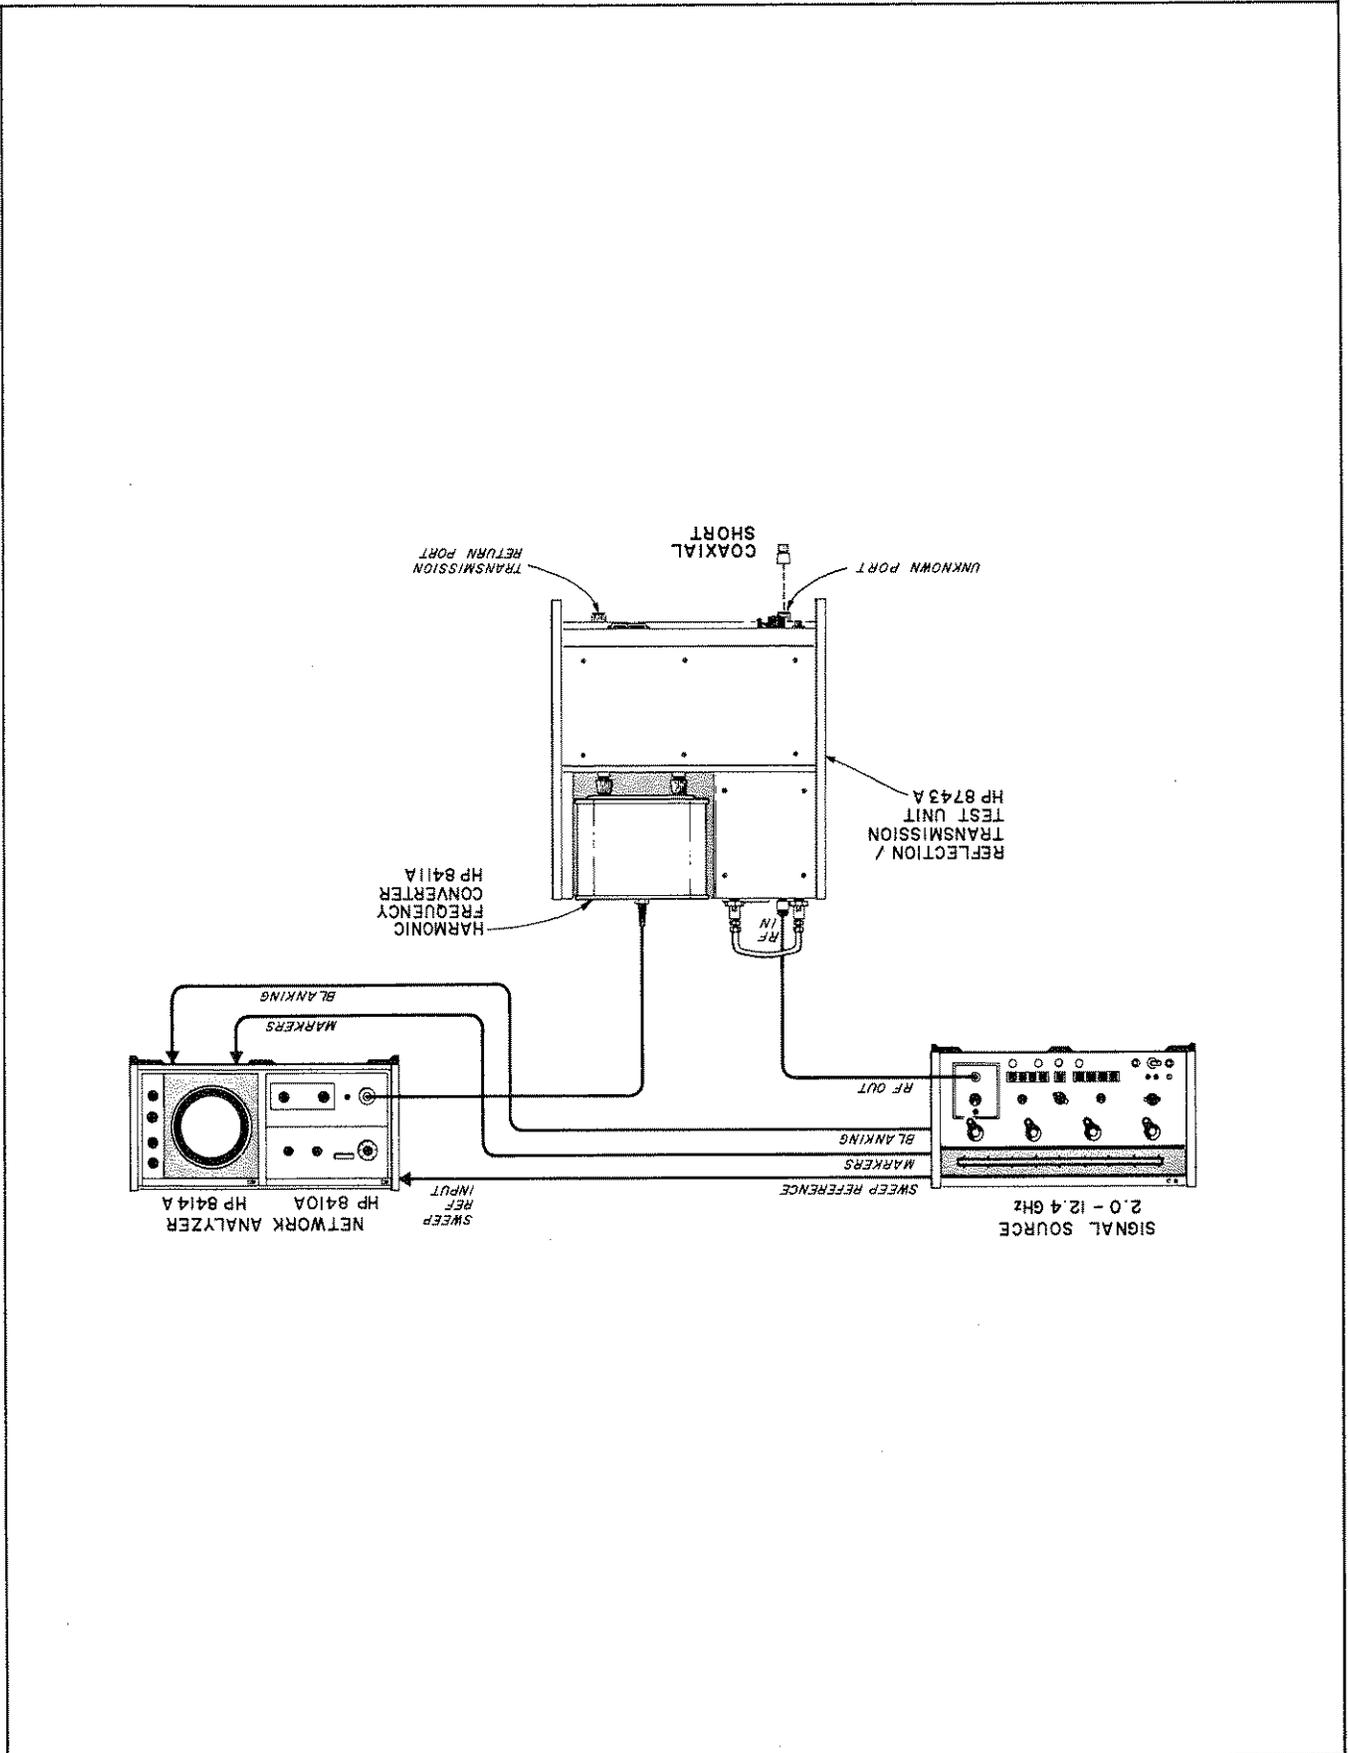


Figure 3-2. Reflection Measurement with 8410S-200 System Using 8414A Polar Display (Sheet 2 of 2)

REFLECTION MEASUREMENT WITH 8410S-200 SYSTEM

6. Adjust the 8410A PHASE VERNIER, TEST CHANNEL GAIN, and AMPL VERNIER controls to place the dot or cluster for a reference indication of $\Gamma = 1/180^\circ$.

NOTE

Calibration for greater accuracy is discussed in paragraph 3-12.

MEASUREMENT

1. Remove the coaxial short and connect the device to be tested to the 8743A UNKNOWN port.
2. Read the reflection coefficient magnitude and phase (or impedance using a Smith Chart overlay) from the 8414A display.

NOTE

For small reflection coefficients, the 8414A resolution can be improved by increasing the 8410A test channel gain. For example, increasing the full scale reflection by 20 dB changes the full scale reflection coefficient calibration from 1.0 to 0.1 at the outer circle.
- 3. The effective load plane of the device under test may be determined by adjusting the 8743A REFERENCE PLANE EXTENSION to again collapse the trace to a dot or smallest cluster. The distance from reference plane to load plane may be read directly from 8743A digital counter (counter set to zero during calibration).

CALIBRATION DESCRIPTION

Calibration consists of adjusting the 8743A REFERENCE PLANE EXTENSION to obtain equal reference and test channel electrical lengths, then obtaining a reference magnitude and phase indication.

CALIBRATION PROCEDURE

1. Connect equipment as shown in setup above.
2. Connect coaxial short, HP 11565A to the 8743A UNKNOWN port and depress the REFL push-button.
3. Set the signal source to sweep the band of interest. Adjust the signal source RF power and the 8410A SWEEP STABILITY control to obtain a REF CHANNEL LEVEL meter indication in the middle of the OPERATE range.
4. Push and hold the 8414A BEAM CTR push-button and adjust the centering controls to place the dot in the center of the polar display.
5. Obtain equal reference and test channel electrical lengths by adjusting the 8743A REFERENCE PLANE EXTENSION to collapse the trace to a dot or smallest cluster. If the plane of measurement is to be extended beyond the plane of the short, the digital counter should be set to zero so that it can be used to set the required extension accurately. A convenient way to do this is as follows:
 - a. Adjust 8743A REFERENCE PLANE EXTENSION crank until counter reads all zeros.
 - b. Hold thumbwheel to retain zero indication and readjust REFERENCE PLANE EXTENSION to collapse the trace to a dot or smallest cluster.

Figure 3-3. Transmission Measurements with 8410S-200 System Using 8414A Polar Display (Sheet 1 of 2)


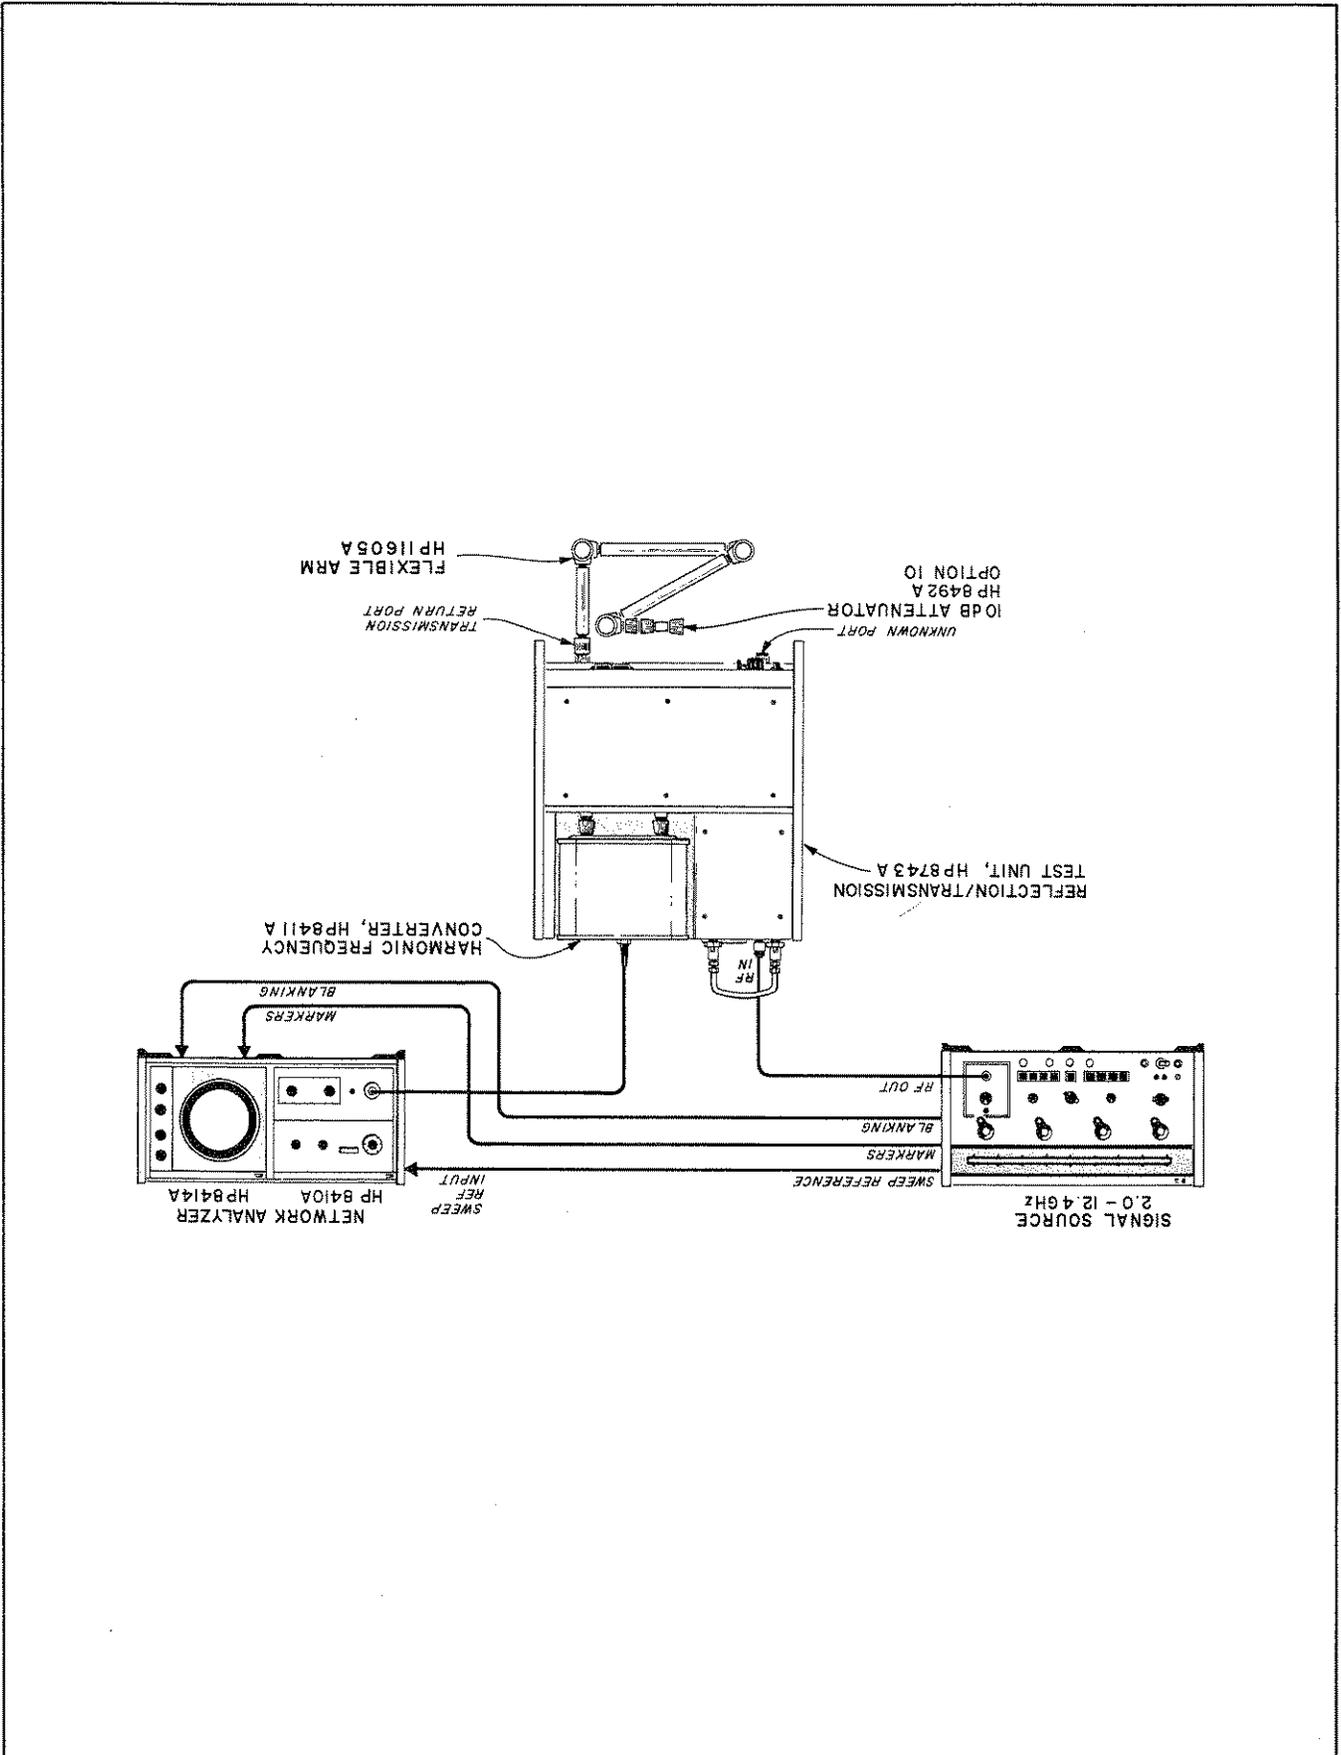


Figure 3-3. Transmission Measurements with 8410S-200 System Using 8414A Polar Display (Sheet 2 of 2)

TRANSMISSION MEASUREMENT WITH 8410S-200 SYSTEM																																															
<p>CALIBRATION DESCRIPTION</p> <ol style="list-style-type: none"> 1. Note the 8410A TEST CHANNEL GAIN setting. 2. This is the calibration gain setting. Adjust the TEST CHANNEL GAIN controls to locate the point of the CRT display representing the frequency of interest on the outside ring. The difference in TEST CHANNEL GAIN settings is the magnitude of the transmission gain or loss of the device under test at the frequency of interest. Note from the table below that the 8414A magnitude scale may be changed to convenient multiples by changing the 8410A TEST CHANNEL GAIN control setting as listed. 3. To determine the electrical length of the device under test, perform the following: <ol style="list-style-type: none"> a. Adjust the 8743A REFERENCE PLANE EXTENSION to again collapse the trace to a dot or smallest cluster. b. The electrical length of the device under test is two times the digital counter reading. 	<p>MEASUREMENT</p> <ol style="list-style-type: none"> 1. Connect equipment as shown in setup above. Connect a 10-dB attenuator, such as the HP 8492A Option 10, to the Flexible Arm (paragraph 3-17), and connect the attenuator to the 8743A UNKNOWN port. 2. Depress the 8743A TRANS pushbutton. 3. Set the signal source to sweep the band of interest. Adjust the signal source RF power and the 8410A SWEEP STABILITY control to obtain a REF CHANNEL LEVEL meter indication in the middle of the OPERATE range. 4. Push and hold the 8414A beam center pushbutton and adjust the centering controls to place the dot in the center of the polar display. 5. Obtain equal reference and test channel electrical lengths by adjusting the 8743A REFERENCE PLANE EXTENSION to collapse the trace to a dot or smallest cluster. If the digital counter is to be used to determine the electrical length of the device under test, it should be set to zero. A convenient way to do this is as follows: <ol style="list-style-type: none"> a. Adjust REFERENCE PLANE EXTENSION crank until counter reads all zeros. b. Hold thumbwheel to retain zero indication and readjust REFERENCE PLANE EXTENSION to collapse the trace to a dot or smallest cluster. 6. Adjust the 8410A amplitude and phase controls to place the dot or cluster at a reference indication of $\tau = 1/0^\circ$. 7. Insert the device to be tested between the UNKNOWN port and the 10-dB attenuator. 																																														
<p>Table of Magnitude Scale</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="width: 33%;">8410A TEST CHANNEL GAIN Change</th> <th style="width: 33%;">Full Scale</th> <th style="width: 33%;">Each Ring</th> </tr> </thead> <tbody> <tr> <td>From Cal. Setting</td> <td></td> <td></td> </tr> <tr> <td>+32</td> <td>0.025</td> <td>0.005</td> </tr> <tr> <td>+26</td> <td>0.05</td> <td>0.01</td> </tr> <tr> <td>+20</td> <td>0.1</td> <td>0.02</td> </tr> <tr> <td>+14</td> <td>0.2</td> <td>0.04</td> </tr> <tr> <td>+12</td> <td>0.25</td> <td>0.05</td> </tr> <tr> <td>+6</td> <td>0.5</td> <td>0.1</td> </tr> <tr> <td>Calibration Setting</td> <td>1.0</td> <td>0.2</td> </tr> <tr> <td>-6</td> <td>2.0</td> <td>0.4</td> </tr> <tr> <td>-12</td> <td>4.0</td> <td>0.8</td> </tr> <tr> <td>-14</td> <td>5.0</td> <td>1.0</td> </tr> <tr> <td>-20</td> <td>10.0</td> <td>2.0</td> </tr> <tr> <td>-26</td> <td>20.0</td> <td>4.0</td> </tr> <tr> <td>-32</td> <td>40.0</td> <td>8.0</td> </tr> </tbody> </table>			8410A TEST CHANNEL GAIN Change	Full Scale	Each Ring	From Cal. Setting			+32	0.025	0.005	+26	0.05	0.01	+20	0.1	0.02	+14	0.2	0.04	+12	0.25	0.05	+6	0.5	0.1	Calibration Setting	1.0	0.2	-6	2.0	0.4	-12	4.0	0.8	-14	5.0	1.0	-20	10.0	2.0	-26	20.0	4.0	-32	40.0	8.0
8410A TEST CHANNEL GAIN Change	Full Scale	Each Ring																																													
From Cal. Setting																																															
+32	0.025	0.005																																													
+26	0.05	0.01																																													
+20	0.1	0.02																																													
+14	0.2	0.04																																													
+12	0.25	0.05																																													
+6	0.5	0.1																																													
Calibration Setting	1.0	0.2																																													
-6	2.0	0.4																																													
-12	4.0	0.8																																													
-14	5.0	1.0																																													
-20	10.0	2.0																																													
-26	20.0	4.0																																													
-32	40.0	8.0																																													

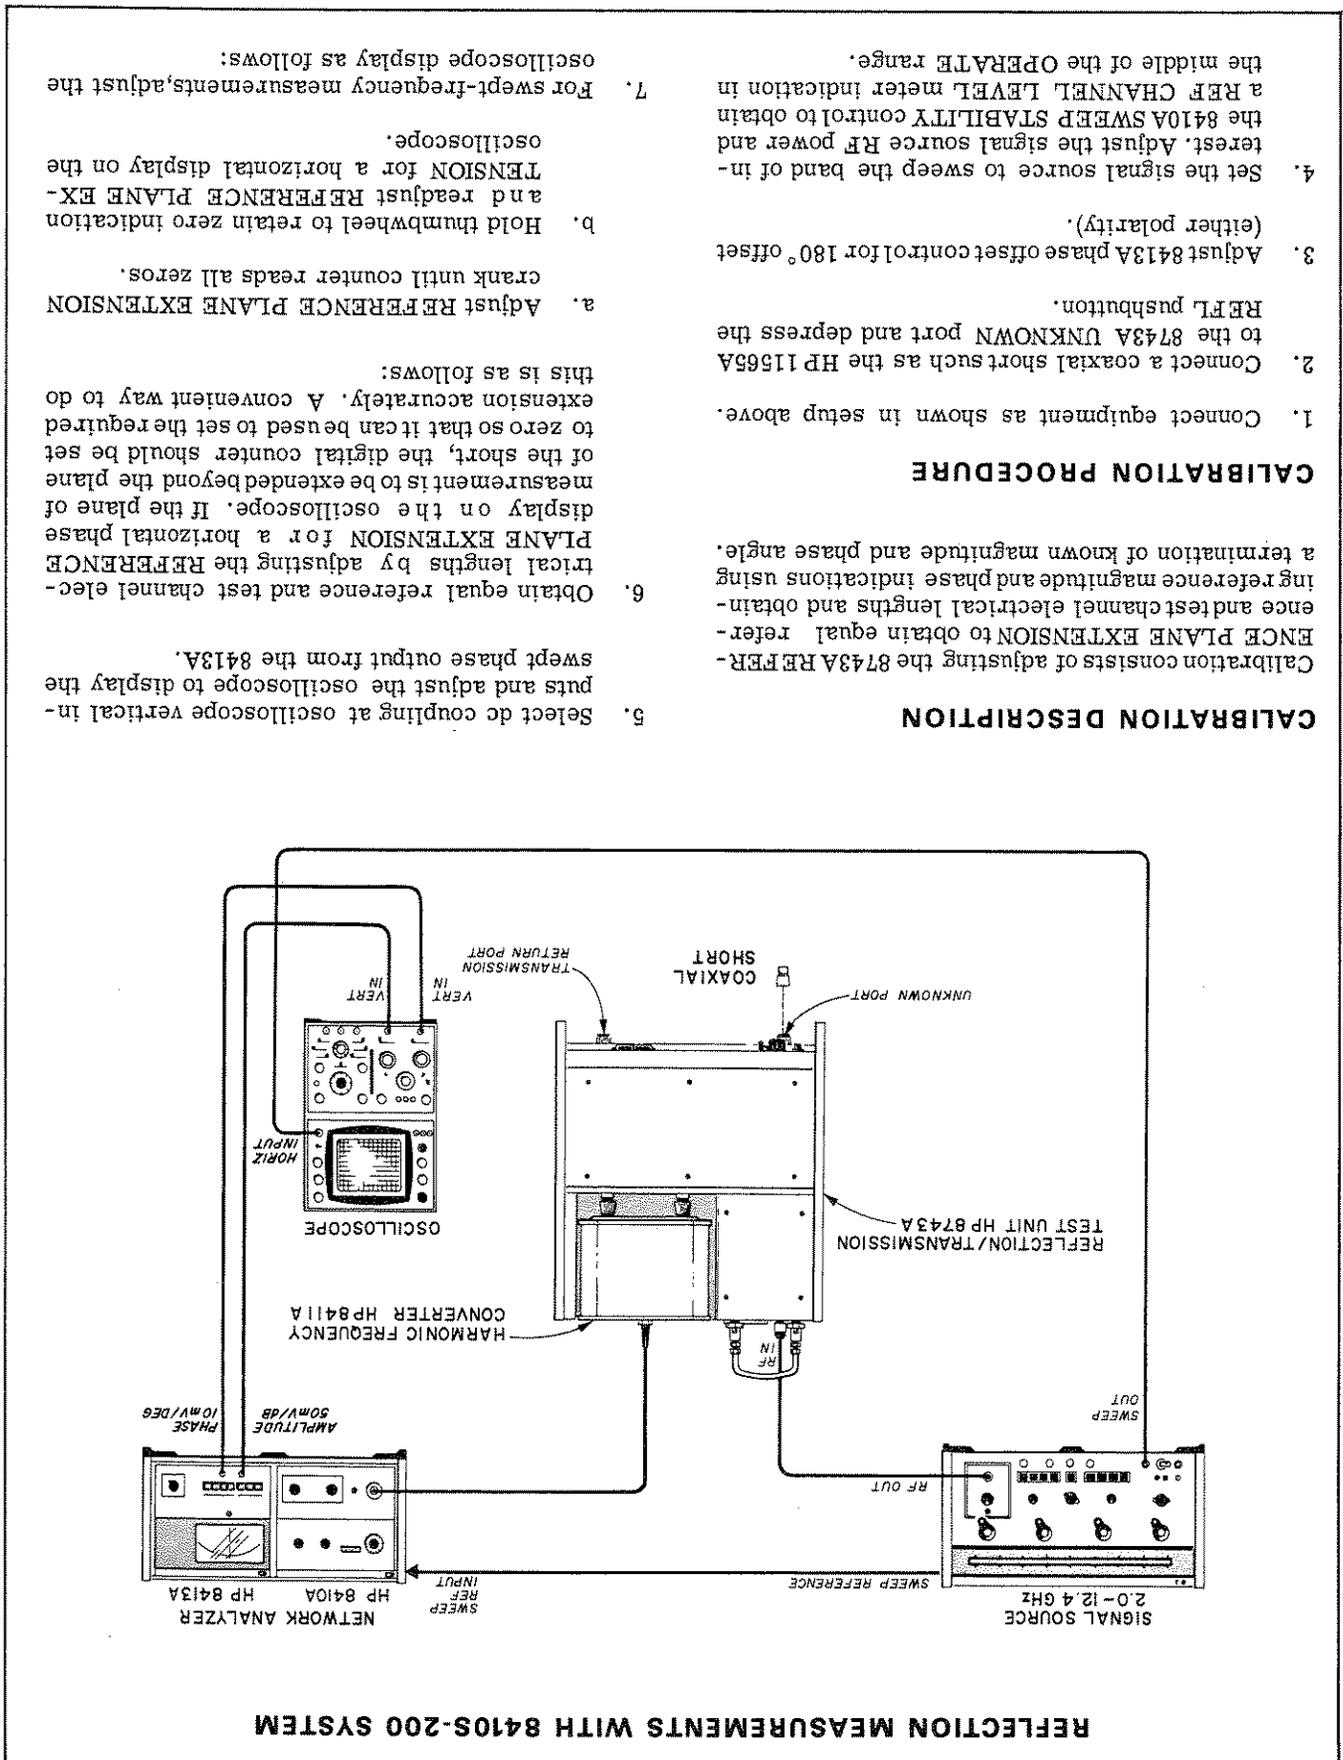Figure 3-4. Reflection Measurements with 8410S-200 System Using 8413A Display Unit. (Sheet 1 of 2)



CALIBRATION DESCRIPTION

Calibration consists of adjusting the 8743A REFERENCE PLANE EXTENSION to obtain equal reference and test channel electrical lengths and obtaining reference magnitude and phase indications using a termination of known magnitude and phase angle.

CALIBRATION PROCEDURE

1. Connect equipment as shown in setup above.
2. Connect a coaxial short such as the HP 11565A to the 8743A UNKNOWN PORT and depress the REFL pushbutton.
3. Adjust 8413A phase offset control for 180° offset (either polarity).
4. Set the signal source to sweep the band of interest. Adjust the signal source RF power and the 8410A SWEEP STABILITY control to obtain a REF CHANNEL LEVEL meter indication in the middle of the OPERATE range.
5. Select dc coupling at oscilloscope vertical inputs and adjust the oscilloscope to display the swept phase output from the 8413A.
6. Obtain equal reference and test channel electrical lengths by adjusting the REFERENCE PLANE EXTENSION for a horizontal phase display on the oscilloscope. If the plane of measurement is to be extended beyond the plane of the short, the digital counter should be set to zero so that it can be used to set the required extension accurately. A convenient way to do this is as follows:
 - a. Adjust REFERENCE PLANE EXTENSION crank until counter reads all zeros.
 - b. Hold thumbwheel to retain zero indication and readjust REFERENCE PLANE EXTENSION for a horizontal display on the oscilloscope.
7. For swept-frequency measurements, adjust the oscilloscope display as follows:

Figure 3-4. Reflection Measurements with 8410S-200 System Using 8413A Display Unit. (Sheet 2 of 2)

REFLECTION MEASUREMENTS WITH 8410S-200 SYSTEM

NOTE

Calibration for greater accuracy is discussed in Paragraph 3-12.

MEASUREMENT

1. Remove the coaxial short and connect the device to be tested to the 8743A UNKNOWN port.
2. Return the 8413A phase offset to zero.
3. For swept-frequency measurements, read magnitude and phase as follows:

a. For magnitude, note 8410A TEST CHANNEL GAIN settings. Increase TEST CHANNEL GAIN to return oscilloscope display to reference obtained during calibration. The difference in TEST CHANNEL GAIN settings is the reflection magnitude in return loss.

b. For phase, adjust oscilloscope vertical sensitivity and position controls to view the swept-phase display of the device under test. Use the calibrated 8413A output (10 mV/degree) and the oscilloscope vertical calibration to determine phase angle.

4. For single-frequency measurements, read magnitude and phase as follows:

a. For magnitude, note 8410A TEST CHANNEL GAIN settings. Increase TEST CHANNEL GAIN to return the 8413A meter indication to zero. The difference in TEST CHANNEL GAIN settings is the reflection magnitude in return loss.

b. For phase, adjust the 8413A phase offset for an on-scale meter indication on the most sensitive scale. The phase angle is the algebraic sum of phase offset and meter indication.

$$\Gamma_p = \text{Log}^{-1} (0.05 \times \text{return loss})$$

- a. Disconnect oscilloscope vertical input from 8413A amplitude channel to simulate no amplitude signal from 8413A. Note trace position.
- b. Reconnect vertical input and adjust 8410A TEST CHANNEL GAIN and AMPLITUDE VERNIER controls so that the average of the trace falls on the zero position noted in step (a) opposite.
- c. Adjust oscilloscope vertical position for a convenient amplitude reference.
- d. Disconnect oscilloscope vertical input from 8413A phase channel to simulate no phase signal from 8413A. Note trace position.
- e. Reconnect vertical input and adjust 8410A PHASE VERNIER control so that the average of the trace falls on the zero trace position noted in step (d) above.
- f. Adjust oscilloscope vertical position for a convenient phase reference.

8. To calibrate for single-frequency measurements, perform the following:

- a. Set the signal source for single-frequency operation.

- b. Set 8413A PHASE OFFSET switch to zero and depress PHASE 180 degree pushbutton. Adjust 8410A PHASE VERNIER control for a zero degree indication on the 8413A. Depress PHASE 6 degree pushbutton and again zero meter with 8410A PHASE VERNIER.
- c. Depress 8413A AMPLITUDE 30 dB pushbutton. Adjust 8410A TEST CHANNEL GAIN and AMPLITUDE VERNIER controls for a zero dB indication on the 8413A meter. Depress AMPLITUDE 3 dB pushbutton and again zero meter with 8410A AMPLITUDE VERNIER control.

Figure 3-5. Transmission Measurement with 8410S-200 System Using 8413A Display Unit. (Sheet 1 of 2)

1. Connect equipment as shown in setup above. Connect a 10-dB attenuator, such as the HP 8492A Option 10, to the HP 11605A Flexible Arm (paragraph 3-17) and connect the attenuator to the 8743A UNKNOWN port. Depress 8743A TRANS pushbutton.
2. Set the signal source to sweep the band of interest. Adjust the signal source RF power and the 8410A SWEEP STABILITY control to obtain a REF CHANNEL LEVEL meter indication in the middle of the OPERATE range.
3. Select dc coupling at oscilloscope vertical inputs and adjust the oscilloscope to display the swept phase output from the 8413A.
4. Obtain equal reference and test channel electrical lengths by adjusting the 8743A REFERENCE PLANE EXTENSION for a horizontal phase display on the oscilloscope. If the digital counter is to be used to determine the electrical length of the device under test, it should be set to zero. A convenient way to do this is as follows:
 - a. Adjust REFERENCE PLANE EXTENSION crank until counter reads all zeros.
 - b. Hold thumbwheel to retain zero indication and readjust REFERENCE PLANE EXTENSION for a horizontal display on the oscilloscope.
5. For swept-frequency measurements, adjust the oscilloscope display as follows:
 - a. Disconnect oscilloscope vertical input from 8413A amplitude signal from 8413A. Note late no amplitude signal from 8413A. Note trace position.

CALIBRATION PROCEDURE

Calibration consists of adjusting the 8743A REFERENCE PLANE EXTENSION to obtain equal reference and test channel electrical lengths and obtaining reference magnitude and phase indication.

CALIBRATION DESCRIPTION

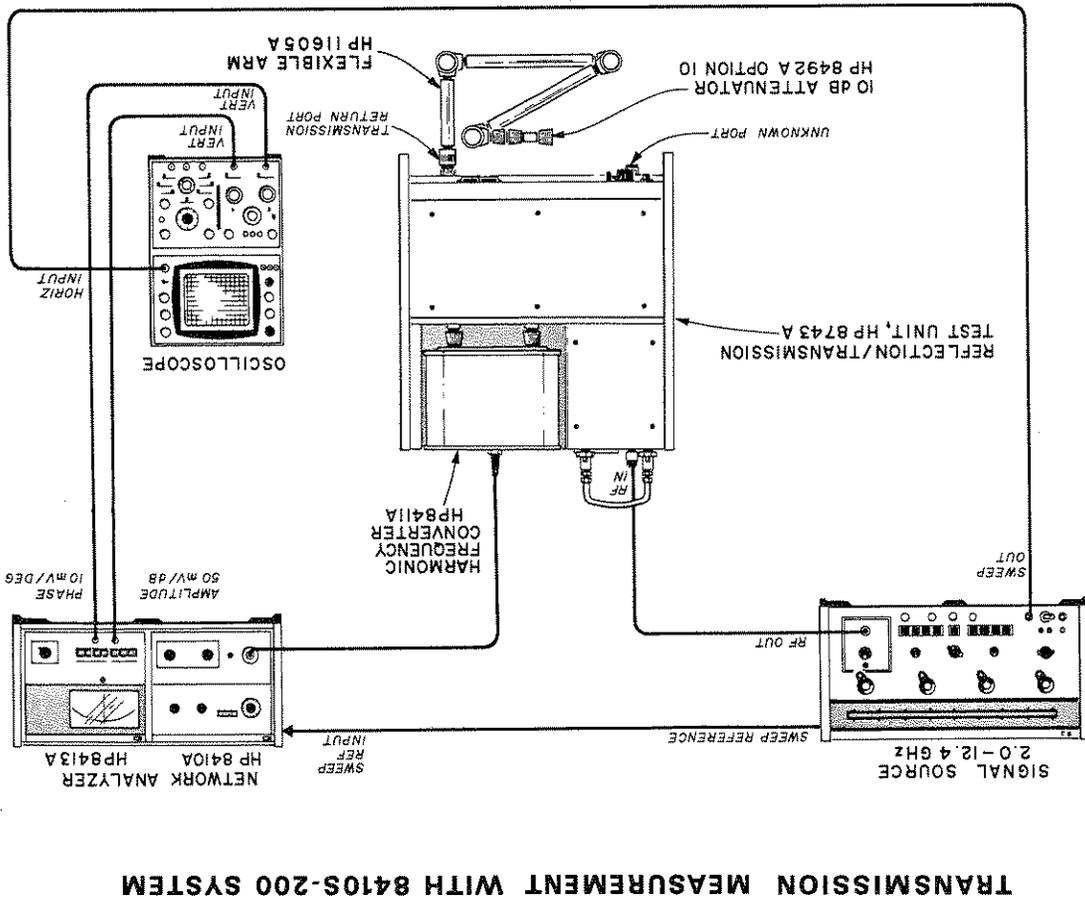


Figure 3-5. Transmission Measurement Using 8410S-200 System With 8413A Display Unit. (Sheet 2 of 2)

TRANSMISSION MEASUREMENT WITH 8410S-200 SYSTEM

MEASUREMENT


1. Insert the device to be tested between the 8743A UNKNOWN port and the 10-dB attenuator.
 2. For swept-frequency measurements, read magnitude and phase as follows:
 - a. For magnitude, note 8410A TEST CHANNEL GAIN settings. Adjust TEST CHANNEL GAIN to return oscilloscope display to reference obtained during calibration. The difference in TEST CHANNEL GAIN settings is the transmission gain or loss in dB of the device under test.
 - b. For phase, adjust oscilloscope vertical sensitivity and position controls to view the swept-phase display of the device under test. Use the calibrated 8413A output (10 mV/degree) and the oscilloscope vertical calibration to determine phase angle.
- NOTE**
- The phase display is the combination of linear phase shift (due to electrical length) and non-linear phase shift. Group delay can be determined from this display. (See HP Application Note 92.)
3. For single-frequency measurements, read magnitude and phase as follows:
 - a. For magnitude, note 8410A TEST CHANNEL GAIN settings. Adjust TEST CHANNEL GAIN to return the 8413A meter indication to zero. The difference in TEST CHANNEL GAIN settings is the transmission gain or loss in dB of the device under test.
 - b. For phase, adjust the 8413A PHASE OFFSET for an on-scale meter indication on the most sensitive scale. The phase angle is the algebraic sum of PHASE OFFSET and meter indication.
- a. Adjust oscilloscope vertical position for a convenient amplitude reference.
 - b. Disconnect oscilloscope vertical input from 8413A phase channel, to simulate no phase signal from 8413A. Note trace position.
 - c. Reconnect vertical input and adjust 8410A PHASE VERNIER controls so that the average of the trace falls on the zero trace position noted in step (d) above.
 - d. Adjust oscilloscope vertical position for a convenient phase reference.
6. To calibrate for single-frequency measurements, perform the following:
 - a. Set the signal source for single-frequency operation.
 - b. Set 8413A PHASE OFFSET switch to zero and depress PHASE 180 degree pushbutton. Adjust 8410A PHASE VERNIER control for zero degree indication on the 8413A. Depress PHASE 6-degree pushbutton and again zero meter with PHASE VERNIER.
 - c. Depress 8413A AMPLITUDE 30 dB pushbutton. Adjust 8410A TEST CHANNEL GAIN and AMPLITUDE VERNIER controls for a zero dB indication on the 8413A meter. Depress AMPLITUDE 3 dB pushbutton and again zero meter with 8410A AMPLITUDE VERNIER control.

b. For single frequencies below 1 GHz, set up the 8745A to measure the desired reflection coefficient (S11 or S22). Calibrate the display unit and connect a low reflection termination ($\rho = 0.005$ or $VSWR = 1.01$ max.), such as an HP Model H01-909A, to the 8745A incident power port (INPUT PORT A or B) at the reference plane. Since the magnitude of the Model H01-909A reflection is very small, the measured reflection coefficient on the 8414A can be considered the directionality.

2. For single frequencies above 1 GHz, set up the 8743A or 8745A to measure the desired reflection coefficient. Calibrate the display unit and attach the sliding load (HP Model 907A) to the 8743A UNKNOWN port or to the 8745A incident power port (INPUT PORT A or B). Slide the load and adjust the horizontal and vertical controls until the circle rotates about the center of the 8414A CRT, as shown in Figure 3-8. Directionality is now cancelled for this frequency and this TEST CHANNEL GAIN setting on the 8410A.

3-15. On the 8414A polar display, the vector subtraction can be performed directly with the horizontal and vertical position controls. Increase the 8410A test channel gain so full scale reflection on the polar display is suitable for the component you wish to measure and perform the following:

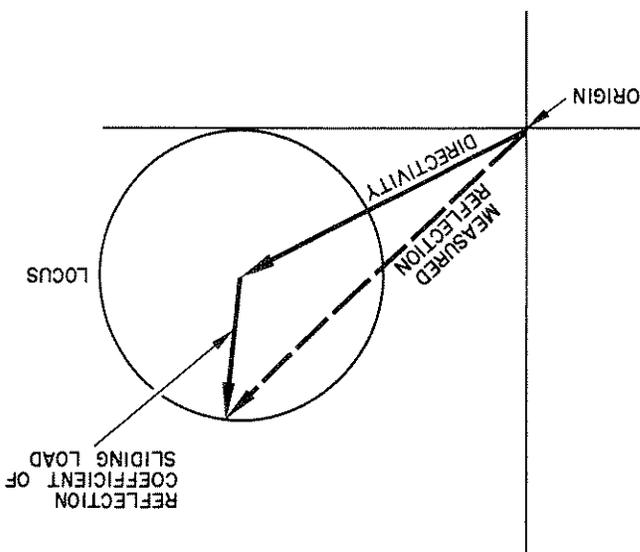Figure 3-7. Typical Polar Plot Showing Locus of Measured Reflection when Sliding Load is Moved.



load. Figure 3-7 depicts the sliding load in one position. As the sliding load is moved, the magnitude of its reflection remains constant but the phase of the reflection changes. As the load is moved, its reflection indication rotates in a circle of constant magnitude about the directionality vector. The center of this circle is the tip of the directionality vector. When the location of the center of the circle is known, the error can be vectorially subtracted from the measured reflection to obtain the reflection coefficient of the device under test.

vector. Adjust the 8414A horizontal and vertical controls to place the dot in the center of the CRT. Directionality is now cancelled for this frequency and this TEST CHANNEL GAIN setting on the 8410A.

3-16. System tracking, or response also introduces an error into a measurement. This error occurs only in sweep mode and is eliminated by simply making CW (single frequency) measurements.

3-17. INCREASED ACCURACY FOR TRANSMISSION MEASUREMENTS IN 8410S-200 SYSTEMS.

3-18. A 50-ohm coaxial attenuator is recommended for transmission measurements. An attenuator connected between the output of the device under test and the HP 11605A Flexible Arm reduces the ambiguity due to mismatch between the 11605A, 8743A, and 8411A. A 10-dB low-reflection attenuator, such as an HP 8492A Option 10, reduces this ambiguity to essentially that due to the mismatch of the attenuator ($VSWR < 1.25$). Greater values of attenuation may be used, however, values greater than 10 dB will not reduce mismatch. For values less than 10 dB the multiple mismatch between the 11605A, 8743A, and 8411A should be taken into consideration.

3-19. In addition to reducing ambiguity due to mismatch, the 10-dB attenuator makes the test channel power level during calibration the same for transmission and reflection. Also, the combined electrical lengths of the 8492A and the 11605A makes the electrical length of the test channel in the transmission mode nearly equal to its length in the reflection mode. This means that it is possible to calibrate in reflection mode of operation, then switch to transmission mode and be in approximate calibration. However, for best accuracy, it is necessary to recalibrate in each mode.

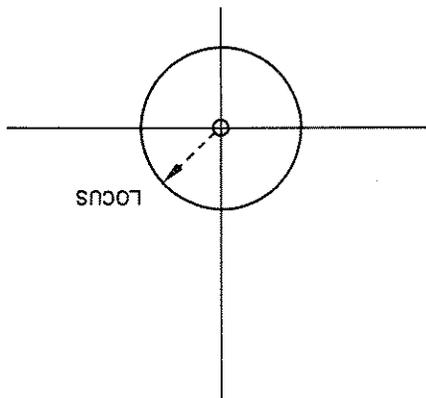


Figure 3-8. Center of Polar Display, Showing Locus of Sliding Load Vector with Directionality Cancelled.

Item No.	System Used in	Instrument	Critical Specifications	Recommended HP Model
1	-100 -200 -300	Signal Source	Frequency Range: 0.11 to 12.4 GHz Output Power: +8 dBm	8690B/8699B (0.1 to 4 GHz) 8690B/8693A, B (4 to 8 GHz) 8690B/8694A, B (8 to 12.4 GHz)
2	-100 -200 -300	Power Meter and Thermistor Mount	Frequency Range: 0.11 to 12.4 GHz Power Range: +5 to -30 dBm Instrument Accuracy: ±3% Input Impedance: 50 ohms SWR: 1.35 maximum Connector: APC-7*	432A with 8478B Option 11 Thermistor Mount
3	-200 -300	Swept Slotted-Line	Any frequency in range: 2.0 to 12.4 GHz Impedance: 50 ohm ±0.2 ohms Output Connector: APC-7* Residual SWR: 1.03 or less	817A
4	-100 -200 -300	Dual Trace Oscilloscope	Vertical Amplifier: Dual trace, DC Coupled Vertical Sensitivity: 5 mV/cm Bandwidth: 450 KHz minimum Horizontal Sweep Rate: 1µs/cm to 5 s/cm External Horizontal Input	1200A or 140A/1401A/1422A or 180A/1801A/1820A or 181A/1801A/1820A
5	-100 -200 -300	Narrow Band AC Voltmeter	Frequency Range: 270 through 290 KHz Selectivity: 200 and 1000 Hz at 278 KHz Dynamic Range: 75 dB Meter Scale: dB	310A or 312A

*Amphenol RF Division, Danbury, Connecticut.

Table 4-1. Recommended Test Equipment (Sheet 1 of 2)

4-1. INTRODUCTION.

This section provides instructions for checking the performance of the system, as well as isolating trouble to an individual instrument. For adjustment or alignment procedures, see the individual instrument Operating and Service Manual.

4-3. PERFORMANCE TEST.

The performance tests are presented in Figures 4-1 through 4-3. These procedures may be used during incoming inspection to verify the electrical operation of all of the instruments in the system. They may also be used during periodic evaluation of the system or after repair or alignment of one of the individual instruments. Test equipment required for these procedures is listed in Table 4-1. Other equipment required for the tests is furnished in the accessory kit that is included with the system.

**SECTION IV
MAINTENANCE**

4-6. TROUBLESHOOTING.

Figure 4-1 contains performance test procedures which are to be performed on all system configurations (8410S-100, -200, and -300). The procedures in Figure 4-2 check the transducer in the 8410S-100 system and Figure 4-3 checks the transducer in the 8410S-200 system. Therefore, to check an 8410S-100 system, perform the procedures in Figures 4-1 and 4-2. For an 8410S-200 system, perform procedures in Figures 4-1 and 4-3. For an 8410S-300 system, perform all of the procedures in Figures 4-1 through 4-3. The troubleshooting procedures are presented in Figures 4-6 and 4-8. They isolate a fault to an individual instrument. When the malfunctioning instrument is found, refer to the Operating and Service Manual for the faulty instrument to further isolate the trouble within the instrument.


Item No.	Used in System	Instrument	Critical Specifications	Recommended HP Model
6	-100 -200 -300	Variable Attenuator (Calibrated)	Attenuation: 0 and 60 dB Input and Output Impedance: 50 ohms nominal Calibration: at 60 dB setting referenced from 0 dB setting Calibration Accuracy: ± 0.3 dB Calibration Frequency: 2.0 GHz	354A calibrated by Standards Laboratory
7	-100 -200 -300	Fixed Air Line (2 Required)	50-ohm, 10-cm air line extension with APC-7* connectors	11566A
8	-100 -200 -300	50-ohm Load	Impedance: 50 ohms Power Rating: 10 mW maximum VSWR: 1.01 maximum, 0.11 to 2 GHz; 1.1 maximum 2 to 12.4 GHz Connector: APC-7*	H01-909A
9	-100 -200 -300	Sliding Load	50-ohm coaxial sliding termina- tion with APC-7* connector SWR: < 1.05 Frequency Range: 1 to 12.4 GHz	907A
10	-100 -200 -300	DC Power Supply	Range: 0-5 Vdc	721A
11	-100 -200 -300	Signal Generator	Frequency Range: 270 through 290 kHz Output Level: 0 to 3V rms Output Impedance: 50 to 600 ohms	200CD or 651A
12	-100 -200 -300	Variable Attenuator	Range: 12 dB in 1-dB steps Frequency: 278 kHz and 1 GHz Accuracy: ± 0.35 dB at 278 kHz and 1 GHz	355C
13	-100 -200 -300	Variable Attenuator	Range: 120 dB in 10-dB steps Frequency: 278 kHz and 1 GHz Accuracy: ± 1.5 dB at 278 kHz and 1 GHz	355D
14	-100 -200 -300	DC Digital Voltmeter	Accuracy: 0.05% Input Impedance: 10 megohm minimum Automatic Range Selection: range to 50V	3440A with 3442A Automatic Range Selector Plug-in

*Amphenol RF Division, Danbury, Connecticut.

Table 4-1. Recommended Test Equipment (Sheet 2 of 2)

Figure 4-1. Performance Test Procedures Common to all Systems. (Sheet 1 of 20)

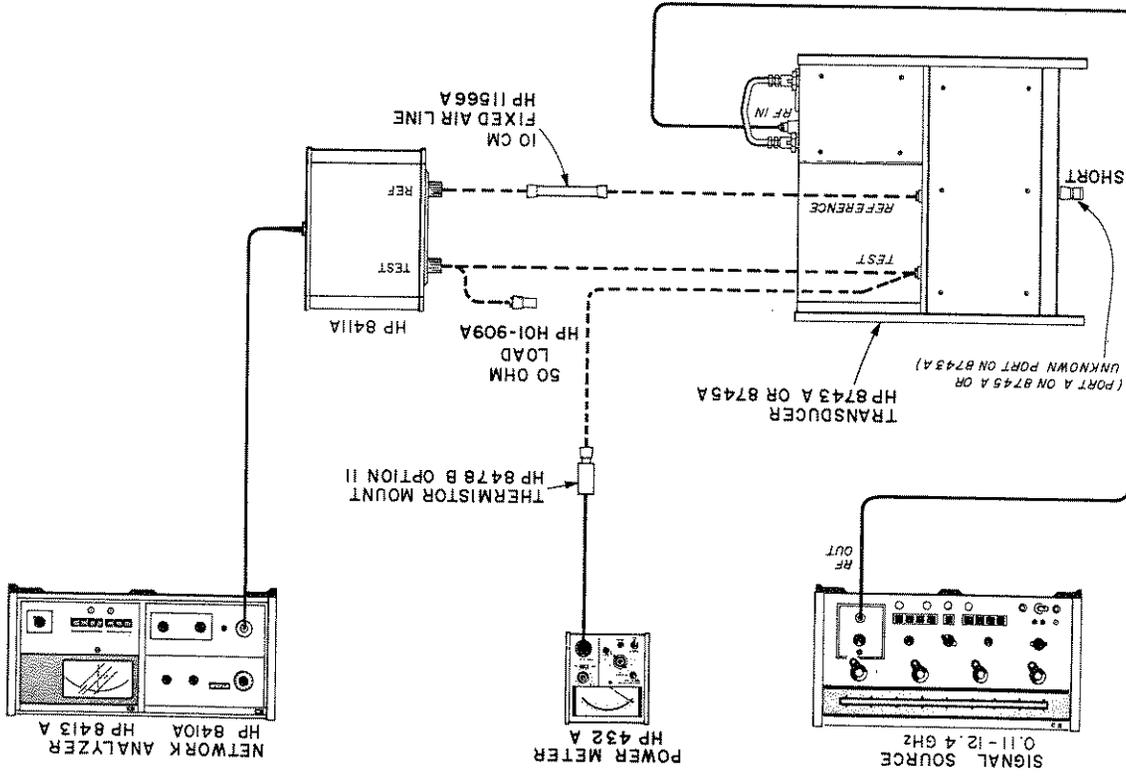EQUIPMENT: Items 1, 2, 7, and 8, Table 4-1.



TEST SETUP

A -30 dbm signal at the TEST input of the 8411A is used to set a reference at the 8413A. The TEST port of the 8411A is terminated, leaving only TEST CHANNEL noise to be measured at the 8413A. Noise level of -78 dbm is 48 dB lower than the -30 dbm reference level. 40 dB of gain is added with the TEST CHANNEL GAIN control and -8 dB from zero reference is indicated on the 8413A, totaling 48 dB.

TEST DESCRIPTION

TEST CHANNEL NOISE: Less than -78 dbm.

SPECIFICATION TESTED

1

DESCRIPTION AND PROCEDURE

TEST

Figure 4-1. Performance Test Procedures Common to all Systems. (Sheet 2 of 20)


TEST	DESCRIPTION AND PROCEDURE
1 (Contd)	<p><u>PROCEDURE</u></p> <p>a. Connect equipment as shown above. Install short on port A of 8745A or UNKNOWN Port of 8743A. If 8745A is used, depress INPUT PORT A and S11 pushbuttons. If 8743A is used, depress REFLECT pushbutton. Set signal source for single-frequency (CW) operation in range of transducer used.</p> <p>b. Disconnect 8411A from 8743A or 8745A and check for -30 dBm signal level at 8743A or 8745A TEST port with power meter. If necessary, adjust signal source for -30 dBm indication. Reconnect 8411A to 8743A or 8745A.</p> <p>c. Check that 8410A REF CHANNEL LEVEL meter indicates in the OPERATE range.</p> <p>d. Press 8413A PHASE 180 degree pushbutton then adjust the 8410A PHASE VERNIER control: the 8413A meter indication should change smoothly indicating the 8410A is phase locked.</p> <p>e. Press 8413A AMPLITUDE 10 dB pushbutton. Adjust 8410A AMPL VERNIER and TEST CHANNEL GAIN controls to obtain a zero (center of scale) indication on 8413A meter.</p> <p>f. Disconnect 8411A from 8743A or 8745A, extend reference channel with 10-cm air line, and connect 50-ohm termination to 8411A TEST input.</p> <p>g. Increase 8410A TEST CHANNEL GAIN by 40 dB. The 8413A meter should indicate in the negative direction at least -8 dB. (This indicates less than -78 dBm equivalent input noise.)</p>
2	<p><u>SPECIFICATION TESTED</u></p> <p>IF GAIN CONTROL RANGE: 69 dB total in 10- and 1-dB steps; vernier provides continuous adjustment over at least 2 dB.</p> <p>IF GAIN CONTROL ACCURACY: ± 0.1 dB per 10-dB step and ± 0.05 dB per 1-dB step. A combination of both 10 dB and 1 dB steps not to exceed ± 0.2 dB.</p> <p><u>TEST DESCRIPTION</u></p> <p>The TEST CHANNEL GAIN control is tested for accuracy and the AMPL VERNIER control operation is checked. This is done by feeding a constant RF signal through the test channel and monitoring the rear-panel test channel 278 KHz IF output signal on a narrow-band ac voltmeter. The attenuators are set at each position and the resultant change in signal level is read on the ac voltmeter.</p>

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 3 of 20)

- a. Change equipment test setup as shown above. Install short on port A of 8745A or UNKNOWN PORT if 8743A is used, depress REFL pushbutton. Set signal source for single-frequency (CW) operation in the range of the transducer used.
- b. Check for phase-locked condition in the 8410 as follows:
 - (1) REF CHANNEL LEVEL meter should indicate in the OPERATE range. If not, adjust signal source power output to obtain OPERATE indication on meter.
 - (2) Depress 8413A PHASE 180 degree pushbutton and adjust PHASE OFFSET for near zero degree meter indication. Adjust the 8410A PHASE VEERNER control: the 8413A phase meter indication should change smoothly, indicating the 8410A is phase locked.
- c. Set the 8410A TEST CHANNEL GAIN 10 dB/step control to 0 dB.

PROCEDURE

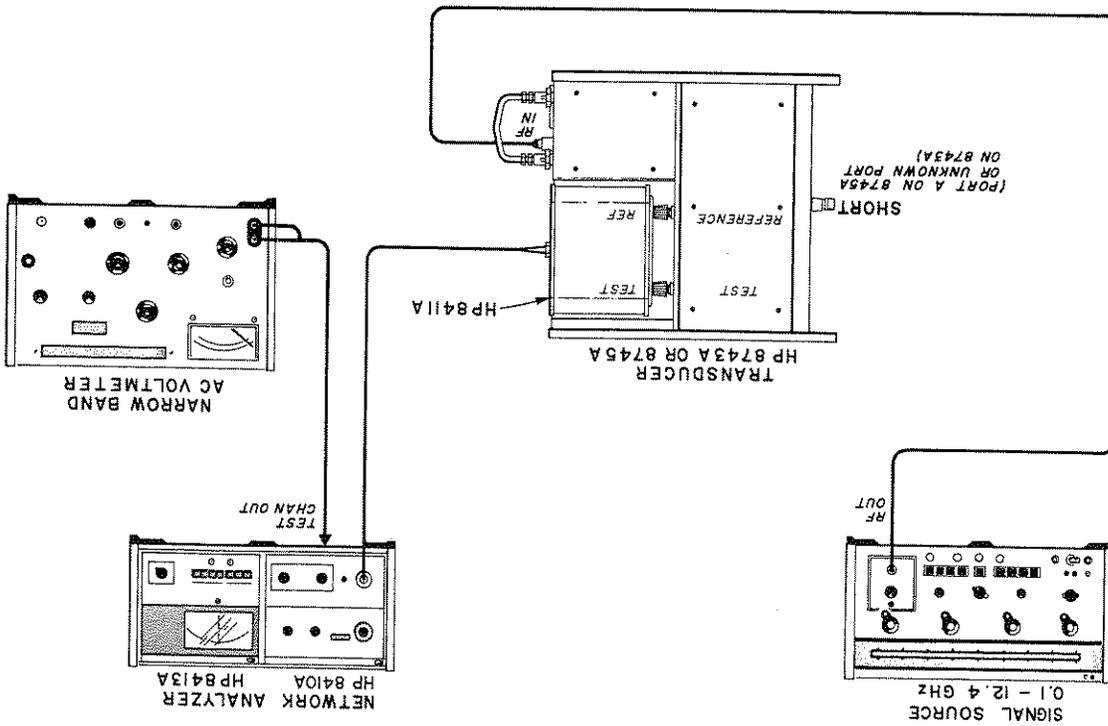EQUIPMENT: Items 1 and 5, Table 4-1.



TEST SETUP

2 (Contd)

DESCRIPTION AND PROCEDURE

TEST

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 4 of 20)

TEST	DESCRIPTION AND PROCEDURE																					
2 (Contd)	<p>PROCEDURE</p> <p>d. Set narrow band ac voltmeter to 1-kHz bandwidth and frequency to 278 kHz. Adjust 8410A AMPL VERNIER control and TEST CHANNEL GAIN 1 dB/step control for a -60 dB reference indication on the ac voltmeter. (Set ac voltmeter to -60 dB range and adjust reference level, 8410A AMPL VERNIER control, and TEST CHANNEL GAIN 1 dB/step control for a zero dB ac voltmeter indication.)</p> <p>e. Increase 8410A TEST CHANNEL GAIN in 10-dB steps and check accuracy as indicated below.</p> <table border="1" data-bbox="402 1200 1281 1570"> <thead> <tr> <th>Model 8410A TEST CHANNEL GAIN</th> <th>AC Voltmeter Range Setting</th> <th>AC Voltmeter Indication</th> </tr> </thead> <tbody> <tr> <td>10 dB</td> <td>-50 dB</td> <td>0(±0.1) dB ± voltmeter error</td> </tr> <tr> <td>20 dB</td> <td>-40 dB</td> <td>0(±0.2) dB ± voltmeter error</td> </tr> <tr> <td>30 dB</td> <td>-30 dB</td> <td>0(±0.2) dB ± voltmeter error</td> </tr> <tr> <td>40 dB</td> <td>-20 dB</td> <td>0(±0.2) dB ± voltmeter error</td> </tr> <tr> <td>50 dB</td> <td>-10 dB</td> <td>0(±0.2) dB ± voltmeter error</td> </tr> <tr> <td>60 dB</td> <td>0 dB</td> <td>0(±0.2) dB ± voltmeter error</td> </tr> </tbody> </table> <p>f. Set ac voltmeter to -40 dB range, set 8410A TEST CHANNEL GAIN 10 dB/step control to 20 dB, and set 1 dB/step control to zero dB. Adjust AMPL VERNIER control for a reference indication on the ac voltmeter at any one-dB scale division.</p> <p>g. Increase 8410A TEST CHANNEL GAIN 1 dB/step control in 1-dB steps; ac voltmeter indications should increase in corresponding 1-dB steps. If necessary, change ac voltmeter range to a higher or lower scale. Each meter indication must be within ±0.1 dB of a 1-dB major scale division on the meter, ± the error of the voltmeter.</p> <p>h. Using the ac voltmeter, check AMPL VERNIER range. It should be at least 2 dB.</p>	Model 8410A TEST CHANNEL GAIN	AC Voltmeter Range Setting	AC Voltmeter Indication	10 dB	-50 dB	0(±0.1) dB ± voltmeter error	20 dB	-40 dB	0(±0.2) dB ± voltmeter error	30 dB	-30 dB	0(±0.2) dB ± voltmeter error	40 dB	-20 dB	0(±0.2) dB ± voltmeter error	50 dB	-10 dB	0(±0.2) dB ± voltmeter error	60 dB	0 dB	0(±0.2) dB ± voltmeter error
Model 8410A TEST CHANNEL GAIN	AC Voltmeter Range Setting	AC Voltmeter Indication																				
10 dB	-50 dB	0(±0.1) dB ± voltmeter error																				
20 dB	-40 dB	0(±0.2) dB ± voltmeter error																				
30 dB	-30 dB	0(±0.2) dB ± voltmeter error																				
40 dB	-20 dB	0(±0.2) dB ± voltmeter error																				
50 dB	-10 dB	0(±0.2) dB ± voltmeter error																				
60 dB	0 dB	0(±0.2) dB ± voltmeter error																				
3	<p>SPECIFICATION TESTED</p> <p>REFERENCE CHANNEL INPUT POWER RANGE: 20 dB variation causes less than 1.5 dB amplitude and less than 4 degree phase change at output. The 20-dB range should be between -16 dBm and -44 dBm.</p> <p>TEST DESCRIPTION</p> <p>The 8410A AGC circuit is checked for a 20-dB range within the input power range of -16 dBm and -44 dBm. This is done by changing RF input power levels to the two operating extremes of the AGC circuit and checking for constant reference channel output. Phase and amplitude are then monitored through the 20 dB AGC range to determine that they remain within specifications through the entire range.</p>																					

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 5 of 20)

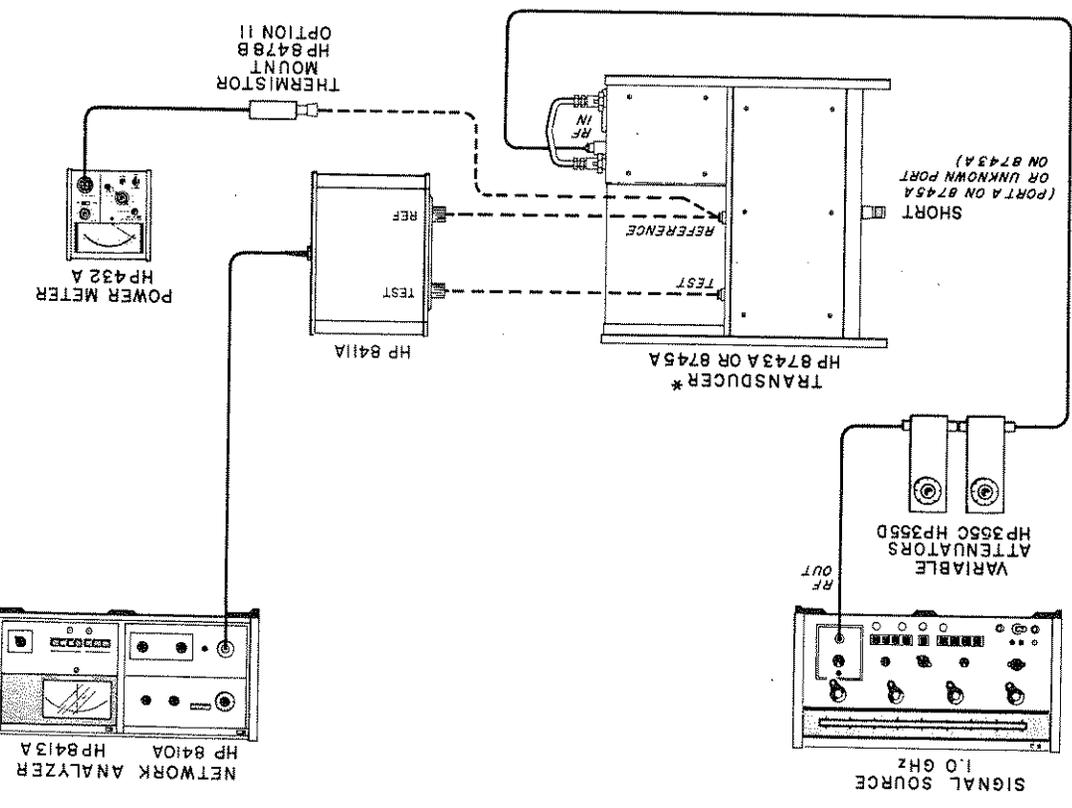
TEST	DESCRIPTION AND PROCEDURE
3 (Contd)	<p style="text-align: center;"><u>TEST SETUP</u></p>  <p>*The coupling of the 8743A internal directional coupler rolls off below 2.0 GHz; however, this unit may be used at 1.0 GHz for this test.</p> <p>EQUIPMENT: Items 1, 2, 12, and 13, Table 4-1.</p>
	<p style="text-align: center;"><u>PROCEDURE</u></p> <ol style="list-style-type: none"> a. Change test setup as shown above. Install short on port A of 8745A or UNKNOWN port of 8743A. If 8743A is used, depress INPUT PORT A and S11 pushbuttons. If 8743A is used, depress REFL pushbutton. Set signal source for single-frequency (CW) operation at 1.0 GHz. Set HP 355C and 355D attenuators to zero dB. b. Check for phase-locked condition in the 8410A as follows: <ol style="list-style-type: none"> (1) The 8410A REF CHANNEL LEVEL meter should indicate in the OPERATE range. If not, adjust signal source power output to obtain an OPERATE indication on meter. (2) Depress 8413A PHASE 180 degree pushbutton. Adjust the PHASE VERNIER control: the 8413A meter indication should change smoothly indicating the 8410A is phase locked.

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 6 of 20)


TEST	DESCRIPTION AND PROCEDURE
3 (Contd)	<p><u>PROCEDURE</u></p> <p>c. Depress 8413A AMPLITUDE 10-dB pushbutton and zero meter by adjusting 8410A AMPL VERNIER and AMPLITUDE TEST CHANNEL GAIN controls.</p> <p>d. Slowly increase signal source power until the 8413A meter indication increases rapidly, indicating the top of the AGC range. Reduce signal source power slightly to return the 8413A meter to zero so that the AGC is operating just at the top of its range.</p> <p>e. Disconnect the 8411A from the 8743A or the 8745A and connect power meter thermistor mount to 8743A or 8745A REFERENCE port. Measure and note power meter indication.</p> <p>f. Reconnect 8411A to 8743A or 8745A. Reduce signal source power to 8743A or 8745A by adding attenuation with HP 355C and 355D attenuators until the 8413A meter indication starts to decrease rapidly. This is the lower limit of the AGC range. Increase the signal with the attenuators until the 8413A meter returns to zero reference just at the edge of the AGC lower limit. Record this attenuator setting. Calculate the AGC lower power level at the 8743A or 8745A REFERENCE port by subtracting the total attenuation set at the HP 355C and 355D attenuators from the AGC upper limit noted in step e. The AGC range should be 20 dB or greater and should be between the limits of -16 dBm and -44 dBm. Note the limits of the AGC range.</p> <p>g. Select the middle 20 dB segment from the AGC range noted in step f. (For example, if the measured AGC range were -20 dBm to -44 dBm, the middle 20 dB segment would be -22 dBm to -42 dBm. This would be a range of settings on the 355C and 355D attenuators between 2 dB and 22 dB.) Set the 355C and 355D attenuators for the upper end of selected 20 dB AGC range. (In the example, this would be a 2 dB setting.)</p> <p>h. Press the 8413A PHASE 6 degree pushbutton to select the lowest phase scale. Adjust the 8413A meter to zero by adjusting the 8413A PHASE OFFSET switches, the 8410A PHASE VERNIER control, and the 8743A or 8745A REFERENCE PLANE EXTENSION control.</p> <p>i. Slowly increase attenuation of 355C and 355D attenuators, one dB at a time, until 20 dB of attenuation is added and the lower end of the 20-dB AGC segment is reached. The difference between the maximum and minimum indication on the 8413A meter should not be more than 4 degrees.</p> <p>j. Press the 8413A AMPLITUDE 3 dB pushbutton to select the lowest amplitude range. Adjust the 8410A AMPL VERNIER and AMPLITUDE TEST CHANNEL GAIN controls to obtain a zero indication on the 8413A meter. Adjust the 355C and 355D attenuators through the same 20-dB range used in step i. The difference between the maximum and minimum indication on the 8413A meter should not be more than 1.5 dB.</p>
4	<p><u>SPECIFICATION TESTED</u></p> <p>TEST CHANNEL DYNAMIC RANGE: 60 dB or greater.</p> <p><u>TEST DESCRIPTION</u></p> <p>A known signal level of -15 dBm is applied to the 8411A TEST channel RF input. The corresponding amplitude indication on the 8413A meter is noted. This represents the top of the test channel input power range. A variable attenuator is used to reduce the RF signal at the input of the 8411A to -75 dBm (a change of 60 dB). The corresponding indication is</p>

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 7 of 20)

- a. Change equipment test setup as shown above. Install short on port A of 8745A or UNKNOWN port of 8743A. If 8745A is used, depress INPUT PORT A and S11 pushbuttons. If 8743A is used, depress REF L pushbutton. Set signal source for single-frequency (CW) operation at 2 GHz.
- b. Check for phase-locked condition in the 8410A as follows:
 - (1) REF CHANNEL LEVEL meter should indicate in the OPERATE range. If not, adjust signal source power output to obtain OPERATE indication on meter.
 - (2) Depress 8413A PHASE 180 degree pushbutton. Adjust the 8410A PHASE VERNIER control: the 8413A meter indication should change smoothly indicating the 8410A is phase locked.
- c. Connect thermistor mount to variable attenuator output.
- d. Set variable attenuator and 8410A TEST CHANNEL GAIN controls to zero dB.

PROCEDURE

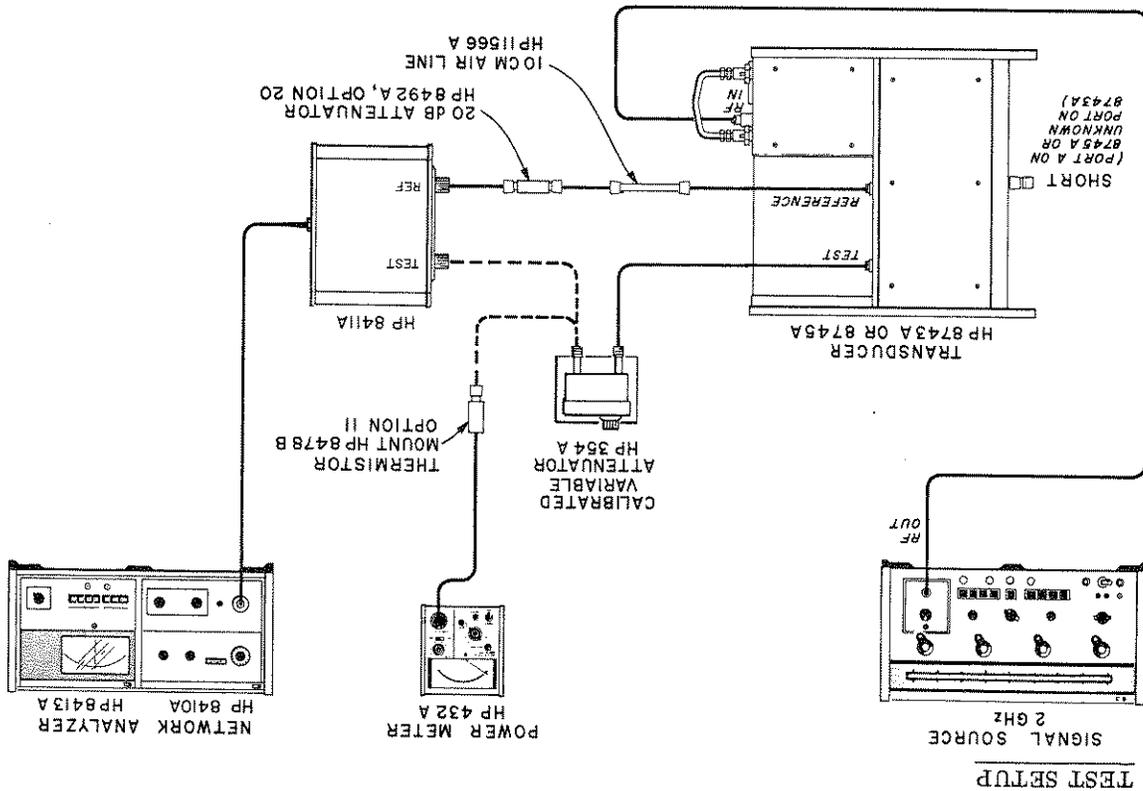EQUIPMENT: Items 1, 2, 6, and 7, Table 4-1.



then read on the 8413A meter. The indication is corrected by accounting for the ambiguity due to noise at this low signal level, and by using the calibration data from the variable attenuator.

4 (Contd)

DESCRIPTION AND PROCEDURE

TEST

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 8 of 20)

TEST	DESCRIPTION AND PROCEDURE	SPECIFICATION TESTED	DESCRIPTION
4 (Contd)	<p><u>PROCEDURE</u></p> <p>e. Adjust signal source for -15 dBm indication on power meter. Signal source output power should not be adjusted again during the remainder of the test. Disconnect the resistor mount from variable attenuator and connect variable attenuator output to 8411A TEST input.</p> <p>f. Depress 8413A AMPLITUDE 3 dB pushbutton. Adjust 8410A AMPL. VERNIER control and TEST CHANNEL GAIN units (1 dB/step) control for zero indication on the 8413A meter.</p> <p>g. Set variable attenuator to 60 dB then set 8410A TEST CHANNEL GAIN tens (10 dB/step) control to 60 dB. The 8413A meter indication should remain at zero. Any deviation should be due only to the effect of signal-to-noise ratio, cross talk, TEST CHANNEL GAIN control error, and variable attenuator error. The deviation limits due to these factors can be calculated as follows:</p> <p>(1) Maximum 8413A meter indication = 0.6 dB noise + 0.2 dB TEST CHANNEL GAIN control tolerance - actual attenuation of variable attenuator at 60-dB setting + 60 dB.</p> <p>(2) Minimum 8413A meter indication = -0.2 dB TEST CHANNEL GAIN tolerance - actual attenuation of variable attenuator at 60 dB setting + 60 dB.</p> <p>For example, if the calibration on the variable attenuator at the 60-dB position is 59.1 dB, then for this example:</p> <p>Maximum = +0.6 dB + 0.2 dB - 59.1 dB + 60 dB = +1.7 dB</p> <p>Minimum = -0.2 dB - 59.1 dB + 60 dB = +0.7 dB</p> <p>Therefore, the 8413A meter indication should be between +0.7 dB and +1.7 dB.</p>	<p><u>PHASE METER AND FRONT-PANEL 10 MV/DEG OUTPUT ACCURACY:</u></p> <p>Phase Meter: ±2% of full scale</p> <p>10 MV/DEG Output: ±2% of DVM indication or ±1 mV, whichever is greater.</p>	<p><u>DESCRIPTION</u></p> <p>An accurate phase shift is established by setting the signal source to a single frequency and inserting electrical length in one channel to unbalance the channels a given portion of a wavelength. The accuracies of the 8413A meter indications and 10 MV/DEG output are compared against these precise phase shifts.</p>

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 9 of 20)

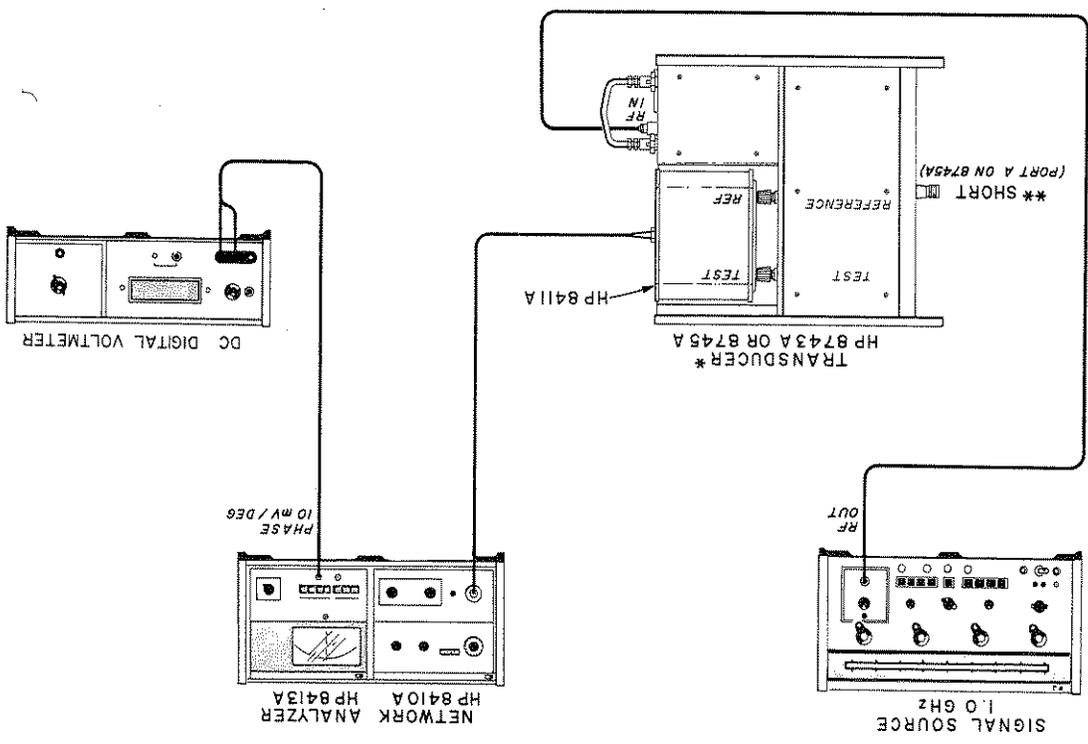
TEST	DESCRIPTION AND PROCEDURE
5 (Contd)	<p style="text-align: center;"><u>TEST SETUP</u></p>  <p style="text-align: center;"><u>PROCEDURE</u></p> <ol style="list-style-type: none"> a. Change equipment test setup as shown above. If an 8743A is used, leave UNKNOWN port open and depress REF.L pushbutton. If an 8745A is used, connect APC-7 short to PORT A and depress INPUT PORT A and S11 pushbuttons. Set signal source for single-frequency (CW) operation at 1.0 GHz. b. Check for phase-locked condition in the 8410A as follows: <ol style="list-style-type: none"> (1) REF CHANNEL LEVEL meter should indicate in the OPERATE range. If not, adjust signal source power output to obtain OPERATE indication on meter. (2) Depress 8413A PHASE 180 degree pushbutton. Adjust the 8410A PHASE VERNIER control: the 8413A phase meter indication should change smoothly, indicating the 8410A is phase locked. c. Obtain an RF signal with 30-cm wavelength as follows: <p>*The coupling of the 8743A internal directional coupler rolls off below 2.0 GHz; however, this unit may be used at 1.0 GHz for these tests.</p> <p>**If 8743A is used, leave UNKNOWN port open; if 8745A is used, connect short to PORT A.</p> <p>EQUIPMENT: Items 1 and 14, Table 4-1.</p>

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 10 of 20)

TEST	DESCRIPTION AND PROCEDURE
5 (Contd)	<p style="text-align: center;"><u>PROCEDURE</u></p> <p style="text-align: center;">NOTE</p> <p>To eliminate mechanical backlash error when adjusting the transducer REFERENCE PLANE EXTENSION, always approach each setting from the same direction.</p> <p>(1) Adjust transducer REFERENCE PLANE EXTENSION crank for zero digital counter indication, then hold thumbwheel and adjust crank fully counterclockwise.</p> <p>(2) Adjust 8413A PHASE OFFSET and 8410A PHASE VERNIER for a zero ± 0.5 millivolt indication on the DVM.</p> <p>(3) Adjust REFERENCE PLANE EXTENSION for 15.00 cm digital counter indication. DVM should indicate zero ± 1 millivolt. If not, adjust signal source frequency for zero ± 1 millivolt DVM indication. Adjust REFERENCE PLANE EXTENSION fully counterclockwise and repeat steps (2) and (3) until DVM indication is zero when digital counter is set to both zero and 15.00 cm.</p> <p>d. Readjust the REFERENCE PLANE EXTENSION as follows:</p> <p>(1) Adjust the crank to obtain a digital counter indication of 7.5 cm.</p> <p>(2) Hold thumbwheel to retain this indication, and adjust crank fully clockwise.</p> <p>(3) Release thumbwheel and adjust crank counterclockwise until the digital counter indicates zero.</p> <p>e. Adjust the 8413A PHASE OFFSET switch and 8410A PHASE VERNIER control for a zero ± 0.5 millivolt indication on the DVM.</p> <p>f. Check the 8413A phase meter and 10 MV/DEG output voltage accuracy as indicated in table below.</p> <p style="text-align: center;">NOTE</p> <p>The signal source frequency and REFERENCE PLANE EXTENSION settings are critical; therefore, if any indication is out of tolerance, readjust signal source frequency (step c), recheck zero settings (step d), and repeat the digital counter setting.</p>

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 11 of 20)

TEST	DESCRIPTION AND PROCEDURE																																				
5 (Contd)	<p style="text-align: center;"><u>PROCEDURE</u></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 25%;">8743A or 8745A Digital Counter Setting*</td> <td style="width: 25%;">8413A Phase Range</td> <td style="width: 25%;">Digital Voltmeter Indication</td> <td style="width: 25%;">8413A Phase Meter Indication</td> </tr> <tr> <td>0.21 cm</td> <td>6°</td> <td>+50 mV ± 1 mV</td> <td>+5° ± 0.12°</td> </tr> <tr> <td>99.79 cm</td> <td>6°</td> <td>-50 mV ± 1 mV</td> <td>-5° ± 0.12°</td> </tr> <tr> <td>0.62 cm</td> <td>18°</td> <td>+150 mV ± 3 mV</td> <td>+15° ± 0.36°</td> </tr> <tr> <td>99.38 cm</td> <td>18°</td> <td>-150 mV ± 3 mV</td> <td>-15° ± 0.36°</td> </tr> <tr> <td>2.08 cm</td> <td>60°</td> <td>+500 mV ± 10 mV</td> <td>+50° ± 1.20°</td> </tr> <tr> <td>97.92 cm</td> <td>60°</td> <td>-500 mV ± 10 mV</td> <td>-50° ± 1.20°</td> </tr> <tr> <td>6.25 cm</td> <td>180°</td> <td>+1.5 Vdc ± 30 mV</td> <td>+150° ± 3.60°</td> </tr> <tr> <td>93.75 cm</td> <td>180°</td> <td>-1.5 Vdc ± 30 mV</td> <td>-150° ± 3.60°</td> </tr> </table> <p>*Adjust the 8743A or 8745A REFERENCE PLANE EXTENSION to obtain digital counter settings. Instructions for obtaining initial setting are given in step d. To eliminate mechanical backlash error, always approach each setting from the same direction.</p>	8743A or 8745A Digital Counter Setting*	8413A Phase Range	Digital Voltmeter Indication	8413A Phase Meter Indication	0.21 cm	6°	+50 mV ± 1 mV	+5° ± 0.12°	99.79 cm	6°	-50 mV ± 1 mV	-5° ± 0.12°	0.62 cm	18°	+150 mV ± 3 mV	+15° ± 0.36°	99.38 cm	18°	-150 mV ± 3 mV	-15° ± 0.36°	2.08 cm	60°	+500 mV ± 10 mV	+50° ± 1.20°	97.92 cm	60°	-500 mV ± 10 mV	-50° ± 1.20°	6.25 cm	180°	+1.5 Vdc ± 30 mV	+150° ± 3.60°	93.75 cm	180°	-1.5 Vdc ± 30 mV	-150° ± 3.60°
8743A or 8745A Digital Counter Setting*	8413A Phase Range	Digital Voltmeter Indication	8413A Phase Meter Indication																																		
0.21 cm	6°	+50 mV ± 1 mV	+5° ± 0.12°																																		
99.79 cm	6°	-50 mV ± 1 mV	-5° ± 0.12°																																		
0.62 cm	18°	+150 mV ± 3 mV	+15° ± 0.36°																																		
99.38 cm	18°	-150 mV ± 3 mV	-15° ± 0.36°																																		
2.08 cm	60°	+500 mV ± 10 mV	+50° ± 1.20°																																		
97.92 cm	60°	-500 mV ± 10 mV	-50° ± 1.20°																																		
6.25 cm	180°	+1.5 Vdc ± 30 mV	+150° ± 3.60°																																		
93.75 cm	180°	-1.5 Vdc ± 30 mV	-150° ± 3.60°																																		
6	<p style="text-align: center;"><u>SPECIFICATION TESTED</u></p> <p>PHASE OFFSET ACCURACY: ±(0.2 degree + 0.3 degree per 10-degree step), not to exceed ±1.5 degrees cumulative, referenced from zero degrees.</p>																																				
	<p style="text-align: center;"><u>DESCRIPTION</u></p> <p>An accurate phase shift is established by setting the signal source to a single frequency and inserting electrical length in one channel to unbalance the channels a given portion of a wavelength. The accuracy of the 8413A PHASE OFFSET is compared against these precise phase shifts.</p>																																				

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 12 of 20)

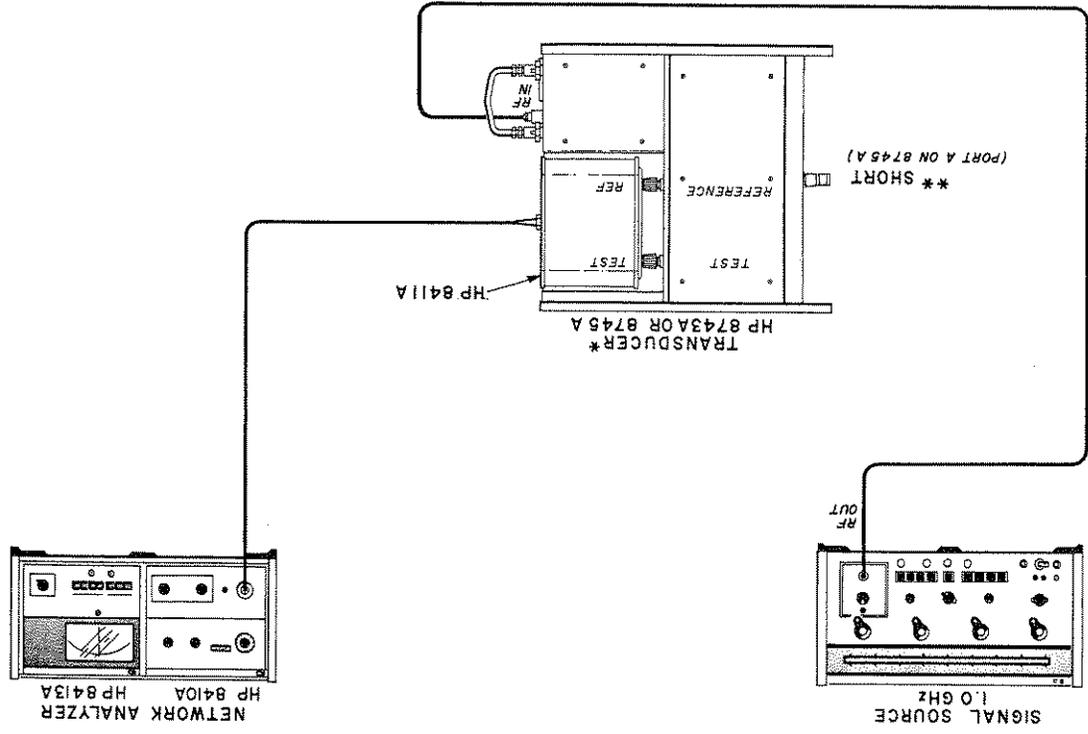
TEST	DESCRIPTION AND PROCEDURE
6 (Contd)	<p style="text-align: center;"><u>TEST SETUP</u></p>  <p style="text-align: center;">*The coupling of the 8743A internal directional coupler rolls off below 2.0 GHz; however, this unit may be used at 1.0 GHz for these tests.</p> <p style="text-align: center;">**If 8743A is used, leave UNKNOWN port open; if 8745A is used, connect short to PORT A.</p> <p style="text-align: center;">EQUIPMENT: Item 1, Table 4-1.</p>
	<p style="text-align: center;"><u>PROCEDURE</u></p> <ol style="list-style-type: none"> a. Change equipment test setup as shown above. If an 8743A is used, leave UNKNOWN port open and depress REF.L pushbutton. If an 8745A is used, connect APC-7 short to PORT A and depress REF.L pushbutton. Set signal source for single-frequency (CW) operation at 1.0 GHz. b. Check for phase-locked condition in the 8410A as follows: <ol style="list-style-type: none"> (1) REF CHANNEL LEVEL meter should indicate in the OPERATE range. If not, adjust signal source power output to obtain OPERATE indication on meter. (2) Depress 8413A PHASE 180 degree pushbutton. Adjust the 8410A PHASE VERNIER control; the 8413A phase meter indication should change smoothly, indicating the 8410A is phase locked.

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 13 of 20)

TEST	DESCRIPTION AND PROCEDURE
6 (Contd)	<p><u>PROCEDURE</u></p> <p>c. If the signal source frequency has not been changed from Test 5, proceed to step d. If the frequency has been changed, obtain an RF signal with 30-cm wavelength as follows:</p>
	<p style="text-align: center;">NOTE</p> <p>To eliminate mechanical backlash error when adjusting the transducer REFERENCE PLANE EXTENSION, always approach each setting from the same direction.</p>
	<p>(1) Adjust transducer REFERENCE PLANE EXTENSION crank for zero digital counter indication, then hold thumbwheel and adjust crank fully counterclockwise.</p> <p>(2) Adjust 8413A PHASE OFFSET and 8410A PHASE VERNIER for a zero phase indication on the 8413A 6 degree range.</p> <p>(3) Adjust REFERENCE PLANE EXTENSION for 15.00 cm digital counter indication. Phase indication should be zero. If not, adjust signal source frequency for 8413A zero degree phase indication. Adjust REFERENCE PLANE EXTENSION fully counterclockwise and repeat steps (2) and (3) until 8413A phase indication is zero when digital counter is set to both zero and 15.00 cm.</p>
	<p>d. Set the 8413A PHASE OFFSET to zero, and depress 180 degree pushbutton.</p> <p>e. Adjust the 8410A PHASE VERNIER to approximately mid-range.</p> <p>f. Adjust the transducer REFERENCE PLANE EXTENSION crank for zero digital counter indication, hold thumbwheel and adjust crank fully counter-clockwise. Continue to hold thumbwheel and adjust crank for a zero 8413A phase indication.</p> <p>g. Depress the 8413A 6 degree pushbutton and adjust the 8410A PHASE VERNIER for a zero degree phase meter indication.</p> <p>h. Check the 8413A + PHASE OFFSET accuracy as indicated in the table below.</p>
	<p style="text-align: center;">NOTE</p> <p>The signal source frequency and REFERENCE PLANE EXTENSION settings are critical; therefore, if any indication is out of tolerance, recheck the frequency in step c and zero setting in step g, then repeat the digital counter setting.</p>

Figure 4-1. Performance Test Procedure Common to all Systems (Sheet 14 of 20)

- i. Adjust the transducer REFERENCE PLANE EXTENSION for zero digital counter indication, hold thumbwheel and adjust crank fully clockwise.
- j. Set the 8413A PHASE OFFSET to minus (-) zero degrees and adjust the 8410A PHASE VERNIER for a zero phase meter indication on the 8413A 6 degree range.
- k. Check the 8413A minus (-) PHASE OFFSET accuracy as indicated in the table on the following page.

*Adjust the 8743A or 8745A REFERENCE PLANE EXTENSION to obtain digital counter settings. Instructions for obtaining initial setting, are given in steps d and e. To eliminate mechanical backlash error, always approach each setting from the same direction.

8743A or 8745A Digital Counter Setting*	8413A PHASE OFFSET Setting	8413A Meter Indication
0.42 cm	+10°	0 ± 0.5°
0.83 cm	+20°	0 ± 0.8°
1.25 cm	+30°	0 ± 1.1°
1.67 cm	+40°	0 ± 1.4°
2.08 cm	+50°	0 ± 1.5°
2.50 cm	+60°	0 ± 1.5°
2.92 cm	+70°	0 ± 1.5°
3.33 cm	+80°	0 ± 1.5°
3.75 cm	+90°	0 ± 1.5°
4.17 cm	+100°	0 ± 1.5°
4.58 cm	+110°	0 ± 1.5°
5.00 cm	+120°	0 ± 1.5°
5.42 cm	+130°	0 ± 1.5°
5.83 cm	+140°	0 ± 1.5°
6.25 cm	+150°	0 ± 1.5°
6.67 cm	+160°	0 ± 1.5°
7.08 cm	+170°	0 ± 1.5°
7.50 cm	+180°	0 ± 1.5°

PROCEDURE

(Contd)
6

TEST DESCRIPTION AND PROCEDURE

TEST

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 15 of 20)

TEST	DESCRIPTION AND PROCEDURE																																																									
6 (Contd)	<p style="text-align: center;"><u>PROCEDURE</u></p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 33%; text-align: center;">8743A or 8745A Digital Counter Setting*</td> <td style="width: 33%; text-align: center;">8413A PHASE OFFSET</td> <td style="width: 33%; text-align: center;">8413A Phase Meter Indication</td> </tr> <tr> <td style="text-align: center;">99.58 cm</td> <td style="text-align: center;">-10°</td> <td style="text-align: center;">0 ± 0.5°</td> </tr> <tr> <td style="text-align: center;">99.17 cm</td> <td style="text-align: center;">-20°</td> <td style="text-align: center;">0 ± 0.8°</td> </tr> <tr> <td style="text-align: center;">98.75 cm</td> <td style="text-align: center;">-30°</td> <td style="text-align: center;">0 ± 1.1°</td> </tr> <tr> <td style="text-align: center;">98.33 cm</td> <td style="text-align: center;">-40°</td> <td style="text-align: center;">0 ± 1.4°</td> </tr> <tr> <td style="text-align: center;">97.92 cm</td> <td style="text-align: center;">-50°</td> <td style="text-align: center;">0 ± 1.5°</td> </tr> <tr> <td style="text-align: center;">97.50 cm</td> <td style="text-align: center;">-60°</td> <td style="text-align: center;">0 ± 1.5°</td> </tr> <tr> <td style="text-align: center;">96.80 cm</td> <td style="text-align: center;">-70°</td> <td style="text-align: center;">0 ± 1.5°</td> </tr> <tr> <td style="text-align: center;">96.67 cm</td> <td style="text-align: center;">-80°</td> <td style="text-align: center;">0 ± 1.5°</td> </tr> <tr> <td style="text-align: center;">96.25 cm</td> <td style="text-align: center;">-90°</td> <td style="text-align: center;">0 ± 1.5°</td> </tr> <tr> <td style="text-align: center;">95.83 cm</td> <td style="text-align: center;">-100°</td> <td style="text-align: center;">0 ± 1.5°</td> </tr> <tr> <td style="text-align: center;">95.42 cm</td> <td style="text-align: center;">-110°</td> <td style="text-align: center;">0 ± 1.5°</td> </tr> <tr> <td style="text-align: center;">95.00 cm</td> <td style="text-align: center;">-120°</td> <td style="text-align: center;">0 ± 1.5°</td> </tr> <tr> <td style="text-align: center;">94.58 cm</td> <td style="text-align: center;">-130°</td> <td style="text-align: center;">0 ± 1.5°</td> </tr> <tr> <td style="text-align: center;">94.17 cm</td> <td style="text-align: center;">-140°</td> <td style="text-align: center;">0 ± 1.5°</td> </tr> <tr> <td style="text-align: center;">93.75 cm</td> <td style="text-align: center;">-150°</td> <td style="text-align: center;">0 ± 1.5°</td> </tr> <tr> <td style="text-align: center;">93.33 cm</td> <td style="text-align: center;">-160°</td> <td style="text-align: center;">0 ± 1.5°</td> </tr> <tr> <td style="text-align: center;">92.92 cm</td> <td style="text-align: center;">-170°</td> <td style="text-align: center;">0 ± 1.5°</td> </tr> <tr> <td style="text-align: center;">92.50 cm</td> <td style="text-align: center;">-180°</td> <td style="text-align: center;">0 ± 1.5°</td> </tr> </table> <p>*Adjust the 8743A or 8745A REFERENCE PLANE EXTENSION to obtain digital counter settings. Instructions for obtaining initial setting are given in steps i and j. To eliminate mechanical backlash error, always approach each setting from the same direction.</p>	8743A or 8745A Digital Counter Setting*	8413A PHASE OFFSET	8413A Phase Meter Indication	99.58 cm	-10°	0 ± 0.5°	99.17 cm	-20°	0 ± 0.8°	98.75 cm	-30°	0 ± 1.1°	98.33 cm	-40°	0 ± 1.4°	97.92 cm	-50°	0 ± 1.5°	97.50 cm	-60°	0 ± 1.5°	96.80 cm	-70°	0 ± 1.5°	96.67 cm	-80°	0 ± 1.5°	96.25 cm	-90°	0 ± 1.5°	95.83 cm	-100°	0 ± 1.5°	95.42 cm	-110°	0 ± 1.5°	95.00 cm	-120°	0 ± 1.5°	94.58 cm	-130°	0 ± 1.5°	94.17 cm	-140°	0 ± 1.5°	93.75 cm	-150°	0 ± 1.5°	93.33 cm	-160°	0 ± 1.5°	92.92 cm	-170°	0 ± 1.5°	92.50 cm	-180°	0 ± 1.5°
8743A or 8745A Digital Counter Setting*	8413A PHASE OFFSET	8413A Phase Meter Indication																																																								
99.58 cm	-10°	0 ± 0.5°																																																								
99.17 cm	-20°	0 ± 0.8°																																																								
98.75 cm	-30°	0 ± 1.1°																																																								
98.33 cm	-40°	0 ± 1.4°																																																								
97.92 cm	-50°	0 ± 1.5°																																																								
97.50 cm	-60°	0 ± 1.5°																																																								
96.80 cm	-70°	0 ± 1.5°																																																								
96.67 cm	-80°	0 ± 1.5°																																																								
96.25 cm	-90°	0 ± 1.5°																																																								
95.83 cm	-100°	0 ± 1.5°																																																								
95.42 cm	-110°	0 ± 1.5°																																																								
95.00 cm	-120°	0 ± 1.5°																																																								
94.58 cm	-130°	0 ± 1.5°																																																								
94.17 cm	-140°	0 ± 1.5°																																																								
93.75 cm	-150°	0 ± 1.5°																																																								
93.33 cm	-160°	0 ± 1.5°																																																								
92.92 cm	-170°	0 ± 1.5°																																																								
92.50 cm	-180°	0 ± 1.5°																																																								
7	<p style="text-align: center;"><u>SPECIFICATION TESTED</u></p> <p style="text-align: center;">AMPLITUDE METER AND 50 MV/DB OUTPUT ACCURACY:</p> <p style="text-align: center;">Amplitude Meter: ±3% of full scale.</p> <p style="text-align: center;">50 MV/DB Output: ±3% of DVM indication.</p> <p style="text-align: center;"><u>DESCRIPTION</u></p> <p>The 8410A AMPLITUDE TEST CHANNEL GAIN control is used to obtain an accurate change in 8413A input signal amplitude. The accuracy of the 8413A meter indication and the 50 MV/DB voltage output are compared against these precise level changes.</p>																																																									

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 16 of 20)

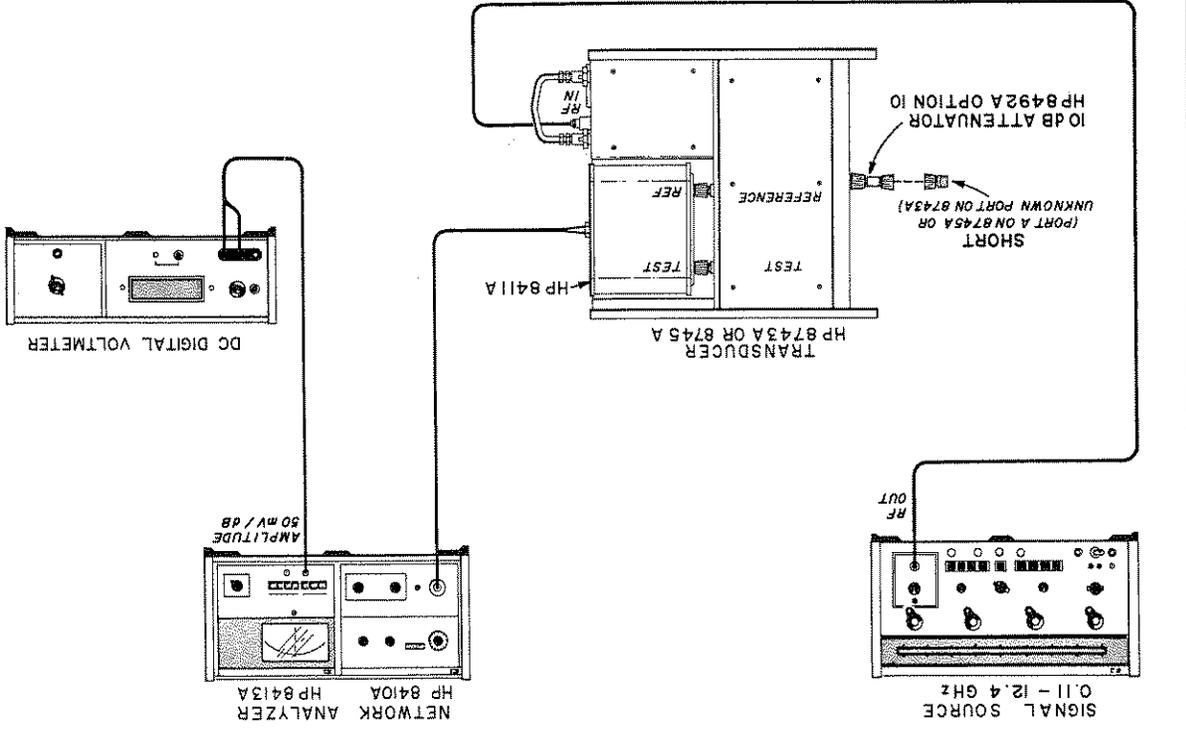
TEST	DESCRIPTION AND PROCEDURE	TEST
7	<p>(Contd)</p> <p style="text-align: center;">TEST SETUP</p>  <p style="text-align: center;">EQUIPMENT: Items 1 and 14, Table 4-1.</p>	7
	<p style="text-align: center;">PROCEDURE</p> <ol style="list-style-type: none"> a. Change equipment test setup as shown above. Install 10-dB attenuator and short on port A of 8745A or UNKNOWN port of 8743A. If 8745A is used, depress INPUT PORT A and S11 pushbuttons. If 8743A is used, depress REFLECT pushbutton. Set signal source for single-frequency (CW) operation in the range of the transducer in the test setup. b. Check for phase-locked condition in 8410A as follows: <ol style="list-style-type: none"> (1) REF CHANNEL LEVEL meter should indicate in the OPERATE range. If not, adjust signal source power output to obtain OPERATE indication on meter. (2) Depress 8413A PHASE 180 degree pushbutton. Adjust the 8410A PHASE VERNIER control; the 8413A phase meter indication should change smoothly, indicating the 8410A is phase locked. c. Set the 8410A TEST CHANNEL GAIN to 20 dB. d. Adjust the 8410A AMPL VERNIER and the 1 dB/step TEST CHANNEL GAIN control for zero dB indication on the 8413A 3-dB range. Note the 8410A TEST CHANNEL GAIN settings. e. Check the 8413A amplitude meter and 50 MV/DB output voltage accuracy as indicated in the table below. 	

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 17 of 20)


TEST	DESCRIPTION AND PROCEDURE																												
7 (Contd)	<p style="text-align: center;"><u>PROCEDURE</u></p> <p style="text-align: center;">NOTE</p> <p style="text-align: center;">Recheck zero adjustment (step d above) after each step.</p> <table border="1" data-bbox="243 1234 1128 1659"> <thead> <tr> <th>Change in 8410A TEST CHANNEL GAIN Setting*</th> <th>8413A Amplitude Range</th> <th>Digital Voltmeter Indication</th> <th>8413A Meter Indication</th> </tr> </thead> <tbody> <tr> <td>+2 dB</td> <td>3 dB</td> <td>+100 mV ±3 mV</td> <td>+2 dB ±0.09 dB</td> </tr> <tr> <td>-2 dB</td> <td>3 dB</td> <td>-100 mV ±3 mV</td> <td>-2 dB ±0.09 dB</td> </tr> <tr> <td>+9 dB</td> <td>10 dB</td> <td>+450 mV ±13.5 mV</td> <td>+9 dB ±0.3 dB</td> </tr> <tr> <td>-9 dB</td> <td>10 dB</td> <td>-450 mV ±13.5 mV</td> <td>-9 dB ±0.3 dB</td> </tr> <tr> <td>+20 dB</td> <td>30 dB</td> <td>+1.00Vdc ±30 mV</td> <td>+20 dB ±0.9 dB</td> </tr> <tr> <td>-20 dB</td> <td>30 dB</td> <td>-1.00Vdc ±30 mV</td> <td>-20 dB ±0.9 dB</td> </tr> </tbody> </table> <p style="text-align: center;">*Instructions for obtaining initial setting are given in step d.</p>	Change in 8410A TEST CHANNEL GAIN Setting*	8413A Amplitude Range	Digital Voltmeter Indication	8413A Meter Indication	+2 dB	3 dB	+100 mV ±3 mV	+2 dB ±0.09 dB	-2 dB	3 dB	-100 mV ±3 mV	-2 dB ±0.09 dB	+9 dB	10 dB	+450 mV ±13.5 mV	+9 dB ±0.3 dB	-9 dB	10 dB	-450 mV ±13.5 mV	-9 dB ±0.3 dB	+20 dB	30 dB	+1.00Vdc ±30 mV	+20 dB ±0.9 dB	-20 dB	30 dB	-1.00Vdc ±30 mV	-20 dB ±0.9 dB
Change in 8410A TEST CHANNEL GAIN Setting*	8413A Amplitude Range	Digital Voltmeter Indication	8413A Meter Indication																										
+2 dB	3 dB	+100 mV ±3 mV	+2 dB ±0.09 dB																										
-2 dB	3 dB	-100 mV ±3 mV	-2 dB ±0.09 dB																										
+9 dB	10 dB	+450 mV ±13.5 mV	+9 dB ±0.3 dB																										
-9 dB	10 dB	-450 mV ±13.5 mV	-9 dB ±0.3 dB																										
+20 dB	30 dB	+1.00Vdc ±30 mV	+20 dB ±0.9 dB																										
-20 dB	30 dB	-1.00Vdc ±30 mV	-20 dB ±0.9 dB																										
8	<p style="text-align: center;"><u>SPECIFICATION TESTED</u></p> <p style="text-align: center;">PHASE RESPONSE VERSUS SIGNAL AMPLITUDE: 1.5 degree maximum phase change for 60-dB amplitude change in test channel.</p>																												
	<p style="text-align: center;"><u>DESCRIPTION</u></p> <p>Two 278-KHz signals of known amplitude are applied to the 8413A inputs. The 8413A phase indication is observed while the test channel input level is varied by 60 dB.</p>																												

Figure 4-1. Performance Test Procedure Common to all Systems. (Sheet 18 of 20)

- a. Remove 8410A top and bottom covers and the cover of rear-panel connector to 8413A plug-in. Disconnect Cable W9 and Cable W4 from J9 and J10 at rear of 8410A bottom casing.
- b. Connect equipment as shown in test setup.
- c. Set 8410A TEST CHANNEL GAIN controls to 00 and AMPL VERNIER control fully counterclockwise.
- d. Adjust output of signal generator set to 278 kHz \pm 0.5 kHz, for 2.3 V p-p at 8410A rear-panel REF CHAN OUTPUT.
- e. Set 0-120 dB variable attenuator to 20 dB.
- f. Set 0-12 dB variable attenuator for 200 mV \pm 10 mV peak-to-peak at 8410A J2, Pin 3.
- g. Turn on the 8410A to supply power to the 8413A.
- h. Set 8413A PHASE OFFSET control for an on-scale meter indication on the \pm 6 degree range.
- i. Record 8413A meter indication (reference at zero attenuation).
- j. Set the 0-120 dB variable attenuator to 80 dB (an increase of 60 dB). The 8413A

PROCEDURE

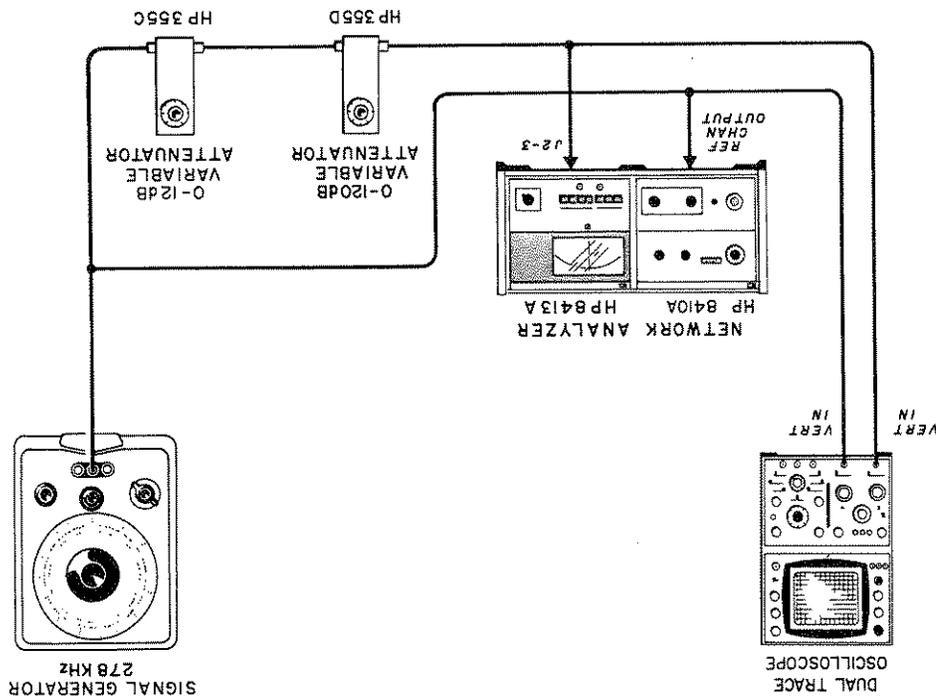EQUIPMENT: Items 4, 11, 12, and 13, Table 4-1



TEST SETUP

8 (Contd)

DESCRIPTION AND PROCEDURE

TEST

Figure 4-1. Performance Test Procedure Common for all Systems. (Sheet 19 of 20)

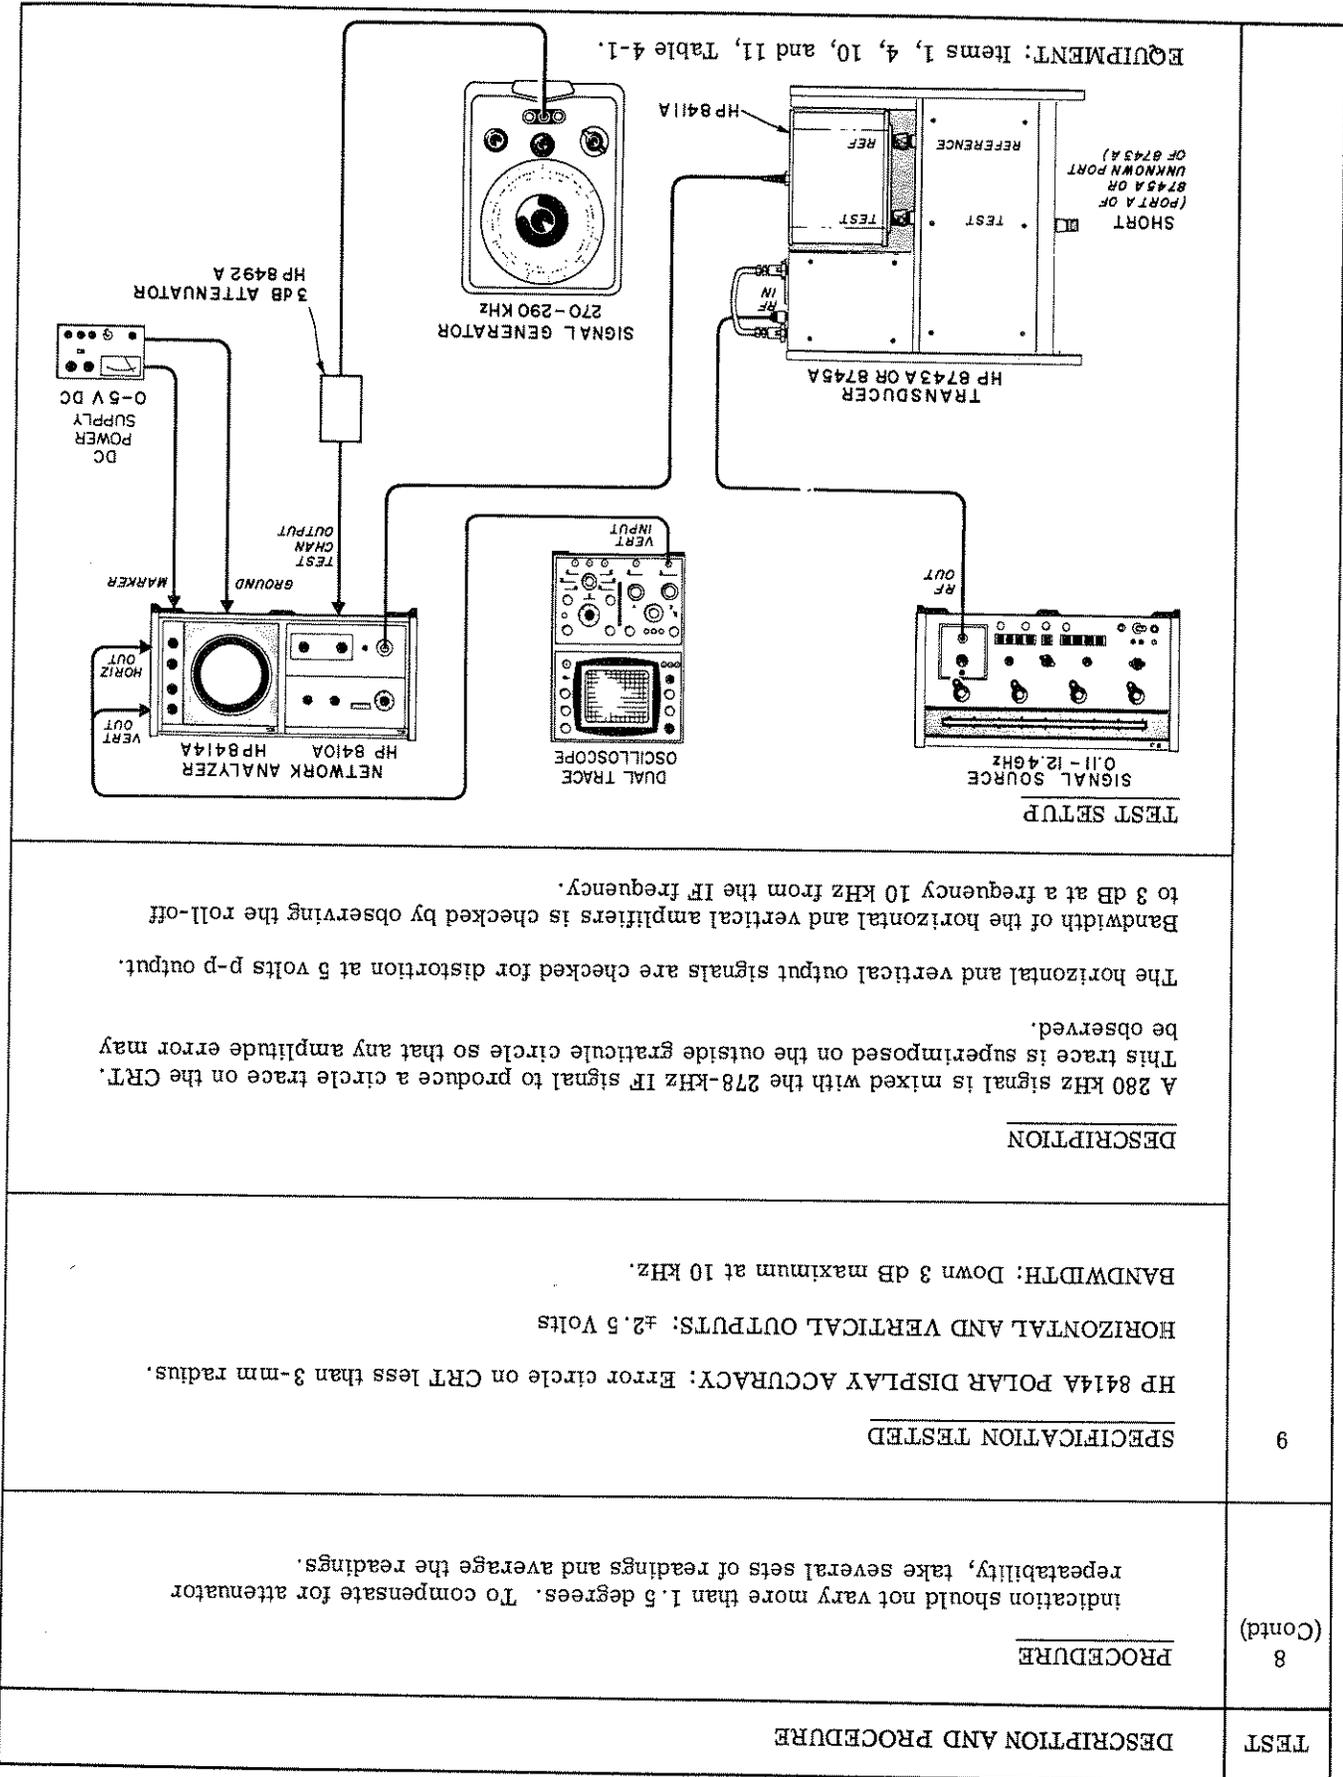


Figure 4-1. Performance Test Procedure Common for all Systems. (Sheet 20 of 20)

TEST	DESCRIPTION AND PROCEDURE
9 (Contd)	<p style="text-align: center;"><u>PROCEDURE</u></p> <p>a. Connect equipment as shown in test setup.</p> <p>b. Set the signal source for single-frequency CW operation in the range of the transducer used. Select reflection mode at transducer (REFL pushbutton on 8743A or A and S11 pushbuttons on 8745A).</p> <p>c. Check for phase-locked condition in the 8410A as follows: (1) The 8410A REF CHANNEL LEVEL meter should indicate in the OPERATE range. If not, adjust signal source power output to obtain OPERATE indication on meter. (2) Adjust the PHASE VERNIER control: the dot on the 8414A should move smoothly, indicating phase lock in the 8410A.</p> <p>d. Depress 8414A BEAM CTR pushbutton and adjust the HORIZ POS and VERT POS controls to place the dot in the center of the CRT.</p> <p>e. Adjust the 270-290 kHz signal generator connected to the 8410A TEST CHAN OUTPUT connector to 280 kHz and increase the amplitude until a trace circle on the 8414A CRT is superimposed on the outside graticule circle.</p> <p>f. Adjust the 8414A HORIZ POS and VERT POS controls if necessary to align the trace on the CRT with the graticule circle.</p> <p>g. The entire trace must be within 3 mm of the outside graticule circle.</p> <p>h. Connect dc-coupled vertical input of oscilloscope to 8414A VERTICAL OUTPUT. Increase 280 kHz signal generator amplitude until a CRT trace of 5 volts peak-to-peak is displayed. There should be no noticeable distortion.</p> <p>i. Connect dc-coupled vertical input of oscilloscope to 8414A HORIZONTAL OUTPUT. If necessary, adjust the 280-kHz signal generator amplitude for a CRT trace of 5 volts peak-to-peak. There should be no noticeable distortion.</p> <p>j. Connect oscilloscope to 8414A VERTICAL output and note peak-to-peak amplitude.</p> <p>k. Connect oscilloscope to TEST CHANNEL OUTPUT connector on 8410A and note peak-to-peak waveform. Change 280-kHz signal generator frequency to 288.0 kHz and adjust waveform to the same peak-to-peak value as noted before frequency change by adjusting signal generator output attenuator.</p> <p>l. Connect oscilloscope to VERTICAL output connector of 8414A and note peak-to-peak amplitude. The waveform must be equal to or greater than 50% of the peak-to-peak amplitude noted in step j.</p> <p>m. Repeat steps j through l with oscilloscope connected to 8414A HORIZONTAL output connector instead of VERTICAL output.</p> <p>n. Adjust 270-290 kHz signal generator near 278 kHz and adjust amplitude to obtain a circle on the 8414A CRT.</p> <p>o. Adjust the power supply to -5 volts. Connect power supply -5V output to 8414A rear-panel MARKER input connector and -5V return to chassis ground. Connect and disconnect -5 volt supply several times. Intensity of CRT trace should brighten when -5 volts is applied.</p> <p>p. Disconnect -5 volts from MARKER input and connect it to BLANKING input. The trace should be blanked off.</p>

Figure 4-2. Performance Test for 8410S-100 System (Sheet 1 of 7)

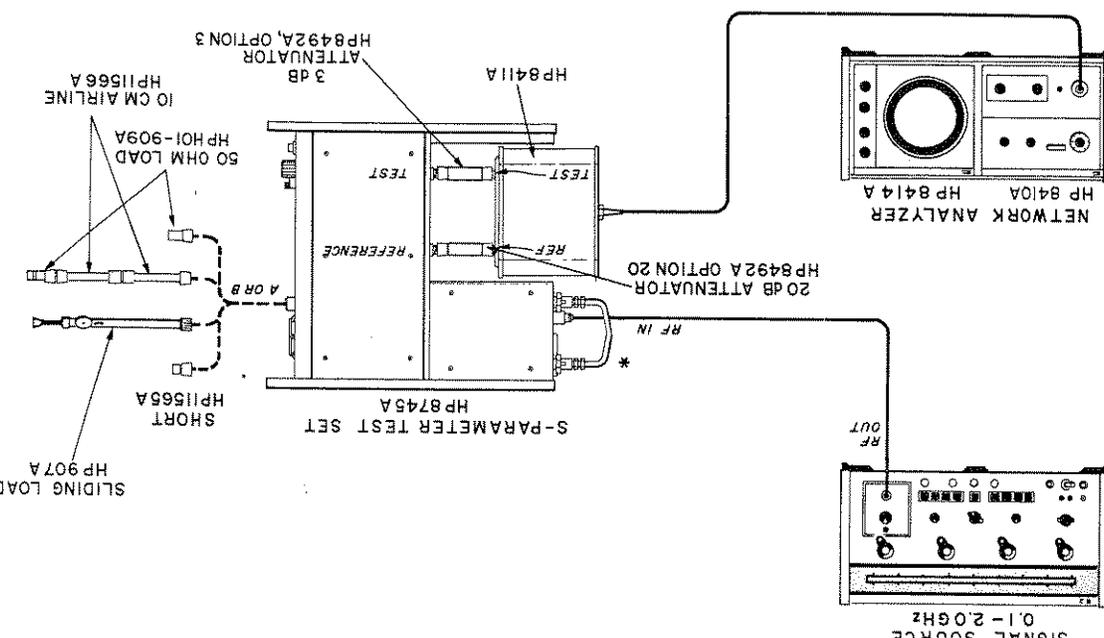
TEST	DESCRIPTION AND PROCEDURE
1	<p>SPECIFICATION TESTED DIRECTIVITY: > 36 dB ($T > 0.016$) from 0.11 to 1.0 GHz > 32 dB ($T > 0.025$) from 1.0 to 2.0 GHz</p> <p>DESCRIPTION Directivity is tested using each internal coupler to measure the reflection coefficient of a standard termination. The reflection coefficient of the termination is cancelled out at single frequencies and the resultant is coupler directivity.</p> <p>TEST SETUP</p>  <p>Use standard link, HP Part No. 08745-20064. EQUIPMENT: Items 1, 7, 8, and 9, Table 4-1.</p>
	<p>NOTE The procedures in Figure 4-2 require that all tests in Figure 4-1 be completed successfully.</p> <p>NOTE The time required to complete the performance test can be significantly reduced by testing across broader frequency ranges than those indicated on the 8410A frequency range selector. Most Network Analyzers can track input frequencies over more than one octave. Factors involved in achieving greater frequency coverage are sweep width and sweep time on the sweep oscillator and the settings of the analyzer. The suggested frequency bands are: 100 to 400 MHz, and 900 MHz to 2.0 GHz. To extend the lower frequency band it may be necessary to adjust the 8410A frequency range selector to the 1.0 to 2.0 GHz range.</p>

Figure 4-2. Performance Test for 8410S-100 System. (Sheet 2 of 7)

TEST	DESCRIPTION AND PROCEDURE
1 (Contd)	<p style="text-align: center;"><u>PROCEDURE</u></p> <p>a. Connect equipment as shown in test setup.</p> <p>b. Calibrate the 8414A display as follows:</p> <p>(1) Connect APC-7 short to 8745A Port A and depress pushbuttons A and S11.</p> <p>(2) Set signal source for automatic sweep.</p> <p style="text-align: center;">NOTE</p> <p>Most network analyzers will phase lock over more than one octave. To cover the entire operating range of the 8745A in a minimum number of frequency segments, set the signal source end frequencies to cover the broadest segment of the 0.1 to 2.0 GHz range to which the network analyzer will phase lock.</p> <p>(3) Adjust the network analyzer and signal source controls for best phase lock over the frequency band selected.</p> <p>(4) Push and hold 8414A BEAM CTR control and adjust HORIZ POS and VERT POS controls to place dot in the center of the polar display.</p> <p>c. Remove APC-7 short and replace with 50-ohm termination.</p> <p>d. Increase 8410A TEST CHANNEL GAIN by 32 dB for 1.0 to 2.0 GHz. This changes the full-scale reflection calibration from 1.0 to 0.025 (directivity of 32 dB) at the outer circle. For 0.1 to 1.0 GHz, increase the TEST CHANNEL GAIN by 36 dB to calibrate the outer circle for a reflection coefficient of 0.016 (directivity of 36 dB).</p> <p style="text-align: center;">NOTE</p> <p>The 8414A display now shows the combination of coupler directivity and reflection coefficient of the 50-ohm termination.</p> <p>e. The 8414A trace of directivity should be within the outer circle. If the trace is within the outer circle, the coupler directivity meets specifications. If the trace is outside of the outer circle, the coupler directivity must be separated from the reflection coefficient vector of the 50-ohm termination to determine if coupler directivity is out of specifications. This is accomplished as follows:</p> <p>(1) Set the signal source for single-frequency (CW) operation and select the frequency which corresponds to the point of greatest reflection on the 8414A display (the point farthest outside the outer circle).</p> <p style="text-align: center;">NOTE</p> <p>In the range of 1 to 2 GHz, a sliding load may be connected in place of the low-reflection 50-ohm load to resolve the directivity vector. For frequencies below 1 GHz, two or more sections of air line are used between the 8745A and load to phase the load reflection vector.</p> <p>(2) Phase the load reflection vector either by adjusting the sliding load or by inserting sections of air line between the 50-ohm load and the 8745A. Use a grease pencil to mark the location on the 8414A display of the circle traced when the sliding load is varied. If sections of air line are used to phase the load reflection vector, obtain a minimum of four points on the 8414A display by connecting different combinations of air lines and mark the points with a grease pencil. Draw a circle connecting the four dots. Variations from a circle are due to reflection variations of the air line. The center of this circle is the tip of the directivity vector. The magnitude at the center of</p>

DESCRIPTION AND PROCEDURE

TEST	PROCEDURE	1 (Contd)	SPECIFICATION TESTED	DESCRIPTION	TEST SETUP
	<p>f. Repeat steps b through e for other frequency segments as necessary to cover the range of 0.1 to 2.0 GHz.</p> <p>g. To check the directivity of the other coupler in the 8745A, connect an APC-7 short to 8745A port B, depress pushbuttons B and S11, and repeat steps b (2) through f.</p>		<p>TERMINATION REFLECTION COEFFICIENT:</p> <p>< 0.11 (< 1.25 VSWR), 100-200 MHz.</p> <p>> 0.09 (< 1.20 VSWR), 200-2000 MHz.</p>	<p>Input (test) port VSWR is tested using the internal coupler associated with the other port in a reflectometer setup canceling, if necessary, coupler directivity and other reflections at single frequencies.</p>	<p>SIGNAL SOURCE 0.1-2.0GHz</p> <p>RF IN RF OUT</p> <p>* HP 8411A</p> <p>S-PARAMETER TEST SET HP 8745A</p> <p>REF TEST</p> <p>HP 8492 A, OPTION 20 HP 8492 A, OPTION 3</p> <p>30dB ATTENUATOR 20dB ATTENUATOR</p> <p>50 OHM LOAD HP H01-909 A</p> <p>UNIVERSAL EXTENSION HP 11604 A</p> <p>SHORT</p> <p>NETWORK ANALYZER HP 8410A HP 8414A</p>

Figure 4-2. Performance Test for 8410S-100 System (Sheet 3 of 7)

*Use long link, HP Part No. 11604-20021.
EQUIPMENT: Items 1 and 8, Table 4-1.

Figure 4-2. Performance Test for 8410S-100 System (Sheet 4 of 7)

TEST	2 (Cont)
DESCRIPTION AND PROCEDURE	<p style="text-align: center;"><u>PROCEDURE</u></p> <p>a. Connect equipment as shown in test setup.</p> <p>b. Calibrate the 8414A display as follows:</p> <p>(1) Connect APC-7 short to port A arm of universal extension and depress pushbuttons A and S11.</p> <p>(2) Set signal source for automatic sweep.</p> <p style="text-align: center;">NOTE</p> <p>Most network analyzers will phase lock over more than one octave. To cover the entire operating range of the 8745A in a minimum number of frequency segments, set the signal source end frequencies to cover the broadest segment of the 0.1 to 2.0 GHz range to which the network analyzer will phase lock.</p> <p>(3) Adjust the network analyzer and signal source controls for best phase lock over frequency band selected. Adjust signal source for 8410A REF CHANNEL LEVEL meter indication at top (right) edge of OPERATE range.</p> <p>(4) Push and hold 8414A BEAM CTR control and adjust HORIZ POS and VERT POS controls to place dot in the center of the polar display.</p> <p>(5) Adjust the 8410A TEST CHANNEL GAIN and AMPL VERNIER controls for a trace on the outer circle of the CRT graticule.</p> <p>c. Remove the APC-7 short and connect the two arms of the universal extension together (8745A port A connected to port B).</p> <p>d. Increase 8410A TEST CHANNEL GAIN by 19 dB for 0.1 to 0.2 GHz. This changes the full-scale reflection calibration from 1.0 to 0.11 at the outer circle. For 0.2 to 2.0 GHz, increase the TEST CHANNEL GAIN by 21 dB to calibrate the outer circle for reflection coefficient of 0.09.</p> <p>e. The 8414A trace of reflection coefficient should be within the outer circle. If the trace is outside of the outer circle, the reflection coefficient of the input port must be separated from the coupler directivity to determine if the input port reflection coefficient is within specification. This is accomplished as follows:</p> <p>(1) Set the signal source for single frequency (CW) operation and select the frequency which corresponds to the point of greatest reflection on the 8414A display (the point farthest outside the outer circle).</p> <p>(2) Terminate the main line of the reflectometer with a low reflection 50-ohm load HP H01-909A. When checking the input reflection of port A, connect the load to port A arm of universal extension and when checking port B, connect the load to port B arm.</p> <p>(3) Without depressing the BEAM CTR, adjust 8414A HORIZ POS and VERT POS controls to place the dot at the CRT center.</p> <p>(4) Disconnect the 50-ohm load. The 8414A display is now the input reflection coefficient only. The directivity has been cancelled and the only ambiguity is due to the small reflection coefficient of the 50-ohm load. (The H01-909A has a maximum reflection coefficient of 0.005 or 50-dB return loss.) If the dot is within the outer circle of the graticule, the input port meets specifications at that frequency.</p> <p>f. To check the reflection coefficient of the other input port, connect short to port B arm of universal extension, depress 8745A pushbuttons B and S11, and repeat steps b (2) through e.</p>

Figure 4-2. Performance Test for 8410S-100 System. (Sheet 5 of 7)

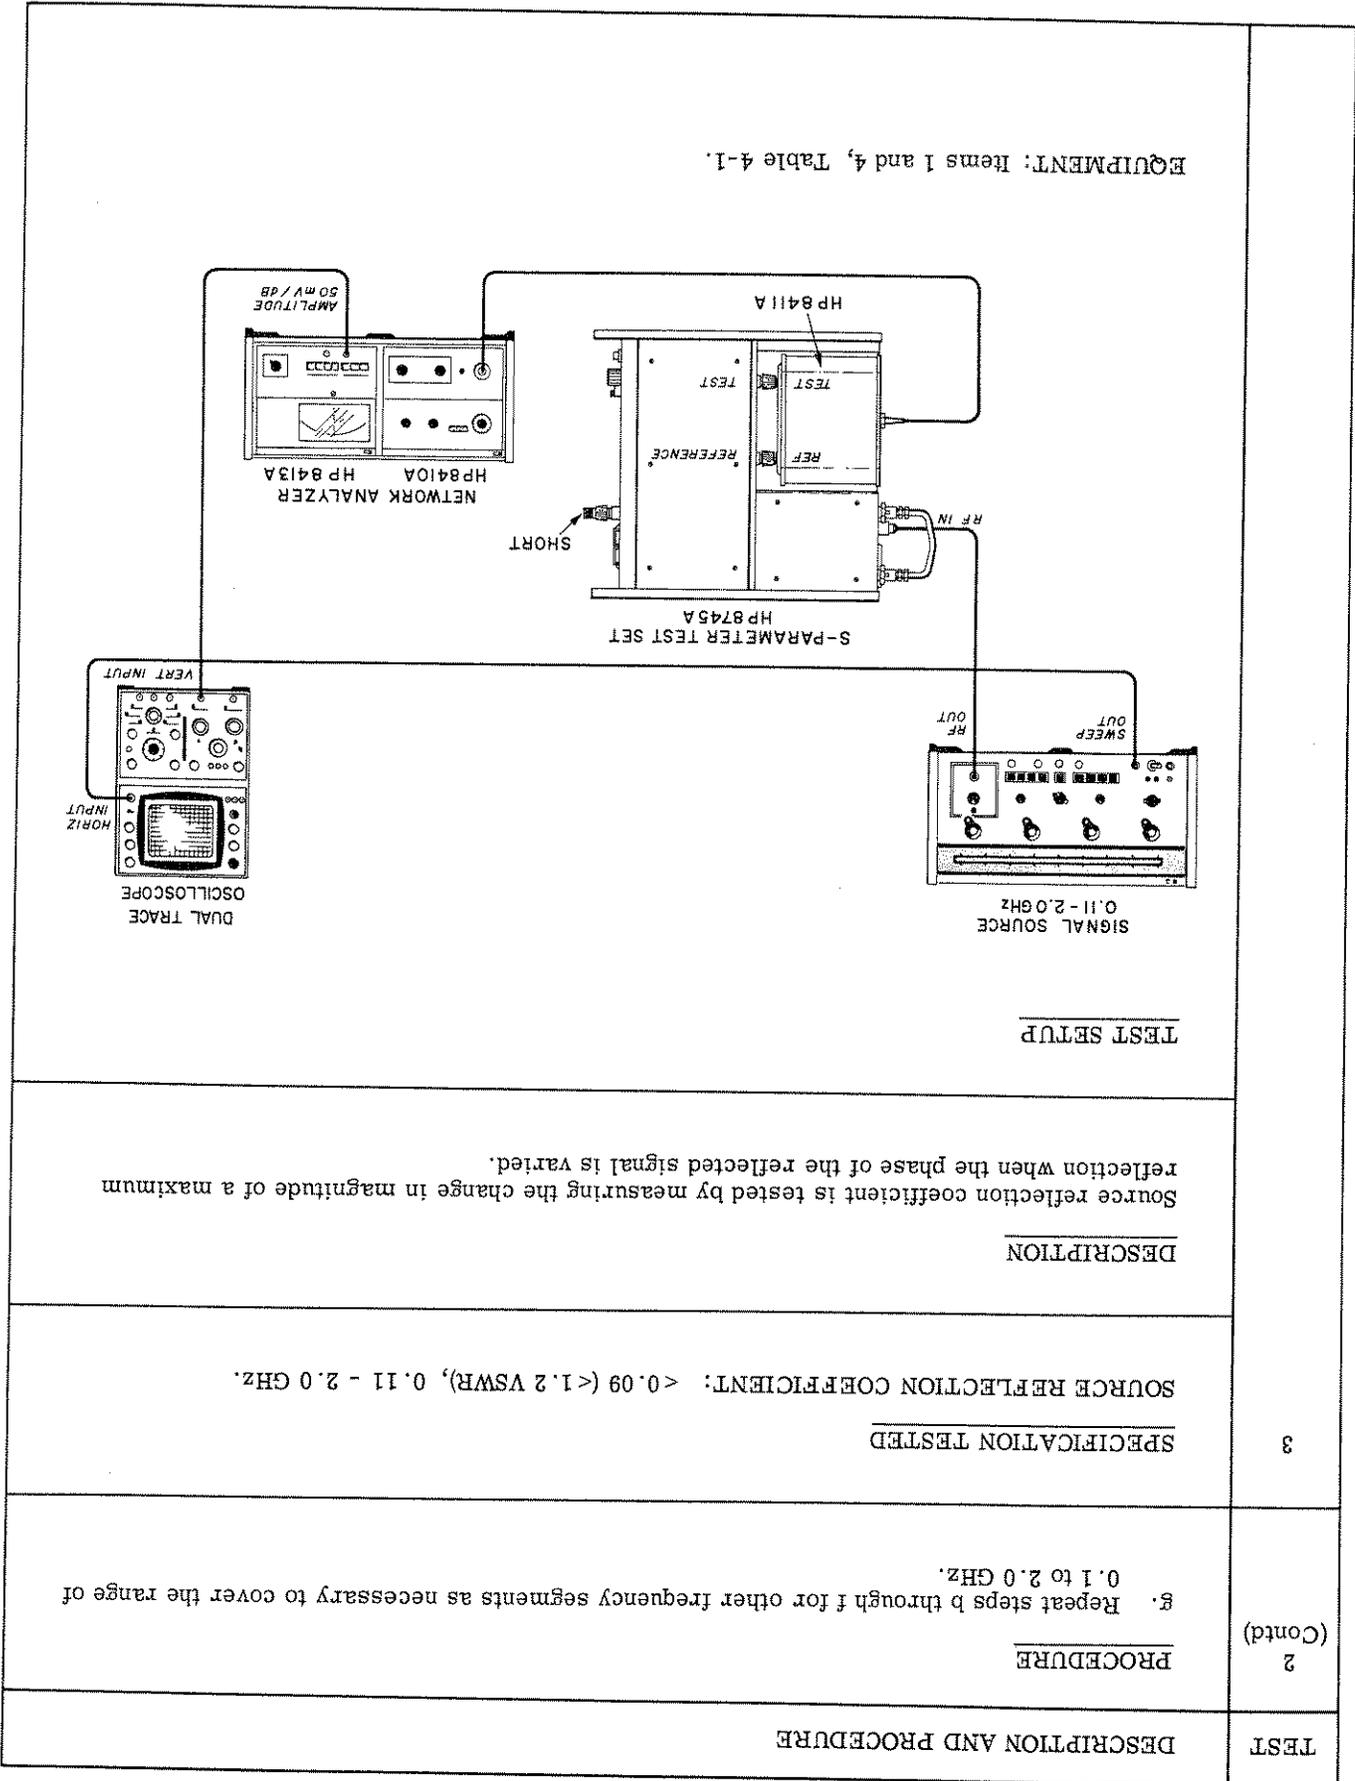


Figure 4-2. Performance Test for 8410S-100 System (Sheet 6 of 7)

TEST	DESCRIPTION AND PROCEDURE
3 (Contd)	<p style="text-align: center;"><u>PROCEDURE</u></p> <p>a. Connect equipment as shown in test setup.</p> <p>b. Connect APC-7 short to 8745A port A and depress pushbuttons A and S11.</p> <p>c. Set signal source for automatic sweep.</p> <p style="text-align: center;">NOTE</p> <p>Most network analyzers will phase lock over more than one octave. To cover the entire operating range of the 8745A in a minimum number of frequency segments, set the signal source end frequencies to cover the broadest segment of the 0.1 to 2.0 GHz range to which the network analyzer will phase lock.</p> <p>d. Adjust the network analyzer frequency range selector and sweep stability control, the signal source sweep time and sweep width, and the oscilloscope vertical and horizontal positioning controls to display the amplitude output of the 8413A.</p> <p>e. Set the oscilloscope vertical sensitivity to display 0.01 V/cm (0.2 dB/cm).</p> <p>f. Draw the oscilloscope trace on the face of the CRT with a grease pencil.</p> <p>g. Remove the APC-7 short and draw the trace of the open circuit on the face of the CRT.</p> <p>h. The maximum deviation between traces should not exceed 1.6 dB, indicating a VSWR < 1.2.</p> <p style="text-align: center;">$VSWR = \log^{-1} (0.05 \times \text{deviation between traces in dB})$</p> <p>i. Repeat steps b through h for other frequency segments as necessary to cover the range of 0.1 to 2.0 GHz.</p> <p>j. To check the source match of port B, connect APC-7 short to 8745A port B, depress pushbuttons B and S11, and repeat steps f through h for each frequency segment to cover the range of 0.1 to 2.0 GHz.</p>
4	<p style="text-align: center;"><u>SPECIFICATION TESTED</u></p> <p style="text-align: center;">CHANNEL ISOLATION: Greater than 65 dB, 0.11 to 2.0 GHz.</p>
	<p style="text-align: center;"><u>TEST DESCRIPTION</u></p> <p>The 278-kHz test channel signal is monitored by an ac voltmeter with 200-Hz bandwidth. This rejects incoming noise and indicates only the test channel signal level. After a reference level is established at the ac voltmeter, the RF signal to the 8411A test channel is disconnected, and the input is terminated with a 50-ohm load. With the RF signal applied only to the reference channel, any signal present in the test channel is due to signal leakage between channels. Isolation between channels is calculated taking the signal level below zero indicated on the ac voltmeter plus the test channel gain added at the 8410A.</p>

Figure 4-2. Performance Test for 8410S-100 System (Sheet 7 of 7)

TEST	DESCRIPTION AND PROCEDURE
4 (Contd)	<p style="text-align: center;"><u>TEST SETUP</u></p>
	<p style="text-align: center;"><u>PROCEDURE</u></p> <ol style="list-style-type: none"> a. Change equipment test setup as shown above. Connect 8411A to 8745A without the air line. Depress 8745A pushbuttons A and S11. b. Check for phase-locked condition in the 8410A as follows: <ol style="list-style-type: none"> (1) Set signal source for single-frequency CW operation and adjust output for a REF CHANNEL LEVEL meter indication at the right edge of the OPERATE range. (2) Depress the 8413A PHASE 180 degree pushbutton. Adjust the 8410A PHASE VERNIER control: the 8413A meter indication should change smoothly, indicating phase lock in the 8410A. c. Set 8410A TEST CHANNEL GAIN controls to zero. Adjust ac voltmeter for maximum output at 278 kHz, select automatic frequency control mode, and select 200-Hz bandwidth. Adjust 8410A AMPL VERNIER control and up to 4 dB on the TEST CHANNEL GAIN control for zero dB ac voltmeter indication on the meter range selected. d. Disconnect 8411A from 8745A and connect 50-ohm termination to 8411A TEST input. Connect 8411A REFERENCE port to 8745A with 10-cm air line. e. Increase the 8410A TEST CHANNEL GAIN control setting by 65 dB. The indication on the ac voltmeter should be zero or lower on the meter range selected.

EQUIPMENT: Items 1, 5, 7, and 8, Table 4-1.

Figure 4-3. Performance Tests for 8410S-200 System (Sheet 1 of 6)

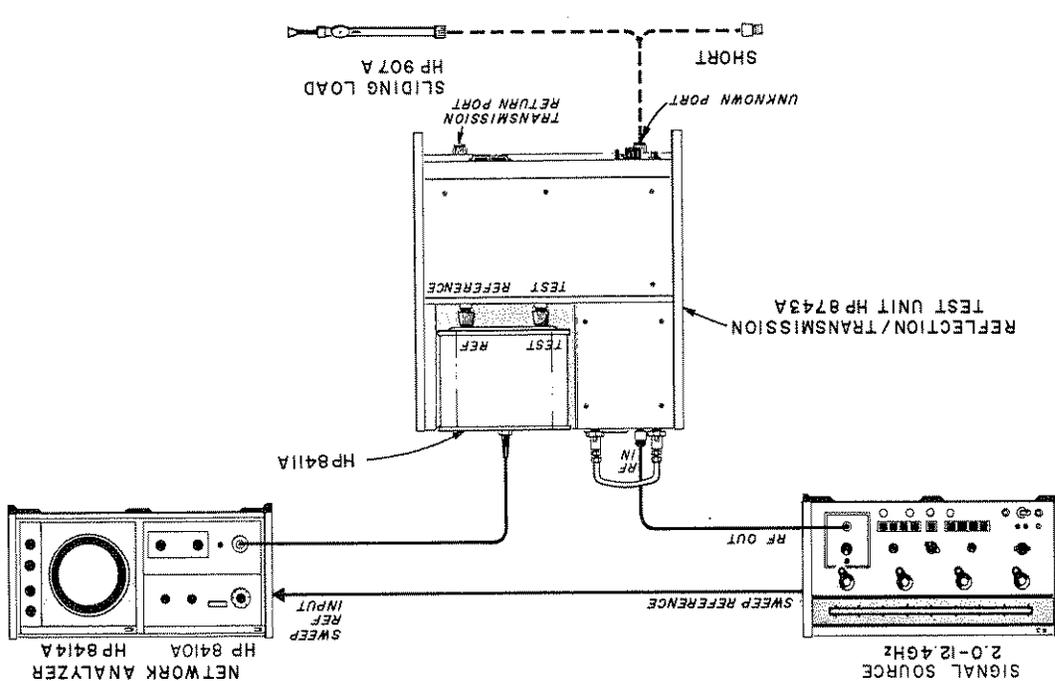
TEST	DESCRIPTION AND PROCEDURE
1	<p style="text-align: center;">NOTE</p> <p>The procedures in Figure 4-3 require that all tests in Figure 4-1 be completed successfully.</p>
	<p style="text-align: center;"><u>SPECIFICATION TESTED</u></p> <p>DIRECTIVITY: 30 dB or greater.</p>
	<p style="text-align: center;"><u>DESCRIPTION</u></p> <p>Directivity is measured by sweeping octave bands, using a sliding load. If the average signal due to the combination of directivity of the coupler and reflection of the sliding load is greater than the directivity specification the directivity value may be isolated from the load reflection at single frequencies by phasing the reflection vector with the sliding load.</p>
	<p style="text-align: center;"><u>TEST SETUP</u></p>  <p style="text-align: center;">EQUIPMENT: Items 1 and 9, Table 4-1.</p>

Figure 4-3. Performance Tests for 8410S-200 System. (Sheet 2 of 6)

TEST	DESCRIPTION AND PROCEDURE
1 (Contd)	<p style="text-align: center;"><u>PROCEDURE</u></p> <p>a. Connect equipment as shown in setup above.</p> <p>b. Connect the coaxial short to the 8743A UNKNOWN port and depress the REFL pushbutton.</p> <p>c. Set the sweep oscillator to automatic sweep. Adjust the sweep oscillator and network analyzer controls to phase lock the network analyzer over the segment of the 8743A frequency range covered by the sweep oscillator. Adjust sweep oscillator for an indication on the 8410A REF CHANNEL LEVEL meter to the upper edge of the OPERATE range.</p> <p>d. Push and hold the 8414A BEAM CTR pushbutton and adjust the centering controls to place the dot in the center of the polar display.</p> <p>e. Adjust the REFERENCE PLANE EXTENSION to collapse the trace to a dot or smallest cluster.</p> <p>f. Adjust the 8410A TEST CHANNEL GAIN and AMPLITUDE VERNIER controls to place the dot or the center of the cluster at the outer circle.</p> <p>g. Remove the coaxial short and replace with the sliding load.</p> <p>h. Increase the 8410A test channel gain by 30 dB. Phase the sliding load, noting the CRT display. The average of this display must be inside the outer circle.</p> <p>i. If the swept-display cannot be resolved satisfactorily, make single-frequency measurements as follows:</p> <p>(1) Set the sweep oscillator to single-frequency operation. Select the frequency which corresponds to the point of greatest reflection on the 8414A display.</p> <p>(2) Adjust the 8414A centering controls, while phasing the load, until the circle rotates about the center of the CRT. (See Figure 3-8).</p> <p>(3) Depress the 8414A beam center pushbutton. The dot must be inside the outer circle.</p> <p>j. Repeat steps b through i for other frequency segments as necessary to cover the range of 2.0 to 12.4 GHz.</p>
2	<p style="text-align: center;"><u>SPECIFICATION TESTED</u></p> <p>TERMINATION REFLECTION COEFFICIENT: < 0.09 (<1.2 VSWR), 2 to 8 GHz; > 0.13 (<1.3 VSWR), 8 to 12.4 GHz.</p>
	<p style="text-align: center;"><u>DESCRIPTION</u></p> <p>The signal source RF output is leveled to provide a constant-amplitude signal to the swept slotted line. The swept slotted line resolves out the reflection coefficient of the TRANSMISSION RETURN port. The reflection measurement includes the contributions made by the 8414A input circuit, the flexible arm, and the 10-dB attenuator.</p>

Figure 4-3. Performance Test for 8410S-200 System (Sheet 3 of 6)

TEST	2 (Cont)	DESCRIPTION AND PROCEDURE
		<p style="text-align: center;"><u>TEST SETUP</u></p> <p style="text-align: center;"><u>EQUIPMENT:</u> Items 1, 3, and 4, Table 4-1.</p> <p style="text-align: center;"><u>PROCEDURE</u></p> <ol style="list-style-type: none"> a. Connect equipment as shown in setup above. b. Either use signal source internal leveling or level the sweep as follows. Connect the oscilloscope vertical input through a BNC tee to the leveling probe output of the HP 448A. Adjust the signal source RF power output to obtain a 25 mV indication on oscilloscope. Adjust the leveling probe into the HP 448A until a flat response is obtained on the oscilloscope. Tighten the probe in place. c. Reconnect vertical input of oscilloscope to slotted line probe. Adjust depth of slotted line probe to get 5 mV output as displayed on oscilloscope. Do not insert probe far enough to touch center conductor or diode may be burned out. d. Press 8743A REFLECT pushbutton. Move slotted-line carriage to obtain a trace on the oscilloscope similar to Figure 4-4. Select spot of maximum trace width and calculate: $SWR = \frac{E_{max}}{E_{min}}$

Figure 4-3. Performance Test for 8410S-200 System (Sheet 4 of 6)

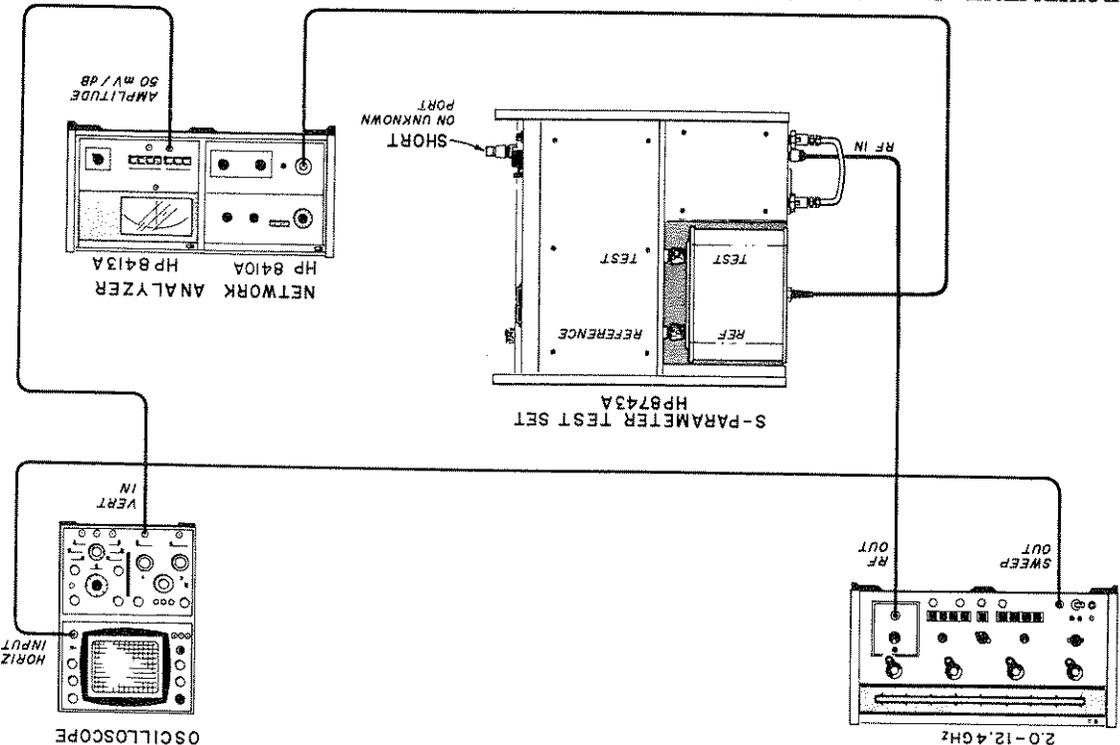
TEST	DESCRIPTION AND PROCEDURE
2 (Contd)	<p><u>PROCEDURE</u></p> <p>SWR must not be greater than 1.2 in range of 2 to 8 GHz and greater than 1.3 in range of 8 to 12.4 GHz.</p> <p>e. Press 8743A TRANS pushbutton. Move slotted-line carriage and observe trace on oscilloscope. Select spot of maximum trace width and calculate:</p> $SWR = \frac{E_{max}}{E_{min}}$ <p>SWR must not be greater than 1.2 in range of 2 to 8 GHz and greater than 1.3 in range of 8 to 12.4 GHz.</p>
3	<p><u>SPECIFICATION TESTED</u></p> <p>SOURCE REFLECTION COEFFICIENT: < 0.09 (< 1.2 VSWR), 2-8 GHz, < 0.13 (< 1.3 VSWR), 8-12.4 GHz</p> <p><u>DESCRIPTION</u></p> <p>Source reflection coefficient is tested by measuring the change in magnitude of a maximum reflection when the phase of the reflected signal is varied.</p>
	<p><u>TEST SETUP</u></p>  <p><u>EQUIPMENT: Items 1 and 4, Table 4-1.</u></p>

Figure 4-3. Performance Test for 8410S - 200 System (Sheet 5 of 6)

TEST	DESCRIPTION
3 (Contd)	<p style="text-align: center;"><u>PROCEDURE</u></p> <p>a. Connect equipment as shown in test setup.</p> <p>b. Connect APC-7 short to 8743A UNKNOWN port and depress REF.L pushbutton.</p> <p>c. Set signal source to automatic sweep.</p> <p style="text-align: center;">NOTE</p> <p>Most network analyzers will phase lock over more than one octave. To cover the entire operating range of the 8743A in a minimum number of frequency segments, set the signal source end frequencies to cover the broadest segment of the 2 to 12.4 GHz range to which the network analyzer will phase lock.</p> <p>d. Adjust the network analyzer frequency range selector and sweep stability control, the signal source sweep time and sweep width, and the oscilloscope vertical and horizontal positioning controls to display the amplitude output of the 8413A.</p> <p>e. Set the oscilloscope vertical sensitivity to display 0.01 V/cm (0.2 dB/cm).</p> <p>f. Draw the oscilloscope trace on the face of the CRT with a grease pencil.</p> <p>g. Remove the APC-7 short and draw the trace of the open circuit on the face of the CRT.</p> <p>h. The maximum deviation between traces in the 2 to 8 GHz range should not exceed 1.6 dB, indicating a VSWR < 1.2 and in the 8 to 12.4 GHz range the deviation should not exceed 2.3 dB, indicating a VSWR < 1.3.</p> <p style="text-align: center;">$VSWR = \log^{-1} (0.05 \times \text{deviation between traces in dB})$</p> <p>i. Repeat steps b through h for other frequency segments as necessary to cover the range of 2 to 12.4 GHz.</p>
4	<p style="text-align: center;"><u>SPECIFICATION TESTED</u></p> <p>CHANNEL ISOLATION: ≥65 dB, 2.0 to 6.0 GHz; ≥60 dB, 6 to 12.4 GHz.</p>
	<p style="text-align: center;"><u>TEST DESCRIPTION</u></p> <p>The 278-kHz test-channel signal is monitored by a narrow band ac voltmeter with 200-Hz bandwidth. This narrow bandwidth rejects incoming noise so that only the test channel signal level is indicated. After a reference level is established at the ac voltmeter, the RF signal to the 8411A test channel is disconnected, and the input is terminated with a 50-ohm load. With the RF signal applied only to the reference channel, any signal present in the test channel is due to signal leakage between channels. Isolation between channels is calculated taking the signal level below zero indicated on the ac voltmeter plus the test channel gain added at the 8410A.</p>

Figure 4-3. Performance Test for 8410S-200 System (Sheet 6 of 6)


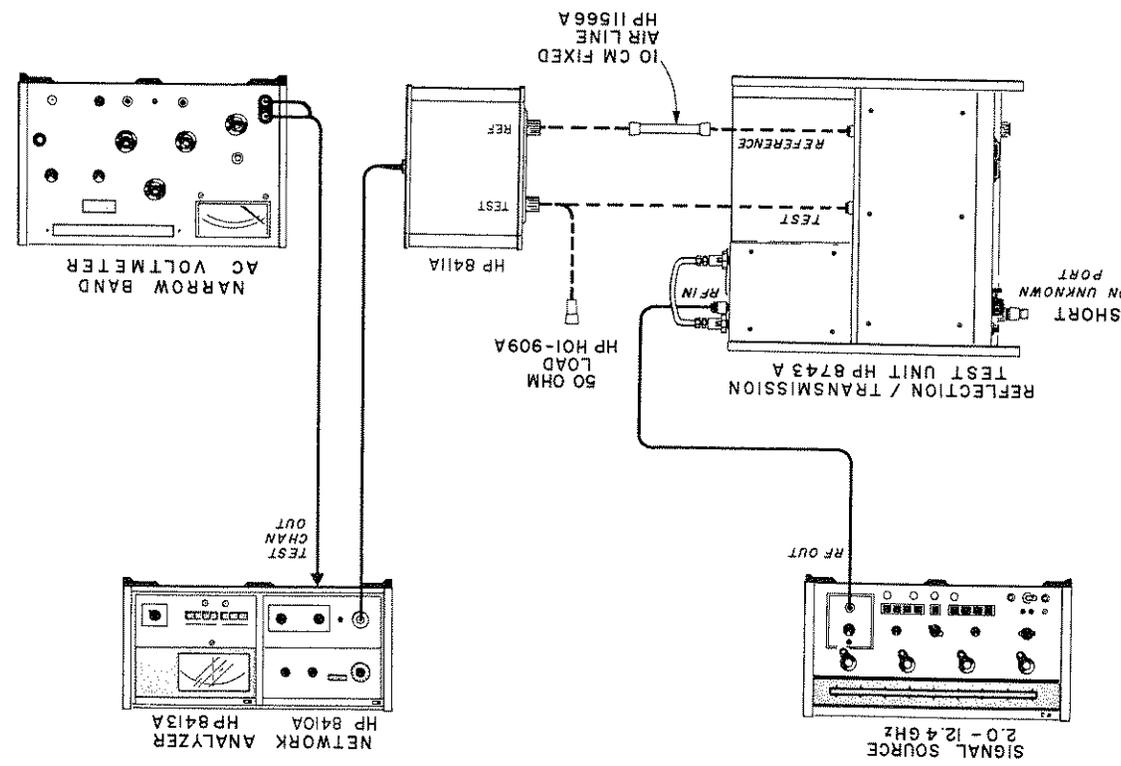
TEST	DESCRIPTION AND PROCEDURE
4 (Contd)	<p style="text-align: center;"><u>TEST SETUP</u></p>  <p style="text-align: center;"><u>EQUIPMENT: Items 1, 5, 7, and 8, Table 4-1.</u></p>
	<p style="text-align: center;"><u>PROCEDURE</u></p> <ol style="list-style-type: none"> a. Change equipment test setup as shown above. Connect 8411A to 8743A without the air line. Depress 8743A REFLECT pushbuttons. b. Check for phase-locked condition in the 8410A as follows: <ol style="list-style-type: none"> (1) Adjust the signal source for a REF CHANNEL LEVEL meter indication at the right edge of the OPERATE range. (2) Depress the 8413A PHASE 180 degree pushbutton. Adjust the 8410A PHASE VERNIER control; the 8413A meter indication should change smoothly, indicating phase lock in the 8410A. c. Set 8410A TEST CHANNEL GAIN controls to zero. Adjust ac voltmeter for maximum output at 278 kHz, select automatic frequency control mode, and select 200 Hz bandwidth. Adjust 8410A AMPL VERNIER control and up to 4 dB on 1 dB/step TEST CHANNEL GAIN control for zero db ac voltmeter indication on the meter range selected. d. Disconnect 8411A from 8743A and connect 50-ohm termination to 8411A TEST input. Connect 8411A REFERENCE port to 8743A with 10 cm air line. e. Increase the 8410A TEST CHANNEL GAIN setting by 65 dB in the range of 2.0 to 6.0 GHz and 60 dB in the range of 6 to 12.4 GHz. The indication on the ac voltmeter should be zero or lower on the meter range selected.

Figure 4-4. Typical Pattern of a Swept VSWR Measurement

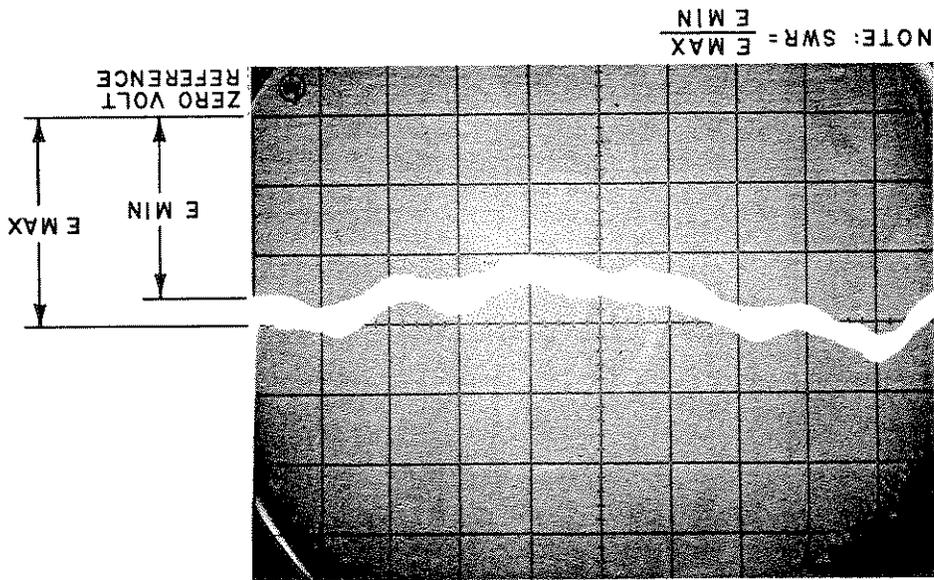


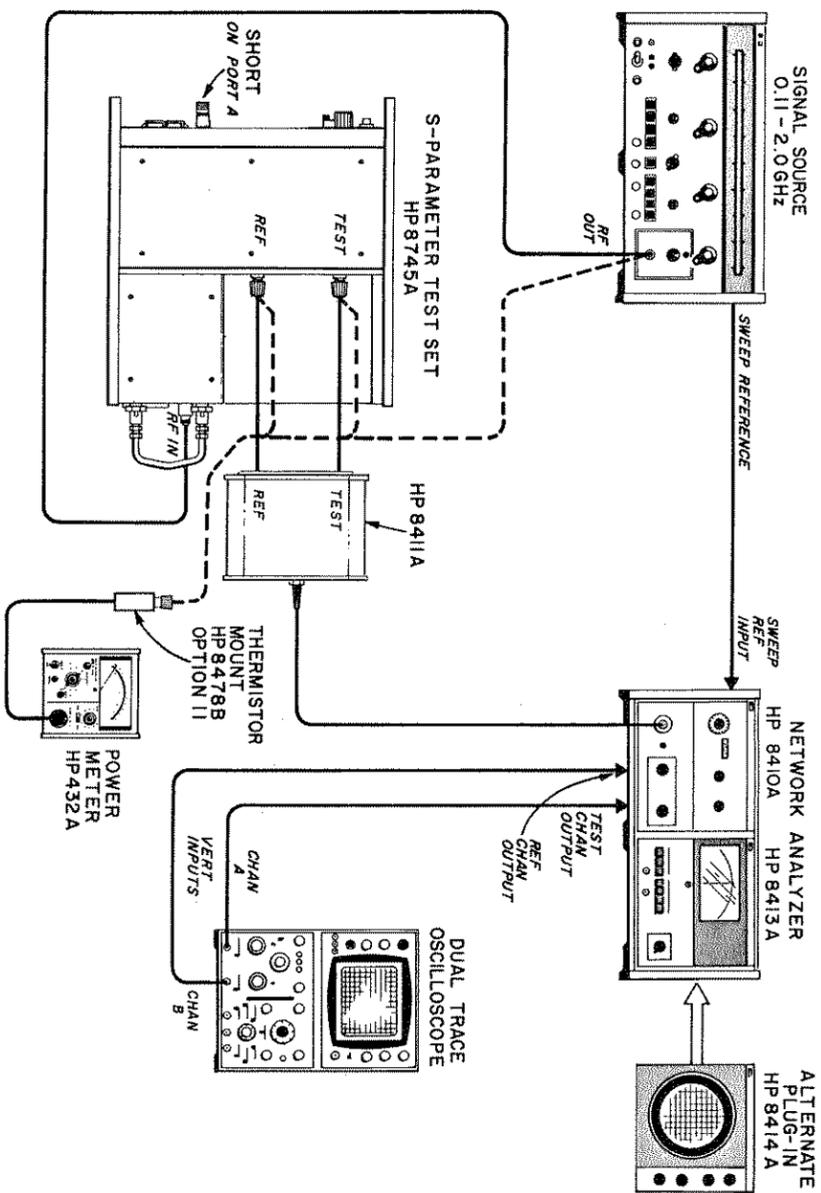


Figure 4-5. Test Setup for Model 8410S-100 and 8410S-300 Troubleshooting

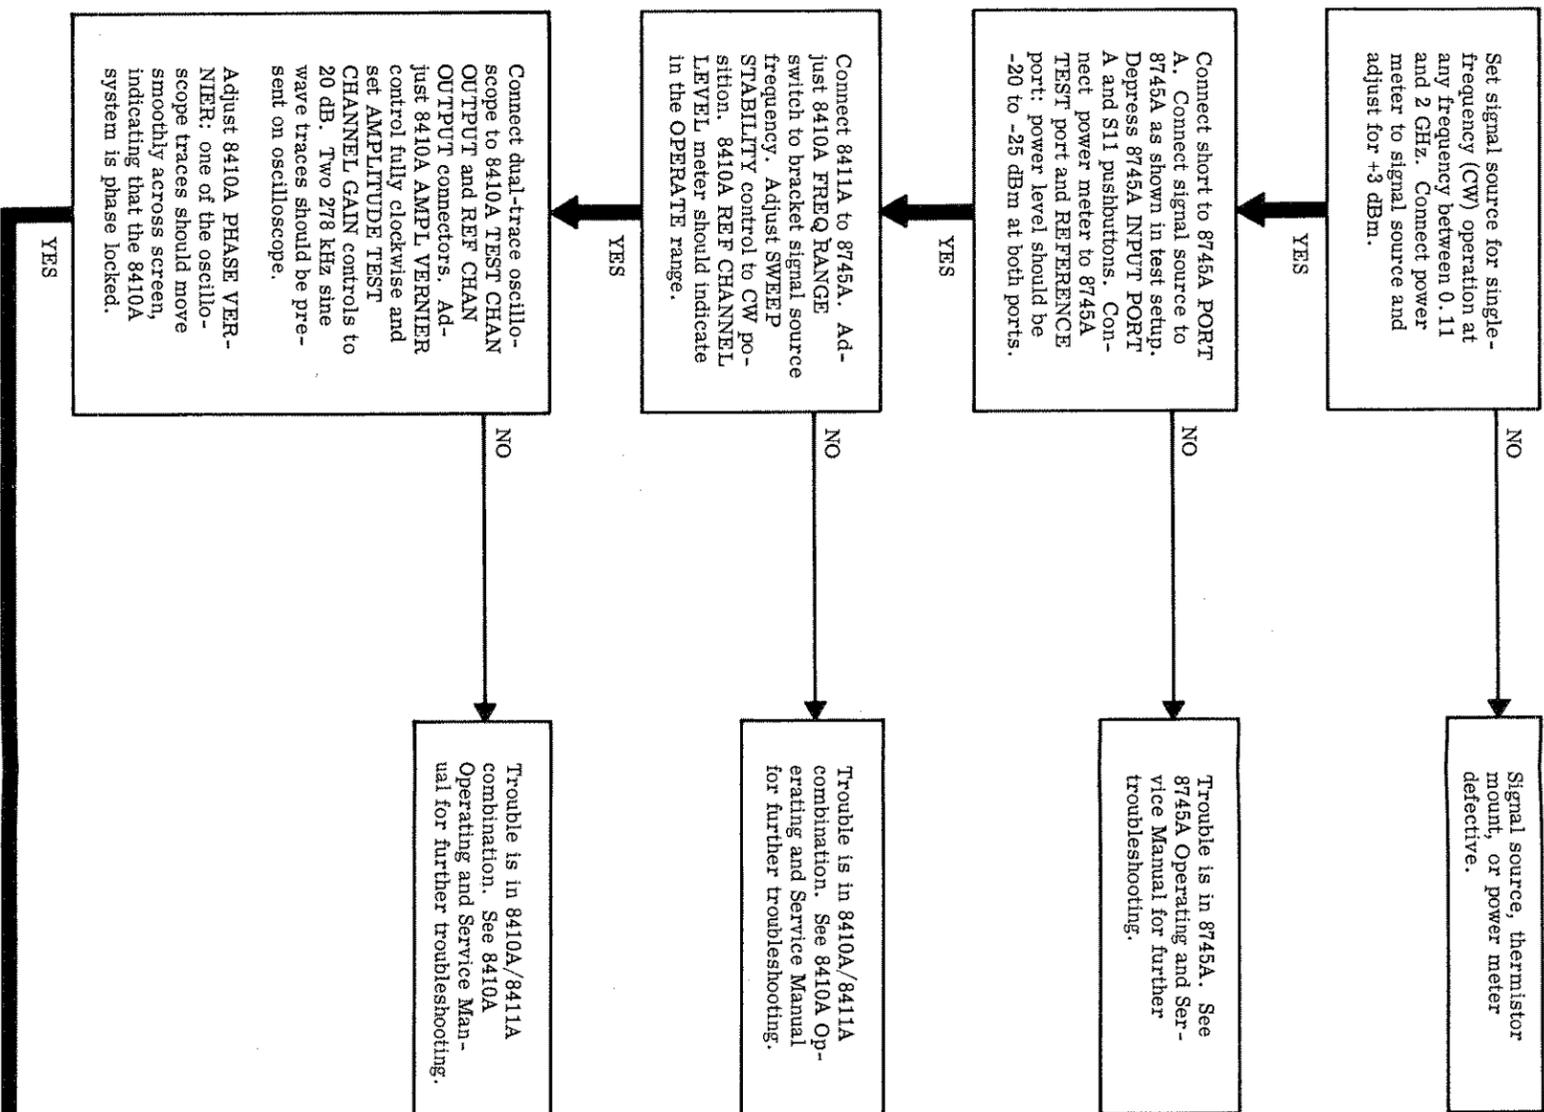

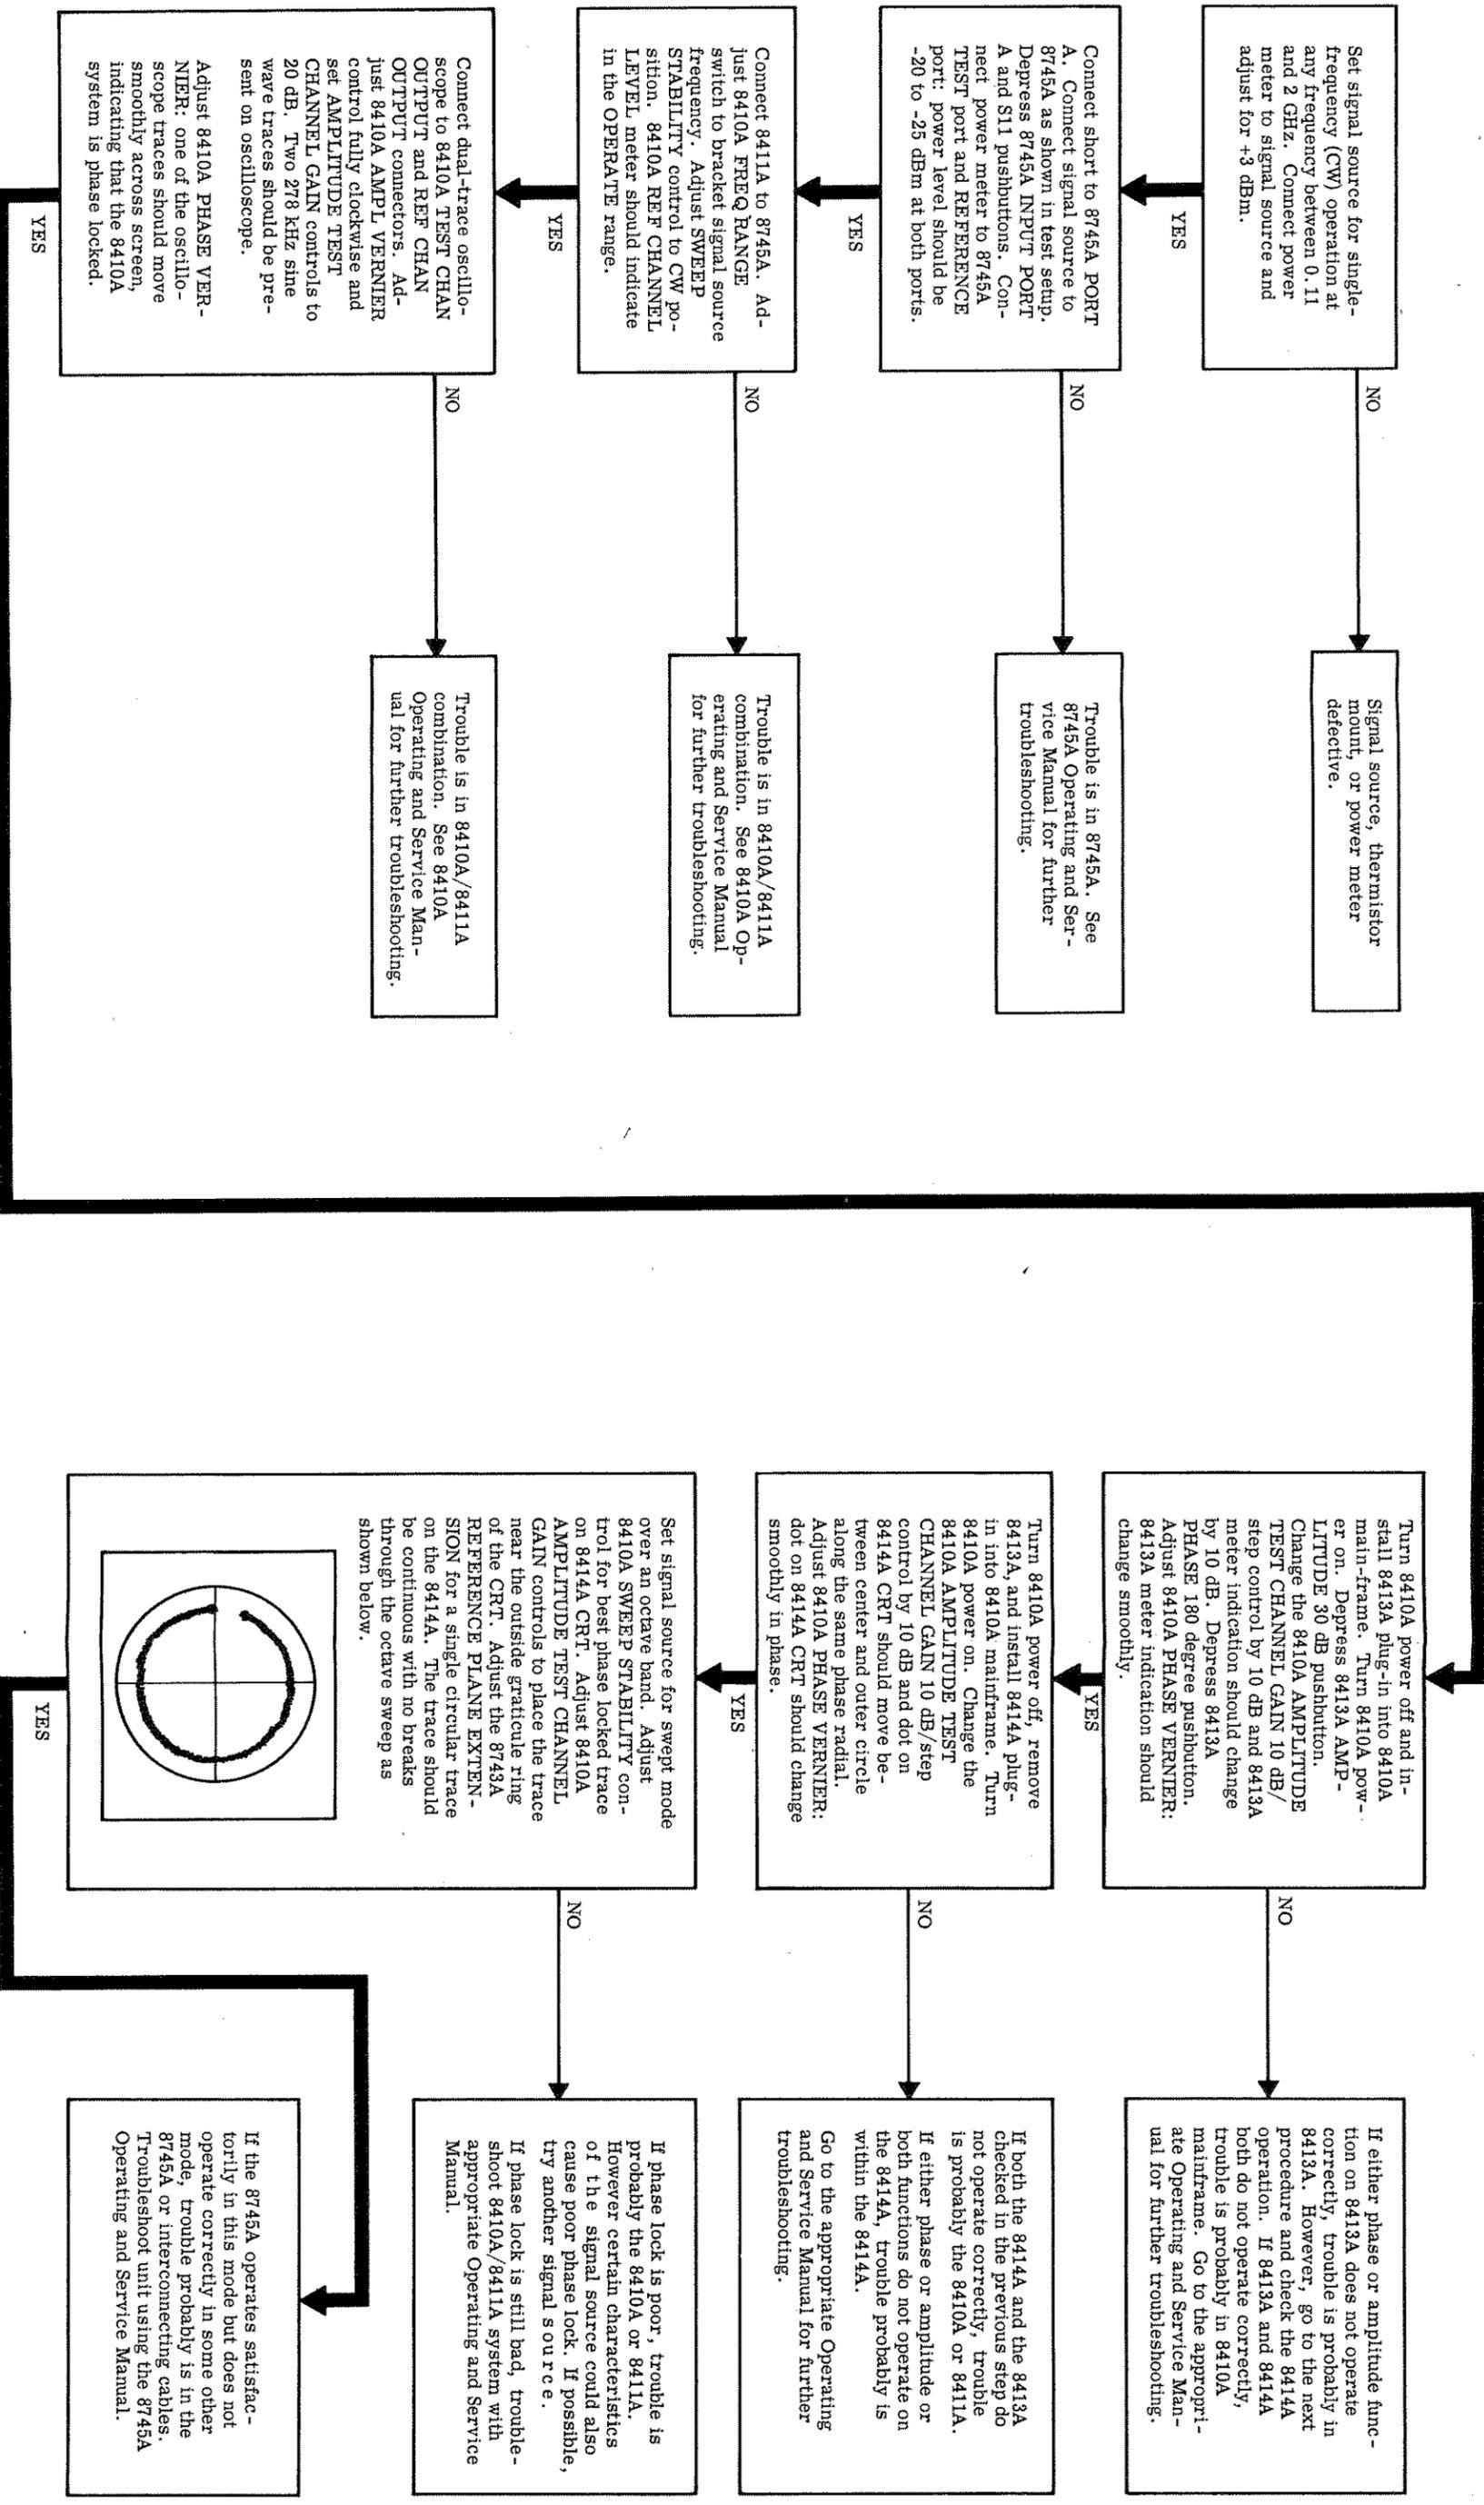


Figure 4-6. Model 8410S-100 and 8410S-300 System Troubleshooting Tree

▶ **MODEL 8410S-100 AND 8410S-300**
TROUBLESHOOTING, Figures 4-5 and 4-6




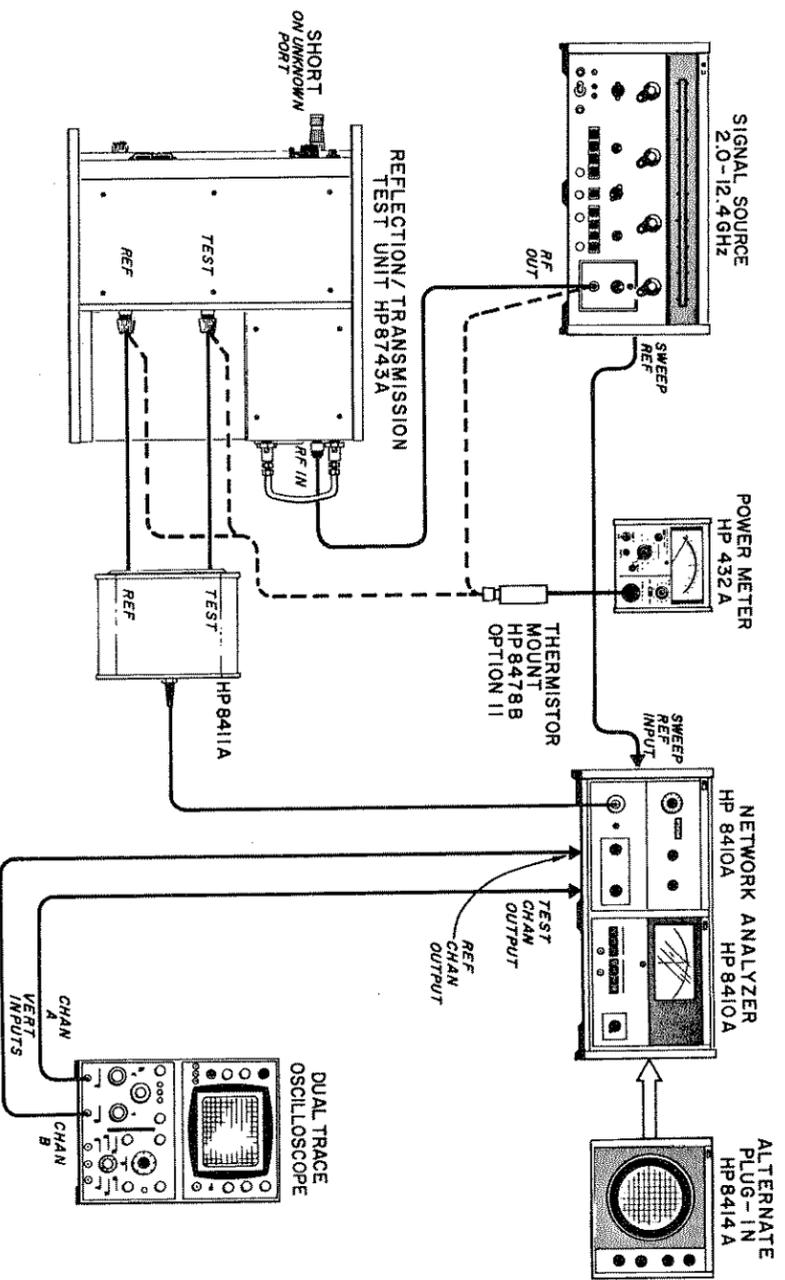


Figure 4-7. Test Setup for Model 8410S-200 and 8410S-300 Troubleshooting

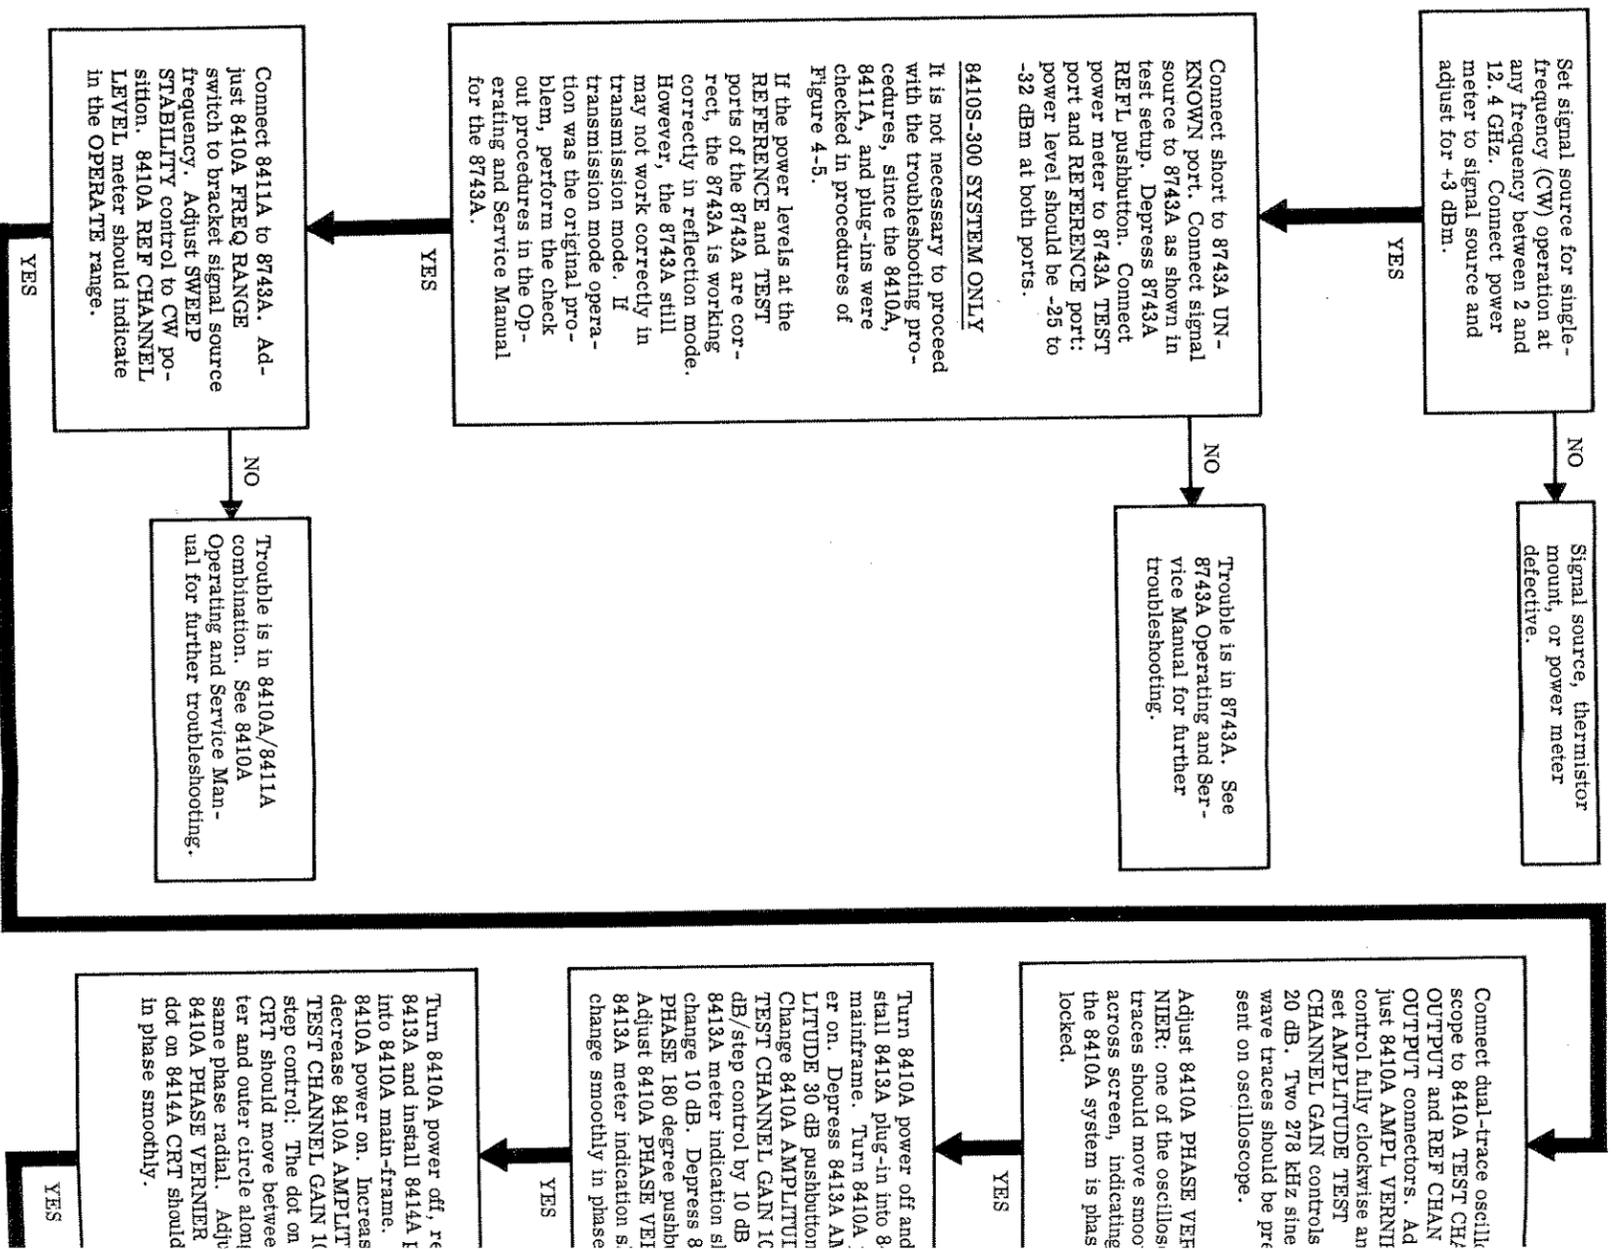

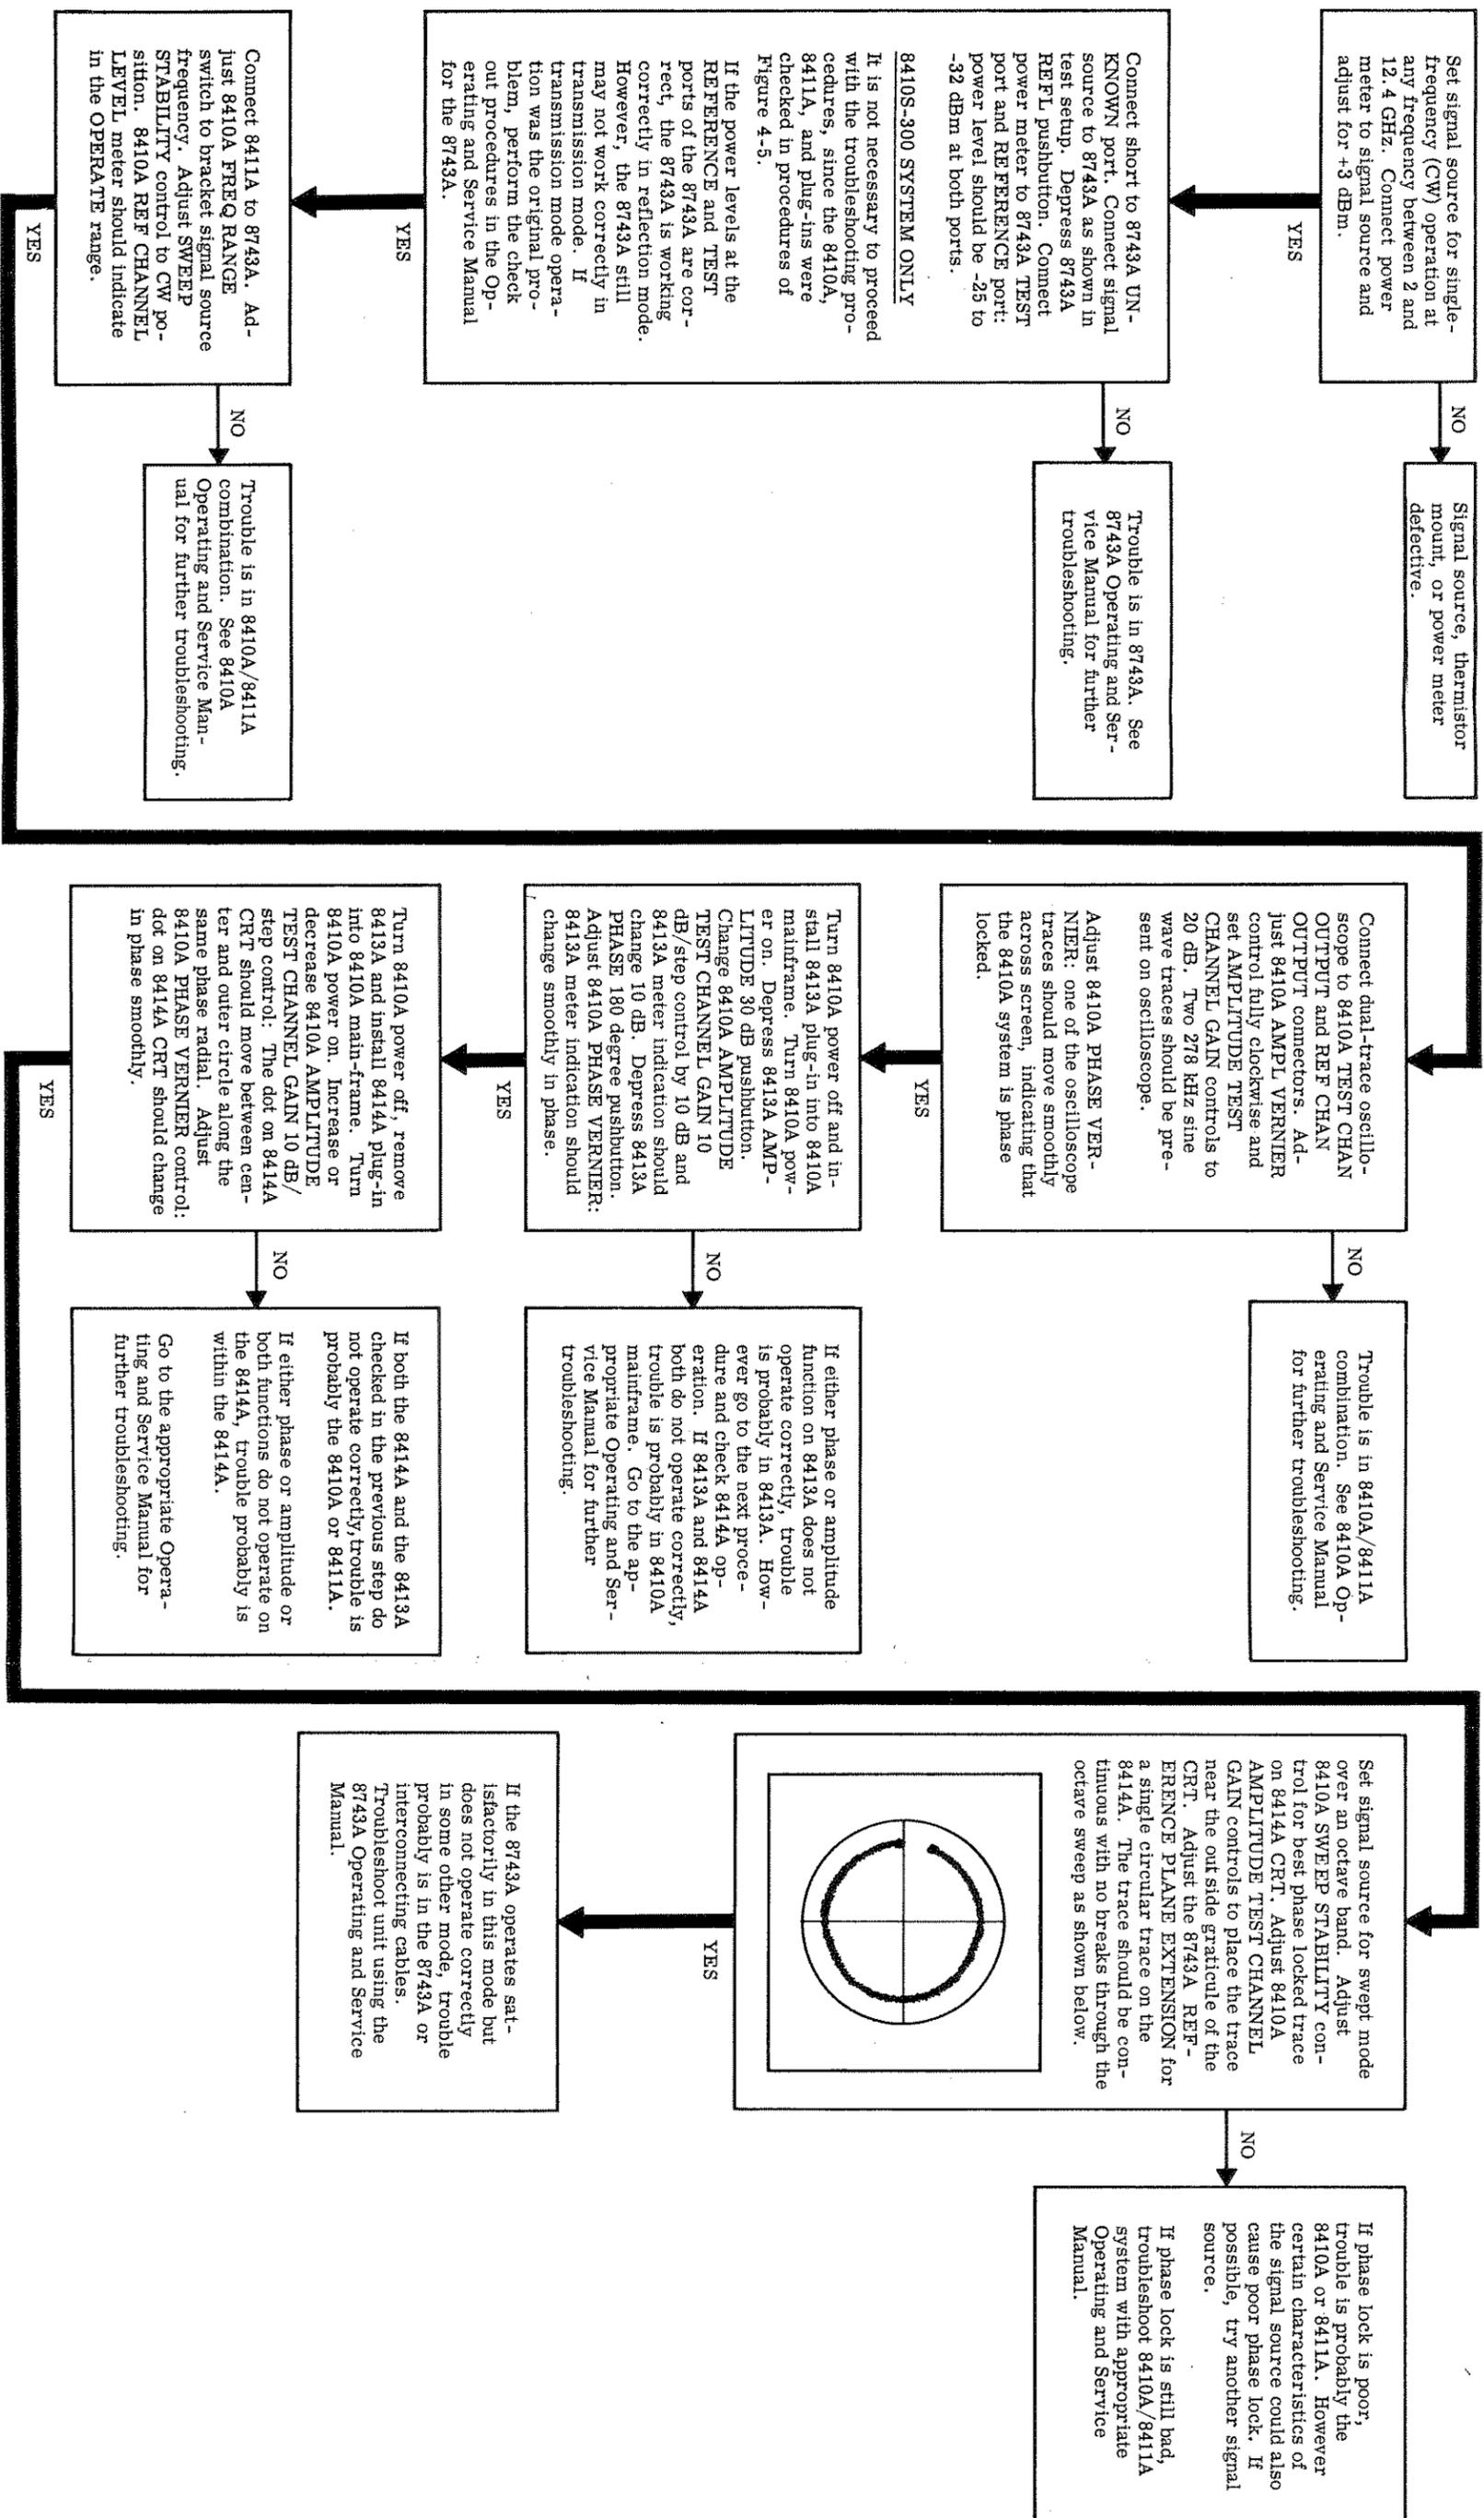


Figure 4-8. Model 8410S-200 and 8410S-300 System Troubleshooting Tree

