

Errata

Title & Document Type: 81533B and 81520A/1B/4A/5A Optical Head User's Guide

Manual Part Number: 81533-90014

Revision Date: May 1994

HP References in this Manual

This manual may contain references to HP or Hewlett-Packard. Please note that Hewlett-Packard's former test and measurement, semiconductor products and chemical analysis businesses are now part of Agilent Technologies. We have made no changes to this manual copy. The HP XXXX referred to in this document is now the Agilent XXXX. For example, model number HP8648A is now model number Agilent 8648A.

About this Manual

We've added this manual to the Agilent website in an effort to help you support your product. This manual provides the best information we could find. It may be incomplete or contain dated information, and the scan quality may not be ideal. If we find a better copy in the future, we will add it to the Agilent website.

Support for Your Product

Agilent no longer sells or supports this product. You will find any other available product information on the Agilent Test & Measurement website:

www.tm.agilent.com

Search for the model number of this product, and the resulting product page will guide you to any available information. Our service centers may be able to perform calibration if no repair parts are needed, but no other support from Agilent is available.

Users Guide

HP 81533B Optical Head Interface Module, HP 81520A, HP 81521B, HP 81524A, and HP 81525A Optical Heads

SERIAL NUMBERS

This manual applies to all instruments listed above, and
also to the HP 81533A Optical Head Interface Module.



**HEWLETT
PACKARD**

**HP Part No. 81533-90014
Printed in the Federal Republic of Germany**

**Fourth Edition
E0594**

Notices

This document contains proprietary information which is protected by copyright. All rights are reserved.

No part of this document may be photocopied, reproduced, or translated to another language without the prior written consent of Hewlett-Packard GmbH.

© Copyright 1992 by:
Hewlett-Packard GmbH
Herrenberger Str. 130
7030 Boeblingen
Federal Republic of Germany

Subject Matter

The information in this document is subject to change without notice.

Hewlett-Packard makes no warranty of any kind with regard to this printed material, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

Hewlett-Packard shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

Printing History

New editions are complete revisions of the manual. Update packages, contain additional and replacement information to be incorporated into the manual by the customer. The date on the title page only changes when a new manual is published. When an edition is reprinted, all the prior updates to the edition are incorporated.

Warranty

This Hewlett-Packard instrument product is warranted against defects in material and workmanship for a period of one year from date of shipment. During the warranty period, HP will, at its option, either repair or replace products which prove to be defective.

For warranty service or repair, this product must be returned to a service facility designated by HP. Buyer shall prepay shipping charges to HP and HP shall pay shipping charges to return the product to Buyer.

However, Buyer shall pay all shipping charges, duties, and taxes for products returned to HP from another country.

HP warrants that its software and firmware designated by HP for use with an instrument will execute its programming instructions when properly installed on that instrument.

HP does not warrant that the operation of the instrument, software, or firmware will be uninterrupted or error free.

Limitation of Warranty

The foregoing warranty shall not apply to defects resulting from improper or inadequate maintenance by Buyer, Buyer-supplied software or interfacing, unauthorized modification or misuse, operation outside of the environmental specifications for the product, or improper site preparation or maintenance.

No other warranty is expressed or implied. Hewlett-Packard specifically disclaims the implied warranties of Merchantability and Fitness for a Particular Purpose.

Exclusive Remedies

The remedies provided herein are Buyer's sole and exclusive remedies. Hewlett-Packard shall not be liable for any direct, indirect, special, incidental, or consequential damages whether based on contract, tort, or any other legal theory.

Assistance

Product maintenance agreements and other customer assistance agreements are available for Hewlett-Packard products. For any assistance contact your nearest Hewlett-Packard Sales and Service Office. Addresses are provided at the back of this manual.

Certification

Hewlett-Packard Company certifies that this product met its published specifications at the time of shipment from the factory.

Hewlett-Packard further certifies that its calibration measurements are traceable to the United States National Institute of Standards and Technology, NIST (formerly the United States National Bureau of Standards, NBS) to the extent allowed by the Institutes's calibration facility, and to the calibration facilities of other International Standards Organization members.

Control Serial Number: Edition 3 applies directly to all instruments.
Edition 1 : 1st May 1990 : 81533-90011 : E0590 ; 1st December 1990 : 81533-90011 : E1290
Edition 2 : 1st December 1991 : 81533-90012 : E1291
Edition 3 : 1st March 1993 : 81533-90013 : E0393
Edition 4 : 1st May 1994 : 81533-90014 : E0594

Safety Considerations

Before operation, review the instrument and manual, including the red safety page, for safety markings and instructions. You must follow these to ensure safe operation and to maintain the instrument in safe condition.

Initial Inspection

Inspect the shipping container for damage. If there is damage to the container or cushioning, keep it until you have checked the contents of the shipment for completeness and verified the module both mechanically and electrically.

The Performance Tests give procedures for checking the operation of the module. If the contents are incomplete, mechanical damage or defect is apparent, or if a module does not pass the operator's checks, notify the nearest Hewlett-Packard office.

Warning



To avoid hazardous electrical shock, do not perform electrical tests when there are signs of shipping damage to any portion of the outer enclosure (covers, panels, etc.).

Power Requirements

The HP 81533B operates when installed into the HP 8153A Optical Multimeter mainframe.

Operating Environment

The HP 8153A safety information summarizes the HP 81533B operating environment ranges. In order for the HP 81533B to meet specifications, the operating environment must be within the limits specified in this section.

Input/Output Signals



Caution

A maximum of 15V can be applied as an external voltage to any BNC connectors.

Storage and Shipment

The module can be stored or shipped at temperatures between -40°C and $+70^{\circ}\text{C}$. Protect the module from temperature extremes that may cause condensation within it.

Contents

C. HP 81533B, HP 81520A, HP 81521B, HP 81524A, and HP 81525A Specifications	
Supplementary Performance Characteristics	C-3
HP 81050AL Lens	C-3
HP 81010BL and HP 81050BL Lens	C-4
Optical Connections	C-4
Compensating for Lens Loss	C-6
D. HP 81533B and Optical Heads Performance Tests	
Introduction	D-1
Test Record	D-1
Test Failure	D-1
Instrument Specification	D-2
Module Function Tests	D-3
Equipment Required	D-3
Function Test	D-3
Static and Dynamic Tests	D-3
Gain/Range Calibration Accuracy Test	D-6
HP 81520A, HP 81521B, HP 81524A, and HP 81525A Performance Tests	D-12
Equipment Required	D-12
HP 81520A	D-12
HP 81521B	D-13
HP 81524A or HP 81525A	D-14
Performance Test	D-14
Accuracy and Linearity Tests	D-15
I. Accuracy Test	D-15
II. Linearity Test	D-16

E. Cleaning Procedures

Cleaning Materials	E-1
Cleaning Fiber/Front-Panel Connectors	E-2
Cleaning Connector Interfaces	E-2
Cleaning Connector Bushings	E-3
Cleaning Detector Windows	E-3
Cleaning Lens Adapters	E-3
Cleaning Detector Lens Interfaces	E-4

Index

Figures

C-1. Optical Connections	C-5
C-2. Optical Connections	C-6
D-1. Accuracy Test Set-Up	D-15
D-2. HP 81525A Linearity Test Test Set-Up	D-17
D-3. Addition of results (example)	D-20

HP 81533B, HP 81520A, HP 81521B, HP 81524A, and HP 81525A Specifications

Specifications describe the instrument's warranted performance. Supplementary performance characteristics describe the instrument's non-warranted typical performance.

Because of the modular nature of the instrument, these performance specifications apply only to this module. You should insert these pages into the appropriate section of the manual.

HP 81533B Specifications

	HP 81533B with HP 81520A Optical Head	HP 81533B with HP 81521B Optical Head	HP 81533B with HP 81524A Optical Head	HP 81533B with HP 81525A Optical Head
Sensor Element	Si, 5mm	Ge, 5mm	InGaAs, 5mm	
Wavelength range	450-1020nm	900-1700nm	800-1650nm	
Power range	+10 to -100dBm	+3 to -80dBm	+3 to -90dBm	+27 to -70dBm (1250 to 1650nm) +23 to -70dBm (800 to 1650nm)
Applicable fiber type	parallel beam, 9/125 μ m - 100/140 μ m, NA \leq 0.3			
Uncertainty (Accuracy) at reference conditions^[1]	\pm 2.2% (600-1020nm)	\pm 2.2% (1000-1650nm)	\pm 2.2% (1000-1600nm)	\pm 3% (900-1600nm)
Total Uncertainty^[2]	\pm 4% \pm 0.5pW (600-1020nm)	\pm 4% \pm 50pW (1000-1650nm)	\pm 4% \pm 5pW (1000-1600nm)	\pm 5% \pm 500pW (900-1600nm)
Linearity 18°C to 28°C const. temp Operating temp. range const. temp	(+3 to -80dBm) \pm 0.04dB \pm 0.5pW \pm 0.15dB \pm 0.5pW	(+3 to -60dBm) \pm 0.04dB \pm 50pW \pm 0.15dB \pm 50pW	(+3 to -70dBm) \pm 0.04dB \pm 5pW \pm 0.15dB \pm 5pW	(-10 to -50dBm) ^[3] \pm 0.04dB \pm 500pW \pm 0.15dB \pm 500pW
Noise peak-peak, avg. time 1sec	<0.5pW (700-900nm)	<50pW (1200-1600nm)	<5pW (1000-1600nm)	<500pW (900-1600nm)
Operating Temperature	0°C to +40°C	0°C to +40°C	0°C to +40°C	0°C to +35°C ^[4]
Dimensions	Module Head			
	75mm H, 32mm W, 335mm D (2.8" \times 1.3" \times 13.2") 37.5mm Diameter, 140mm Long (1.5" \times 5.5")			
Weight	Module Head			
	net 0.6kg (1.3lbs), shipping 1kg (2.2lbs) net 0.45kg (1lbs), shipping 1kg (2.2lbs)			
Recalibration period	2 years			
Warmup time	20 min.			
The display may vary by \pm 1 count.				

Information on the traceability of power meters is available on request

[1] at the following reference conditions:

- Power level 10 μ W (-20dBm), Continuous Wave (CW).
- Parallel beam, 3mm spot diameter on detector.
- Ambient temperature 23 \pm 5°C.
- At day of calibration.
(add 0.3% for aging over one year, add 0.6% over two years).
- Spectral width of source <10nm

[2] at the following operating conditions:

- Parallel beam, 3mm spot diameter on detector, or connectorized fiber with NA ≤ 0.2
 - Ambient temperature 0 to 40°C, non-condensating.
 - Within 1 year after calibration, add 0.3% for the second year.
- [3] Add 0.007dB/dB between 10 and 27dBm.
- [4] 30°C for >20dBm input power.

Supplementary Performance Characteristics

Add 1% to total uncertainty for the full wavelength range.

Outside the specified wavelength range, the noise increases by up to 5 times the value shown above.


For fiber applications with NA between 0.2 and 0.3 use specific lenses and add 0.5% total uncertainty for the 850±50nm, 1300±50nm, and 1550±50nm range.

Analog output	
bandwidth	\geq DC, \leq 300 to 1000Hz depending on range and optical head
output voltage	0 to 2V into open
output impedance	600 Ω typ.
max. input voltage	± 10 V

HP 81050AL Lens

Attenuation at 850 nm (AL-type) is printed on each lens. This value must be entered into the power meter using the CAL parameter, for precise measurements.


Typical attenuation over wavelength for the 81050AL, exactly measured at 850 nm:

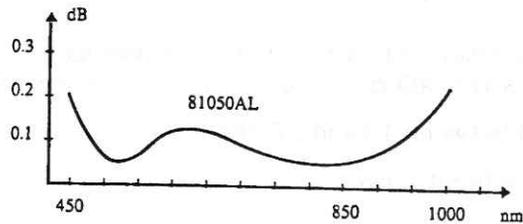

HP 81010BL and HP 81050BL Lens

Attenuation at 1300/1550 nm (BL-type) is printed on each lens. This value must be entered into the power meter using the CAL parameter, for precise measurements.

Typical attenuation over wavelength for the 81010BL and 81050BL, exactly measured at 1300 nm and 1550 nm:

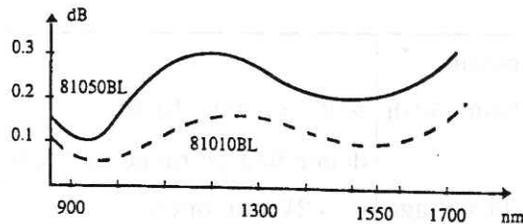

Optical Connections

For the optical head, various accessories can be ordered that aid measurement, as well as connection to bare or terminated fibers. Depending on which accessories you ordered, Figure C-1 shows the sequence in which you attach them to the HP 81520A. Figure C-2 shows the sequence in which you attach them to the HP 81521B and the HP 81524A.

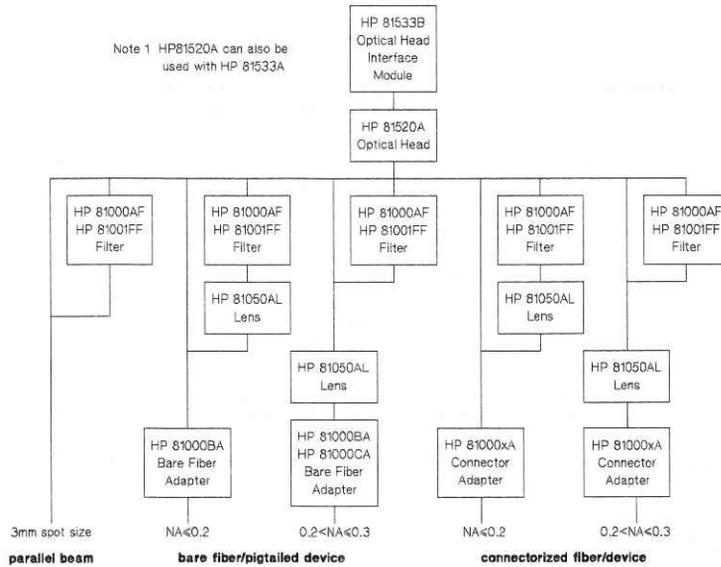


Figure C-1. Optical Connections

You should enter this CAL factor, together with any other known losses for your measurement system, to compensate for the non-ideal nature of the measuring equipment.

HP 81533B and Optical Heads Performance Tests

Introduction

The procedures in this section test the electrical performance of the instrument. The complete specifications to which the HP 81533B, with an optical head, is tested are given in Appendix C. All tests can be performed without access to the interior of the instrument. The test equipment given corresponds to tests carried out with Diamond HMS-10/HP connectors.

Test Record

Results of the performance test may be tabulated on the Test Record provided after the test procedures. It is recommended that you fill out the Test Record and refer to it while doing the test. Since the test limits and setup information are printed on the Test Record for easy reference, the record can also be used as an abbreviated test procedure (if you are already familiar with the test procedures). The Test Record can also be used as a permanent record and may be reproduced without written permission from Hewlett-Packard.

Test Failure

If the HP 81533B or the optical head fails any performance test, return it to the nearest Hewlett-Packard Sales/Service Office for repair.

D Instrument Specification

Specifications are the performance characteristics of the instrument that are certified. These specifications, listed in Appendix C, are the performance standards or limits against which to test. Appendix C also lists some supplemental characteristics. Supplemental characteristics should be considered as additional information.

Any changes in the specifications due to manufacturing changes, design, or traceability to the National Bureau of Standards, are covered in a manual change supplement, or revised manual. Such specifications supersede any that were previously published.

Module Function Tests

Equipment Required

Equipment required for the function test is listed in the table below. Any equipment that satisfies the critical specifications of the equipment given in the table, may be substituted for the recommended models.

Instrument/Accessory	Recommended Model
Multimeter Mainframe	HP 8153A
Optical Head	HP 81520A, HP 81521B, HP 81524A, or HP 81525A
Digital Multimeter	HP 3466A, with test leads.
BNC to BNC cable	HP 10102A
BNC(m) to dual Banana plug	HP 10110B
Test/Cal Box	P/N 08152-63201
Head Recognition Adapter	P/N 08152-63211
Test Cable	P/N 15414-61603
BNC(f) to dual Banana plug	P/N 1251-2277
DC Standard	with adapter cables
Oscilloscope	

Function Test

The function test given in this section is using the HP 8153A with the HP 81533B Optical Head Adapter Module and the 08152- 63201 Test/Cal Box to check voltages and signals to and from the HP 81520A/21B Optical Heads. Perform each step in the tests in the order given, using the corresponding equipment.

Static and Dynamic Tests

1. Insert the HP 81533B into the mainframe channel A position and connect the test/cal box to its input.
2. Make sure that the head recognition adapter is connected to the test/cal box.
3. Turn power on and check that all display segments are lit for approximately 2 seconds and check that the HP 8153A then displays the error message E3200 HEAD-DAT SELFTEST.
4. To test the constant voltages:

D

- a. Using the test cable check the following DC levels at test/cal box receptacles

Receptacle Expected Value

+15V +15±0.8V

-15V -15±0.8V

P.CTRL 0V

STATUS 0V

5. To test the ranging:

- a. The states of RANGE 0 and RANGE 1 depend on the respective HP 8153A range settings.
- b. Press **Auto** to make sure that autoranging is OFF.
- c. Select the following ranges with **Up** and **Down**. In each case, check the status of the range selection signal on the RANGE 0 and RANGE 1 receptacle on the test/cal box.

dBm Range	RANGE 0	RANGE 1
0	H	H
-10	H	H
-20	H	L
-30	H	L
-40	H	L
-50	L	L

6. To test the +5V:

- a. Set the oscilloscope as follows:

Input to 2V/DIV, DC Coupled, 1MΩ.

Timebase to 0.005s/DIV.

Sweep mode to AUTO.

Note

When performing this test and the following tests, each time, after pressing the switch on the head recognition adapter, the message ER 3200 HEAD-DAT appears. To continue the tests or to repeat a test, the error state must be overwritten by pressing any key on the HP 8153A front panel.

- b. Use the test cable to connect the +5V receptacle to the oscilloscope.
 - c. Check that, when you press the switch on the head recognition adapter, the +5V output switches from 0V to +5V and then back to 0V after approximately 2 seconds.
7. To test the data clock (see also the note to step 6):
- a. Use the test cable to connect the CLOCK receptacle to the oscilloscope.
 - b. Check that, when you press the switch on the head recognition adapter, the CLOCK outputs clock pulses for approximately 4 seconds, going from +5V to 0V.
8. To test the \overline{OE} (see also the note to step 6):
- a. Use the test cable to connect the \overline{OE} receptacle to the oscilloscope.
 - b. Check that, when you press the switch on the head recognition adapter, the \overline{OE} output switches from +5V to 0V and then back to +5V after approximately 2 seconds.
9. To test the ON/OFF (see also the note to step 6):
- a. Use the test cable to connect the ON/OFF receptacle to the oscilloscope.
 - b. Check that the ON/OFF output is at +15V while you are pressing the switch on the head recognition adapter, and at +5V when you release the switch.
10. To test the Peltier Control:
- a. Change the input sensitivity of the oscilloscope to 0.05V/DIV and connect the test cable from the P.CTRL receptacle to the oscilloscope.
 - b. Watch the DC level displayed on the oscilloscope and connect instead of the head recognition adapter the HP 81520A, HP 81521B, HP 81524A, or HP 81525A Optical Head.
 - c. After a few seconds, the P.CTRL voltage should change from approximately 130mV to approximately 30mV (HP 81520A), from

D

approximately 150mV to approximately 40mV (HP 81521B)) or from approximately 130mV to approximately 50mV (HP 81524A, or HP 81525A).

Gain/Range Calibration Accuracy Test

Note



These measurements are very dependent on the condition of the test setup. Before beginning these tests, check the equipment for possible ground loops and shielding problems and make sure that the line supply is free of disturbances.

11. To test the gain/range calibration accuracy:
 - a. Connect the DC standard to the BNC connector marked "8152A IN" on the test/cal box. Make sure that the DC standard is set to 0 volts.
 - b. Make sure the instrument is in MEASure mode, and press **(dBm/W)** to make sure that the display is in Watts.
 - c. Press **(Param)** to select the CAL parameter. Reset the calibration to 0 by holding **(Param)** down for 3 seconds.
 - d. Press **(Zero)** to zero the instrument. Select the -20dBm range with **(Up)** and **(Down)**.
 - e. Check that, at the DC standard settings, and Range settings given in the table, you get the readings indicated.

Range DC Standard Setting		Reading
-20	0.0000V	0.00 μ W
-20	+7.6000V	19.000 μ W(\pm 40 counts)
-20	+0.7600V	1.900 μ W(\pm 4 counts)
-30	+0.7600V	1900.0nW(\pm 40 counts)
-30	+0.0760V	190.0nW(\pm 4 counts)
-40	+0.0760V	190.00nW(\pm 40 counts)
-40	+0.0076V	19.00nW(\pm 4 counts)

Function Test for the HP 81533B

D

Test Facility:

_____	Report No.	_____
_____	Date	_____
_____	Customer	_____
_____	Tested By	_____

Model HP 81533B Optical Head Interface Module

Serial No. _____ Ambient temperature _____ °C

Options _____ Relative humidity _____ %

Firmware Rev. _____ Line frequency _____ Hz

Special Notes:

Performance Test for the HP 81533B

Test Equipment Used:

Description	Model No.	Trace No.	Cal. Due Date
1. Lightwave Multimeter (Std.)	HP 8153A	_____	_____
2. Opt. Head Interface Module	HP 81533B	_____	_____
3a. Optical Head 850nm	HP 81520A	_____	_____
3b. Optical Head 1310, 1550nm	HP 81521B	_____	_____
3c. Optical Head 1310, 1550nm	HP 81524A	_____	_____
3d. Optical Head 1310, 1550nm	HP 81525A	_____	_____
4. BNC to BNC Cable	HP 10102A		
5. BNC(m) to dual banana plug	HP 10110B		
6. Test/Cal Box	08152-63201		
7. Head Recognition Adapter	08152-63211		
8. Test Cable	15414-61603		
9. BNC(f) to dual banana plug	1251-2277		
10. DC Standard with Adapter Cables	_____	_____	_____
11. Oscilloscope	_____	_____	_____
12. _____	_____	_____	_____
13. _____	_____	_____	_____

Function Test for the HP 81533B

Page 3 of 4

D

Model HP 81533B Opt. Head Int. Module No. _____ Date _____

Test Description		Pass	Fail
Static and Dynamic Test			
Parameter	Expected Value		
+15V	+15±0.8V	—	—
-15V	-15±0.8V	—	—
P.CTRL	0V	—	—
STATUS	0V	—	—
RANGE 0	High in the 0dBm to -40dBm ranges Low in the -50dBm range	—	—
RANGE 1	High in the 0dBm to -10dBm ranges Low in the -20dBm to -50dBm ranges	—	—
+5V	0V→+5V→0V	—	—
MODE 0	0V→+5V→0V	—	—
MODE 1	0V→+5V→0V	—	—
CLOCK	Pulses from +5V to 0V	—	—
$\overline{\text{OE}}$	+5V→0V→+5V	—	—
ON/OFF	+5V→+15V→+5V	—	—
P.CTRL	Peltier Regulation	—	—

Function Test for the HP 81533B

Page 4 of 4

D

Model HP 81533B Opt. Head Int. Module No. _____ Date _____

Test Description		Result		
Gain/Range Accuracy Test				
Range	DC Standard Setting	Minimum	Actual	Maximum
-20dBm	0.0000V	0.000 μ W	_____	0.000 μ W
-20dBm	+7.6000V	18.960 μ W	_____	19.040 μ W
-20dBm	+0.7600V	1.896 μ W	_____	1.904 μ W
-30dBm	+0.7600V	1896.0nW	_____	1904.0nW
-30dBm	+0.0760V	189.6nW	_____	190.4nW
-40dBm	+0.0760V	189.60nW	_____	190.40nW
-40dBm	+0.0076V	18.96nW	_____	19.04nW

D

HP 81520A, HP 81521B, HP 81524A, and HP 81525A Performance Tests

Equipment Required

Equipment required for the performance test is listed below. Any equipment that satisfies the critical specifications of the equipment given in the table, may be substituted for the recommended models.

HP 81520A

Instrument/Accessory	Rec. Model	Required Characteristic
Power Meter Standard #C01	HP 8153A Lightwave Multimeter Mainframe with HP 81533B Optical Head Interface Module with HP 81520A Optical Head.	Uncertainty $\pm 1.5\%$
CW Laser Source	HP 8153A Lightwave Multimeter Mainframe with HP 81551MM 850nm Laser Source Module.	Wavelength Uncertainty $\pm 2\text{nm}$
Optical Attenuator	HP 8158B Opt.001/011	
Multimode Fiber	HP 81501AC ($\times 2$)	
Lens Adapter	HP 81050AL	
Connector Adapter	HP 81000AA	
Plastic Cap	5040-9361 ($\times 2$)	

HP 81521B

Instrument/Accessory	Rec. Model	Required Characteristic
Power Meter Standard #C01	HP 8153A Lightwave Multimeter Mainframe with HP 81533B Optical Head Interface Module with HP 81521B Optical Head	Uncertainty $\pm 1.5\%$
CW Laser Source	HP 8153A Lightwave Multimeter Mainframe with HP 81552SM 1310nm Laser Source Module and HP 81553SM 1550nm Laser Source Module	Wavelength Uncertainty $\pm 1.5\text{nm}$
	<i>OR</i>	
	HP 8153A Lightwave Multimeter Mainframe with HP 81554SM 1310/1550nm Laser Source Module.	Wavelength Uncertainty $\pm 1.5\text{nm}$
Optical Attenuator	HP 8158B Opt.002/011	
Singlemode Fiber	HP 81101AC ($\times 2$)	
Lens Adapter	HP 81010BL	
Connector Adapter	HP 81000AA	
Plastic Cap	5040-9361 ($\times 2$)	

D

HP 81524A or HP 81525A

Instrument/Accessory	Rec. Model	Required Characteristic
Power Meter Standard #C01	HP 8153A Lightwave Multimeter Mainframe with HP 81533B Optical Head Interface Module with HP 81524A Optical Head	Uncertainty $\pm 1.5\%$
CW Laser Source	HP 8153A Lightwave Multimeter Mainframe with HP 81552SM 1310nm Laser Source Module and HP 81553SM 1550nm Laser Source Module	Wavelength Uncertainty $\pm 1.5\text{nm}$
	<i>OR</i>	
	HP 8153A Lightwave Multimeter Mainframe with HP 81554SM 1310/1550nm Laser Source Module.	Wavelength Uncertainty $\pm 1.5\text{nm}$
Optical Attenuator	HP 8158B Opt.002/011	
Singlemode Fiber	HP 81101AC ($\times 2$)	
Lens Adapter	HP 81010BL	
Connector Adapter	HP 81000AA	
Plastic Cap	5040-9361 ($\times 2$)	

Performance Test

The performance tests given in this section are separated into Accuracy Test and Linearity Test. Perform each step in the tests in the order given, using the corresponding test equipment.

Note

Make sure that all optical connections of the test setups given in the procedure are dry and clean. **DO NOT USE INDEX MATCHING OIL** (see cleaning procedure).

The Optical Cables from the Laser Source to and from the HP 8158B Attenuator to the Power Meter must be fixed on the table to ensure minimum cable movement during the tests.

Accuracy and Linearity Tests

Specifications: HP 81520A

Uncertainty: $\pm 2.5\%$ (600-1020 nm) including aging.

Linearity: $\pm 0.04\text{dB} \pm 0.5\text{pW}$ rel. to -20dBm

Specifications: HP 81521B

Uncertainty: $\pm 2.5\%$ (1000-1650 nm) including aging.

Linearity: $\pm 0.04\text{dB} \pm 50\text{pW}$ rel. to -20dBm

Specifications: HP 81524A

Uncertainty: $\pm 2.5\%$ (1000-1600 nm) including aging.

Linearity: $\pm 0.04\text{dB} \pm 5\text{pW}$ rel. to -20dBm

Specifications: HP 81525A

Uncertainty: $\pm 3.3\%$ (900-1600 nm) including aging.

Linearity: $\pm 0.04\text{dB} \pm 500\text{pW}$ rel. to -20dBm

I. Accuracy Test

The following gives the procedure for performing the accuracy test for the HP 81520A, HP 81521B, HP 81524A, or the HP 81525A with the HP 8153A and the HP 81533B:

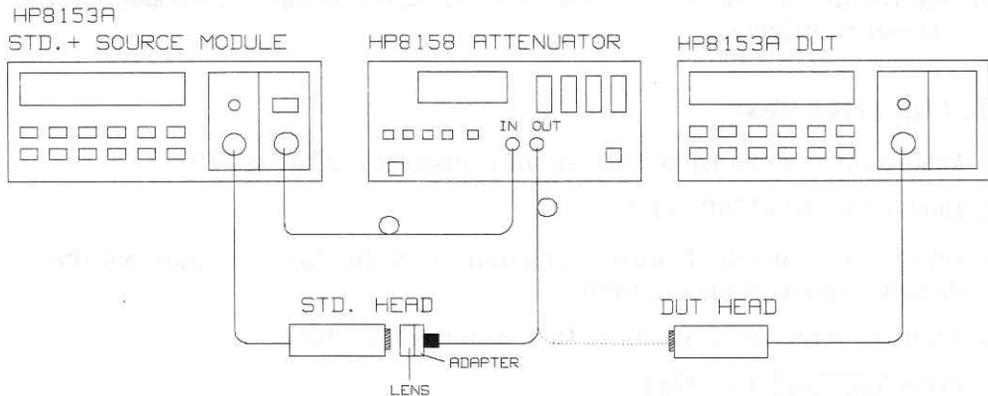


Figure D-1. Accuracy Test Set-Up

D

1. Make sure that the cable connectors, lenses and detector windows are clean. Refer to the cleaning procedure.
2. Connect the equipment as shown in Figure D-1. Ensure that the cables to and from the Attenuator are fixed on the table and both optical heads are close together so that minimum cable movement is achieved when connecting the cable to the Standard or to the DUT Head.
3. Turn the instruments on, enable the laser source, and allow the instruments to warm up for at least 20 minutes.
4. ZERO the power meters with the head connector adapters covered with plastic caps (P/N 5040-9361 or 5040-9351).
5. Set the CAL factor of both instruments to zero.
6. Set the WAVELENGTH of both instruments to the actual wavelength of the Laser Source and note the wavelength in the Test Record.
7. Set both instruments to MEASure, (display in μW), switch AUTOrange off and select the -20dBm range.
8. Enable the HP 8158B output, and change the HP 8158B attenuation until the Power Meter Standard displays 10.00 μW .
9. Connect the attenuator output cable, with the same lens and adapter, to the DUT and check that the DUT display is between 9.75 μW and 10.25 μW . Note the result in the Test Record.
10. For the HP 81521B, HP 81524A, or HP 81525A, repeat steps 8 and 9 at the second wavelength.

II. Linearity Test

1. Make sure that the HP 8158B output is disabled. ZERO the DUT.
2. Enable the HP 8158B output.
3. On the DUT, switch off autoranging and select the -20dBm range. Set the display to show results in dBm.
4. Alter the attenuation until the DUT displays -17.4dBm.
5. Press **Disp→Ref**, then **dB**.
6. Press **Up** to select the -10dBm range.
7. Note the deviation, displayed in dB, as R1 on the test record.

- a. In the -10dBm range. Set the display to show results in dBm.
 - b. Alter the attenuation until the DUT displays -7.4dBm.
 - c. Press **(Disp→Ref)**, then **(dB)**.
 - d. Select the 0dBm range.
 - e. Note the deviation, displayed in dB, as R2 on the test record.
8. Repeat the steps a to e at the all the range and level settings shown in the test record.

Note



- For the HP 81520A, HP 81524A, or HP 81525A, it might be necessary to use the attenuation of the laser source itself, as well as the attenuator, to set the power to -67.2dBm in the -60dBm range.
- For the HP 81525A in the +10, +20, and +30dBm ranges.
 - a. Connect the laser source to the DUT Head as shown in Figure D-2.

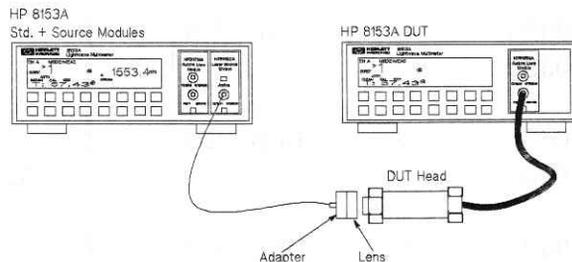


Figure D-2. HP 81525A Linearity Test Test Set-Up

- b. Use the attenuation of the laser source itself to set the power to 0dBm for the 0dBm range before selecting the +10dBm range. You do not need to alter this attenuation of the source before selecting the +20dBm and +30dBm ranges.
-
9. Calculate the non-linearity using the formulae in the test record. An example calculation follows here.

D

**Example Results for the Linearity test (for an HP 81525A
Optical Head)**

Test No.	Test Description	Min. Spec.	Result	Max. Spec.	Measurement Uncertainty
II.	Linearity Test		dB		
	Range Power (dBm)				
	-20dBm -17.4	Disp→Ref			
	-10dBm		0.01 = R1		
	-10dBm -7.4	Disp→Ref			
	0dBm		-0.02 = R2		
	-20dBm -27.4	Disp→Ref			
	-30dBm		-0.02 = R3		
	-30dBm -37.4	Disp→Ref			
	-40dBm		-0.01 = R4		
	0dBm 0	Disp→Ref			
	+10dBm		0.03 = R11		
	0dBm 0	Disp→Ref			
	+20dBm		-0.02 = R21		
	0dBm 0	Disp→Ref			
	+30dBm		0.03 = R31		

**Example Calculated Results for the Linearity Test (for an
HP 81525A Optical Head)**

Test No.	Test Description	Min. Spec.	Result	Max. Spec.	Measurement Uncertainty
Non-Linearity					
	Range Formula				
	0dBm R1 + R2	-0.04dB	-0.01dB	+0.04dB	±0.011dB
	-10dBm R1	-0.04dB	0.01dB	+0.04dB	±0.010dB
	-20dBm		0.000dB		±0.000dB
	-30dBm R3	-0.04dB	-0.02dB	+0.04dB	±0.010dB
	-40dBm R3 + R4	-0.04dB	-0.03dB	+0.04dB	±0.014dB
	+ 10dBm R1 + R2 + R11	-0.04dB	0.02dB	+0.04dB	
	+ 20dBm R1 + R2 + R21	-0.04dB	-0.03dB	+0.04dB	
	+ 30dBm R1 + R2 + R31	-0.04dB	0.01dB	+0.04dB	

Shown graphically, these results look add as shown in the following figure:

D

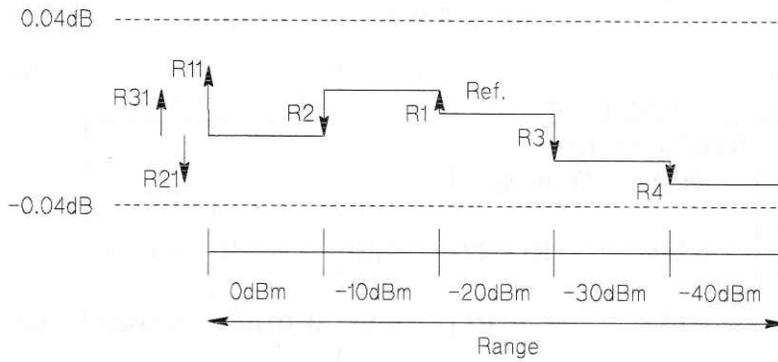


Figure D-3. Addition of results (example)

Performance Test for the HP 81520A

Test Facility:

_____	Report No.	_____
_____	Date	_____
_____	Customer	_____
_____	Tested By	_____

Model HP 81520A Optical Head

Serial No.	_____	Ambient temperature	_____ °C
Options	_____	Relative humidity	_____ %
Firmware Rev.	_____	Line frequency	_____ Hz

Special Notes:

Performance Test for the HP 81520A

Page 2 of 4

Test Equipment Used:

Description	Model No.	Trace No.	Cal. Due Date
1. Lightwave Multimeter (Std.)	HP 8153A	_____	_____
2a. Opt. Head Interface Module	HP 81533B	_____	_____
2b. Optical Head 850nm	HP 81520A	_____	_____
3. Laser Module	HP 81551MM	_____	_____
4. Lens Adapter	HP 81050AL		
5. Connector Adapter	HP 81000AA		
6. Optical Attenuator	HP 8158B Opt.001/011		
7. Multimode Fiber (x2)	HP 81501AC		
8. Lightwave Multimeter (DUT)	HP 8153A		
9. Opt. Head Interface Module (DUT)	HP 81533B		
10. _____	_____	_____	_____
11. _____	_____	_____	_____
12. _____	_____	_____	_____
13. _____	_____	_____	_____
14. _____	_____	_____	_____
15. _____	_____	_____	_____
16. _____	_____	_____	_____

Performance Test for the HP 81520A

Test No.	Test Description	Min. Spec.	Result	Max. Spec.	Measurement Uncertainty
I.	Accuracy Test		μW		
	measured at _____ nm Output Power	9.75 μW	_____	10.25 μW	$\pm 2.00\%$
II.	Linearity Test		dB		
	Range Power (dBm)				
	-20dBm -17.4 Disp→Ref		_____ = R1		
	-10dBm				
	-10dBm -7.4 Disp→Ref		_____ = R2		
	0dBm				
	-20dBm -27.4 Disp→Ref		_____ = R3		
	-30dBm				
	-30dBm -37.4 Disp→Ref		_____ = R4		
	-40dBm				
	-40dBm -47.4 Disp→Ref		_____ = R5		
	-50dBm				
	-50dBm -57.4 Disp→Ref		_____ = R6		
	-60dBm				

Performance Test for the HP 81520A

Page 4 of 4

Model HP 81520A Optical Head No. _____ Date _____

Test No.	Test Description	Min. Spec.	Result	Max. Spec.	Measurement Uncertainty
Non-Linearity					
	Range Formula				
	0dBm R1 + R2	-0.04dB	_____dB	+0.04dB	±0.011dB
	-10dBm R1	-0.04dB	_____dB	+0.04dB	±0.010dB
	-20dBm		0.000dB		±0.000dB
	-30dBm R3	-0.04dB	_____dB	+0.04dB	±0.010dB
	-40dBm R3 + R4	-0.04dB	_____dB	+0.04dB	±0.014dB
	-50dBm R3 + R4 + R5	-0.04dB	_____dB	+0.04dB	±0.017dB
	-60dBm R3 + R4 + R5 + R6	-0.04dB	_____dB	+0.04dB	±0.022dB

Performance Test for the HP 81521B

Test Facility:

_____	Report No.	_____
_____	Date	_____
_____	Customer	_____
_____	Tested By	_____

Model HP 81521B Optical Head

Serial No.	_____	Ambient temperature	_____ °C
Options	_____	Relative humidity	_____ %
Firmware Rev.	_____	Line frequency	_____ Hz

Special Notes:

Performance Test for the HP 81521B

Page 2 of 4

Test Equipment Used:

Description	Model No.	Trace No.	Cal. Due Date
1. Lightwave Multimeter (Std.)	HP 8153A	_____	_____
2a. Opt. Head Interface Module	HP 81533B	_____	_____
2b. Optical Head 1310, 1550nm	HP 81521B	_____	_____
3a1. Laser Module	HP 81552SM	_____	_____
3a2. Laser Module	HP 81553SM	_____	_____
3b. Laser Module	HP 81554SM	_____	_____
4. Lens Adapter	HP 81010BL		
5. Connector Adapter	HP 81000AA		
6. Optical Attenuator	HP 8158B		
7. Singlemode Fiber (×2)	Opt.002/011 HP 81101AC		
8. Lightwave Multimeter (DUT)	HP 8153A		
9. Opt. Head Interface Module (DUT)	HP 81533B		
10. _____	_____	_____	_____
11. _____	_____	_____	_____
12. _____	_____	_____	_____
13. _____	_____	_____	_____
14. _____	_____	_____	_____

Performance Test for the HP 81521B

Model HP 81521B Optical Head No. _____ Date _____

Test No.	Test Description	Min. Spec.	Result	Max. Spec.	Measurement Uncertainty
I.	Accuracy Test		μW		
	measured at 13_____nm Output Power	9.75 μW	_____	10.25 μW	$\pm 2.00\%$
	measured at 15_____nm Output Power	9.75 μW	_____	10.25 μW	$\pm 2.00\%$
II.	Linearity Test		dB		
	Range Power (dBm)				
	-20dBm -17.4 Disp→Ref		_____ = R1		
	-10dBm		_____ = R2		
	-10dBm -7.4 Disp→Ref		_____ = R3		
	0dBm		_____ = R4		
	-20dBm -27.4 Disp→Ref		_____ = R5		
	-30dBm				
	-30dBm -37.4 Disp→Ref				
	-40dBm				
	-40dBm -47.4 Disp→Ref				
	-50dBm				

Performance Test for the HP 81521B

D

Model HP 81521B Optical Head No. _____ Date _____

Test No.	Test Description	Min. Spec.	Result	Max. Spec.	Measurement Uncertainty
	Non-Linearity				
	Range Formula				
	0dBm R1 + R2	-0.04dB	_____dB	+0.04dB	±0.011dB
	-10dBm R1	-0.04dB	_____dB	+0.04dB	±0.010dB
	-20dBm		0.000dB		±0.000dB
	-30dBm R3	-0.04dB	_____dB	+0.04dB	±0.010dB
	-40dBm R3 + R4	-0.04dB	_____dB	+0.04dB	±0.014dB
	-50dBm R3 + R4 + R5	-0.051dB	_____dB	+0.051dB	±0.017dB

Performance Test for the HP 81524A

Test Facility:

_____	Report No.	_____
_____	Date	_____
_____	Customer	_____
_____	Tested By	_____

Model HP 81524A Optical Head

Serial No. _____ Ambient temperature _____ °C

Options _____ Relative humidity _____ %

Firmware Rev. _____ Line frequency _____ Hz

Special Notes:

Performance Test for the HP 81524A

Page 2 of 4

Test Equipment Used:

Description	Model No.	Trace No.	Cal. Due Date
1. Lightwave Multimeter (Std.)	HP 8153A	_____	_____
2a. Opt. Head Interface Module	HP 81533B	_____	_____
2b. Optical Head 1310, 1550nm	HP 81524A	_____	_____
3a1. Laser Module	HP 81552SM	_____	_____
3a2. Laser Module	HP 81553SM	_____	_____
3b. Laser Module	HP 81554SM	_____	_____
4. Lens Adapter	HP 81010BL	_____	_____
5. Connector Adapter	HP 81000AA	_____	_____
6. Optical Attenuator	HP 8158B	_____	_____
7. Singlemode Fiber (x2)	Opt.002/011 HP 81101AC	_____	_____
8. Lightwave Multimeter (DUT)	HP 8153A	_____	_____
9. Opt. Head Interface Module (DUT)	HP 81533B	_____	_____
10. _____	_____	_____	_____
11. _____	_____	_____	_____
12. _____	_____	_____	_____
13. _____	_____	_____	_____
14. _____	_____	_____	_____

Performance Test for the HP 81524A

Model HP 81524A Optical Head No. _____ Date _____

Test No.	Test Description	Min. Spec.	Result	Max. Spec.	Measurement Uncertainty
I.	Accuracy Test		μW		
	measured at 13_____nm Output Power	9.75 μW	_____	10.25 μW	$\pm 2.00\%$
	measured at 15_____nm Output Power	9.75 μW	_____	10.25 μW	$\pm 2.00\%$
II.	Linearity Test		dB		
	Range Power (dBm)				
	-20dBm -17.4 Disp→Ref				
	-10dBm		_____ = R1		
	-10dBm -7.4 Disp→Ref				
	0dBm		_____ = R2		
	-20dBm -27.4 Disp→Ref				
	-30dBm		_____ = R3		
	-30dBm -37.4 Disp→Ref				
	-40dBm		_____ = R4		
	-40dBm -47.4 Disp→Ref				
	-50dBm		_____ = R5		
	-50dBm -57.4 Disp→Ref				
	-60dBm		_____ = R6		

Performance Test for the HP 81524A

Page 4 of 4

Model HP 81524A Optical Head No. _____ Date _____

Test No.	Test Description	Min. Spec.	Result	Max. Spec.	Measurement Uncertainty
Non-Linearity					
	Range Formula				
	0dBm R1 + R2	-0.04dB	_____dB	+0.04dB	±0.011dB
	-10dBm R1	-0.04dB	_____dB	+0.04dB	±0.010dB
	-20dBm		0.000dB		±0.000dB
	-30dBm R3	-0.04dB	_____dB	+0.04dB	±0.010dB
	-40dBm R3 + R4	-0.04dB	_____dB	+0.04dB	±0.014dB
	-50dBm R3 + R4 + R5	-0.04dB	_____dB	+0.04dB	±0.017dB
	-60dBm R3 + R4 + R5 + R6	-0.04dB	_____dB	+0.04dB	±0.022dB

Performance Test for the HP 81525A

Test Facility:

_____	Report No.	_____
_____	Date	_____
_____	Customer	_____
_____	Tested By	_____

Model HP 81525A Optical Head

Serial No. _____ Ambient temperature _____ °C

Options _____ Relative humidity _____ %

Firmware Rev. _____ Line frequency _____ Hz

Special Notes:

Performance Test for the HP 81525A

Page 2 of 4

Test Equipment Used:

Description	Model No.	Trace No.	Cal. Due Date
1. Lightwave Multimeter (Std.)	HP 8153A	_____	_____
2a. Opt. Head Interface Module	HP 81533B	_____	_____
2b. Optical Head 1310, 1550nm	HP 81524A	_____	_____
3a1. Laser Module	HP 81552SM	_____	_____
3a2. Laser Module	HP 81553SM	_____	_____
3b. Laser Module	HP 81554SM	_____	_____
4. Lens Adapter	HP 81010BL		
5. Connector Adapter	HP 81000AA		
6. Optical Attenuator	HP 8158B		
7. Singlemode Fiber (×2)	Opt.002/011 HP 81101AC		
8. Lightwave Multimeter (DUT)	HP 8153A		
9. Opt. Head Interface Module (DUT)	HP 81533B		
10. _____	_____	_____	_____
11. _____	_____	_____	_____
12. _____	_____	_____	_____
13. _____	_____	_____	_____
14. _____	_____	_____	_____

Performance Test for the HP 81525A

Test No.	Test Description	Min. Spec.	Result	Max. Spec.	Measurement Uncertainty
Model HP 81524A Optical Head No. _____ Date _____					
I.	Accuracy Test		μW		
	measured at 13_____nm Output Power	9.75 μW	_____	10.25 μW	$\pm 2.00\%$
	measured at 15_____nm Output Power	9.75 μW	_____	10.25 μW	$\pm 2.00\%$
II.	Linearity Test		dB		
	Range Power (dBm)				
	-20dBm -17.4 Disp→Ref		_____ = R1		
	-10dBm		_____ = R2		
	-10dBm -7.4 Disp→Ref		_____ = R3		
	0dBm		_____ = R4		
	-20dBm -27.4 Disp→Ref		_____ = R11		
	-30dBm		_____ = R21		
	-30dBm -37.4 Disp→Ref		_____ = R31		
	-40dBm				
	0dBm 0 Disp→Ref				
	+ 10dBm				
	0dBm 0 Disp→Ref				
	+ 20dBm				
	0dBm 0 Disp→Ref				
	+ 30dBm				

Performance Test for the HP 81525A

Page 4 of 4

Model HP 81524A Optical Head No. _____ Date _____

Test No.	Test Description	Min. Spec.	Result	Max. Spec.	Measurement Uncertainty
Non-Linearity					
	Range Formula				
	0dBm R1 + R2	-0.04dB	_____dB	+0.04dB	±0.011dB
	-10dBm R1	-0.04dB	_____dB	+0.04dB	±0.010dB
	-20dBm		0.000dB		±0.000dB
	-30dBm R3	-0.04dB	_____dB	+0.04dB	±0.010dB
	-40dBm R3 + R4	-0.04dB	_____dB	+0.04dB	±0.014dB
	+10dBm R1 + R2 + R11	-0.04dB	_____dB	+0.04dB	
	+20dBm R1 + R2 + R21	-0.04dB	_____dB	+0.04dB	
	+30dBm R1 + R2 + R31	-0.04dB	_____dB	+0.04dB	

Cleaning Procedures

In general, *whenever possible use physically contacting dry connectors*. Fiber connectors may be used dry or wet. Dry means without index matching compound. If there is a need to use an index matching compound, use only HP index matching oil (part number 8500-4922). Clean the connectors, interfaces and bushings carefully each time after use.

Cleaning Materials

	HP P/N
Lens Cleaning Paper	9300-0761
Special Cleaning Tips	9300-1351
Blow Brush	9300-1131
Adhesive Cleaning tape	15475-68701
Isopropyl Alcohol	Not available from HP. This should be available from any local pharmaceutical supplier.
Pipe Cleaner	

Cleaning Fiber/Front-Panel Connectors

1. In order to clean the instrument front panel connector remove the connector interface.
2. Apply some isopropyl alcohol to the lens cleaning paper and clean the surface and the ferrule of the connectors.
3. Using a new dry piece of cleaning paper wipe the connector surface and ferrule until they are dry and clean.
4. Lightly press the adhesive tape several times against the connector surface to remove any remaining particles. After use store the tape in the container.
5. Protect the connector surface with a cap.

Cleaning Connector Interfaces

- Apply some isopropyl alcohol to the pipe cleaner and wash the inside of the connector interface.
- Using a new dry pipe cleaner, dry the inside of the connector interface.
- Remove the brush part from the blow brush and blow air through the inside of the interface to remove any remaining particles.

Note

If any index matching compound was used, use an ultrasonic bath with isopropyl alcohol to clean the connector interfaces.



Cleaning Connector Bushings

As used on the HP 8158B and HP 81000AS/BS.

Normally the connector bushings require no cleaning. However, if it appears that cleaning is necessary, use only the blow brush with the brush part removed.

Caution



- NEVER insert any cleaning tool into the bushing as this may affect the optical system.
- NEVER use any index matching compound, cleaning fluid or cleaning spray.

Cleaning Detector Windows

As used on the HP 81520A and HP 81521B.

1. Use the blow brush to remove any particles from the surface.
2. Wipe the surface with cleaning paper or special cleaning tips.

Cleaning Lens Adapters

Caution Do not use any cleaning fluid or cleaning spray.



-
1. Using the blow brush, remove dust.
 2. Wipe the surfaces with the special cleaning tips.

Cleaning Detector Lens Interfaces

As used on the HP 81522A and HP 8140A and HP 8153A detector modules.

Normally, the lens interface can be cleaned by using the blow brush. If adhesive dirt must be removed perform as follows:

E

1. Using the blow brush, remove the dust from the lens surface.
2. Press the special cleaning tip to the lens surface and rotate the tip.

Note

Use alcohol for cleaning only then when above procedure does not help or if the dirt is caused by oil or fat.

