



## Instruction Manual

### CP031 Current Probe



CP031 Current Probe  
**Instruction Manual**  
August 2013





700 Chestnut Ridge Road  
Chestnut Ridge, NY, 10977-6499  
Tel: (845) 425-2000  
Fax: (845) 578 5985  
teledynelecroy.com

© 2013 Teledyne LeCroy, Inc. All rights reserved.

Unauthorized duplication of Teledyne LeCroy documentation materials other than for internal sales and distribution purposes is strictly prohibited. However, clients are encouraged to distribute and duplicate Teledyne LeCroy documentation for their own internal educational purposes.

WaveSurfer, WaveRunner, WavePro, WaveMaster and Teledyne LeCroy are registered trademarks of Teledyne LeCroy, Inc. Windows is a registered trademark of Microsoft Corporation. Other product or brand names are trademarks or requested trademarks of their respective holders. Information in this publication supersedes all earlier versions. Specifications are subject to change without notice.

## Warranty

Teledyne Lecroy warrants this oscilloscope accessory for normal use and operation within specification for a period of one year from the date of shipment. Spare parts, replacement parts and repairs are warranted for 90 days.

In exercising its warranty, Teledyne Lecroy, at its option, will either repair or replace any assembly returned within its warranty period to the Customer Service Department or an authorized service center. However, this will be done only if the product is determined by Teledyne LeCroy's examination to be defective due to workmanship or materials, and the defect is not caused by misuse, neglect, accident, abnormal conditions of operation, or damage resulting from attempted repair or modifications by a non-authorized service facility.

The customer will be responsible for the transportation and insurance charges for the return of products to the service facility. Teledyne Lecroy will return all products under warranty with transportation charges prepaid.

This warranty replaces all other warranties, expressed or implied, including but not limited to any implied warranty of merchantability, fitness or adequacy for any particular purposes or use. Teledyne Lecroy shall not be liable for any special, incidental, or consequential damages, whether in contract or otherwise.

923362-00 Rev A  
August 2013

## TABLE OF CONTENTS

Safety Instructions .....	1
Symbols .....	1
Precautions .....	1
Operating Environment .....	2
Overview .....	3
Description .....	3
Key Features.....	3
Accessories.....	3
Operation.....	4
Precautions .....	4
Connecting the Probe to the Test Instrument.....	4
Connecting the Probe to the Test Circuit .....	4
Operation with a Teledyne LeCroy Oscilloscope .....	5
Bandwidth Limit.....	5
Auto Zero .....	5
Degauss Probe .....	5
Care and Maintenance .....	6
Cleaning.....	6
Calibration Interval .....	6
Service Strategy.....	6
Troubleshooting .....	6
Returning a Defective Probe .....	7
Performance Verification .....	8
Test Equipment Required .....	8
Preliminary Procedure.....	9
Functional Check .....	9
Check LF Accuracy.....	10

**CP031 Current Probe**

---

Adjustment Procedure .....	11
Test Equipment Required .....	11
Preliminary Procedure.....	12
Adjust LF Accuracy .....	12
Specifications .....	14
Nominal Characteristics .....	14
Warranted Characteristics.....	14
Typical Characteristics .....	14
Environmental Characteristics .....	15
Physical Characteristics .....	15
Graphs.....	16
Certifications.....	17
EMC Compliance .....	17
EC Declaration of Conformity - EMC .....	17
Australia & New Zealand Declaration of Conformity—EMC .....	17
Safety Compliance.....	18
EC Declaration of Conformity – Low Voltage.....	18
Environmental Compliance .....	18
End-Of-Life Handling .....	18
Restriction of Hazardous Substances (RoHS).....	18
Contact Teledyne LeCroy.....	19
Appendix A .....	20

## Safety Instructions

This section contains instructions that must be observed to keep this oscilloscope accessory operating in a correct and safe condition. You are required to follow generally accepted safety procedures in addition to the precautions specified in this section.

**The overall safety of any system incorporating this accessory is the responsibility of the assembler of the system.**

## Symbols

These symbols may appear on the probe body or in this manual to alert you to important safety considerations.



**WARNING.** High Voltage, risk of electric shock.



**CAUTION.** Potential for damage to probe or instrument it is connected to. Attend to the accompanying information to protect against personal injury or damage. Do not proceed until conditions are fully understood and met.



**ELECTROSTATIC DISCHARGE (ESD) HAZARD.** The probe is susceptible to damage if anti-static measures are not taken.



**DOUBLE INSULATION**



**PROTECTIVE (EARTH) TERMINAL**

## Precautions

- **Connect and disconnect properly.** Connect probe to the measurement instrument before connecting the test leads to a circuit/signal being tested.
- **Use only within operational environment listed.** Do not use in wet or explosive atmospheres.
- **Use indoors only.**
- **Keep product surfaces clean and dry.**
- **Be careful with sharp tips.** The tips may cause bodily injury if not handled properly.
- **Do not operate with suspected failures.** Do not use the probe if any part is damaged. Cease operation immediately and sequester the probe from inadvertent use.
- **Be careful not to damage the insulation surface** when making measurements.

## CP031 Current Probe

---

- **Never install or remove the probe on bare conductors which are energized.** The transformer core and shield are grounded but not insulated and may contact the conductor when the locking lever is open.
- To avoid short circuits and accidents that could result in injury or death, use the CP031 current probe only with conductors carrying 300 V or less.
- To prevent short circuits and electric shock when conductors being measured carry less than 300 V but more than the safe voltage level (SELV-E) make sure that the conductors to be measured are insulated with material conforming to:
  - Overvoltage Category I, basic insulation requirement for working voltage of 300 V
  - Pollution degree 2

## Operating Environment

The accessory is intended for indoor use and should be operated in a clean, dry environment. Before using this product, ensure that its operating environment is maintained within these parameters:

**Temperature:** 0° to 40° C

**Humidity:** ≤ 80% relative humidity (non-condensing)

**Altitude:** up to 2000 m (6562 feet)

# Overview

## Description

The CP031 uses a combination of Hall effect and transformer technology which enables measurements to be made on DC, AC and impulse currents. It has a 100 MHz bandwidth and is designed to measure continuous currents up to 30 Amp.

The probe can be used with a WaveSurfer, WaveRunner 6000, or WavePro 7000 series oscilloscope with firmware 4.3.0.0 or higher. With the ProBus interface, the CP031 becomes an integral part of the oscilloscope. The bandwidth limit, auto zero and degauss functions are all controlled from the oscilloscope's graphical user interface. The oscilloscope provides power to the probe, so no external power supply is needed.

## Key Features

- Highly accurate current measurements
- Easy current measurements
- Wide bandwidth
- Compact
- Over-current protected

## Accessories

Certificate of Calibration

Instruction Manual CP031-OM-E

# Operation

## Precautions

The sensor head is a precision assembly consisting of a molded component with a ferrite core and a Hall effect element. It may be damaged if subjected to sudden changes in temperature, mechanical strain or shock.

The mating surfaces of the sensor are precision ground and should be treated with care. If there is any type of dust or dirt on the mating surfaces of the sensor head, measurements may be impaired.

Accurate measurements may not be possible in locations subject to strong magnetic fields such as transformers and high-current conductors, or in locations subject to strong external electric fields.

## Connecting the Probe to the Test Instrument

The CP031 probe has been designed for use with the WaveSurfer, WaveRunner 6000, WavePro 7000, and WaveMaster series Teledyne Lecroy oscilloscopes equipped with the ProBus interface. Attach the probe output connector to the oscilloscope input connector. The oscilloscope will recognize the probe, set the oscilloscope input termination to 1 M $\Omega$  and activate the probe control functions in the user interface. To use the CP031 with a WaveMaster scope, the AP-1M impedance adapter is required.

## Connecting the Probe to the Test Circuit

The CP031 has been designed with a movable split core, eliminating the need to break the conductor for the core to slip around the conductor.

To connect:

1. Pull the slider, so that the clamp opens.
2. Align the sensor so that the current direction indicator corresponds to the direction of current flow in the conductor.
3. Close the slider on the sensor head until the "UNLOCK" indication disappears and the "LOCK" indication appears.
4. Verify that the opening lever is firmly locked and the clamp is securely closed.

**NOTE:** Never use this probe on bare conductors. The core and shield are grounded and any voltage applied to the conductor may cause damage the probe or the circuit under test.

## Operation with a Teledyne LeCroy Oscilloscope

The probe can be controlled through the Vertical Setup dialog for the channel to which the probe is connected.

Turning the **VOLTS/DIV** knob will control the oscilloscope's scale factor to give full dynamic range from 20 mA/div to 50 A/div.

The CP031 probe dialog (a tab behind the channel setup dialog) allows for the selection of the probe's coupling (**DC, Grounded** or **AC**), **AUTO ZERO**, **DEGAUSS PROBE** and **Probe BWL** functions, limiting the system bandwidth to 20 MHz or maximum bandwidth (BWL Off).

### Bandwidth Limit

The CP031 is capable of switching the bandwidth from **Full** (maximum bandwidth) to **20 MHz** by selecting the bandwidth adjustment in the channel menu.

### Auto Zero

The CP031 incorporates an Auto Zero function to remove the DC offset from the current probe. Auto Zero must be invoked by the user. After several minutes of warm-up, or when the probe is exposed to a large shift in ambient temperature, some DC offset drift may occur. To initiate an Auto Zero cycle, touch the CP031 tab of the (Channel) Vertical Setup dialog, then touch **AUTO ZERO**.

### Degauss Probe

If the probe has been magnetized by external magnetic field or by excessive input, the core can be demagnetized by opening the CP031 dialog and touching **DEGAUSS PROBE**. The demagnetizing process takes about 5 seconds and should always be performed before taking a measurement.

Without clamping the probe around a conductor, slide the opening lever to close and lock the probe and touch **DEGAUSS PROBE** twice.

An Auto Zero is automatically performed as part of the degauss cycle.

## Care and Maintenance

### Cleaning

The exterior of the probe and cable should be cleaned only using a soft cloth moistened with water or isopropyl alcohol. The use of abrasive agent, strong detergents or other solvents may damage the probe.



**CAUTION.** The probe case is not sealed and should never be immersed in any fluid.

### Calibration Interval

The recommended calibration interval is one year. Adjustment should only be performed by qualified personnel. (A Performance Verification / Adjustment procedure is included in this manual.)

### Service Strategy

Defective probes must be returned to a Teledyne Lecroy service facility for diagnosis and exchange. A defective probe under warranty will be replaced with a factory refurbished probe. A probe that is not under warranty can be exchanged for a factory refurbished probe. A modest fee is charged for this service. A defective probe must be returned in order to receive credit for the probe core.

### Troubleshooting

If the probe is not operating properly the problem may be the way in which it is used. Before assuming the probe is defective, perform the following troubleshooting procedures:

1. Verify using on the Teledyne Lecroy oscilloscope running firmware 4.3.0.0 or higher. The firmware version of your oscilloscope can be verified by selecting **Utilities > Utilities Setup > Status** tab.
2. Waveform is inverted — Make sure the arrow on the slider is in the direction of the current flow.
3. No signal — Make sure the slider is closed and locked.

## Returning a Defective Probe

Contact your local Teledyne Lecroy sales representative to find out where to return the product. All returned products should be identified by model number and serial number. Provide your name and contact number and if possible describe the defect or failure. In case of products returned to the factory, a Return Authorization Number (RAN) must be used. Contact your nearest Teledyne Lecroy office, or the New York Customer Care Center, to receive a RAN.

**Return shipment should be prepaid. Teledyne Lecroy cannot accept COD or Collect Return shipments.** We recommend air-freighting.

1. Contact your local Teledyne Lecroy sales or service representative to obtain a Return Authorization Number.
2. Remove all accessories from the probe. Do not include the manual.
3. Pack the probe in its case, surrounded by the original packing material (or equivalent) and box.
4. Label the case with a tag containing:
  - The RAN
  - Name and address of the owner
  - Probe model and serial number
  - Description of failure
5. Package the probe case in a cardboard shipping box with adequate padding to avoid damage in transit.
6. Mark the outside of the box with the shipping address given to you by the Teledyne Lecroy representative; be sure to add the following:
  - ATTN: <RAN assigned by the Teledyne Lecroy representative>
  - FRAGILE
7. Insure the item for the replacement cost of the probe.
8. **If returning a probe to a different country, also:**
  - Mark shipments returned for service as a "Return of US manufactured goods for warranty repair/recalibration."
  - If there is a cost involved in the service, put the service cost in the value column and the replacement value in the body of the invoice marked "For insurance purposes only."
  - Be very specific as to the reason for shipment. Duties may have to be paid on the value of the service.

## Performance Verification

This procedure can be used to verify the warranted characteristics of the CP031 Current Probe. The recommended calibration interval for the model CP031 Current Probe is one year. The complete performance verification procedure should be performed as the first step of annual calibration. Performance verification can be completed without removing the probe covers or exposing the user to hazardous voltages. Test results can be recorded on a photocopy of the Test Record provided at the end of the manual.

Adjustment should only be attempted if a parameter measured in the Performance Verification Procedure is outside the specification limits. Adjustment should only be performed by qualified personnel.

The warranted characteristics of the CP031 Current Probe are valid at any temperature within the Environmental Characteristics listed in the Specifications. However, some of the other test equipment used to verify the performance may have environmental limitations required to meet the accuracy needed for the procedure. Make sure that the ambient conditions meet the requirements of all the test instruments used in his procedure.

**NOTE:** Operation of the CP031 controls as described requires software version 4.3.0.0 or higher. Select **Utilities > Utilities Setup** , then open the **Status tab** to confirm the version. Contact your local Teledyne Lecroy representative if the software in your oscilloscope requires updating.

## Test Equipment Required

The following table lists the test equipment and accessories (or their equivalents) which are required for performance verification of the CP031 Current Probe. Because the input and output connector types may vary on different brands and models of test instruments, additional adapters or cables may be required.

**Table 1. List of required equipment.**

Description	Minimum Requirements	Test Equipment Examples
Wide Band Oscilloscope	Minimum 200 MHz bandwidth ProBus interface equipped Software version 4.3.0.0 or higher	Teledyne LeCroy WaveRunner 6030A
Digital Multimeter (2 required)	DC: 0.1% Accuracy 5½ digit resolution	Agilent Technologies 34401A or Fluke 8842A-09
Function Generator	50 Hz sine wave output 3 Vrms into 50Ω	Agilent Technologies 33120A or Stanford Research Model DS340

Description	Minimum Requirements	Test Equipment Examples
Calibration Fixture, 100 Turn Loop	100 Turn loop in series with $0.5\Omega \pm 0.1\%$ resistor with sense terminals	Teledyne LeCroy CP031-CF02
Calibration Fixture	ProBus Extension Cable	Teledyne LeCroy PROBUS-CF01
Banana Plug Adapter	Female BNC to Dual Banana Plug	Pomona 1269
Patch Cables (4 required)	Male Banana to Male Banana, 12"	Pomona B-12-0 (black) Pomona B-12-2 (red)
BNC Adapter	BNC Male to Dual Banana Jack	Pomona 1296

## Preliminary Procedure

1. Connect the CP031 to the channel 1 input of the oscilloscope and completely close the probe slider.
2. Turn the oscilloscope on and allow at least 30 minutes warmup time for the CP031 and test equipment before performing the Verification Procedure.
3. Turn on the other test equipment and allow these to warm up for the time recommended by the manufacturer.
4. While the instruments are reaching operating temperature, make a photocopy of the Performance Verification Test Record (located in Appendix A), and fill in the necessary data.

## Functional Check


The functional check will verify the basic operation of the probe functions.

It is recommended that the Functional Check be performed prior to the Performance Verification Procedure.

1. Select Channel 1 and verify that the probe bandwidth is set to **Full (BWL OFF)**.
2. Verify that the CP031 is sensed and the **CP031** tab appears behind the channel setup dialog.
3. On the CP031 tab, degauss the probe by touching **DEGAUSS** button, then **OK**.
4. Verify that "**Performing Degauss on CP031....**" is displayed at the bottom of the screen and no error message remains displayed.

## CP031 Current Probe

## Check LF Accuracy

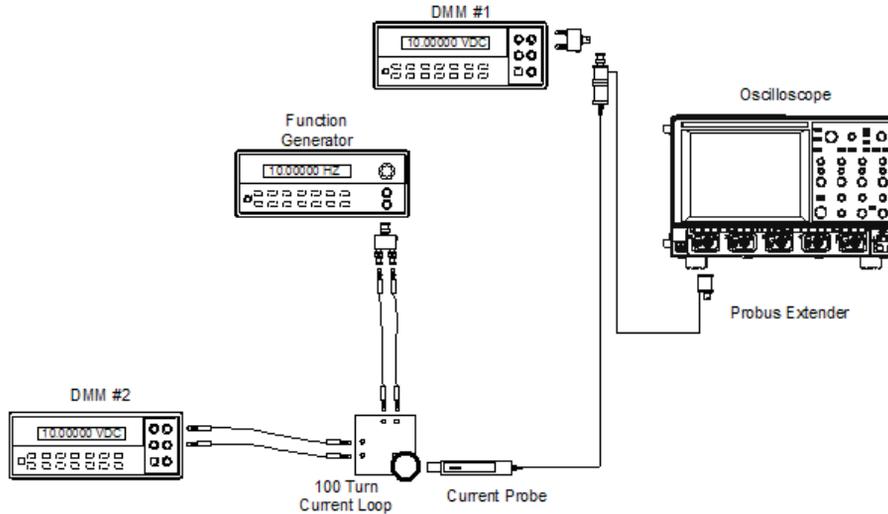

**Figure 1. LF Accuracy Test set up.**

1. Set the Function generator to 50 Hz sine wave. Output voltage at 3 Vrms with 50Ω output.
2. Remove the CP031 from the oscilloscope and reconnect using the ProBus extension cable. Connect the BNC male connector of the ProBus extension to DMM #1 using a BNC Female to Dual Banana adapter.
3. Using Banana Patch cords and the BNC to Dual Banana Plug adapter, connect the 'V Source' and 'V Return' terminals of the 100 Turn Calibration Loop to the output of the Function Generator.
4. Connect the Current Sense terminals of the 100 Turn Calibration Loop to the voltage inputs of DMM #2.
5. Set both DMMs to measure AC Volt.
6. With the CP031 removed from any signal and the slider returned to the LOCKED position, degauss the probe by pressing the **DEGAUSS** button (located in the CP031 dialog), then **OK**.
7. Open the CP031 slider and position the probe input around the 100 Turn loop. Close and LOCK the slider.
8. Adjust the Function generator voltage until the voltage measured at the 'Current Sense' terminals (DMM #2) reads 50 mV ±0.05 mV. (This corresponds to 10 A at the probe head).
9. Record the voltage measured by DMM #1 on the Test Record.
10. Verify that the measured voltage is between 0.989 volt and 1.011 volt.

## Adjustment Procedure

This procedure can be used to adjust the warranted characteristics of the CP031 Current Probe. This procedure should be used if a parameter measured in the Performance Verification Procedure is outside of the specification limits. Adjustment should only be performed by qualified personnel.

The warranted characteristics of the CP031 Current Probe are valid at any temperature within the Environmental Characteristics listed in the Specifications. However, some of the other test equipment used to verify the performance may have environmental limitations required to meet the accuracy needed for the procedure. Make sure that the ambient conditions meet the requirements of all the test instruments used in this procedure.

**NOTE:** Operation of the controls as described requires oscilloscope software version 4.3.0.0 or higher. Select Utilities, Utilities Setup, then open the Status tab to confirm the version. Contact your local Teledyne Lecroy representative if the software in your oscilloscope requires updating.

## Test Equipment Required

The following table lists the test equipment and accessories, or their equivalents, which are required for adjustment of the CP031 Current Probe. Because the input and output connector types may vary on different brands and models of test instruments, additional adapters or cables may be required.

**Table 2. List of required equipment.**


Description	Minimum Requirements	Test Equipment Examples
Wide Band Oscilloscope	Minimum 200 MHz bandwidth ProBus interface equipped Software version 4.3.0.0 or higher	Teledyne LeCroy WaveRunner 6030A
Digital Multimeter (2 required)	DC: 0.1% Accuracy 5½ digit resolution	Agilent Technologies 34401A, or Fluke 8842A-09
Function Generator	50 Hz sine wave output 3 Vrms into 50 Ω	Agilent Technologies 33120A, or Stanford Research Model DS340
Calibration Fixture, 100 Turn Loop	100 Turn loop in series with 0.5 Ω ±0.1% resistor with sense terminals	Teledyne LeCroy CP031-CF02
Banana Plug Adapter	Female BNC to Dual Banana Plug	Pomona 1269
Calibration Fixture	ProBus Extension Cable	Teledyne LeCroy PROBUS-CF01
Patch Cables (4 required)	Male Banana to Male Banana, 12"	Pomona B-12-0 (black) or Pomona B-12-2 (red)
BNC Adapter	BNC Male to Dual Banana Jack	Pomona 1296

## CP031 Current Probe

### Preliminary Procedure

1. Remove the probe compensation box circuit board by removing the two screws from the cable end of the compensation box and sliding the circuit board out of the box.
2. Connect the CP031 compensation board to the channel 1 input of the oscilloscope through the ProBUS extension cable, and completely close the probe slider.
3. Turn the oscilloscope on and allow at least 30 minutes warmup time for the CP031 and test equipment before performing the Verification Procedure.

### Adjust LF Accuracy

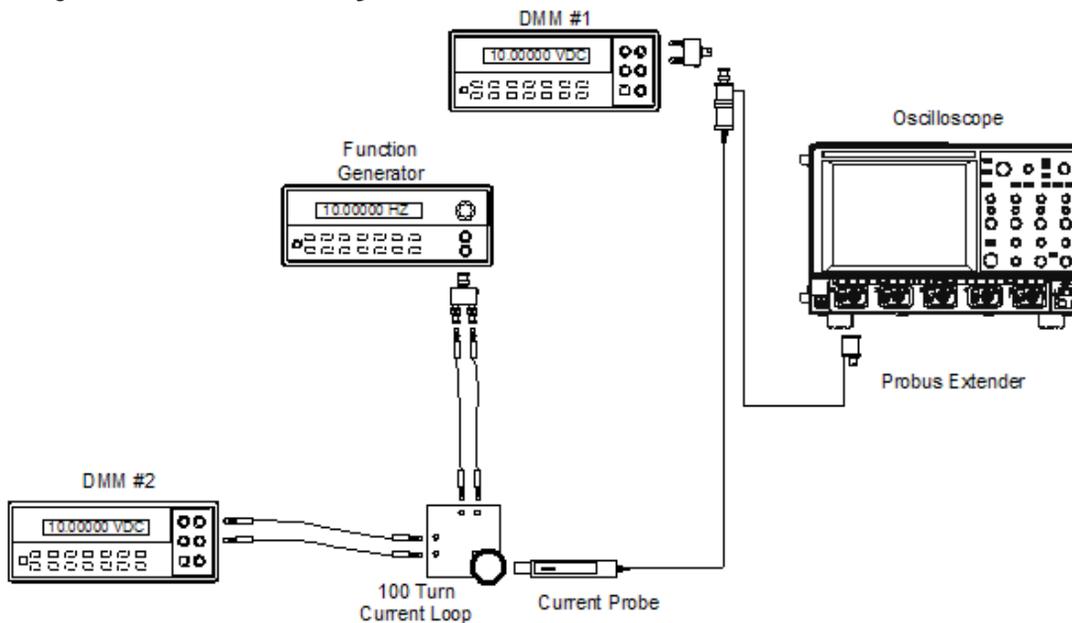

**Figure 2. LF accuracy adjustment set up.**

1. Set the Function Generator to 50 Hz, sinewave output at 3 Vrms with 50  $\Omega$  output.
2. Connect BNC male of ProBUS extension to DMM #1 using BNC Female to Dual Banana adapter.
3. Using banana patch cords, connect the 'V Source' and 'V Return' terminals of the 100 Turn Calibration Loop, to the output of the Function Generator using the BNC to Dual Banana Plug Adapter output. (Refer to Figure 2.)
4. Connect the Current Sense terminals of the 100 Turn Calibration Loop to the voltage inputs of DMM #2.

5. Set both DMMs to measure AC Volt.
6. With the CP031 removed from any signal and the slider returned to the LOCKED position, degauss the probe by touching **DEGAUSS** (on the CP031 dialog), then **OK**.
7. Open the CP031 slider and position the probe input around the 100 Turn loop. Close and LOCK the slider.
8. Adjust the Function Generator voltage until the voltage measured at the 'Current Sense' terminals (DMM #2) is  $50 \text{ mV} \pm 0.05 \text{ mV}$ . (This corresponds to 10 A at the probe head).
9. Adjust variable resistor VR202 on the PCB until the voltage measured on DMM #1 is as close to 2X the voltage measured on DMM #2.
10. Verify that the measured voltage is between 0.990 V and 1.01 V.
11. Disconnect the probe from the test setup.
12. Re-assemble the compensation box by sliding the circuit board back into the box and inserting and fastening the two screws.

# Specifications

## Nominal Characteristics

Nominal characteristics describe parameters and attributes which are guaranteed by design, but do not have associated tolerances.

Maximum Continuous Input Current	30 A <sub>rms</sub> (Refer to Figure 3)
Maximum Peak Current	50 A <sub>peak</sub> , noncontinuous
Insertion Impedance	Refer to Figure 4
Intended Output Load	1 MΩ
Maximum Permitted Circuit Voltage	300 V, CAT I (Insulated conductor)

## Warranted Characteristics

Warranted characteristics describe parameters which have guaranteed performance. Unless otherwise noted, tests are provided in the Performance Verification Procedure for all warranted specifications.

Guaranteed at 23 °C ±5 °C (73 °F ±9 °F) after power has been applied for 30 minutes.

Amplitude Accuracy	±1.0% of reading ±10 mA; to 30 A <sub>rms</sub> ±2.0% of reading; to 50 A <sub>peak</sub> (DC, 45 to 65 Hz)
--------------------	---

## Typical Characteristics

Typical characteristics describe parameters which do not have guaranteed performance; however are representative of the average performance from a sample of several probes. Tests for typical characteristics are not provided in the Performance Verification procedure.

Sensitivity*	20 mA/div* to 50 A/div.
Output voltage	0.1 V/A
Sensitivity Temperature Coefficient	±2% or less. (from 0° to +40 °C, 32 °F to 104 °F)
Noise	Equivalent to 2.5 mA <sub>rms</sub> or less (BW of measuring instrument: 20 MHz)
Bandwidth	DC to 100 MHz. Rise Time ≤ 3.5 ns

\* Lower sensitivity may change with different oscilloscope models.

## Environmental Characteristics

Operating Temperature Humidity	0 to 40 °C (32 °F to 104 °F) ≤ 80% relative humidity (non-condensing)
Storage Temperature Humidity	-10 °C to 50 °C (14 °F to 122 °F) ≤ 80% relative humidity (non-condensing)
Usage	Indoor
Altitude	up to 2000 m (6562 feet)
Effect of External Magnetic Field	Equivalent to a maximum of 5 mA (in a DC or 60 Hz, 400 A/m magnetic field)

## Physical Characteristics

### Dimensions Probe

Length	175 mm (6.9 inch)
Width	18 mm (0.7 inch)
Height	40 mm (1.57 inch)

### Dimensions Compensation Box

Length	65 mm (2.6 inch)
Width	39 mm (1.5 inch)
Height	24 mm (0.9 inch)
Weight	240 g (8.5 oz.)
Maximum diameter of conductors to be measured	5 mm (0.2 inch)

# Graphs

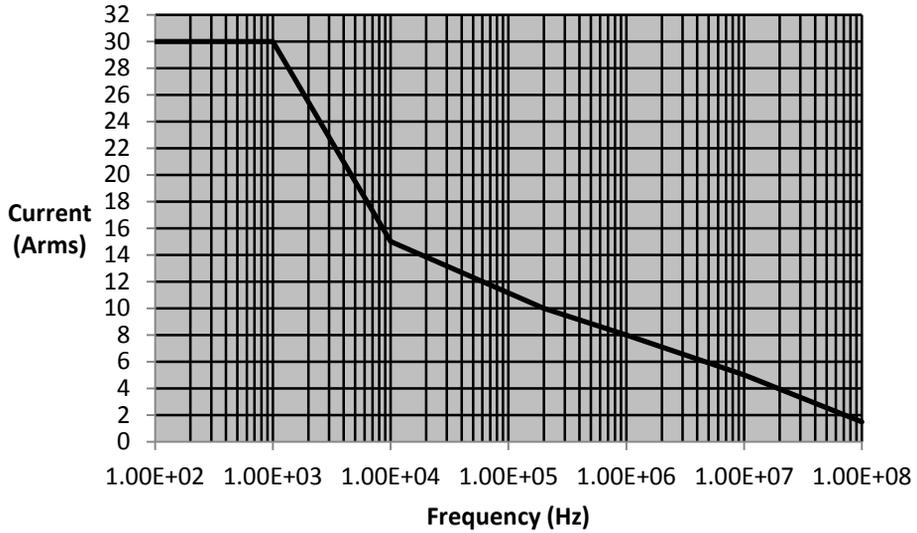


Figure 3. Maximum input current vs. frequency.

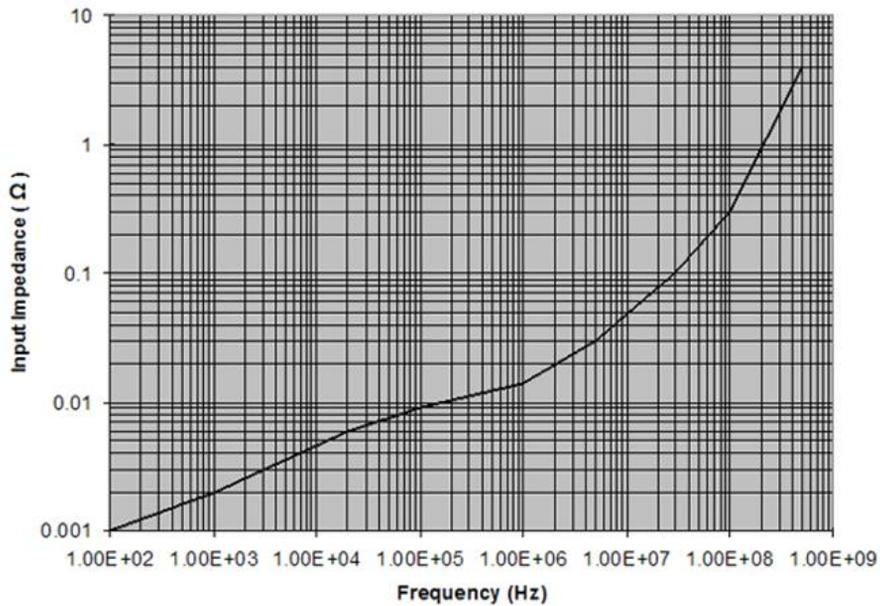


Figure 4. Insertion impedance vs. frequency.

## Certifications

This section contains the instrument's Electromagnetic Compatibility (EMC), Safety and Environmental certifications.

### EMC Compliance

#### ***EC Declaration of Conformity - EMC***

The probe meets intent of EC Directive 2004/108/EC for Electromagnetic Compatibility. Compliance was demonstrated to the following specifications as listed in the Official Journal of the European Communities:

EN 61326-1:2006, EN 61326-2-1:2006 EMC requirements for electrical equipment for measurement, control, and laboratory use.

#### **ELECTROMAGNETIC EMISSIONS:**

CISPR 11:2003, Radiated and Conducted Emissions Group 1, Class A <sup>1 2</sup>

#### **ELECTROMAGNETIC IMMUNITY:**

EN 61000-4-2:2001 Electrostatic Discharge, 4 kV contact, 8 kV air, 4 kV vertical/horizontal coupling planes <sup>3</sup>

EN 61000-4-3:2006 RF Radiated Electromagnetic Field, 3 V/m, 80-1000 MHz; 3 V/m, 1400 MHz - 2 GHz; 1 V/m, 2 GHz - 2.7 GHz <sup>3</sup>

- 1 Emissions which exceed the levels required by this standard may occur when the probe is connected to a test object.
- 2 This product is intended for use in nonresidential areas only. Use in residential areas may cause electromagnetic interference.
- 3 Meets Performance Criteria "B" limits of the respective standard: during the disturbance, product undergoes a temporary degradation or loss of function or performance which is self-recoverable.

#### **EUROPEAN CONTACT:**

Teledyne LeCroy Europe GmbH  
Waldhofer Str 104  
D-69123 Heidelberg  
Germany  
Tel: (49) 6221 82700

### ***Australia & New Zealand Declaration of Conformity—EMC***

Probe complies with the EMC provision of the Radio Communications Act per the following standards, in accordance with requirements imposed by Australian Communication and Media Authority (ACMA):

## CP031 Current Probe

---

CISPR 11:2003 Radiated and Conducted Emissions, Group 1, Class A, in accordance with EN61326-1:2006 and EN61326-2-1:2006.

### AUSTRALIA / NEW ZEALAND CONTACTS:

Vicom Australia Ltd.  
1064 Centre Road  
Oakleigh, South Victoria 3167  
Australia

Vicom New Zealand Ltd.  
60 Grafton Road  
Auckland  
New Zealand

## Safety Compliance

### *EC Declaration of Conformity – Low Voltage*

The probe meets intent of EC Directive 2006/95/EC for Product Safety. Compliance was demonstrated to the following specifications as listed in the Official Journal of the European Communities:

EN 61010-1:2010 Safety requirements for electrical equipment for measurement, control, and laboratory use – Part 1: General requirements

EN 61010-2:032:2002 Safety requirements for electrical equipment for measurement, control, and laboratory use – Part 2-032: Particular requirements for hand-held and hand-manipulated current sensors for electrical test and measurement

## Environmental Compliance

### *End-Of-Life Handling*



The probe is marked with this symbol to indicate that it complies with the applicable European Union requirements to Directives 2002/96/EC and 2006/66/EC on Waste Electrical and Electronic Equipment (WEEE) and Batteries.

The probe is subject to disposal and recycling regulations that vary by country and region. Many countries prohibit the disposal of waste electronic equipment in standard waste receptacles. For more information about proper disposal and recycling of your Teledyne LeCroy product, please visit [teledynelecroy.com/recycle](http://teledynelecroy.com/recycle).

### *Restriction of Hazardous Substances (RoHS)*

The product and its accessories conform to the 2011/65/EU RoHS2 Directive, as it has been classified as Industrial Monitoring and Control Equipment (per Article 3, Paragraph 24) and is exempt from RoHS compliance until 22 July 2017 (per Article 4, Paragraph 3).

# Contact Teledyne LeCroy

Teledyne LeCroy Service Centers	
<p><b>United States and Canada - World Wide Corporate Office</b> Teledyne LeCroy Corporation 700 Chestnut Ridge Road Chestnut Ridge, NY, 10977-6499, USA Ph: 800-553-2769 / 845-425-2000 FAX: 845-578-5985 teledynelecroy.com <b>Support:</b> contact.corp@teledynelecroy.com <b>Sales:</b> customersupport@teledynelecroy.com</p>	<p><b>United States - Protocol Solutions Group</b> Teledyne LeCroy Corporation 3385 Scott Boulevard Santa Clara, CA, 95054, USA FAX: 408-727-0800 teledynelecroy.com <b>Sales and Service:</b> Ph: 800-909-7211 / 408-727-6600 contact.corp@teledynelecroy.com <b>Support:</b> Ph: 800-909-7112 / 408-653-1260 psgsupport@teledynelecroy.com</p>
<p><b>European Headquarters</b> Teledyne LeCroy SA 4, Rue Moïse Marcinihes Case postale 341 1217 Meyrin 1 Geneva, Switzerland Ph: + 41 22 719 2228 / 2323 /2277 FAX:+41 22 719 2233 contact.sa@teledynelecroy.com applications.indirect@teledynelecroy.com teledynelecroy.com/europe <b>Protocol Analyzers:</b> Ph: +44 12 765 03971</p>	<p><b>Singapore, Oscilloscopes</b> Teledyne LeCroy Singapore Pte Ltd. Blk 750C Chai Chee Road #02-08 Technopark @ Chai Chee Singapore 469003 Ph: ++ 65 64424880 FAX: ++ 65 64427811 <b>Singapore, Protocol Analyzers</b> Genetron Singapore Pte Ltd. 37 Kallang Pudding Road, #08-08 Tong Lee Building Block B Singapore 349315 Ph: ++ 65 9760-4682</p>
<p><b>China</b> Teledyne LeCroy Corporation Beijing Rm. 2001 - Office; Rm. 2002 - Service Center Unit A, Horizon Plaza No. 6, Zhichun Road, Haidian District Beijing 100088, China Ph: ++86 10 8280 0318 / 0319 / 0320 FAX:++86 10 8280 0316 <b>Service:</b> Rm. 2002 Ph: ++86 10 8280 0245</p>	<p><b>Korea</b> Teledyne LeCroy Korea 10th fl.Ildong Bldg. 968-5 Daechi-dong, Gangnam-gu Seoul 135-280, Korea Ph: ++ 82 2 3452 0400 FAX: ++ 82 2 3452 0490</p>
<p><b>Taiwan</b> LeColn Technology Co Ltd. Far East Century Park, C3, 9F No. 2, Chien-8th Road, Chung-Ho Dist., New Taipei City, Taiwan Ph: ++ 886 2 8226 1366 FAX: ++ 886 2 8226 1368</p>	<p><b>Japan</b> Teledyne LeCroy Japan Hobunsha Funchu Bldg, 3F 3-11-5, Midori-cho, Fuchu-Shi Tokyo 183-0006, Japan Ph: ++ 81 4 2402 9400 FAX: ++ 81 4 2402 9586 teledynelecroy.com/japan</p>

## CP031 Current Probe

# Appendix A

## Performance Verification Test Record

Photocopy this page and record the results of measurements made during the performance verification of the CP031 Current Probe on the copy. File the completed record as required by applicable internal quality procedures.

The sections in the test record correspond to the parameters tested in the performance verification procedure. The numbers preceding the individual data records correspond to the steps in the procedure that require the recording of data. Results recorded in the column labeled "Test Result" are the actual specification limit check. The test limits are included in all of these steps. Other measurements and the results of intermediate calculations that support the limit check are to be recorded in the column labeled "Intermediate Results".

Permission is granted to reproduce these pages for the purpose of recording test results.

**Model:** \_\_\_\_\_  
**Serial Number:** \_\_\_\_\_  
**Asset or Tracking Number:** \_\_\_\_\_  
**Date:** \_\_\_\_\_  
**Technician:** \_\_\_\_\_

## Equipment Used

	MODEL	SERIAL NUMBER	CALIBRATION DUE DATE
Digital Multimeter #1			
Digital Multimeter #2			
Function Generator <sup>1</sup>			N/A

<sup>1</sup>The function generator used in this Performance Verification Procedure is used for making relative measurements. The output of the generator is measured with a DMM or oscilloscope in this procedure. Thus, the generator is not required to be calibrated.

## CP031 Test Record

Step	Description	Test Result
Gain Accuracy	10 Probe Output (Spec limit: 0.495 - 0.505 V)	_____ V





700 Chestnut Ridge Road  
Chestnut Ridge, NY 10977  
USA

[teledynelecroy.com](http://teledynelecroy.com)